

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092318\
 Data File : PL040235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2018 12:24
 Operator : AJ\SJ
 Sample : J4777-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-02-0920-18-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:24:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.249	3.843	132.2E6	54229614	17.372	16.606
28)	SA Decachlor...	7.876	8.795	130.3E6	51021632	14.718	15.946
Target Compounds							
7)	B delta-BHC	0.000	4.885	0	8723451	N.D.	1.929 #
15)	B Endosulfa...	5.923f	0.000	188.6E6	0	18.151	N.D. #
16)	A 4,4'-DDD	5.834	6.566f	26341375	79146714	3.048	24.713 #
23)	Chlordane-1	4.009	0.000	70315407	0	186.819	N.D. #
24)	Chlordane-2	4.595	0.000	33028039	0	86.089	N.D. #
27)	Chlordane-5	5.923	0.000	188.6E6	0	454.645	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092318\
Data File : PL040235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2018 12:24
Operator : AJ\SJ
Sample : J4777-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:24:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

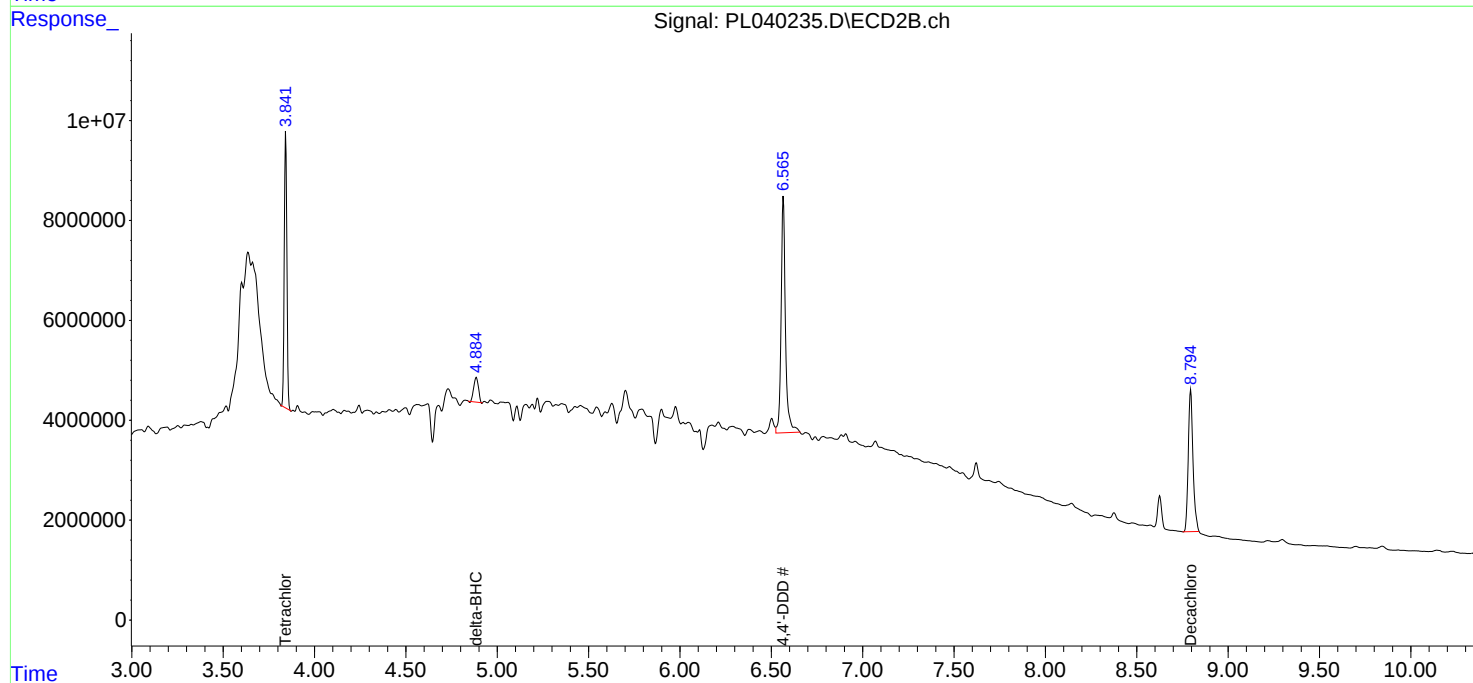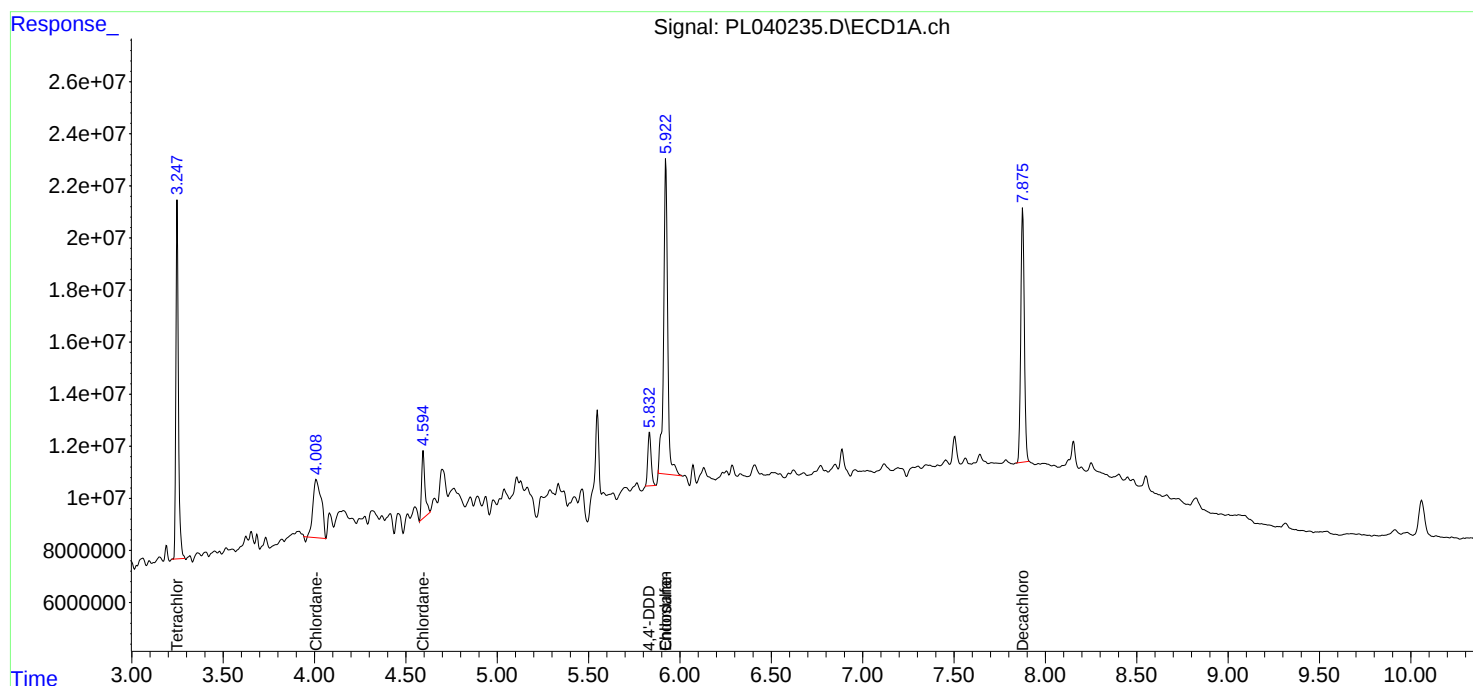


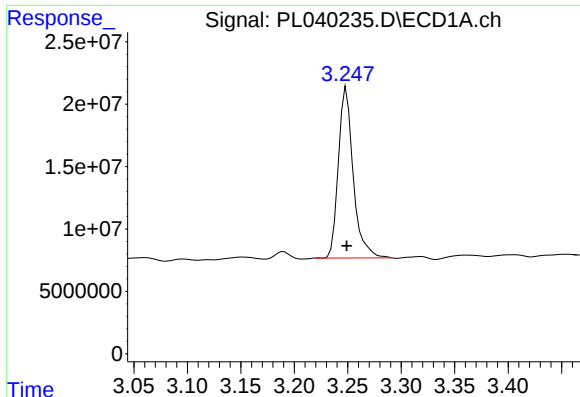

#1 Tetrachloro-m-xylene


R.T.: 3.249 min
Delta R.T.: 0.000 min
Response: 132164802
Conc: 17.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-D

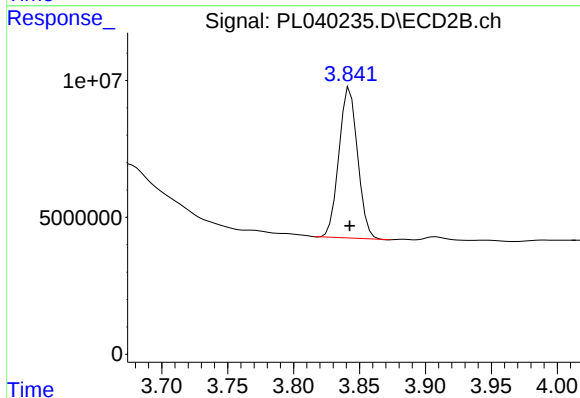


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 54229614
Conc: 16.61 ng/ml

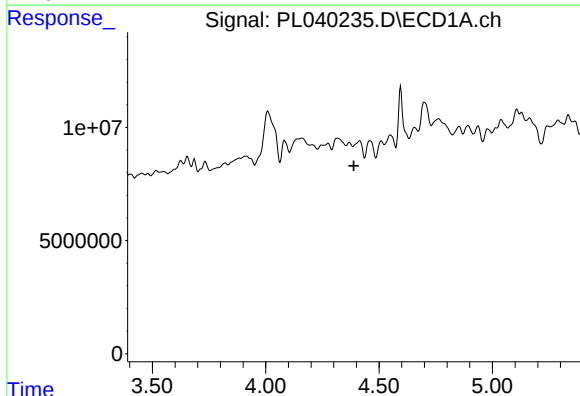


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.389 min
Response: 0
Conc: N.D.

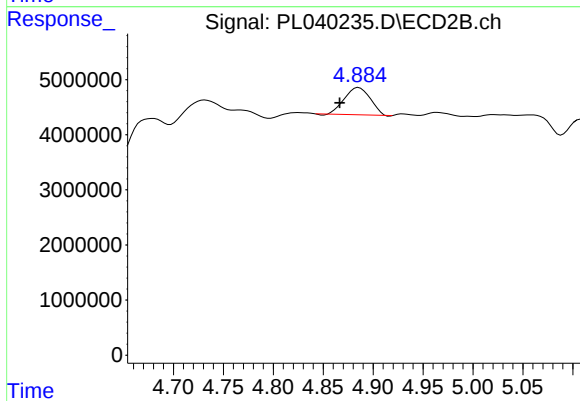

#7 delta-BHC


R.T.: 4.885 min
Delta R.T.: 0.019 min
Response: 8723451
Conc: 1.93 ng/ml

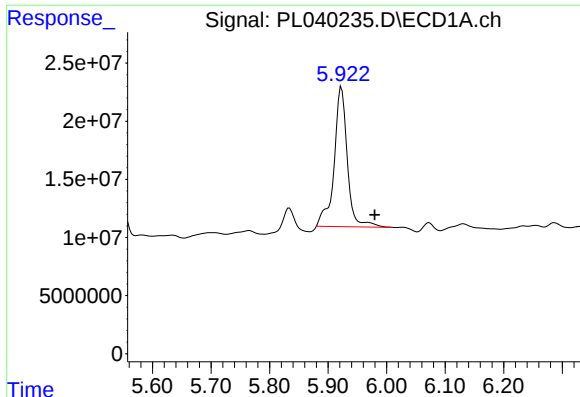

#15 Endosulfan II


R.T.: 5.923 min
Delta R.T.: -0.057 min
Response: 188561800
Conc: 18.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-D

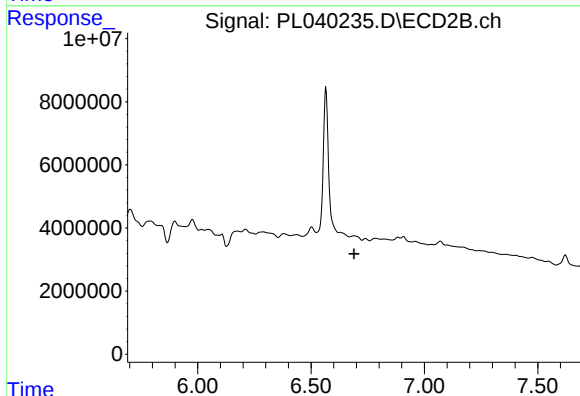


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.690 min
Response: 0
Conc: N.D.

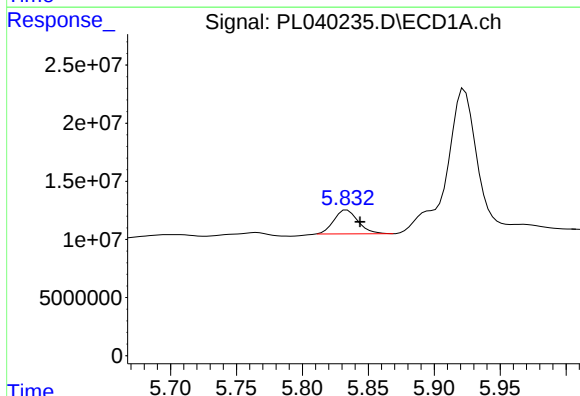


#16 4,4'-DDD

R.T.: 5.834 min
Delta R.T.: -0.010 min
Response: 26341375
Conc: 3.05 ng/ml

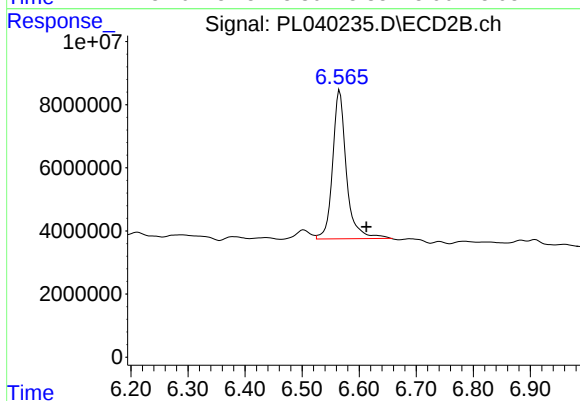

#16 4,4'-DDD


R.T.: 6.566 min
Delta R.T.: -0.047 min
Response: 79146714
Conc: 24.71 ng/ml

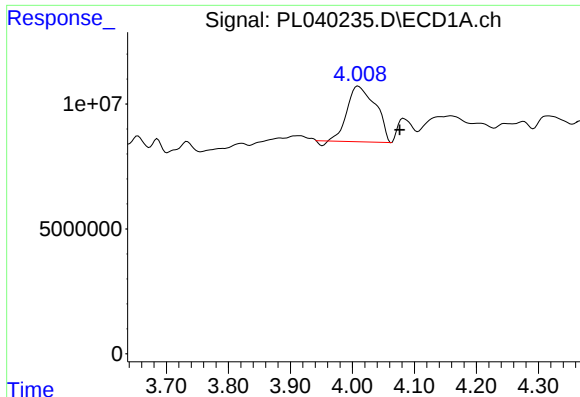

#23 Chlordane-1


R.T.: 4.009 min
Delta R.T.: -0.067 min
Response: 70315407
Conc: 186.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-D

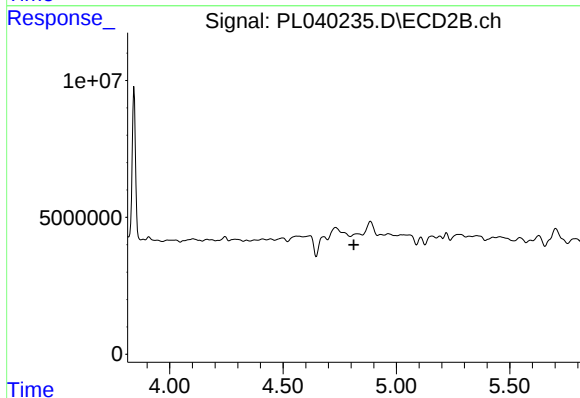


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.812 min
Response: 0
Conc: N.D.

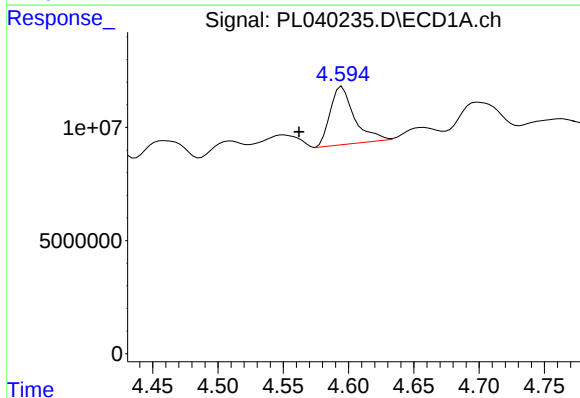


#24 Chlordane-2

R.T.: 4.595 min
Delta R.T.: 0.033 min
Response: 33028039
Conc: 86.09 ng/ml

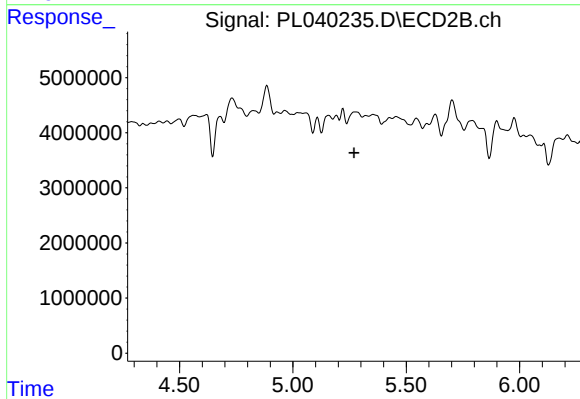

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.270 min
Response: 0
Conc: N.D.

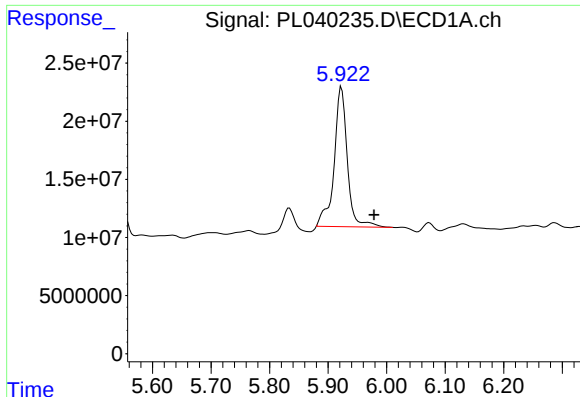

#27 Chlordane-5


R.T.: 5.923 min
Delta R.T.: -0.056 min
Response: 188561800
Conc: 454.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-D

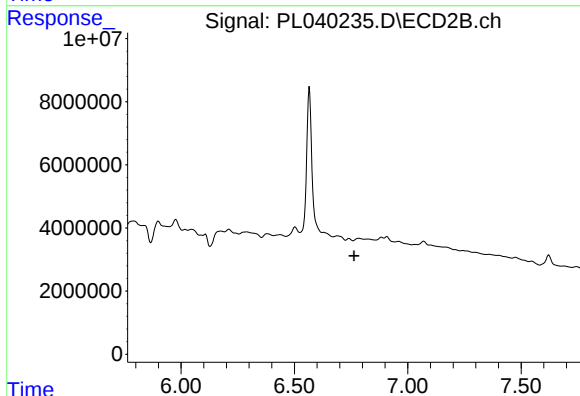


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

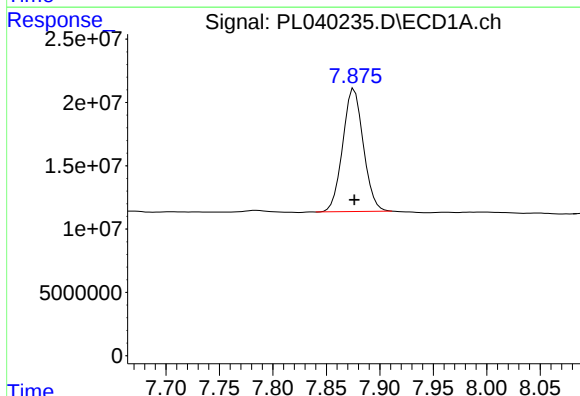

#28 Decachlorobiphenyl

R.T.: 7.876 min
Delta R.T.: 0.000 min
Response: 130341988
Conc: 14.72 ng/ml

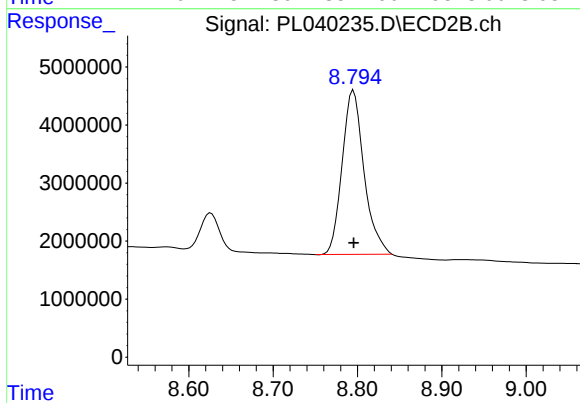

#28 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 51021632
Conc: 15.95 ng/ml