

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092318\
 Data File : PL040236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Sep 2018 12:38
 Operator : AJ\SJ
 Sample : J4777-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PL-02-0920-18-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:24:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.249	3.843	98431753	40465241	12.938	12.391
28)	SA Decachlor...	7.877	8.795	88706224	35119940	10.017	10.976
Target Compounds							
7)	B delta-BHC	0.000	4.886	0	9894799	N.D.	2.187 #
9)	A Endosulfan I	0.000	5.976f	0	8451690	N.D.	2.385 #
10)	B gamma-Chl...	0.000	5.901	0	2957902	N.D.	0.768 #
11)	B alpha-Chl...	0.000	5.976	0	8451690	N.D.	2.222 #
15)	B Endosulfa...	5.923f	0.000	171.1E6	0	16.470	N.D. #
16)	A 4,4'-DDD	5.834	6.566f	23642031	71693318	2.736	22.386 #
23)	Chlordane-1	4.008	0.000	66175266	0	175.819	N.D. #
24)	Chlordane-2	4.595	5.220	39461940	4362405	102.859	26.445 #
25)	Chlordane-3	0.000	5.901	0	2957902	N.D.	5.531 #
26)	Chlordane-4	0.000	5.976	0	8451690	N.D.	13.235 #
27)	Chlordane-5	5.923	0.000	171.1E6	0	412.546	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092318\
Data File : PL040236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Sep 2018 12:38
Operator : AJ\SJ
Sample : J4777-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:24:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

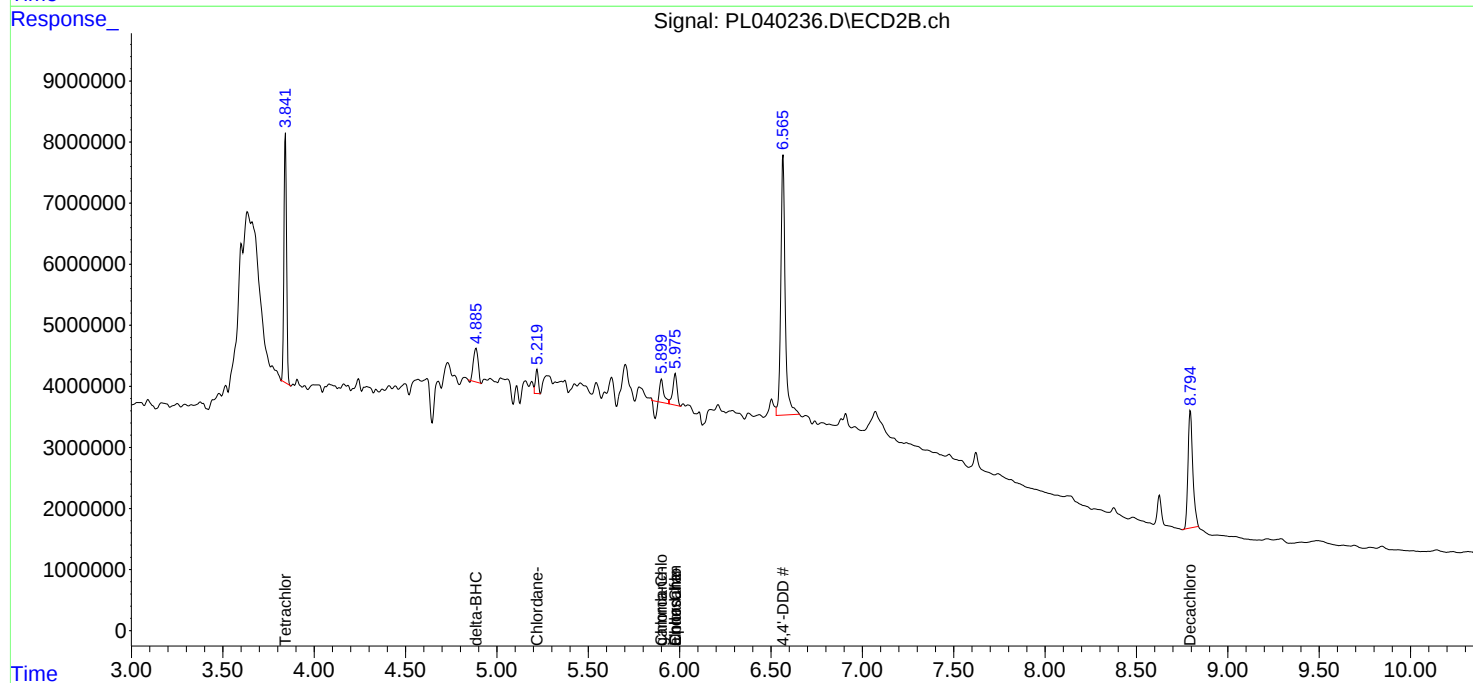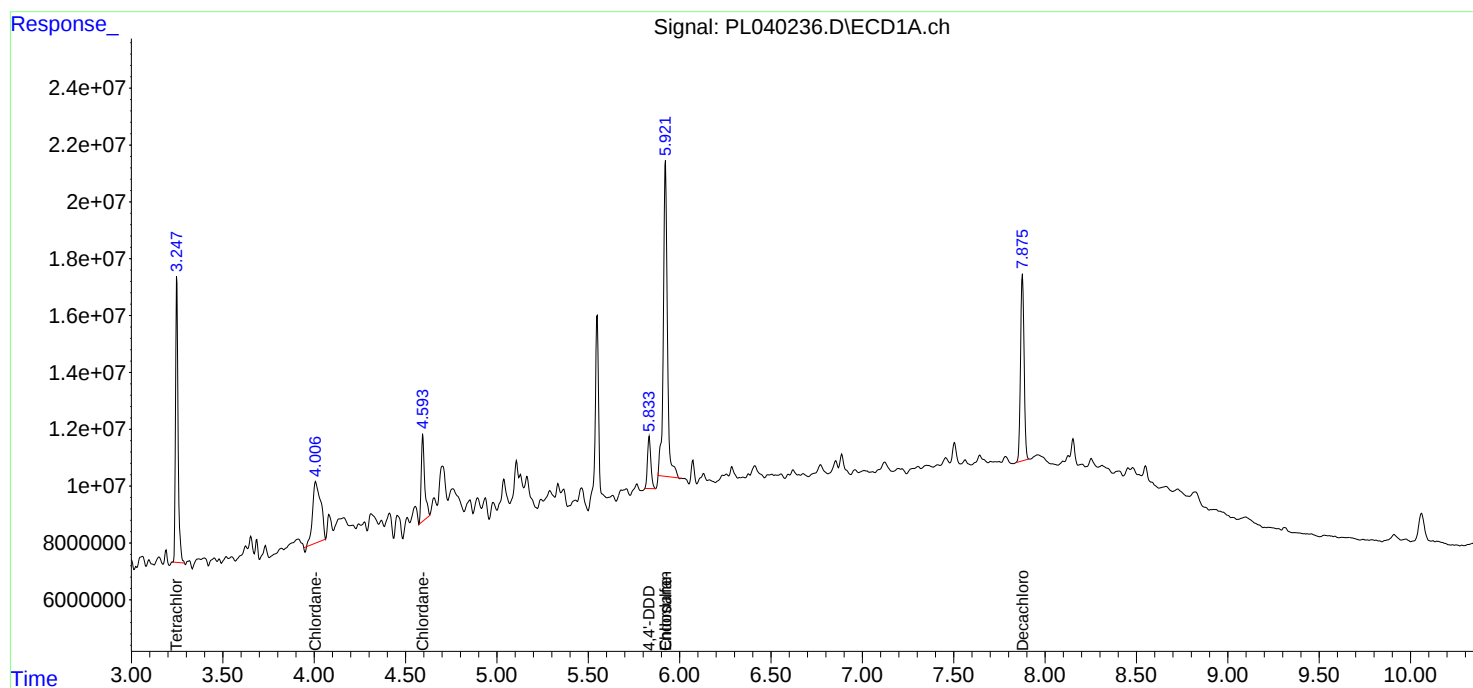


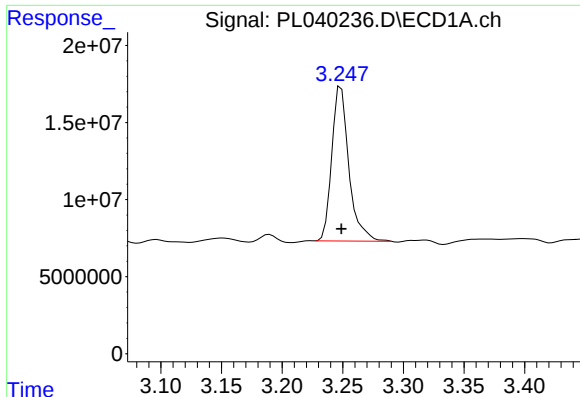

#1 Tetrachloro-m-xylene


R.T.: 3.249 min
Delta R.T.: 0.000 min
Response: 98431753
Conc: 12.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

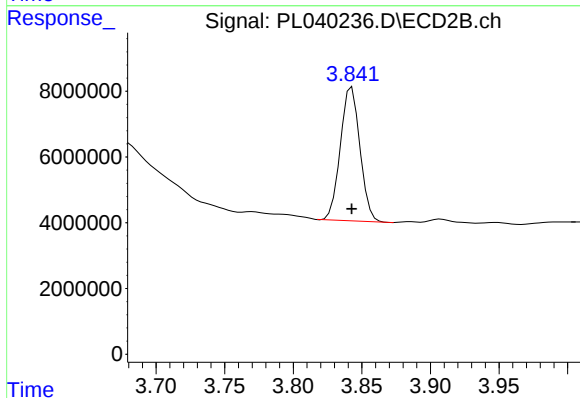


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 40465241
Conc: 12.39 ng/ml

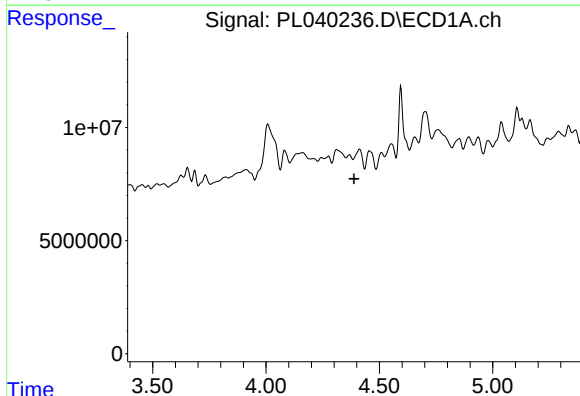


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.389 min
Response: 0
Conc: N.D.

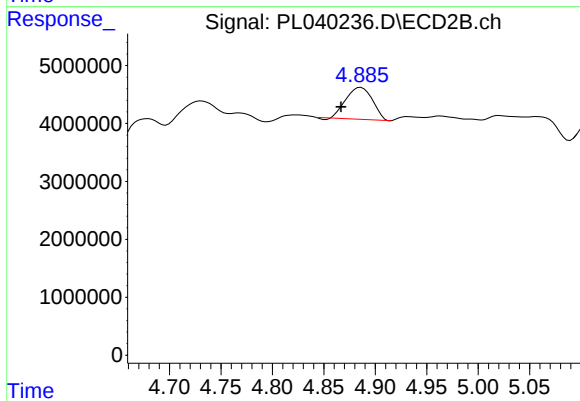

#7 delta-BHC


R.T.: 4.886 min
Delta R.T.: 0.019 min
Response: 9894799
Conc: 2.19 ng/ml

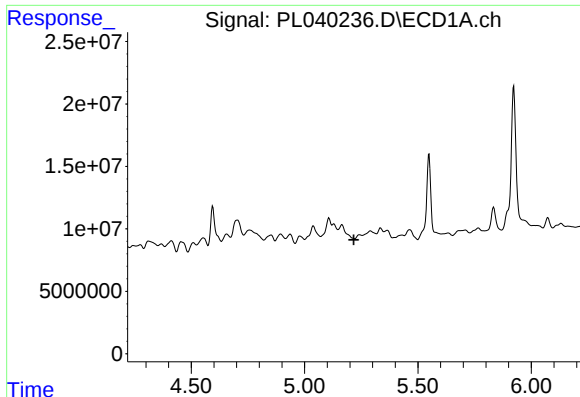

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.217 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

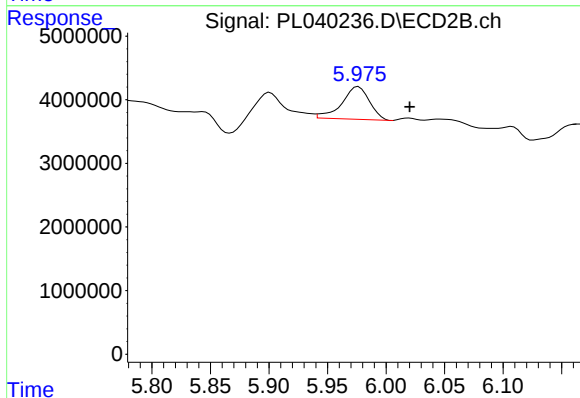


#9 Endosulfan I

R.T.: 5.976 min
Delta R.T.: -0.044 min
Response: 8451690
Conc: 2.38 ng/ml

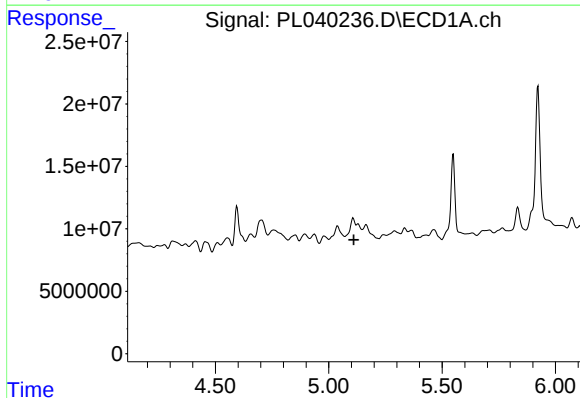


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.110 min
Response: 0
Conc: N.D.

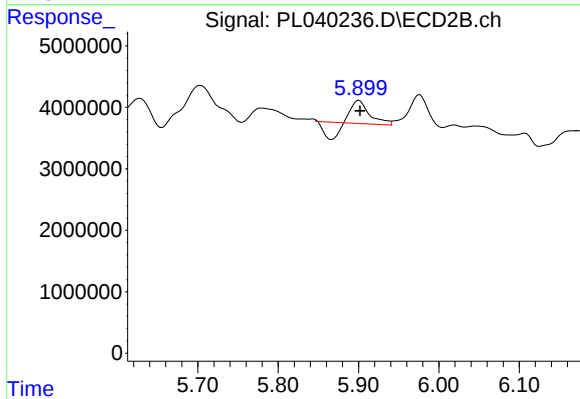

#10 gamma-Chlordane


R.T.: 5.901 min
Delta R.T.: -0.001 min
Response: 2957902
Conc: 0.77 ng/ml

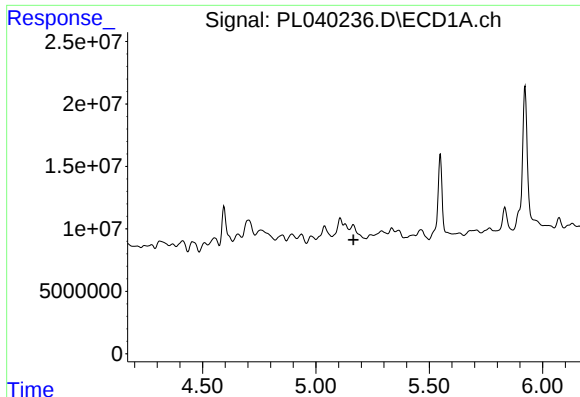

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

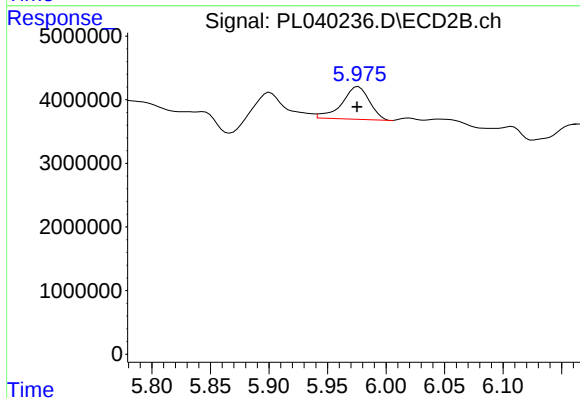


#11 alpha-Chlordane

R.T.: 5.976 min
Delta R.T.: 0.001 min
Response: 8451690
Conc: 2.22 ng/ml

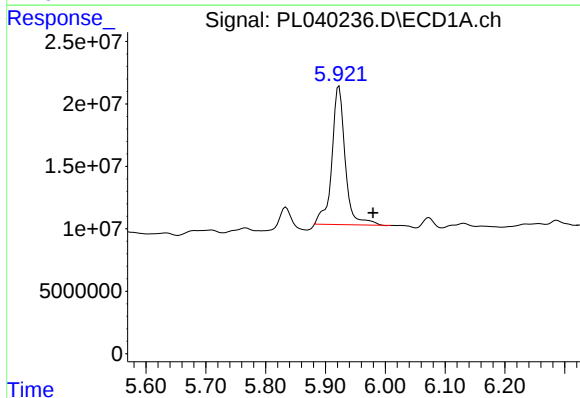


#15 Endosulfan II

R.T.: 5.923 min
Delta R.T.: -0.057 min
Response: 171101671
Conc: 16.47 ng/ml

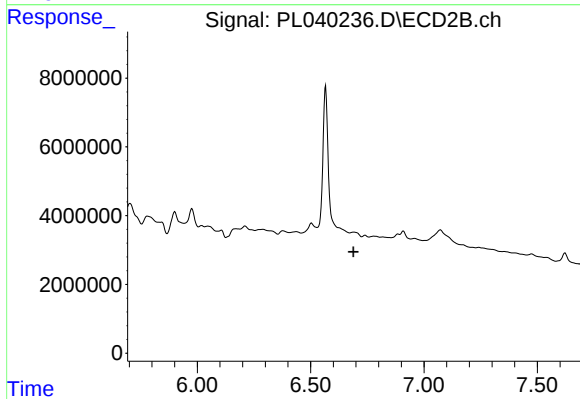

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.690 min
Response: 0
Conc: N.D.

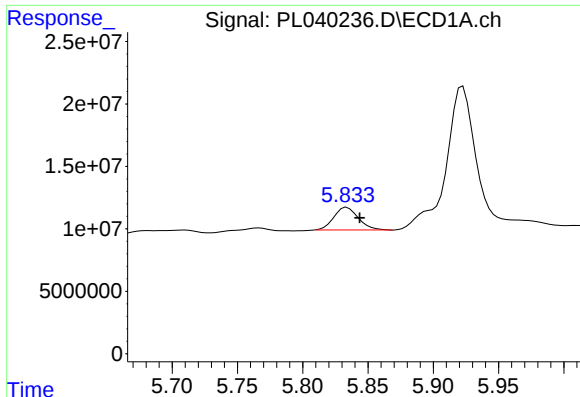

#16 4,4'-DDD


R.T.: 5.834 min
Delta R.T.: -0.010 min
Response: 23642031
Conc: 2.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

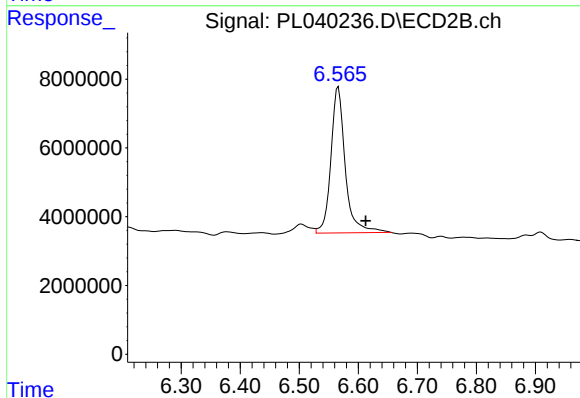


#16 4,4'-DDD

R.T.: 6.566 min
Delta R.T.: -0.047 min
Response: 71693318
Conc: 22.39 ng/ml

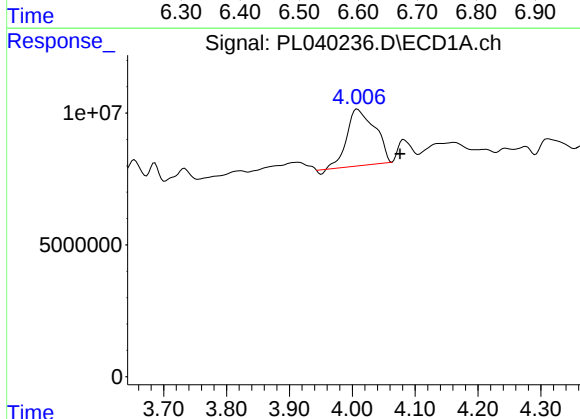


#23 Chlordane-1

R.T.: 4.008 min
Delta R.T.: -0.068 min
Response: 66175266
Conc: 175.82 ng/ml

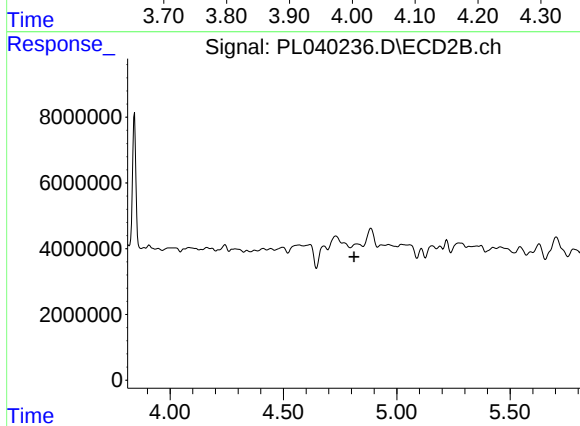

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.812 min
Response: 0
Conc: N.D.

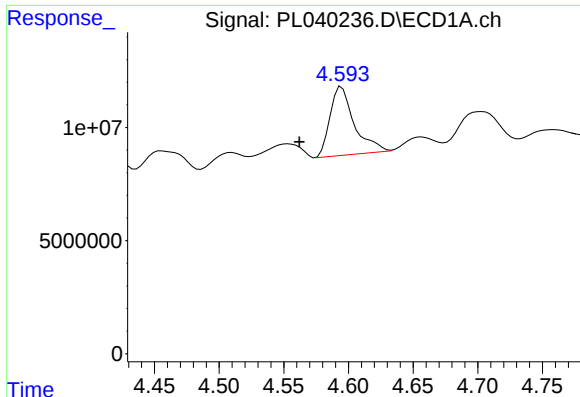

#24 Chlordane-2


R.T.: 4.595 min
Delta R.T.: 0.033 min
Response: 39461940
Conc: 102.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

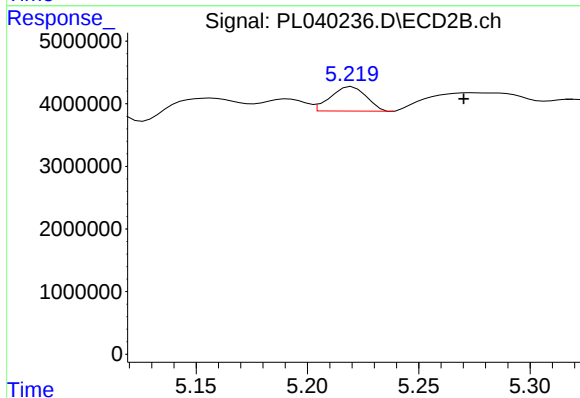


#24 Chlordane-2

R.T.: 5.220 min
Delta R.T.: -0.050 min
Response: 4362405
Conc: 26.44 ng/ml

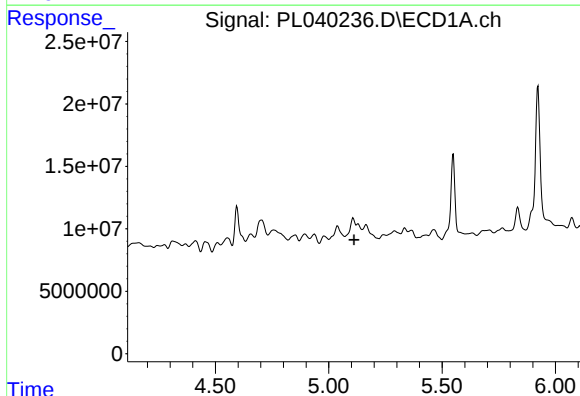


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

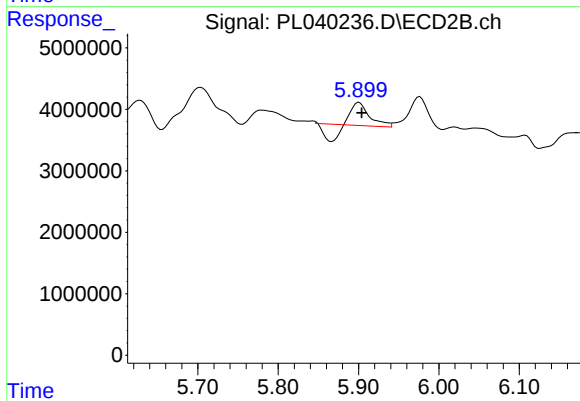

#25 Chlordane-3


R.T.: 5.901 min
Delta R.T.: -0.003 min
Response: 2957902
Conc: 5.53 ng/ml

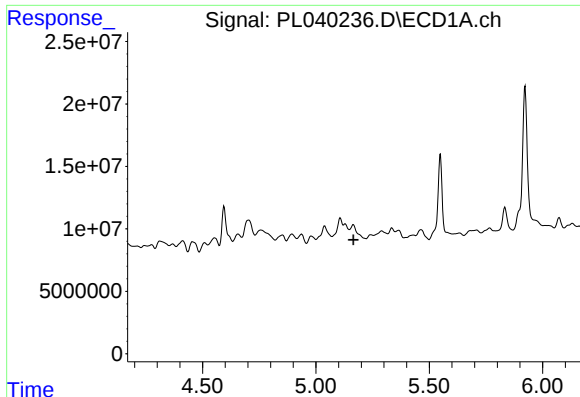

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

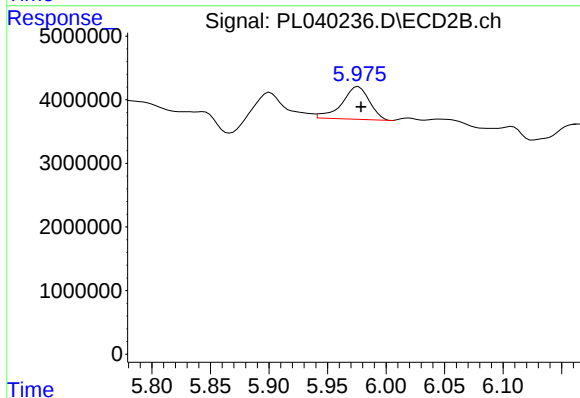


#26 Chlordane-4

R.T.: 5.976 min
Delta R.T.: -0.002 min
Response: 8451690
Conc: 13.23 ng/ml

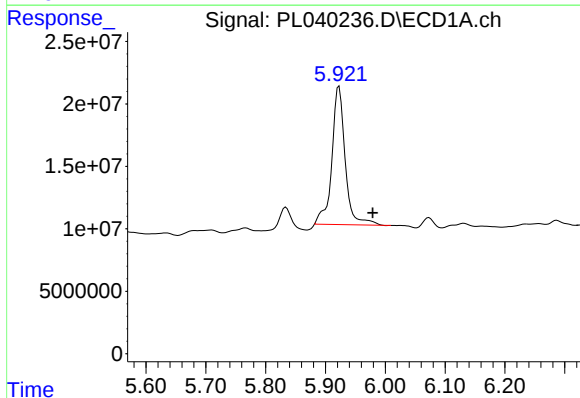


#27 Chlordane-5

R.T.: 5.923 min
Delta R.T.: -0.056 min
Response: 171101671
Conc: 412.55 ng/ml

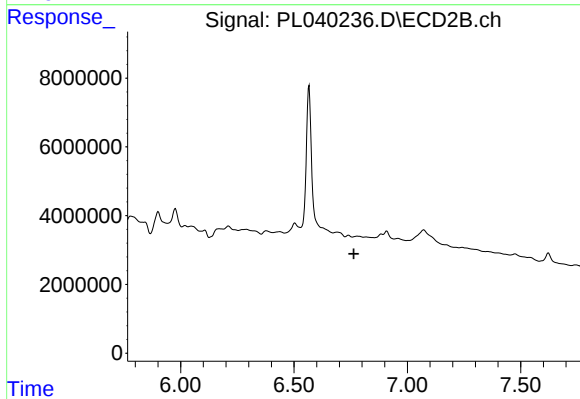

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

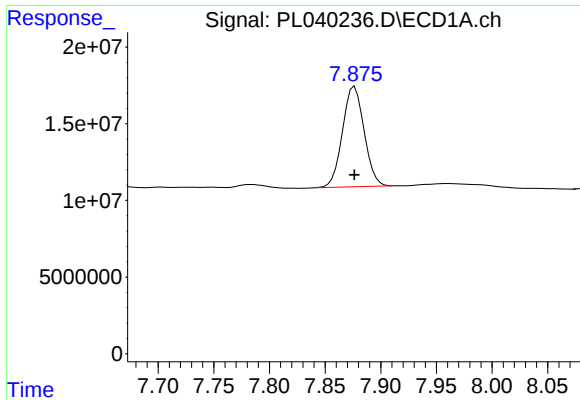

#28 Decachlorobiphenyl

R.T.: 7.877 min
Delta R.T.: 0.000 min
Response: 88706224
Conc: 10.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PL-02-0920-18-B

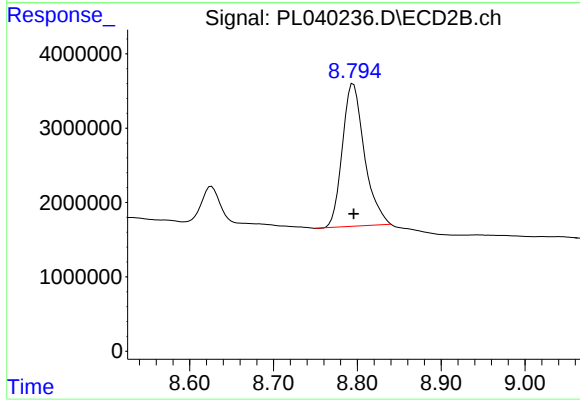

#28 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 35119940
Conc: 10.98 ng/ml