

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092319\
 Data File : PL052660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2019 08:59
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:08:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	0.000	4.424	0	736119	N.D.	0.241 #
3) MA	gamma-BHC...	0.000	4.723	0	385960	N.D.	0.134 #
4) MA	Heptachlor	4.576f	5.243	45023027	235564	3.985	0.080 #
5) MB	Aldrin	0.000	5.546	0	10446697	N.D.	3.944 #
6) B	beta-BHC	0.000	4.910f	0	3642591	N.D.	2.731 #
7) B	delta-BHC	0.000	5.103	0	665185	N.D.	0.232 #
10) B	gamma-Chl...	0.000	6.163	0	237557	N.D.	0.093 #
23)	Chlordane-1	0.000	5.017f	0	2080684	N.D.	26.797 #
25)	Chlordane-3	0.000	6.163	0	237557	N.D.	0.776 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092319\
Data File : PL052660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2019 08:59
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:08:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

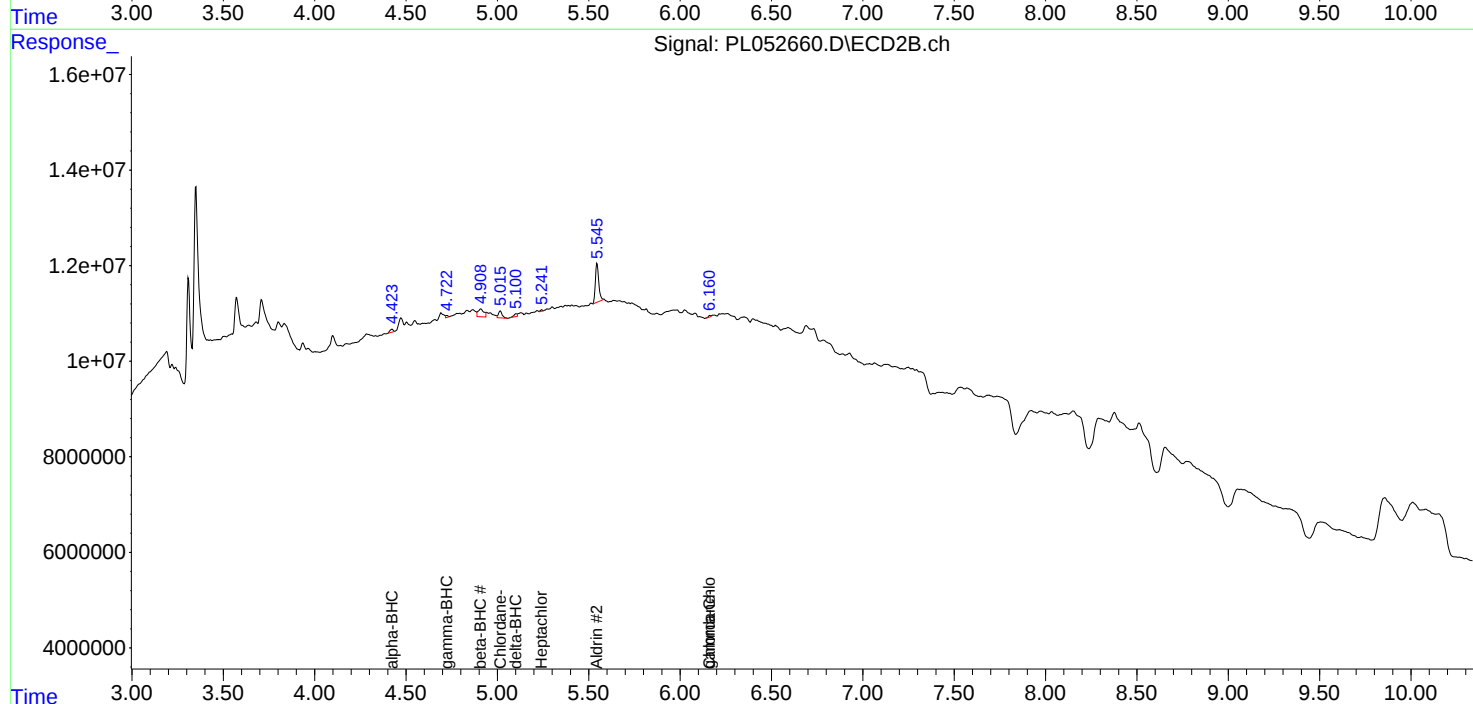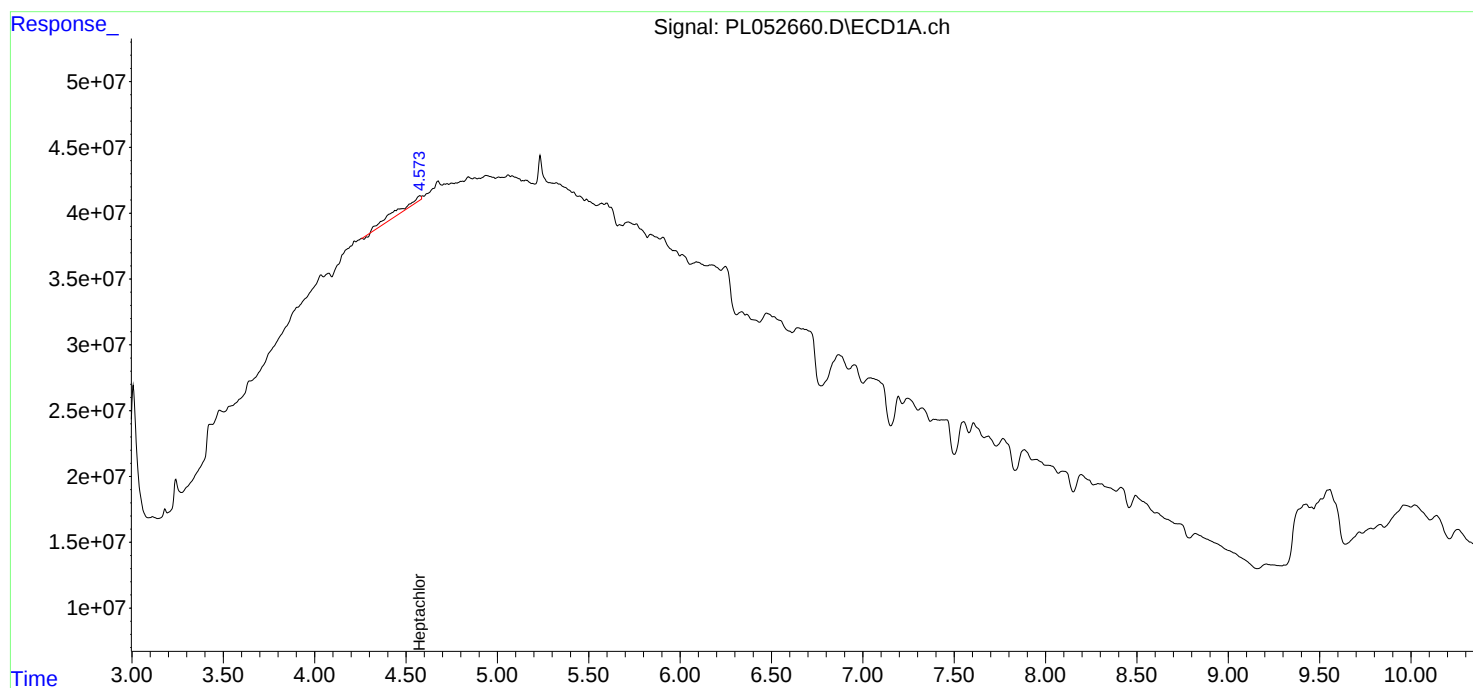


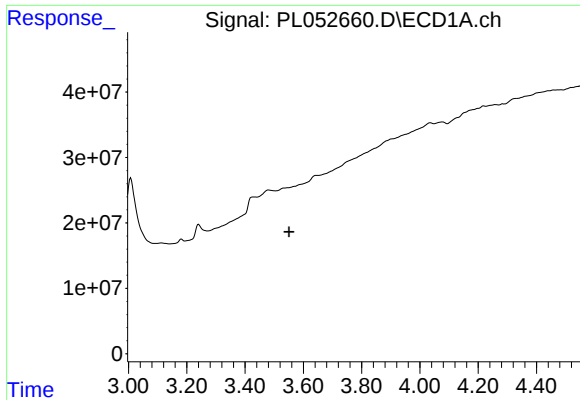

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

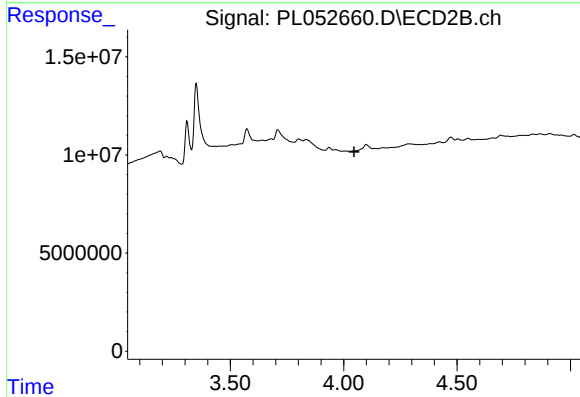


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.045 min
Response: 0
Conc: N.D.

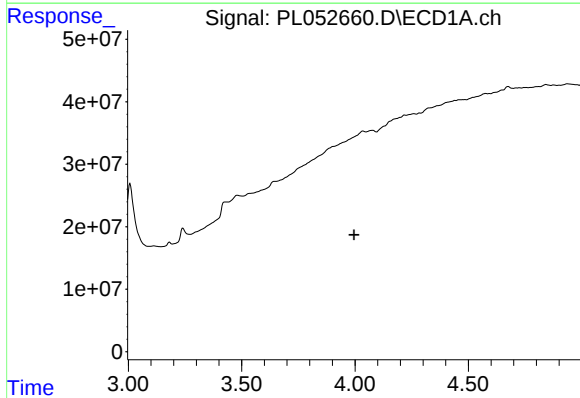


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

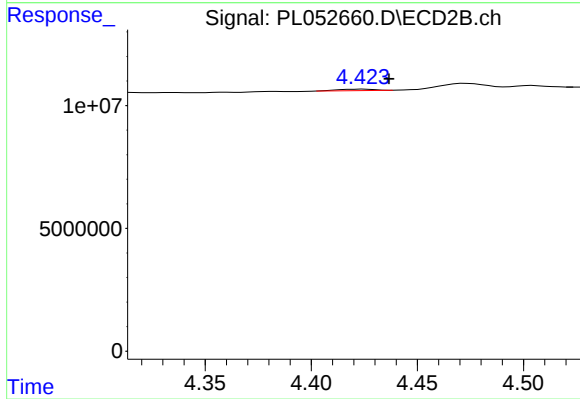

#2 alpha-BHC


R.T.: 4.424 min
Delta R.T.: -0.012 min
Response: 736119
Conc: 0.24 ng/ml

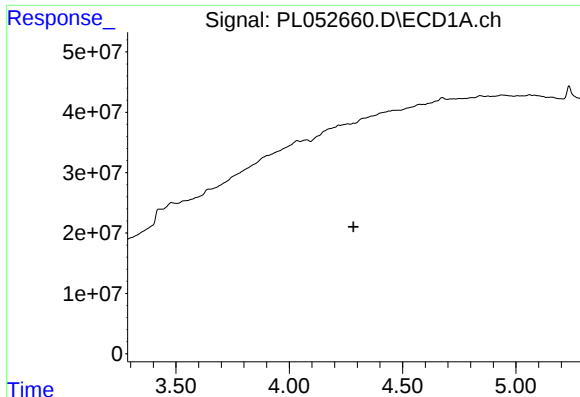

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

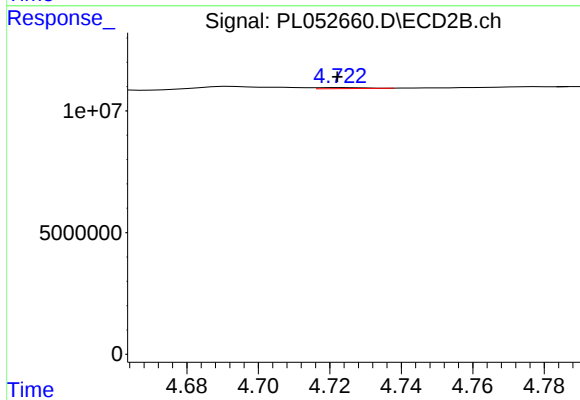


#3 gamma-BHC (Lindane)

R.T.: 4.723 min
Delta R.T.: 0.001 min
Response: 385960
Conc: 0.13 ng/ml

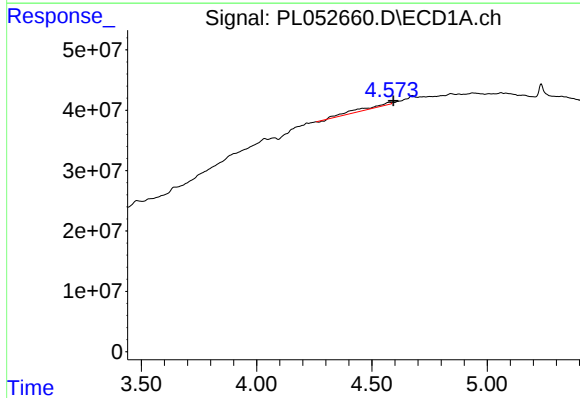


#4 Heptachlor

R.T.: 4.576 min
Delta R.T.: -0.018 min
Response: 45023027
Conc: 3.98 ng/ml

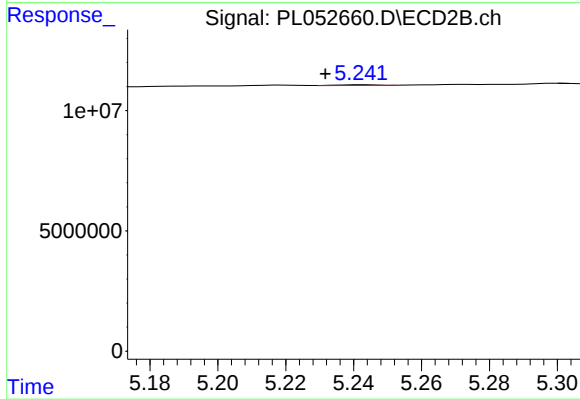

#4 Heptachlor


R.T.: 5.243 min
Delta R.T.: 0.011 min
Response: 235564
Conc: 0.08 ng/ml

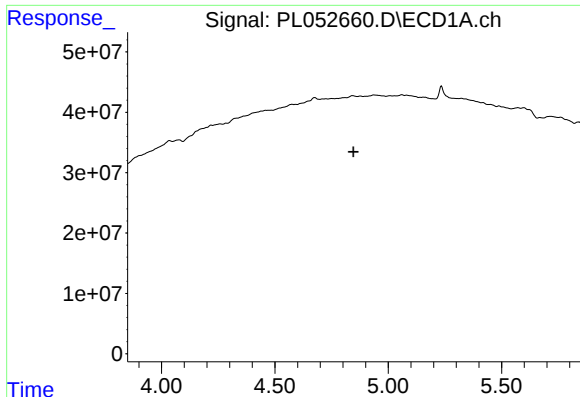

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 4.847 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

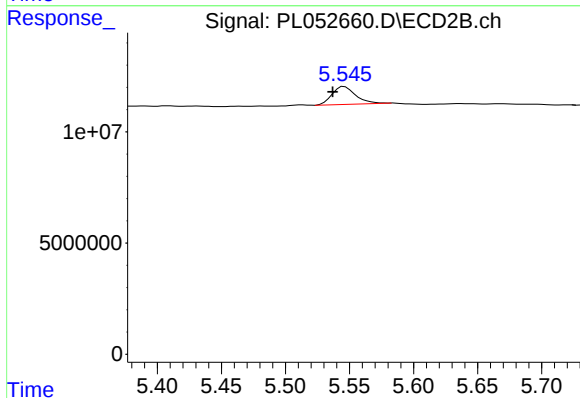


#5 Aldrin

R.T.: 5.546 min
Delta R.T.: 0.009 min
Response: 10446697
Conc: 3.94 ng/ml

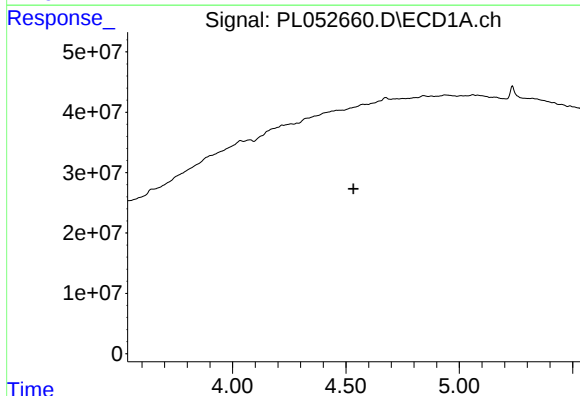


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.534 min
Response: 0
Conc: N.D.

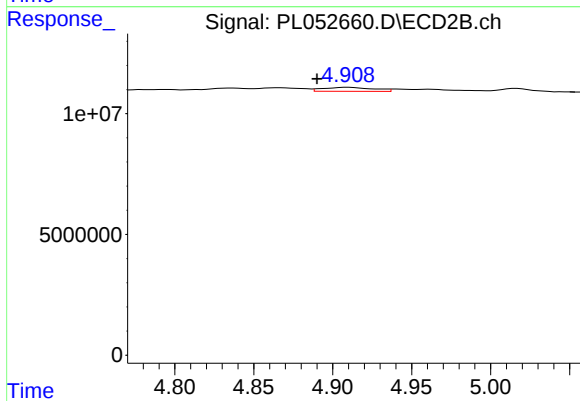

#6 beta-BHC


R.T.: 4.910 min
Delta R.T.: 0.020 min
Response: 3642591
Conc: 2.73 ng/ml

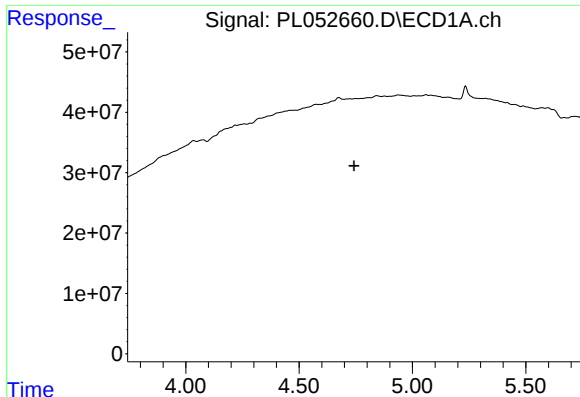

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

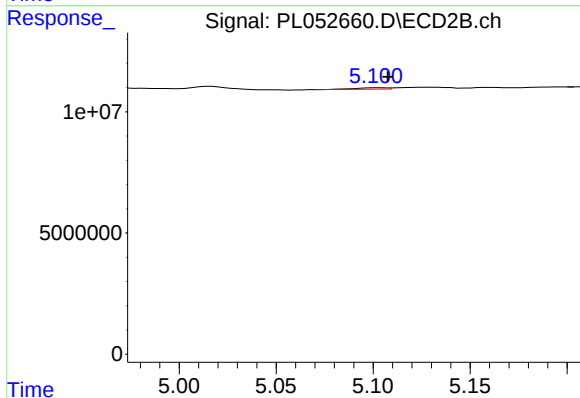


#7 delta-BHC

R.T.: 5.103 min
Delta R.T.: -0.005 min
Response: 665185
Conc: 0.23 ng/ml

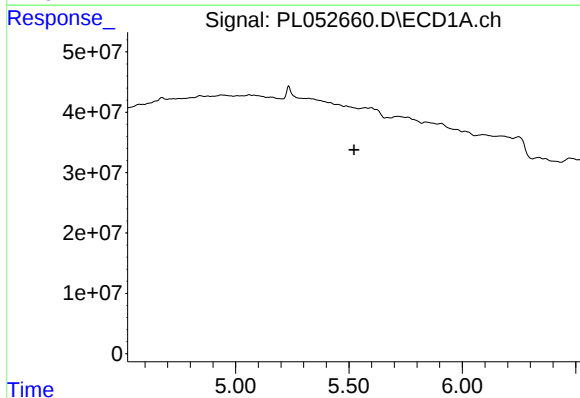


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.523 min
Response: 0
Conc: N.D.

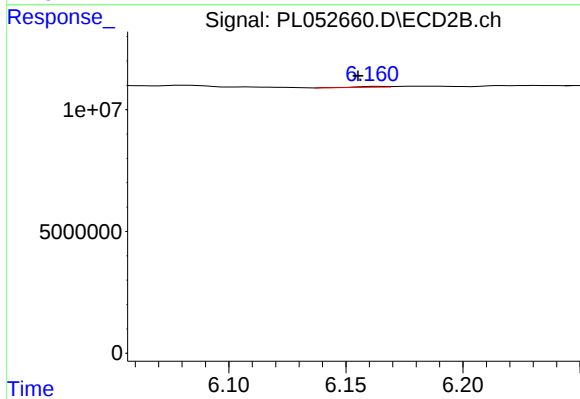

#10 gamma-Chlordane


R.T.: 6.163 min
Delta R.T.: 0.008 min
Response: 237557
Conc: 0.09 ng/ml

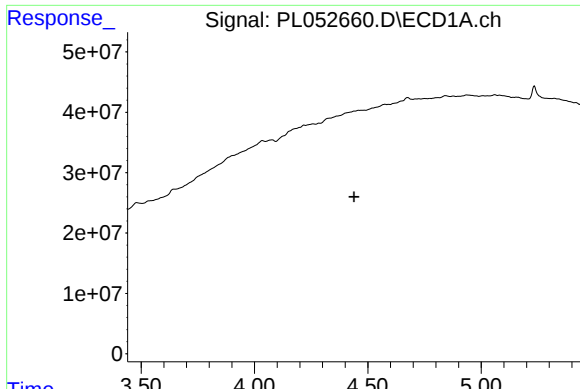

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

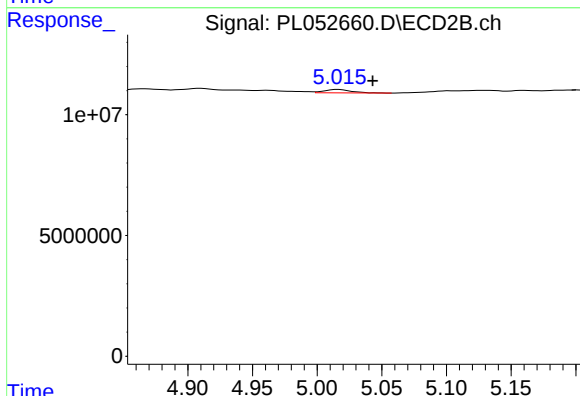


#23 Chlordane-1

R.T.: 5.017 min
Delta R.T.: -0.027 min
Response: 2080684
Conc: 26.80 ng/ml

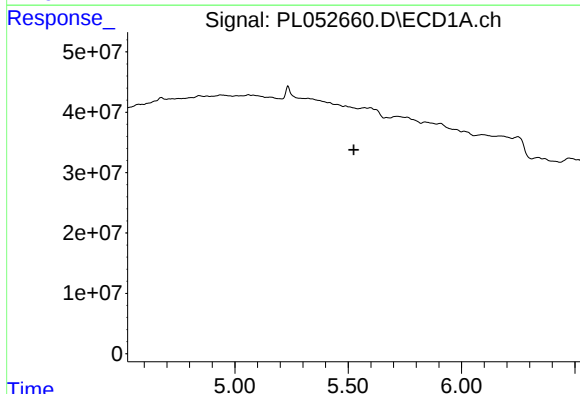


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

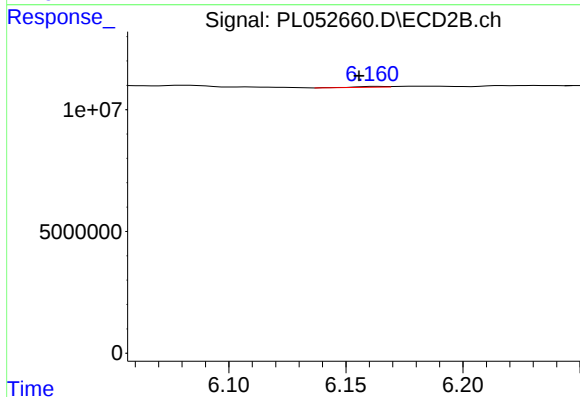

#25 Chlordane-3


R.T.: 6.163 min
Delta R.T.: 0.007 min
Response: 237557
Conc: 0.78 ng/ml

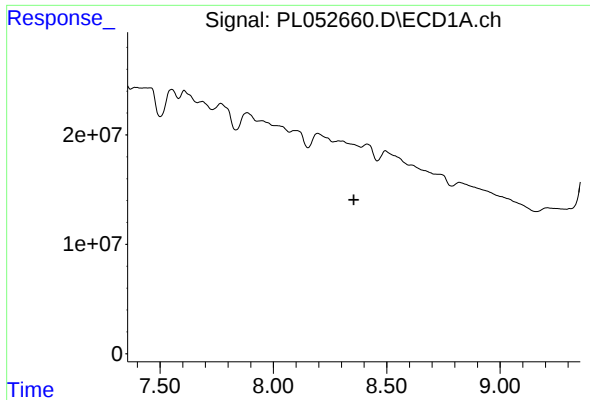

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

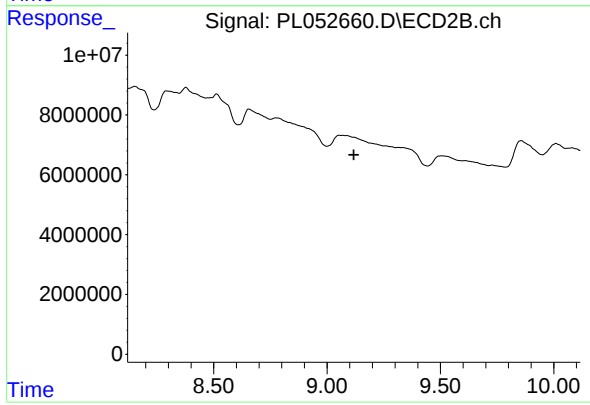

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.118 min
Response: 0
Conc: N.D.