

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092319\
 Data File : PL052661.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2019 09:13
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:08:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	4.047	185.0E6	53469851	23.724	24.539
28)	SA Decachlor...	8.353	9.125	181.3E6	60092632	20.735	25.095
Target Compounds							
4)	MA Heptachlor	0.000	5.244	0	205281	N.D.	0.070 #
9)	A Endosulfan I	0.000	6.275	0	636075	N.D.	0.273 #
11)	B alpha-Chl...	0.000	6.256f	0	1556163	N.D.	0.623 #
23)	Chlordane-1	0.000	5.038	0	108934	N.D.	1.403 #
26)	Chlordane-4	0.000	6.256f	0	1556163	N.D.	4.046 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092319\
Data File : PL052661.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2019 09:13
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:08:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

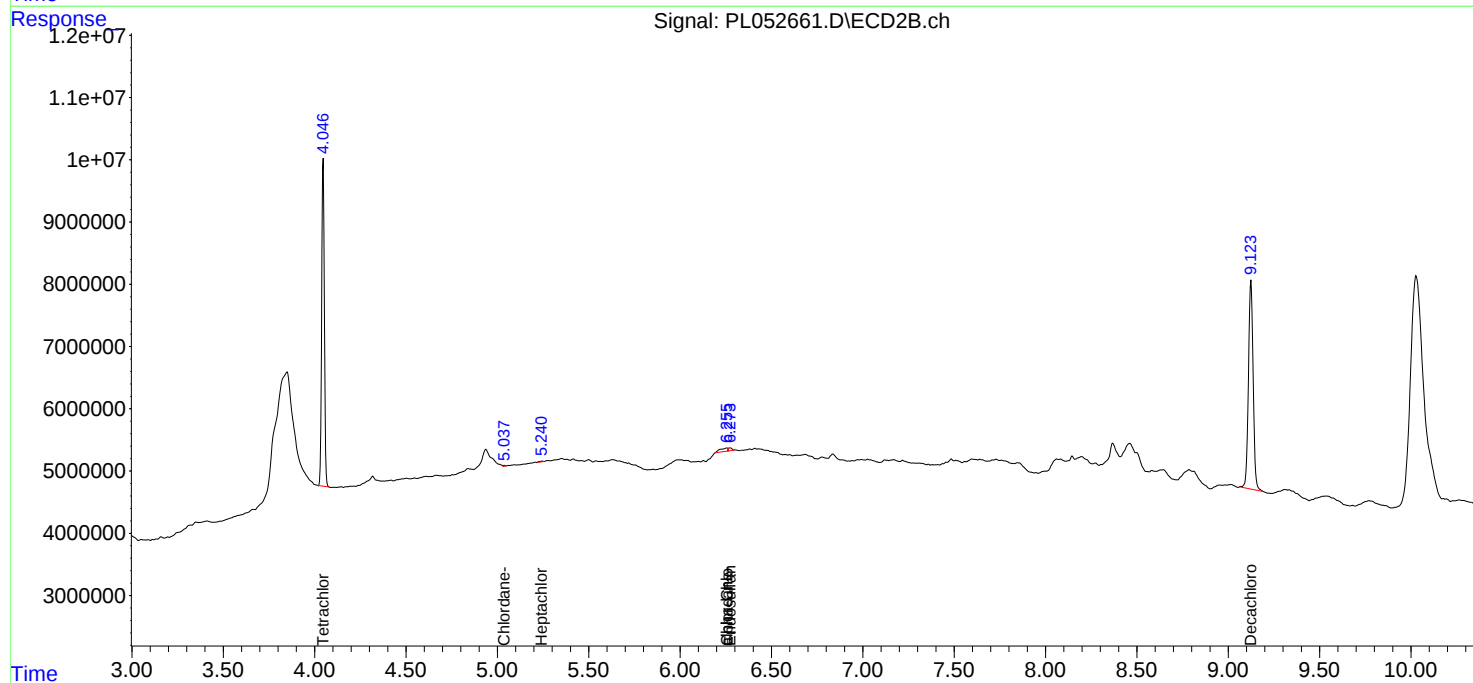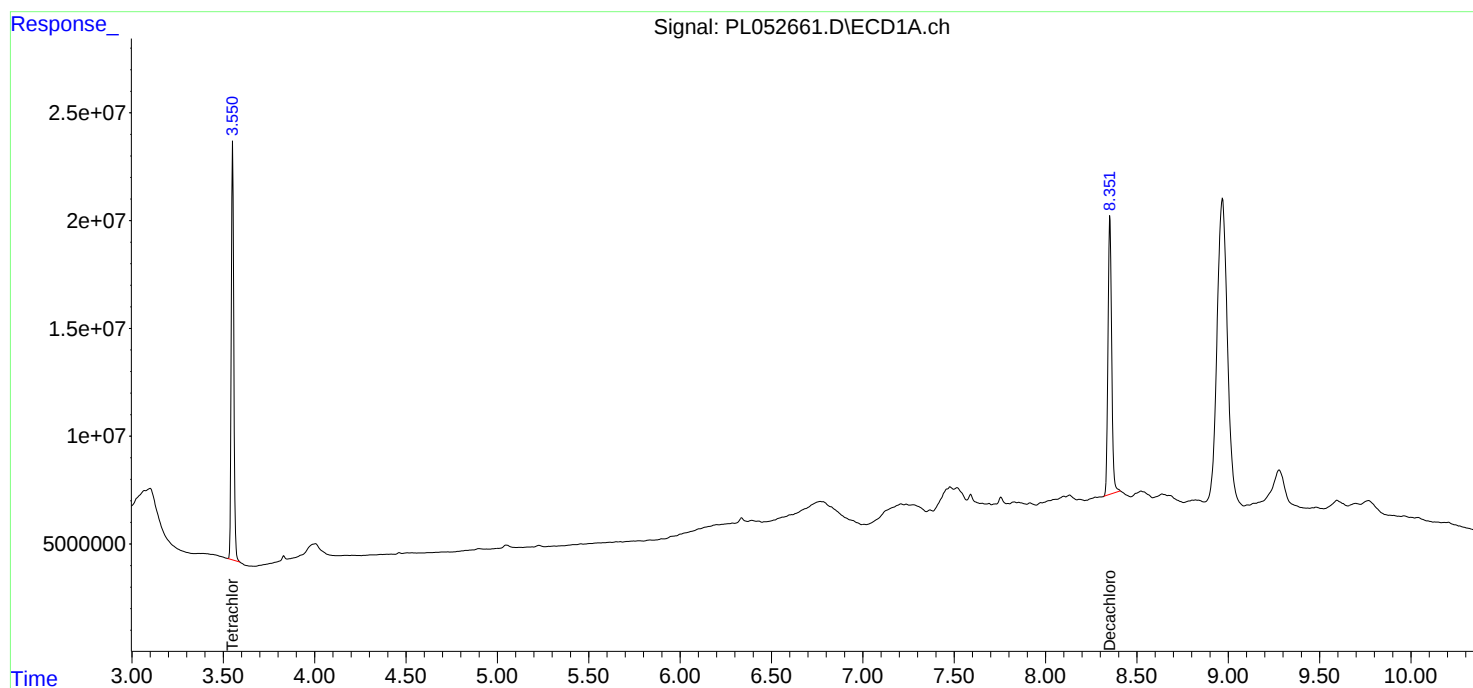


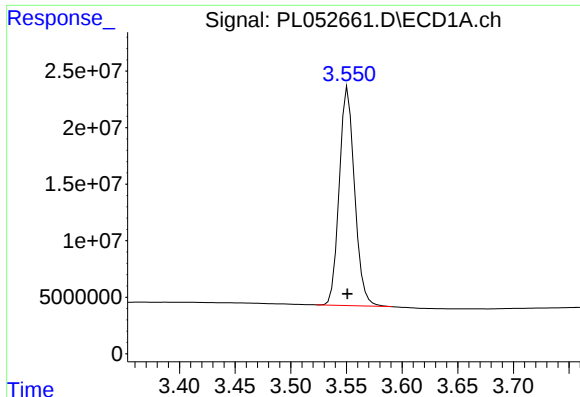

#1 Tetrachloro-m-xylene


R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 184989322
Conc: 23.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

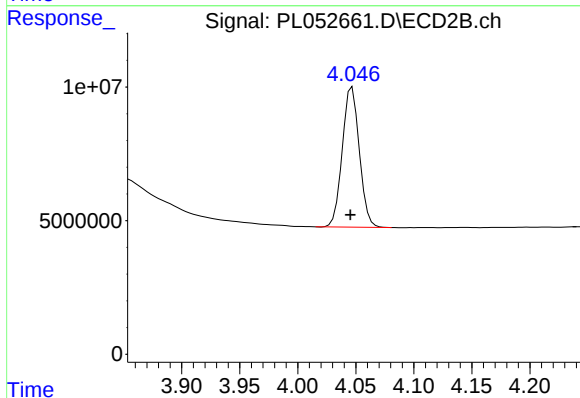


#1 Tetrachloro-m-xylene

R.T.: 4.047 min
Delta R.T.: 0.001 min
Response: 53469851
Conc: 24.54 ng/ml

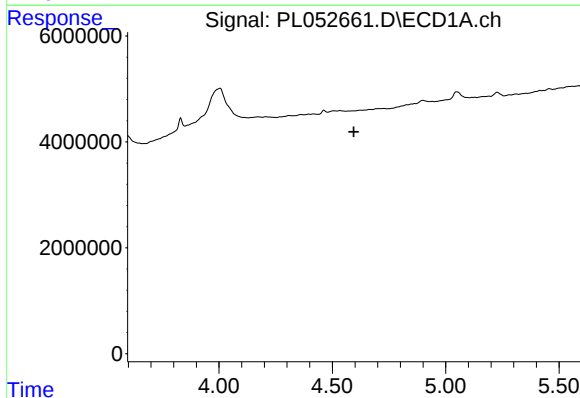


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.594 min
Response: 0
Conc: N.D.

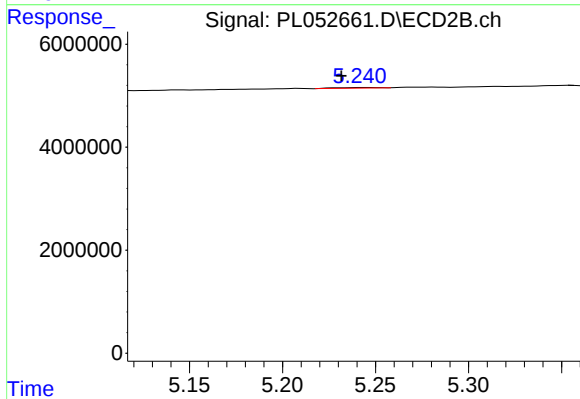

#4 Heptachlor


R.T.: 5.244 min
Delta R.T.: 0.012 min
Response: 205281
Conc: 0.07 ng/ml

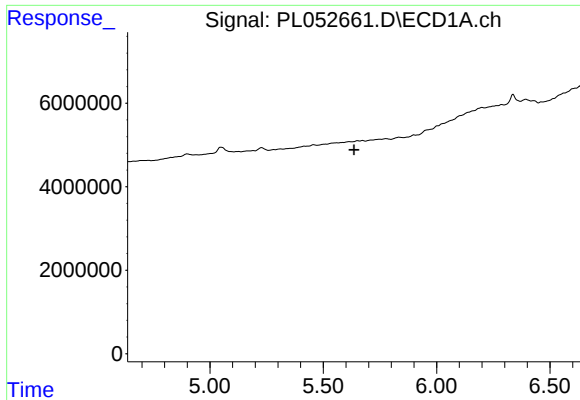

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.636 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

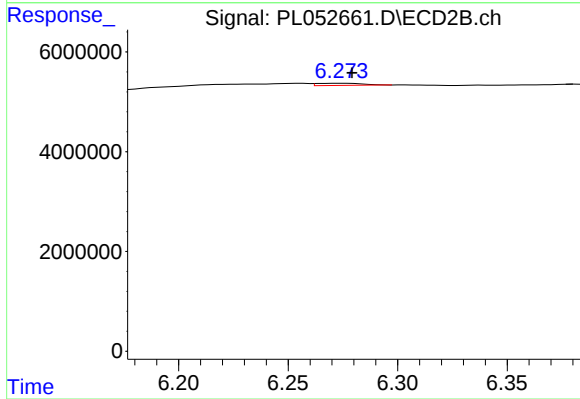


#9 Endosulfan I

R.T.: 6.275 min
Delta R.T.: -0.005 min
Response: 636075
Conc: 0.27 ng/ml

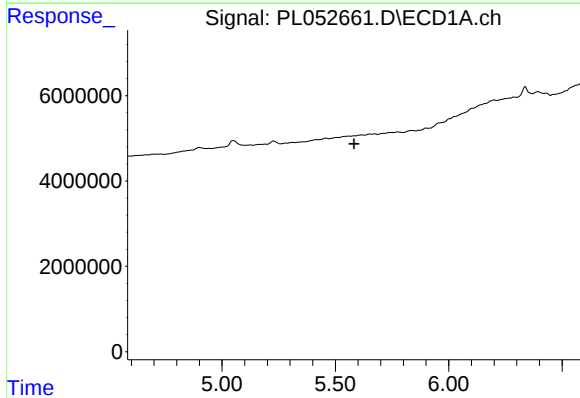


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.582 min
Response: 0
Conc: N.D.

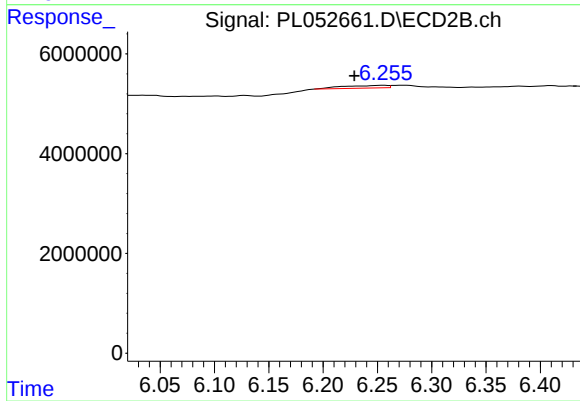

#11 alpha-Chlordane


R.T.: 6.256 min
Delta R.T.: 0.027 min
Response: 1556163
Conc: 0.62 ng/ml

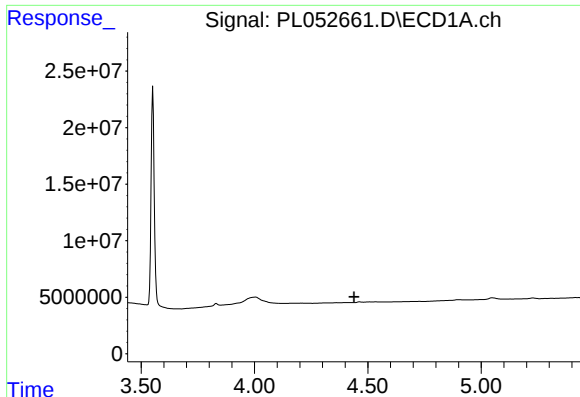

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

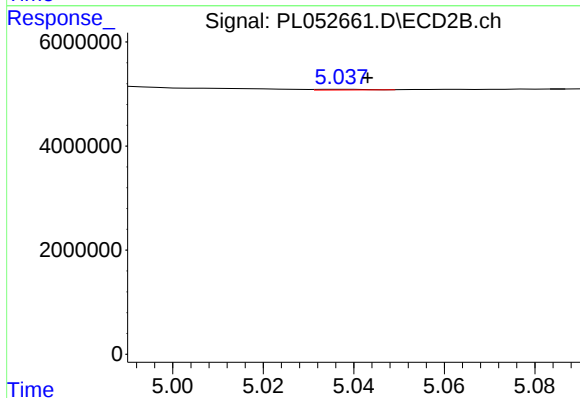


#23 Chlordane-1

R.T.: 5.038 min
Delta R.T.: -0.005 min
Response: 108934
Conc: 1.40 ng/ml

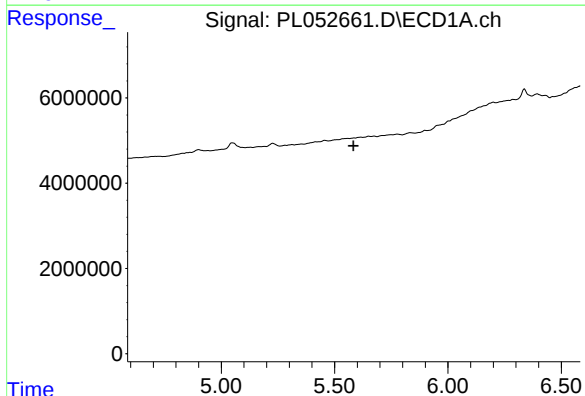


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.583 min
Response: 0
Conc: N.D.

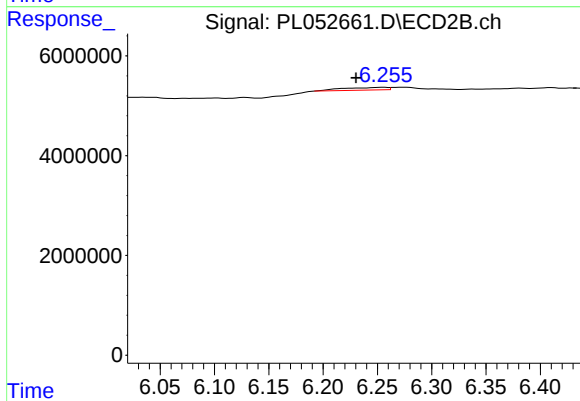

#26 Chlordane-4

R.T.: 6.256 min
Delta R.T.: 0.026 min
Response: 1556163
Conc: 4.05 ng/ml

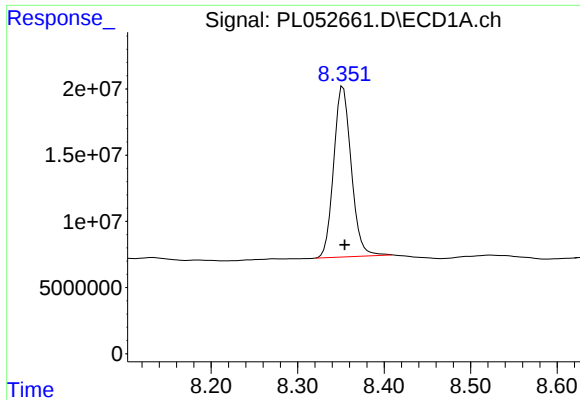

#28 Decachlorobiphenyl


R.T.: 8.353 min

Delta R.T.: -0.002 min

Response: 181321223

Conc: 20.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

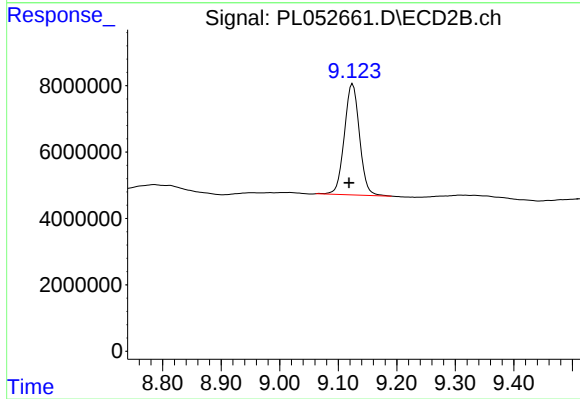

#28 Decachlorobiphenyl

R.T.: 9.125 min

Delta R.T.: 0.006 min

Response: 60092632

Conc: 25.09 ng/ml