

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092319\
 Data File : PL052677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2019 18:36
 Operator : SG\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 01:11:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	4.048	187.7E6	54178255	24.068	24.864
28)	SA Decachlor...	8.353	9.127	164.0E6	56673794	18.754	23.667 #
Target Compounds							
2)	A alpha-BHC	3.991	0.000	72482652	0	6.029	N.D. #
8)	B Heptachlo...	0.000	5.917	0	2073439	N.D.	0.791 #
10)	B gamma-Chl...	0.000	6.133f	0	1225340	N.D.	0.482 #
18)	B Endrin al...	6.604f	0.000	168.6E6	0	21.812	N.D. #
23)	Chlordane-1	0.000	5.017f	0	222184	N.D.	2.861 #
25)	Chlordane-3	0.000	6.133f	0	1225340	N.D.	4.005 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092319\
Data File : PL052677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2019 18:36
Operator : SG\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 01:11:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

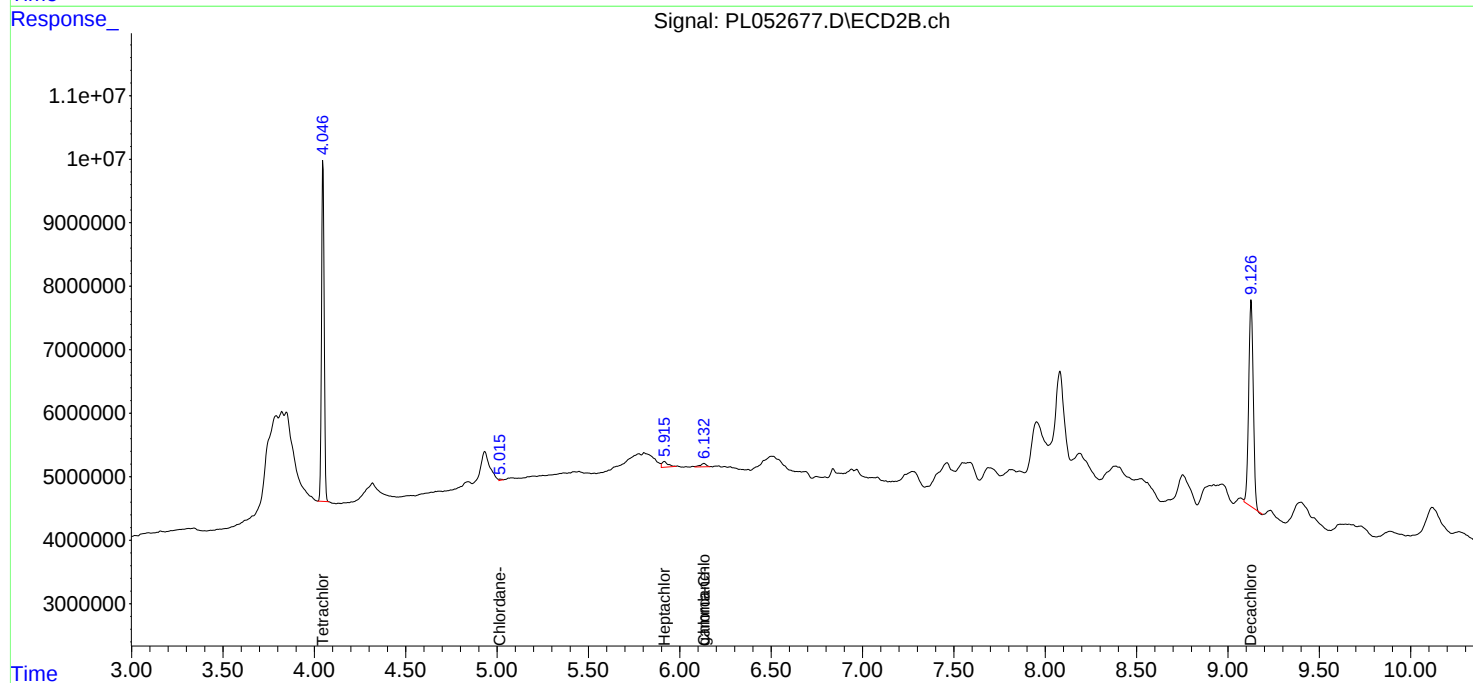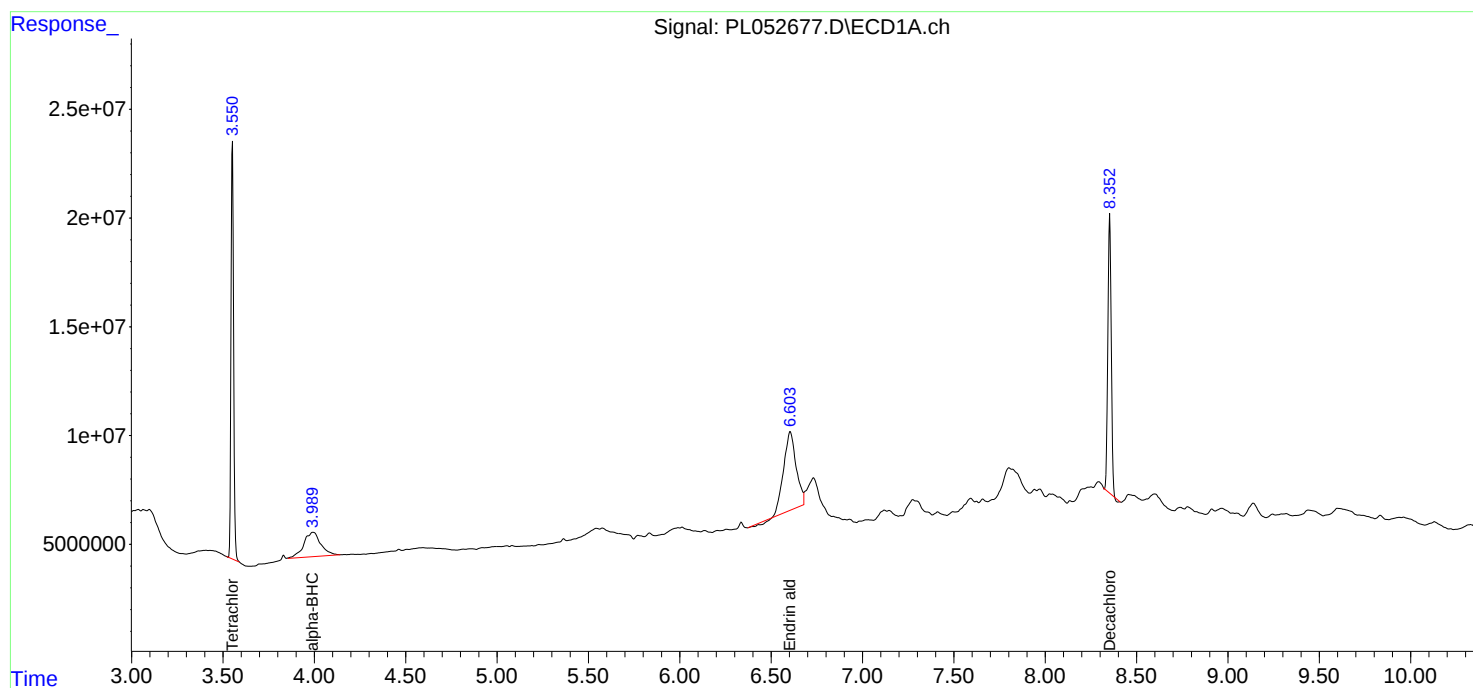


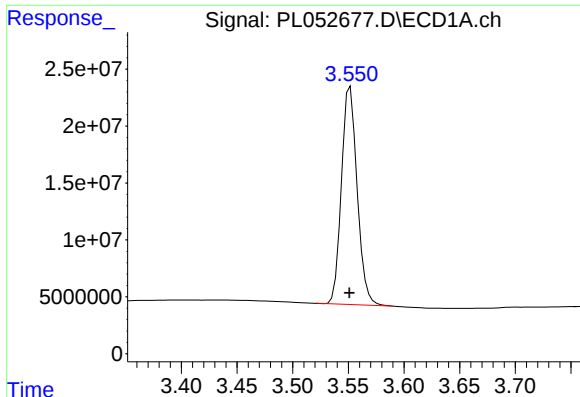

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 187673145
Conc: 24.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

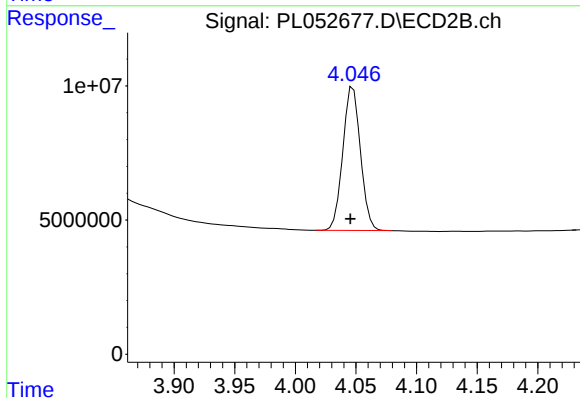


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.002 min
Response: 54178255
Conc: 24.86 ng/ml

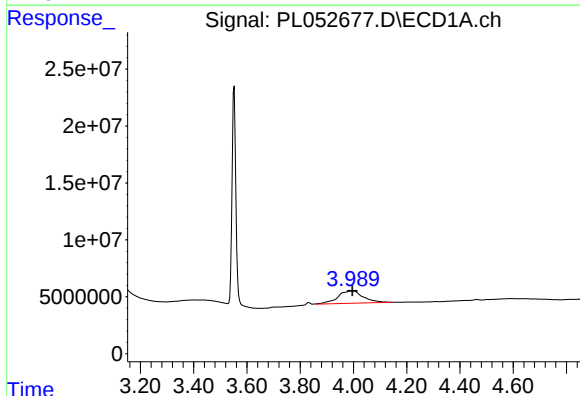


#2 alpha-BHC

R.T.: 3.991 min
Delta R.T.: -0.005 min
Response: 72482652
Conc: 6.03 ng/ml

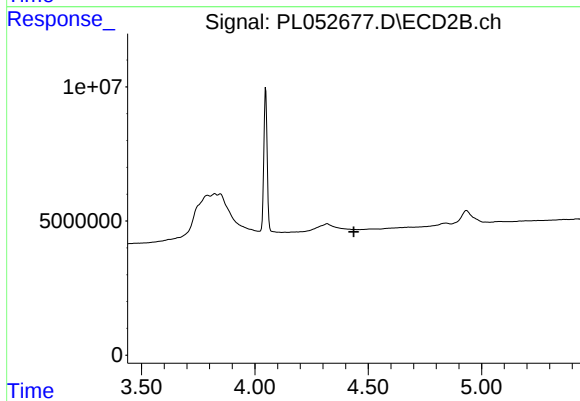

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.437 min
Response: 0
Conc: N.D.

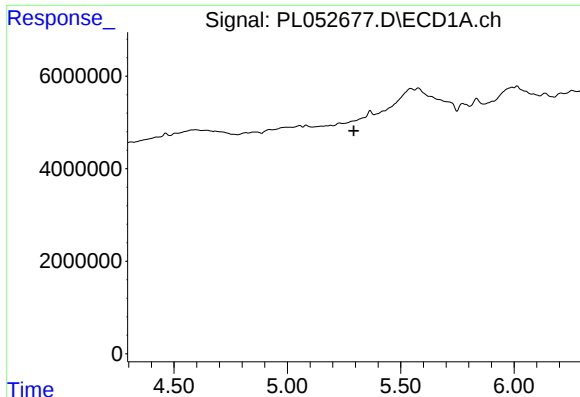

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

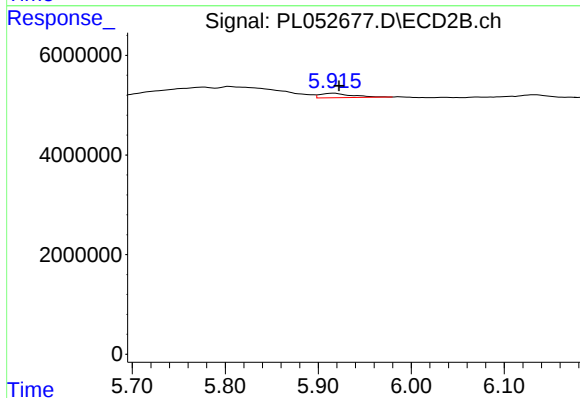


#8 Heptachlor epoxide

R.T.: 5.917 min
Delta R.T.: -0.006 min
Response: 2073439
Conc: 0.79 ng/ml

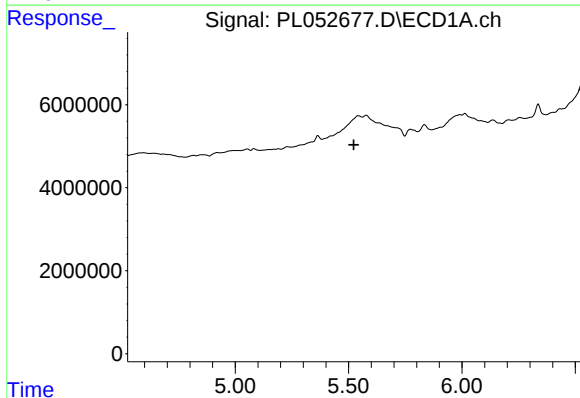


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.523 min
Response: 0
Conc: N.D.

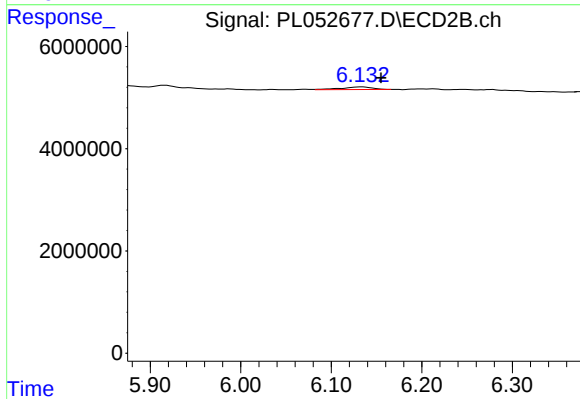

#10 gamma-Chlordane


R.T.: 6.133 min
Delta R.T.: -0.022 min
Response: 1225340
Conc: 0.48 ng/ml

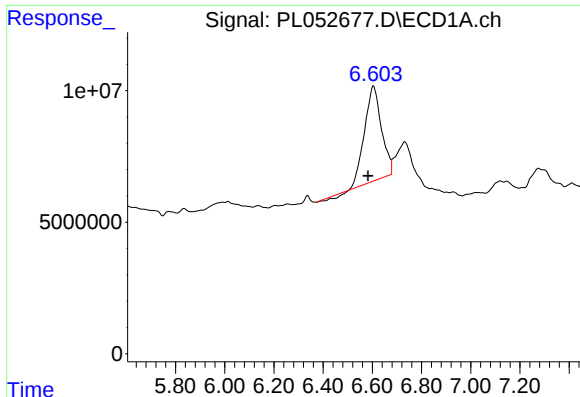

#18 Endrin aldehyde


R.T.: 6.604 min
Delta R.T.: 0.022 min
Response: 168648386
Conc: 21.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

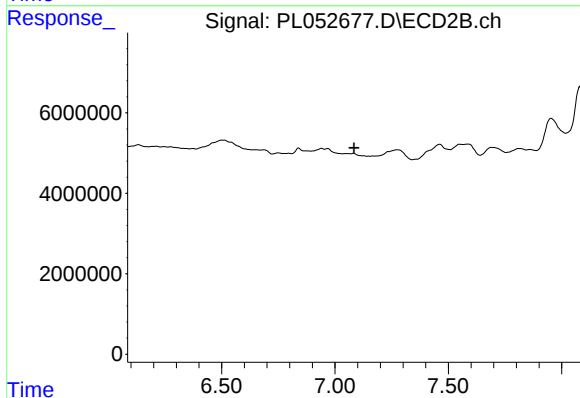


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.085 min
Response: 0
Conc: N.D.

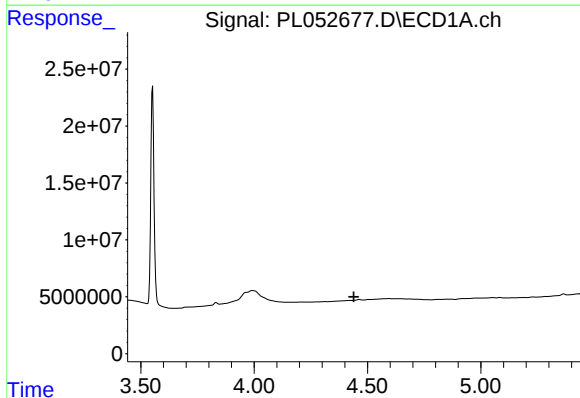


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.440 min
Response: 0
Conc: N.D.

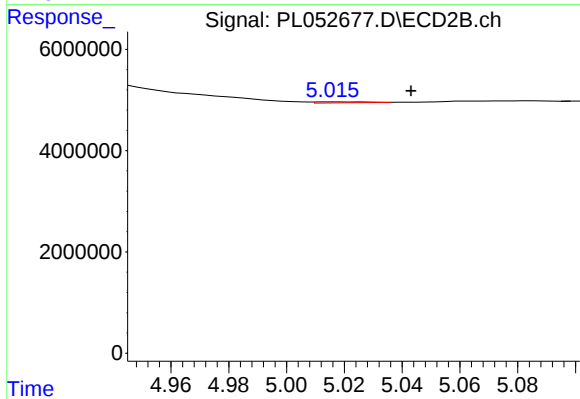

#23 Chlordane-1


R.T.: 5.017 min
Delta R.T.: -0.026 min
Response: 222184
Conc: 2.86 ng/ml

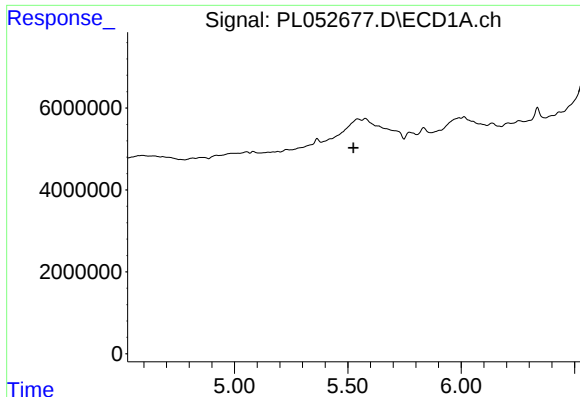

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

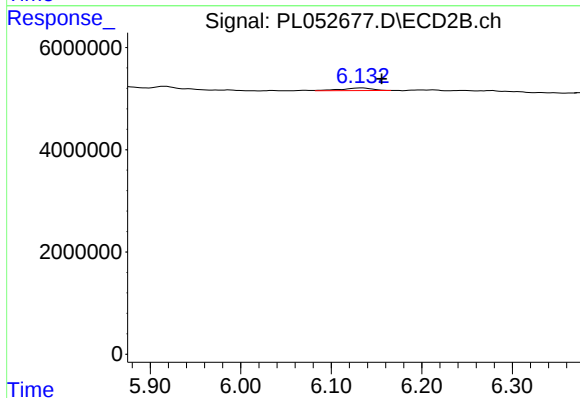


#25 Chlordane-3

R.T.: 6.133 min
Delta R.T.: -0.023 min
Response: 1225340
Conc: 4.00 ng/ml

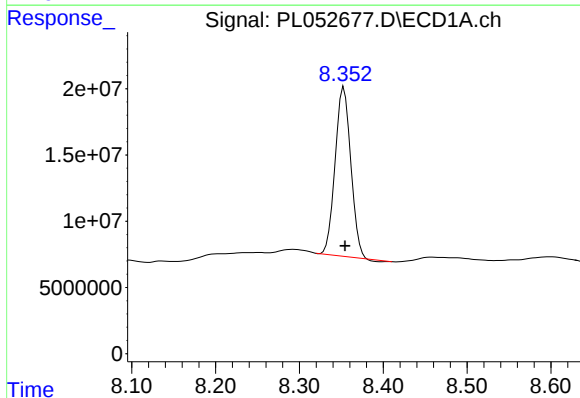

#28 Decachlorobiphenyl

R.T.: 8.353 min
Delta R.T.: -0.001 min
Response: 163996871
Conc: 18.75 ng/ml

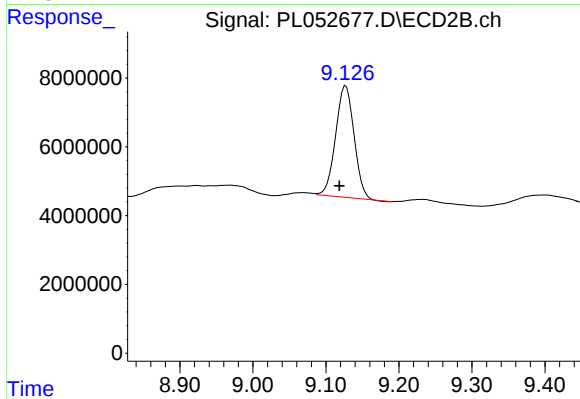

#28 Decachlorobiphenyl

R.T.: 9.127 min
Delta R.T.: 0.009 min
Response: 56673794
Conc: 23.67 ng/ml