

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 12:44
 Operator : DD\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 13:33:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:32:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.457	4.007	148.7E6	194.2E6	73.768	73.580
28)	SA Decachlor...	8.211	9.094	120.7E6	155.8E6	72.561	72.650
Target Compounds							
23)	Chlordane-1	4.327	5.004	36377953	70276413	717.292	737.242
24)	Chlordane-2	4.828	5.473	46383817	72367037	760.203	726.560
25)	Chlordane-3	5.397	6.122	121.5E6	280.6E6	757.034	753.962
26)	Chlordane-4	5.455	6.197	100.9E6	340.5E6	747.180	747.911
27)	Chlordane-5	6.290	7.003	41182139	54398325	748.833	749.939



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 12:44
Operator : DD\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 13:33:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:32:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

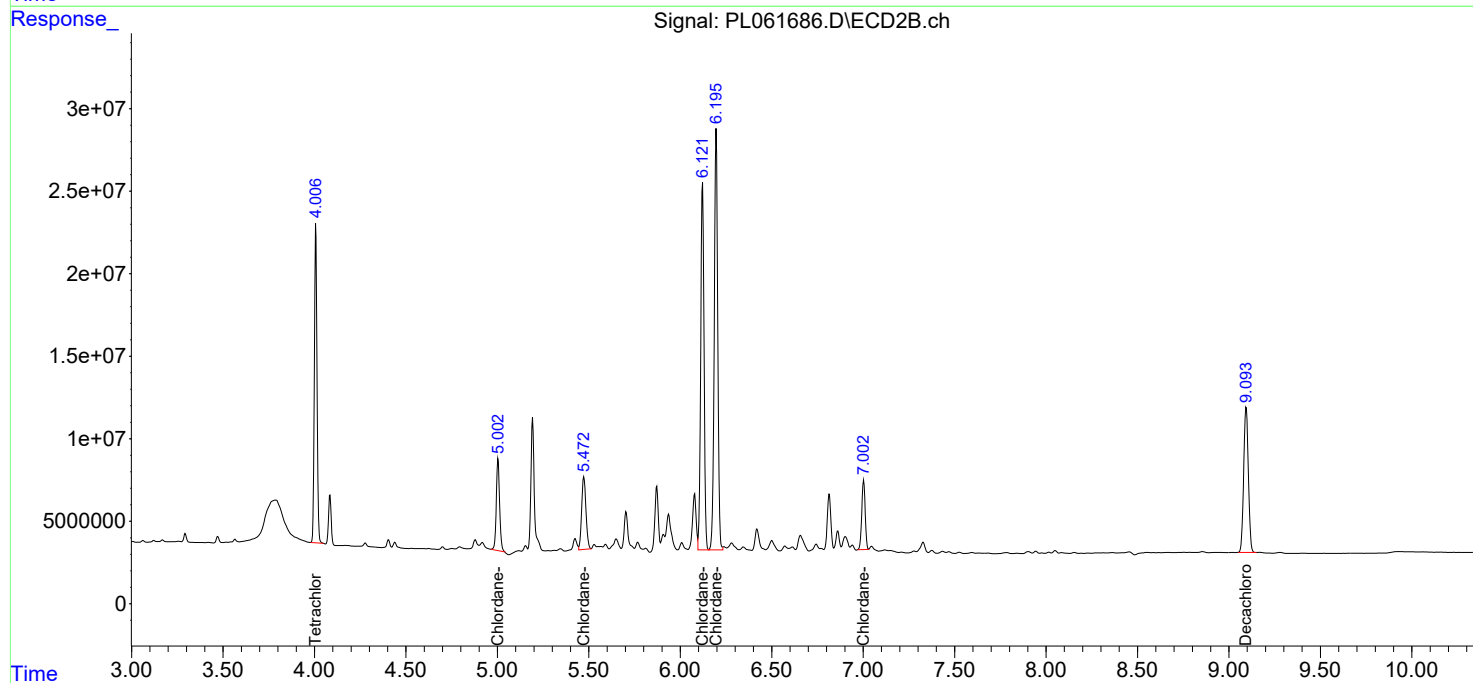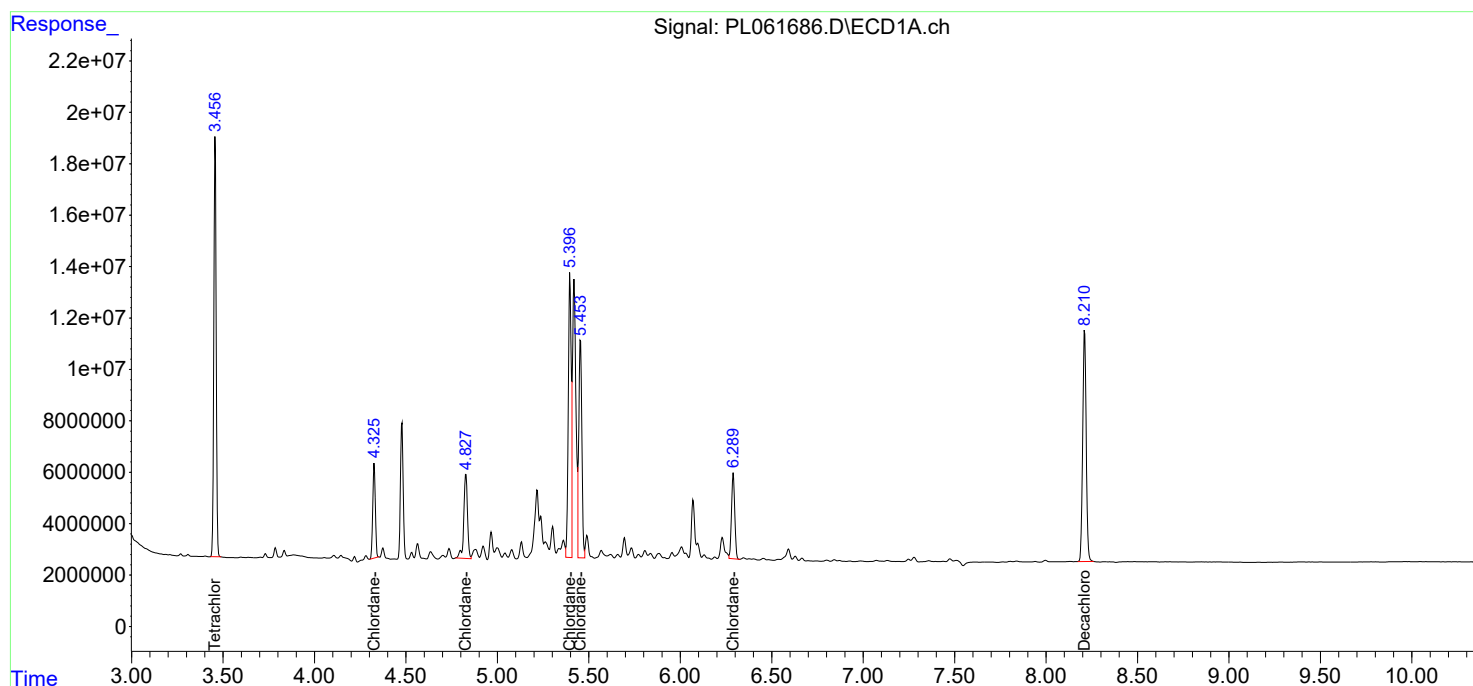


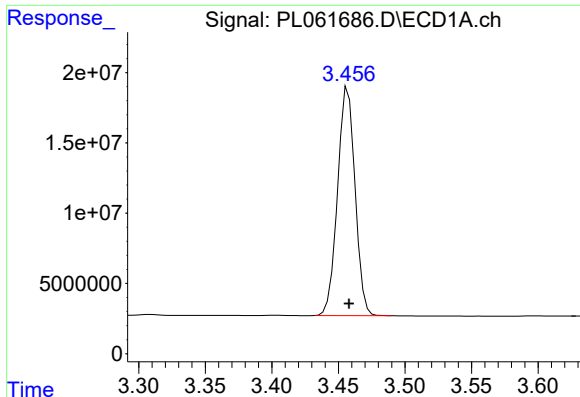

#1 Tetrachloro-m-xylene


R.T.: 3.457 min
Delta R.T.: 0.000 min
Response: 148709236
Conc: 73.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

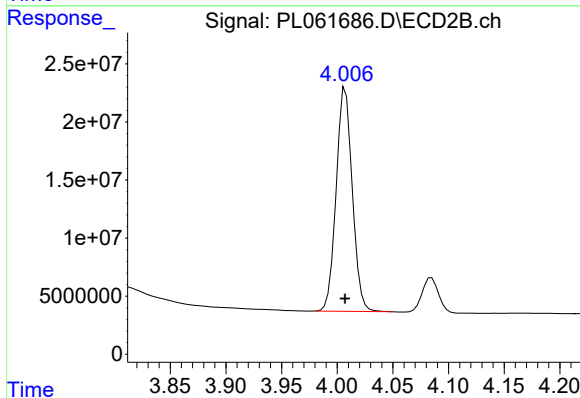


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 194174923
Conc: 73.58 ng/ml

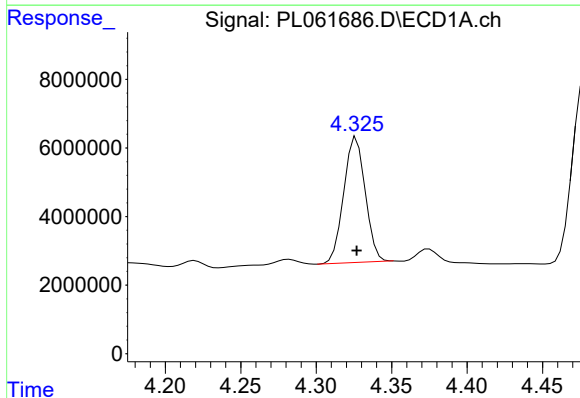


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 36377953
Conc: 717.29 ng/ml

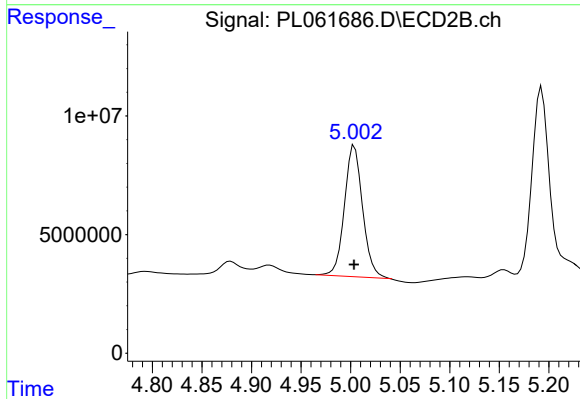

#23 Chlordane-1


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 70276413
Conc: 737.24 ng/ml

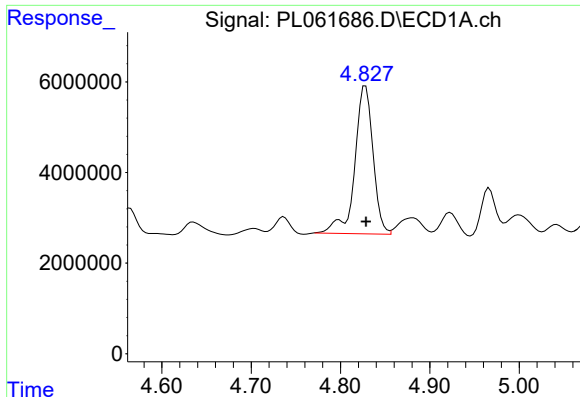

#24 Chlordane-2


R.T.: 4.828 min
Delta R.T.: 0.000 min
Response: 46383817
Conc: 760.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

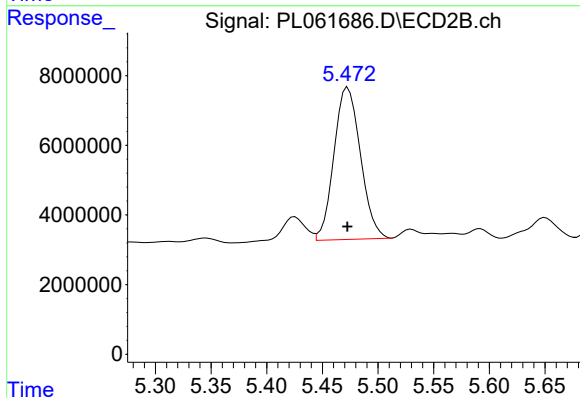


#24 Chlordane-2

R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 72367037
Conc: 726.56 ng/ml

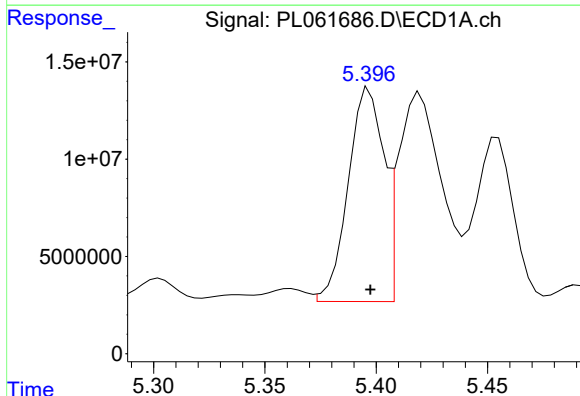


#25 Chlordane-3

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 121539712
Conc: 757.03 ng/ml

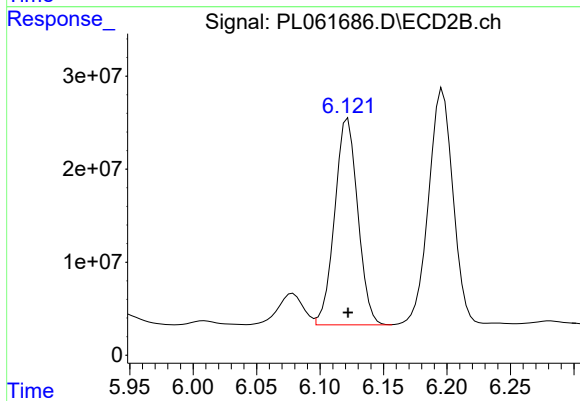

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 280647807
Conc: 753.96 ng/ml

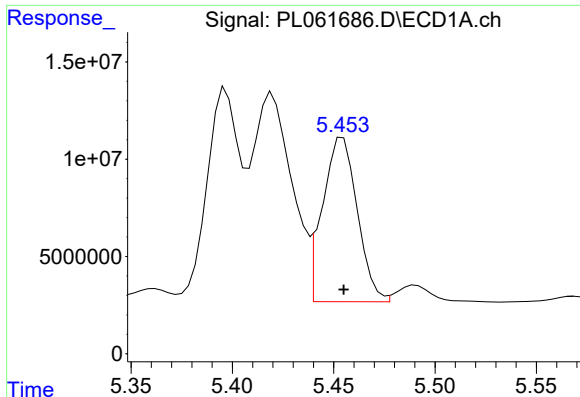

#26 Chlordane-4


R.T.: 5.455 min
Delta R.T.: 0.000 min
Response: 100932110
Conc: 747.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

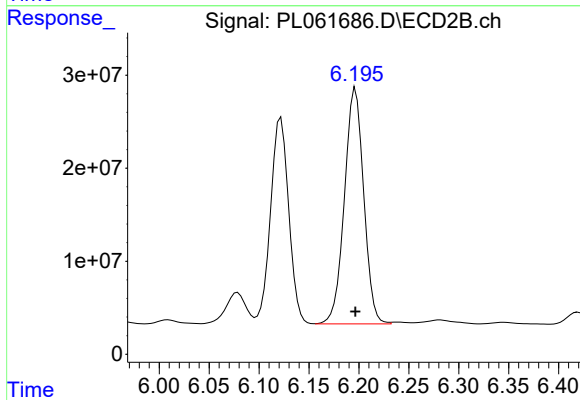


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 340536836
Conc: 747.91 ng/ml

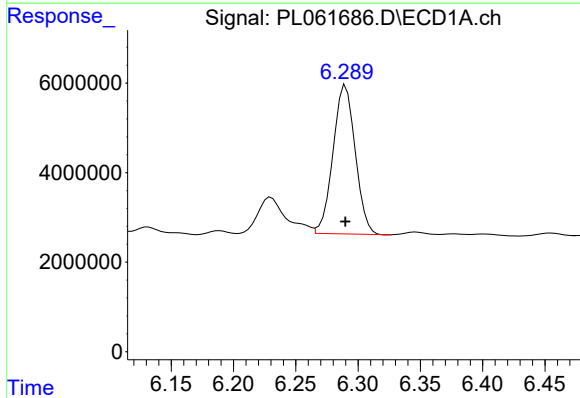


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 41182139
Conc: 748.83 ng/ml

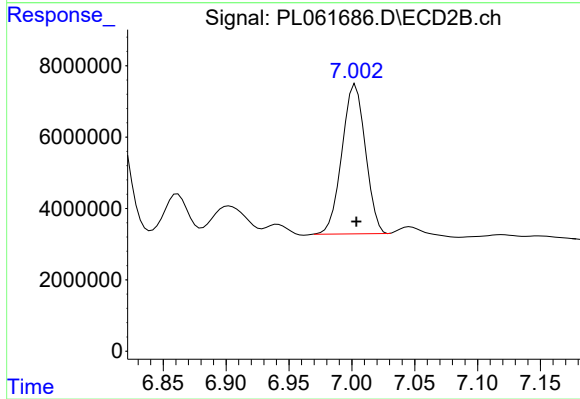

#27 Chlordane-5


R.T.: 7.003 min
Delta R.T.: 0.000 min
Response: 54398325
Conc: 749.94 ng/ml

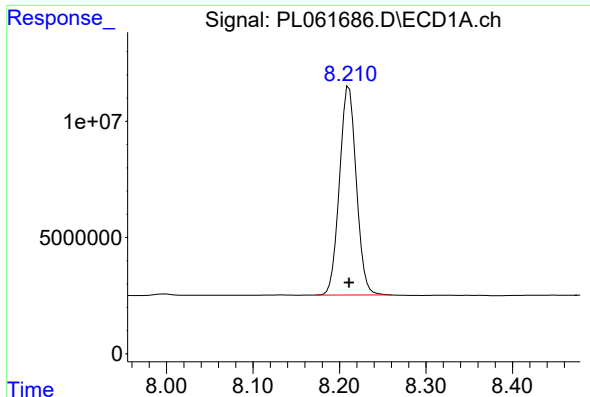

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 120710110
Conc: 72.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

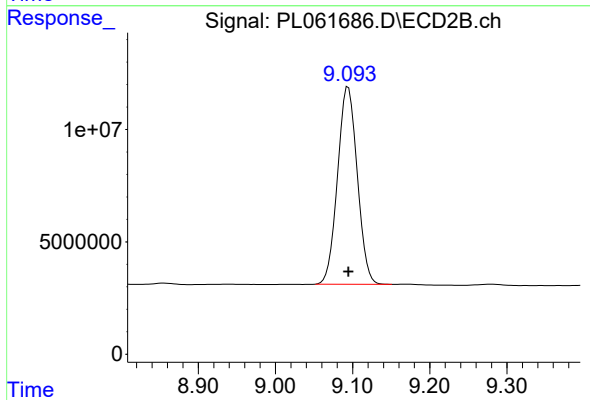

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 155814831
Conc: 72.65 ng/ml