

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061728.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 22:40
 Operator : DD\AJ
 Sample : L4105-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MTB-SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:16:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	24659741	42353079	14.455	15.524
28)	SA Decachlor...	8.211	9.094	25739121	36325805	15.822	16.501
Target Compounds							
9)	A Endosulfan I	5.529f	0.000	2856990	0	1.763	N.D. #
10)	B gamma-Chl...	5.386	0.000	9688133	0	5.579	N.D. #
12)	B 4,4'-DDE	0.000	6.352	0	2666194	N.D.	0.977 #
15)	B Endosulfa...	6.295	6.947f	6384501	11309464	3.949	4.376
19)	B Endosulfa...	6.645f	7.281	4118524	14780692	2.662	6.312 #
21)	B Endrin ke...	0.000	7.747	0	4394514	N.D.	1.872 #
25)	Chlordane-3	5.386	0.000	9688133	0	61.636	N.D. #
27)	Chlordane-5	6.295	0.000	6384501	0	117.090	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061728.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 22:40
Operator : DD\AJ
Sample : L4105-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MTB-SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:16:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

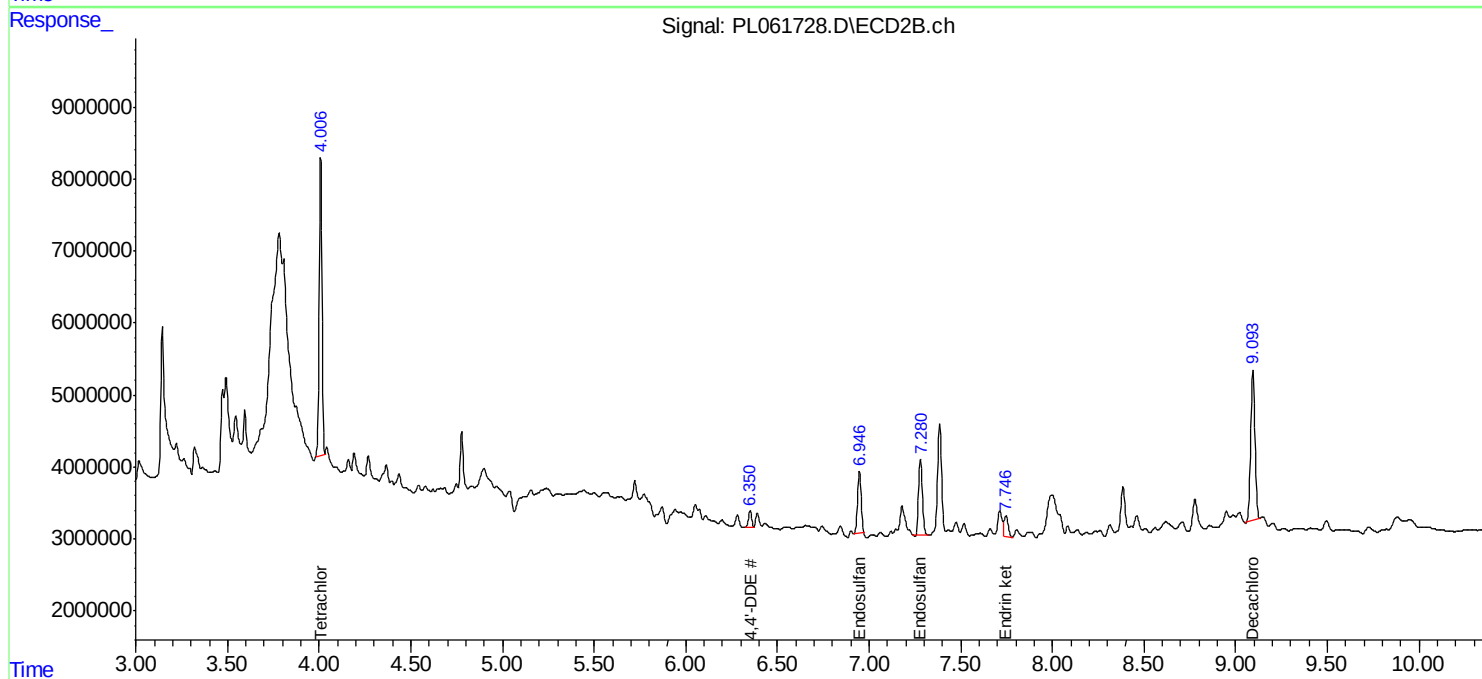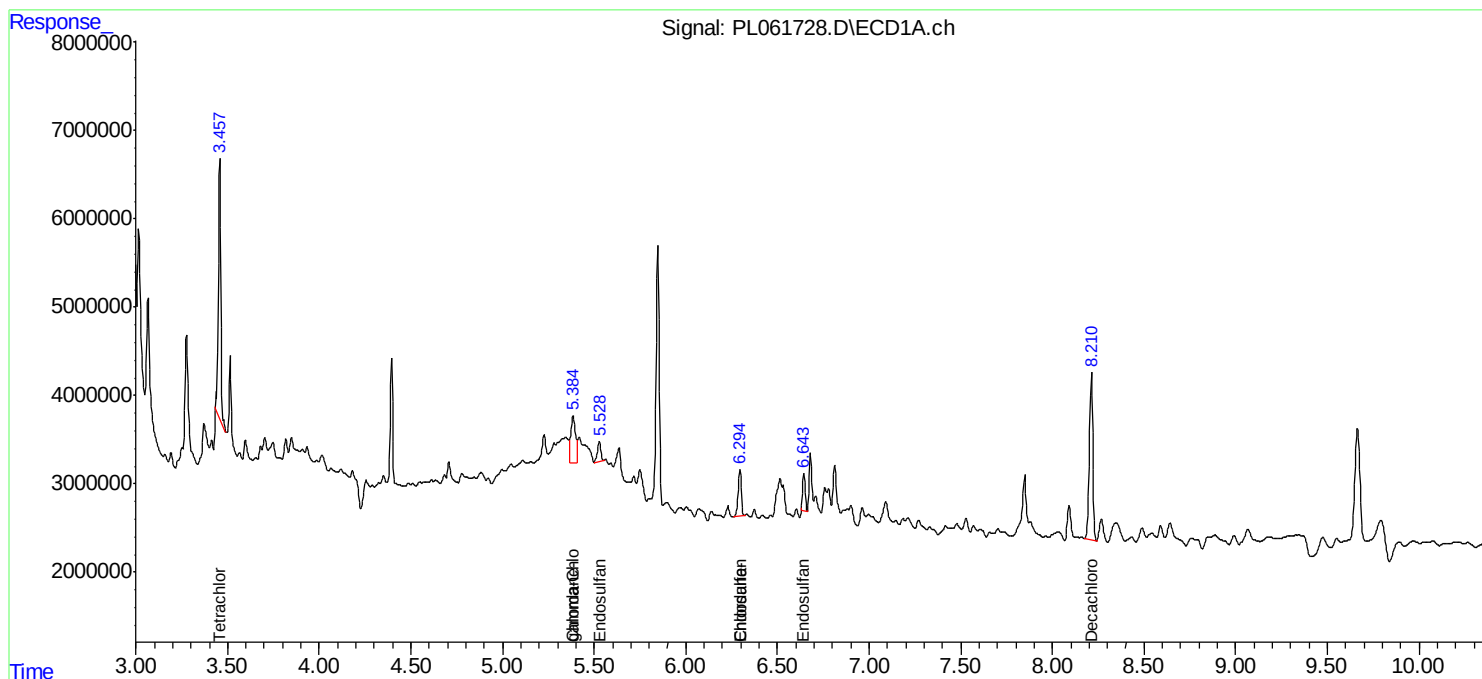


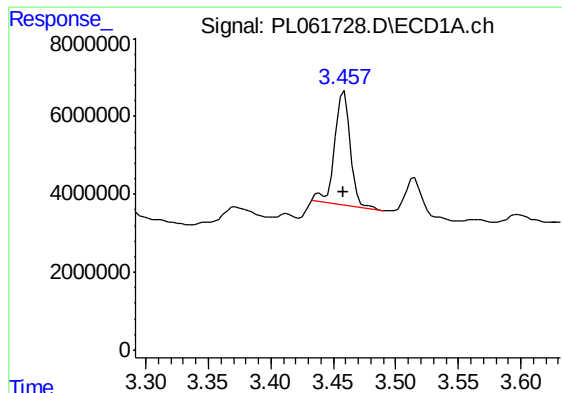

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 24659741
Conc: 14.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
MTB-SP

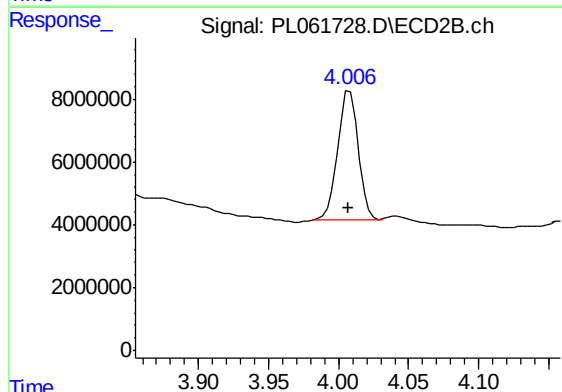


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 42353079
Conc: 15.52 ng/ml

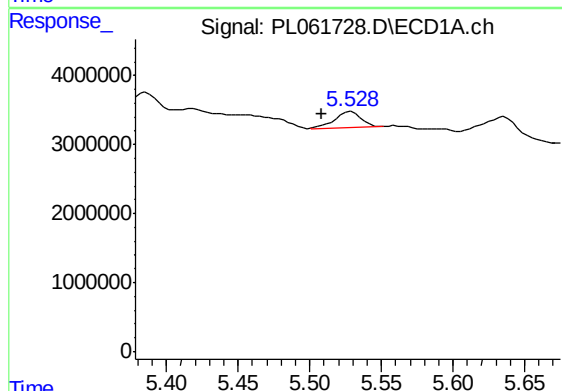


#9 Endosulfan I

R.T.: 5.529 min
Delta R.T.: 0.021 min
Response: 2856990
Conc: 1.76 ng/ml

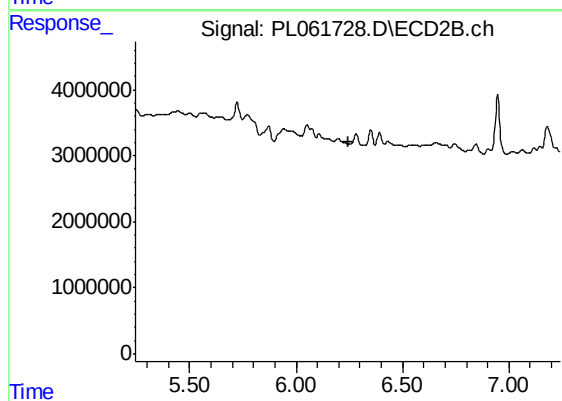

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

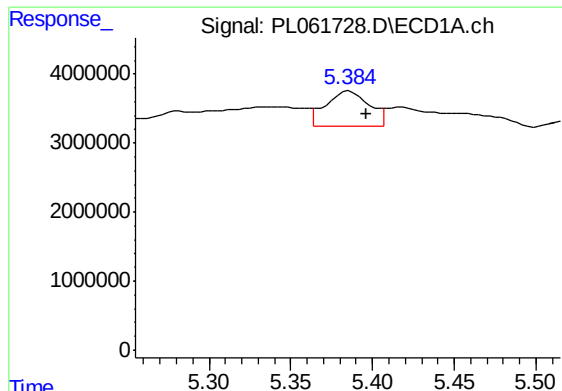

#10 gamma-Chlordane


R.T.: 5.386 min
Delta R.T.: -0.011 min
Response: 9688133
Conc: 5.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
MTB-SP

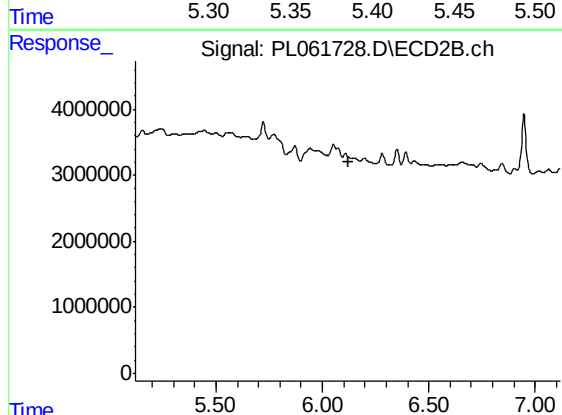


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

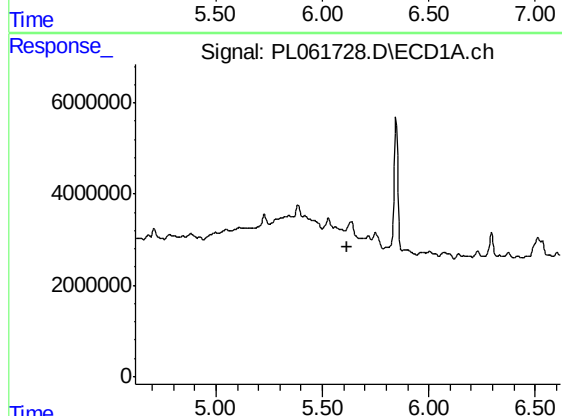


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.620 min
Response: 0
Conc: N.D.

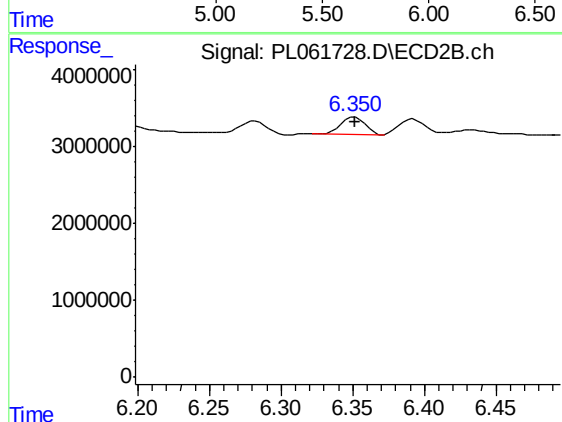

#12 4,4'-DDE


R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 2666194
Conc: 0.98 ng/ml

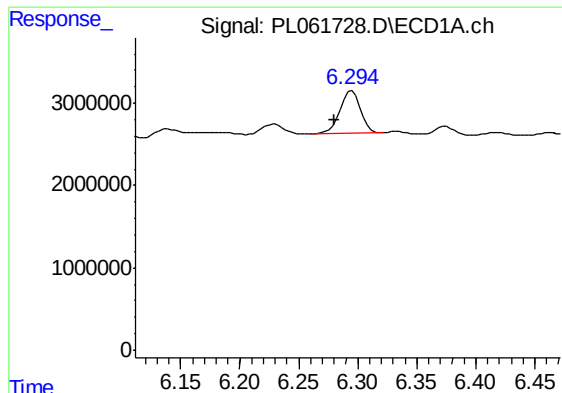

#15 Endosulfan II


R.T.: 6.295 min
Delta R.T.: 0.014 min
Response: 6384501
Conc: 3.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
MTB-SP

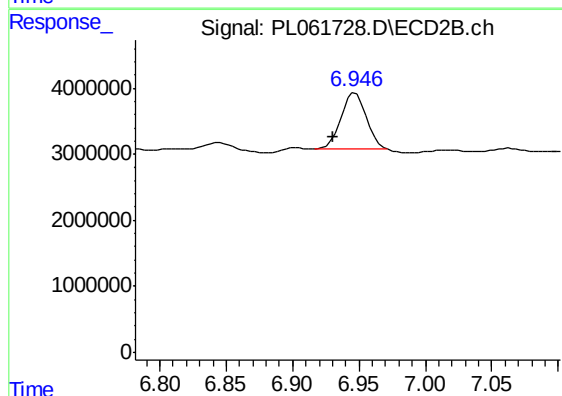


#15 Endosulfan II

R.T.: 6.947 min
Delta R.T.: 0.017 min
Response: 11309464
Conc: 4.38 ng/ml

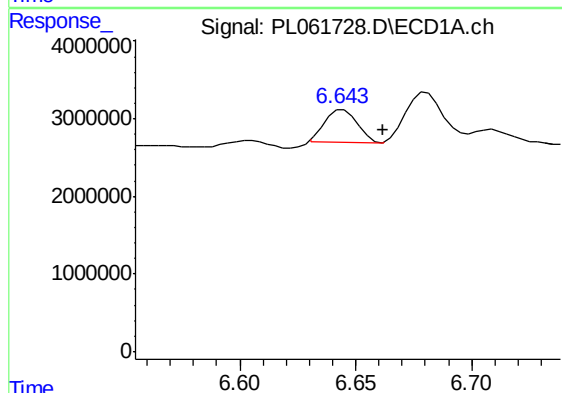


#19 Endosulfan Sulfate

R.T.: 6.645 min
Delta R.T.: -0.017 min
Response: 4118524
Conc: 2.66 ng/ml

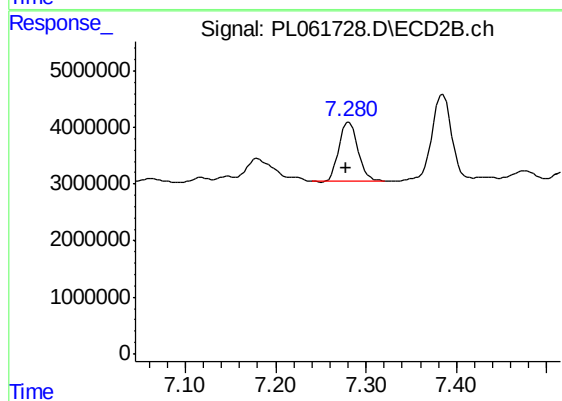

#19 Endosulfan Sulfate


R.T.: 7.281 min
Delta R.T.: 0.003 min
Response: 14780692
Conc: 6.31 ng/ml

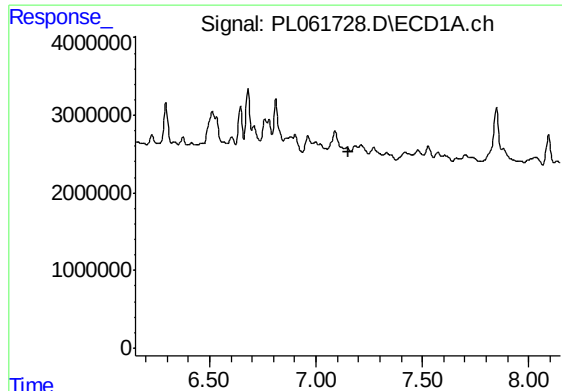

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
MTB-SP

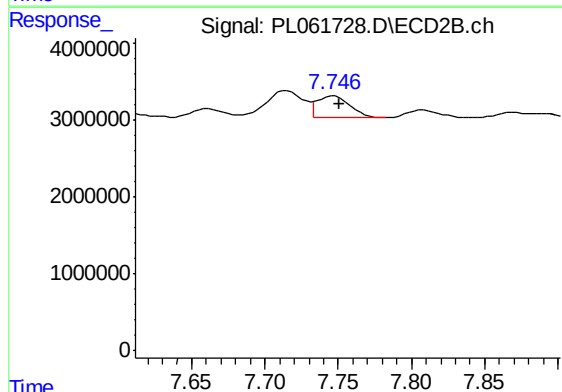


#21 Endrin ketone

R.T.: 7.747 min
Delta R.T.: -0.003 min
Response: 4394514
Conc: 1.87 ng/ml

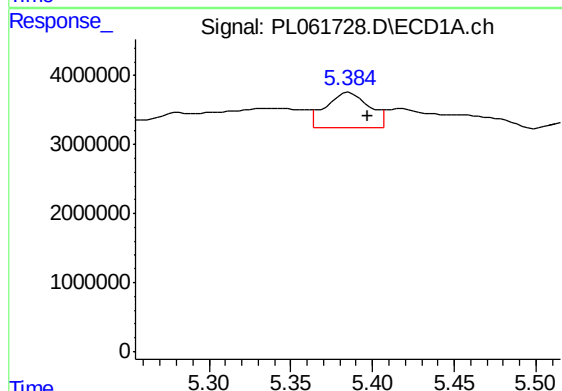


#25 Chlordane-3

R.T.: 5.386 min
Delta R.T.: -0.012 min
Response: 9688133
Conc: 61.64 ng/ml

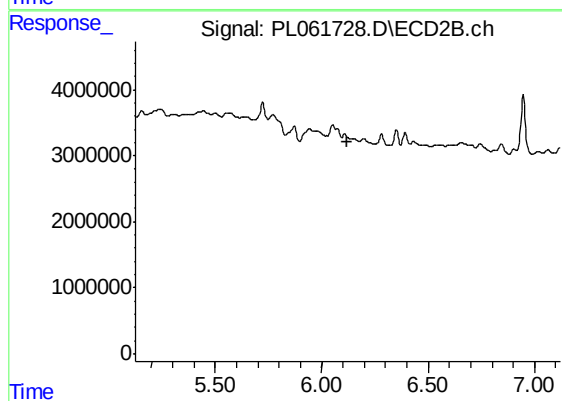

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.122 min
Response: 0
Conc: N.D.

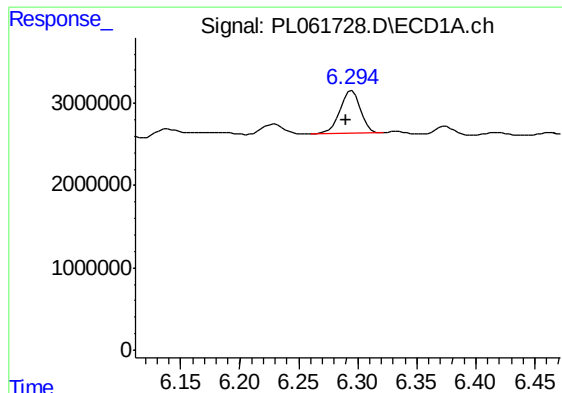

#27 Chlordane-5


R.T.: 6.295 min
Delta R.T.: 0.005 min
Response: 6384501
Conc: 117.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
MTB-SP

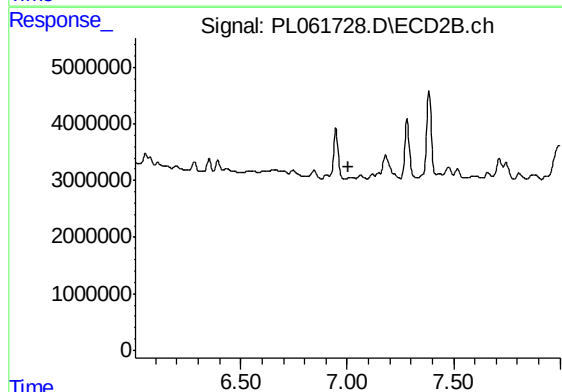


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.004 min
Response: 0
Conc: N.D.

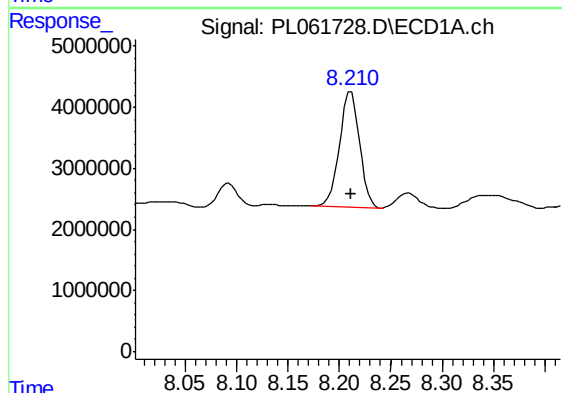

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 25739121
Conc: 15.82 ng/ml

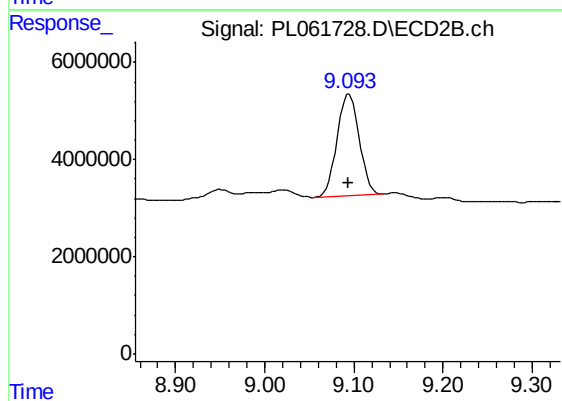

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 36325805
Conc: 16.50 ng/ml