

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 03:08
 Operator : DD\AJ
 Sample : L4094-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS-WC-L-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:21:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.459	4.008	27116774	36662463	15.895	13.438
28) SA	Decachlor...	8.211	9.096	15956922	18715155	9.809	8.502
Target Compounds							
8) B	Heptachlo...	0.000	5.900	0	17244756	N.D.	6.958 #
10) B	gamma-Chl...	0.000	6.128	0	5194601	N.D.	1.769 #
13) MA	Dieldrin	0.000	6.510	0	13599669	N.D.	4.794 #
16) A	4,4'-DDD	0.000	6.830	0	13361430	N.D.	6.010 #
20) A	Methoxychlor	0.000	7.611	0	2515695	N.D.	1.997 #
23)	Chlordane-1	4.332	0.000	1517178	0	30.640	N.D. #
25)	Chlordane-3	0.000	6.128	0	5194601	N.D.	14.176 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 03:08
Operator : DD\AJ
Sample : L4094-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:21:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

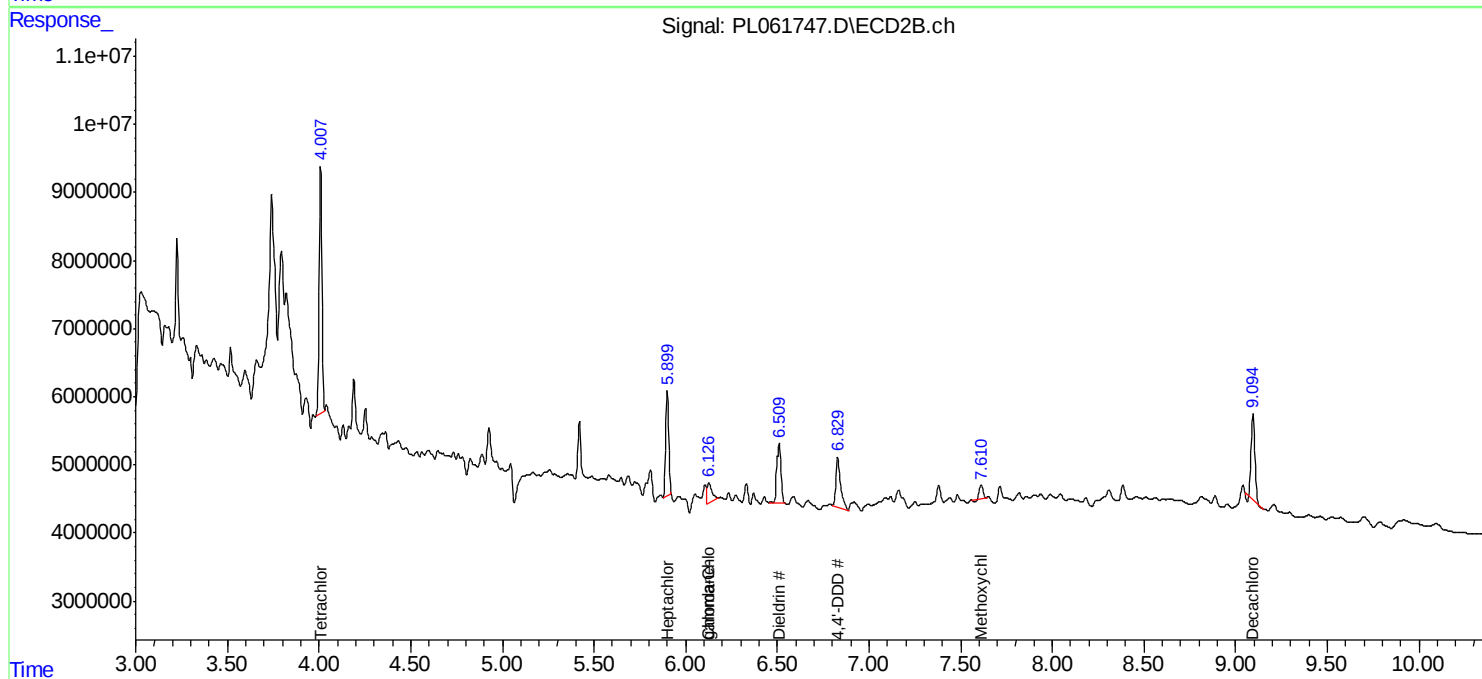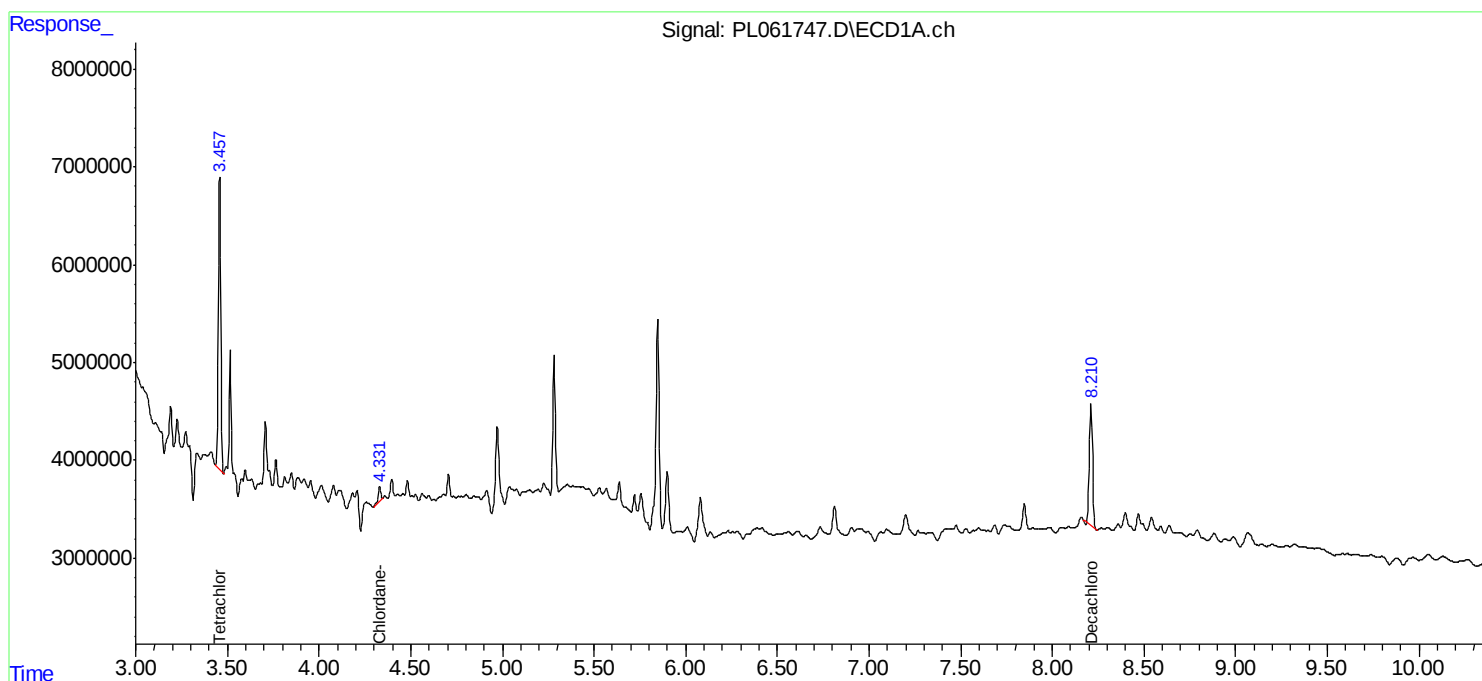


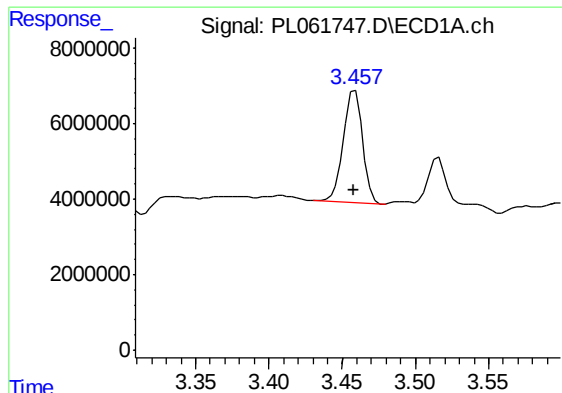

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 27116774
Conc: 15.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01

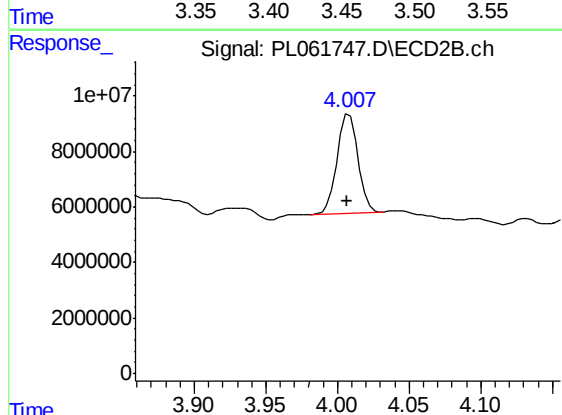


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 36662463
Conc: 13.44 ng/ml

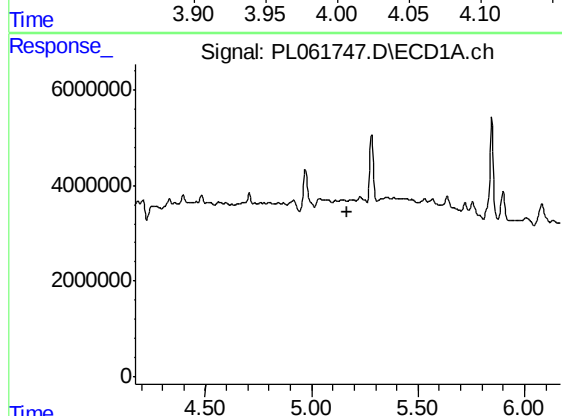


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

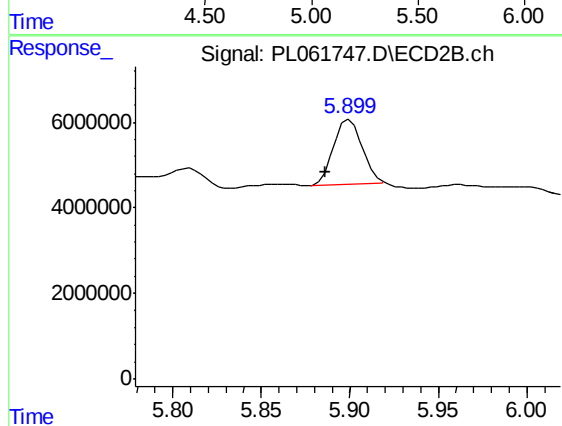

#8 Heptachlor epoxide


R.T.: 5.900 min
Delta R.T.: 0.014 min
Response: 17244756
Conc: 6.96 ng/ml

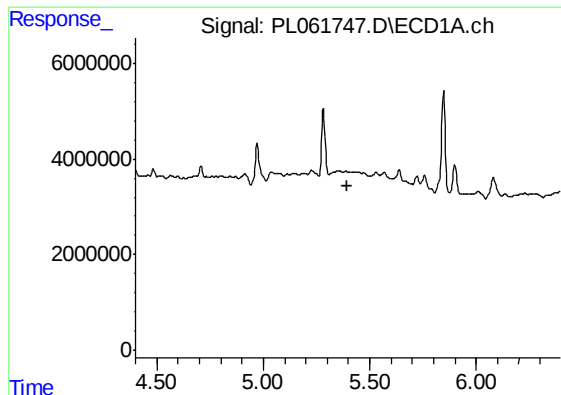

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01

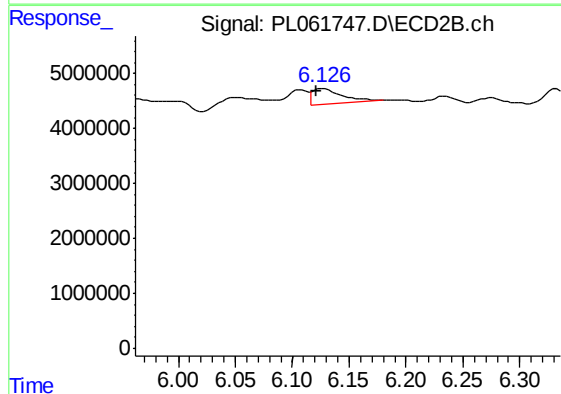


#10 gamma-Chlordane

R.T.: 6.128 min
Delta R.T.: 0.006 min
Response: 5194601
Conc: 1.77 ng/ml

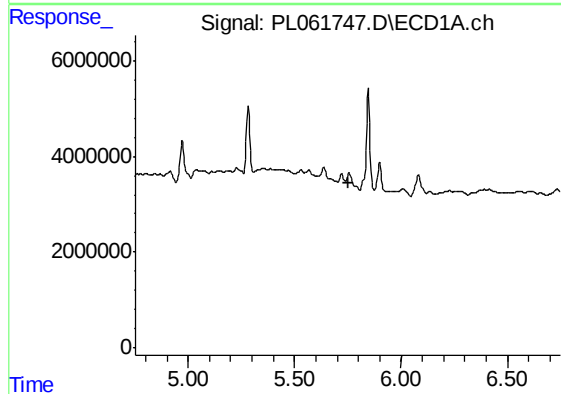


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

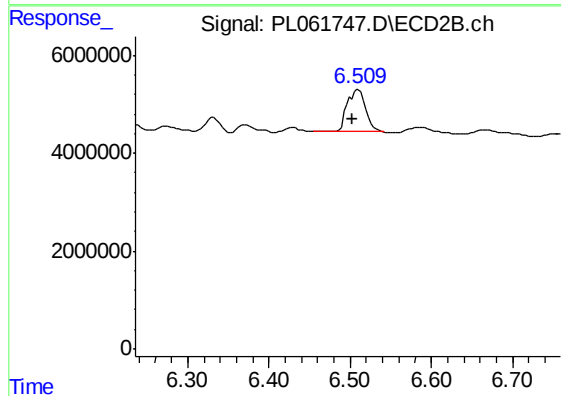

#13 Dieldrin


R.T.: 6.510 min
Delta R.T.: 0.008 min
Response: 13599669
Conc: 4.79 ng/ml

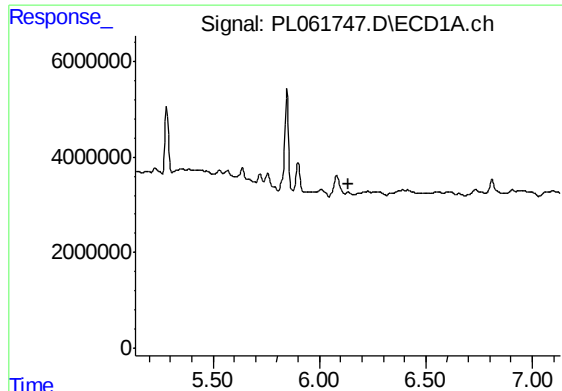

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01

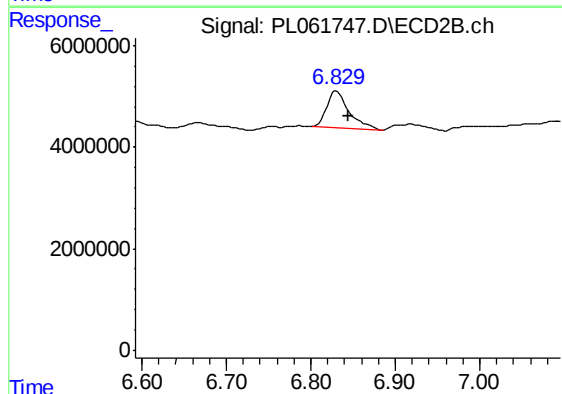


#16 4,4'-DDD

R.T.: 6.830 min
Delta R.T.: -0.014 min
Response: 13361430
Conc: 6.01 ng/ml

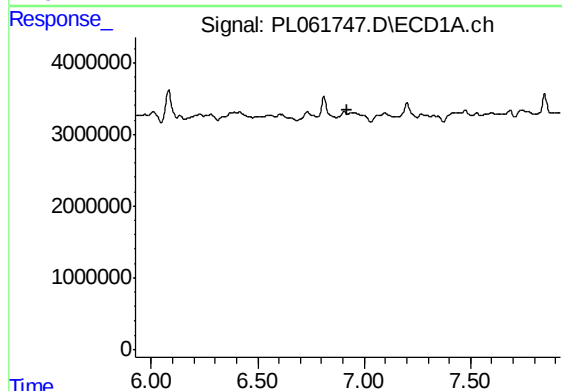


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

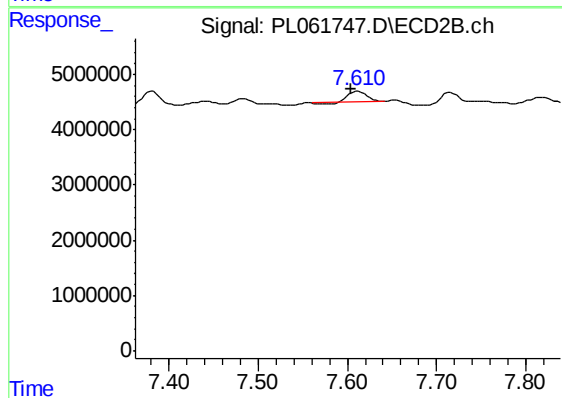

#20 Methoxychlor


R.T.: 7.611 min
Delta R.T.: 0.007 min
Response: 2515695
Conc: 2.00 ng/ml

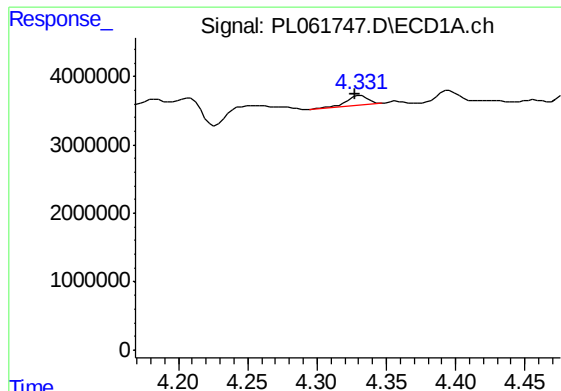

#23 Chlordane-1


R.T.: 4.332 min
Delta R.T.: 0.005 min
Response: 1517178
Conc: 30.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01

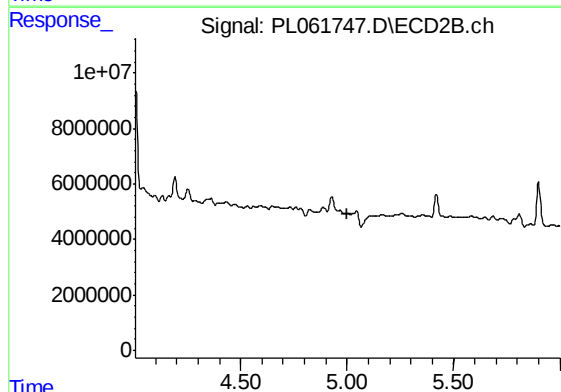


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.004 min
Response: 0
Conc: N.D.

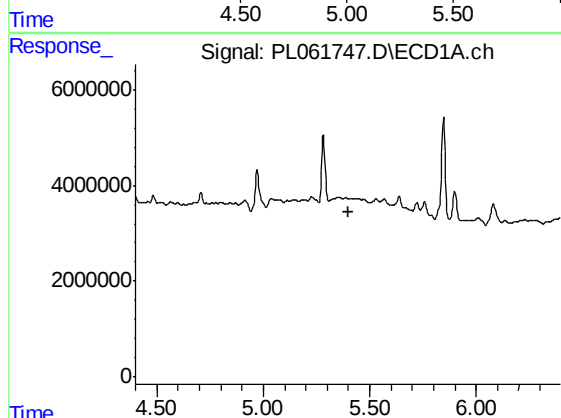


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

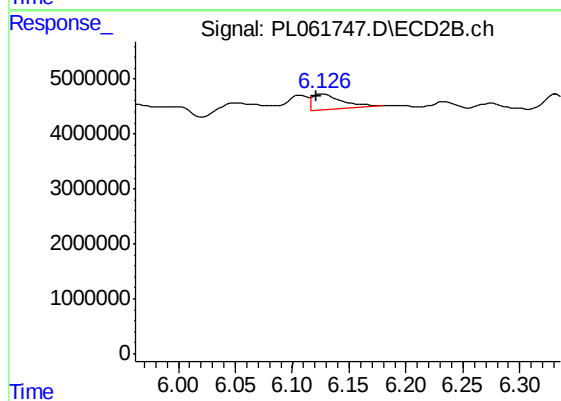

#25 Chlordane-3


R.T.: 6.128 min
Delta R.T.: 0.006 min
Response: 5194601
Conc: 14.18 ng/ml

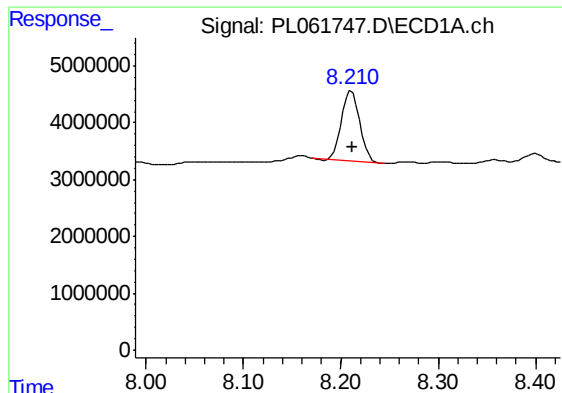

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 15956922
Conc: 9.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01

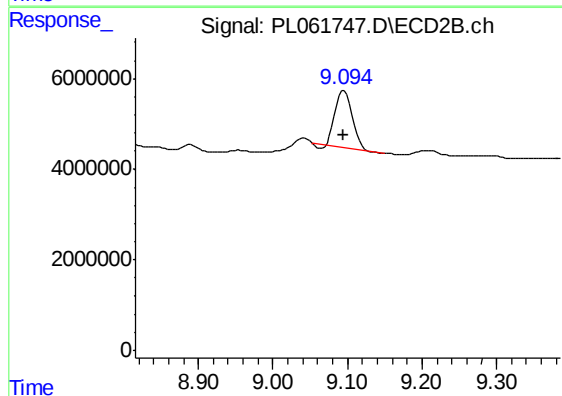

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 18715155
Conc: 8.50 ng/ml