

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 12:30
 Operator : DD\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 13:33:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:32:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	196.6E6	263.4E6	97.500	99.824
28)	SA Decachlor...	8.211	9.095	153.4E6	206.0E6	92.185	96.049
Target Compounds							
23)	Chlordane-1	4.327	5.004	47273160	93295522	932.121	978.727
24)	Chlordane-2	4.829	5.473	55529035	94361279	910.088	947.381
25)	Chlordane-3	5.398	6.122	158.8E6	370.0E6	989.313	994.068
26)	Chlordane-4	5.455	6.197	131.4E6	447.2E6	972.414	982.160
27)	Chlordane-5	6.290	7.004	53867458	72885415	979.495	1004.804



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 12:30
Operator : DD\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 13:33:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:32:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

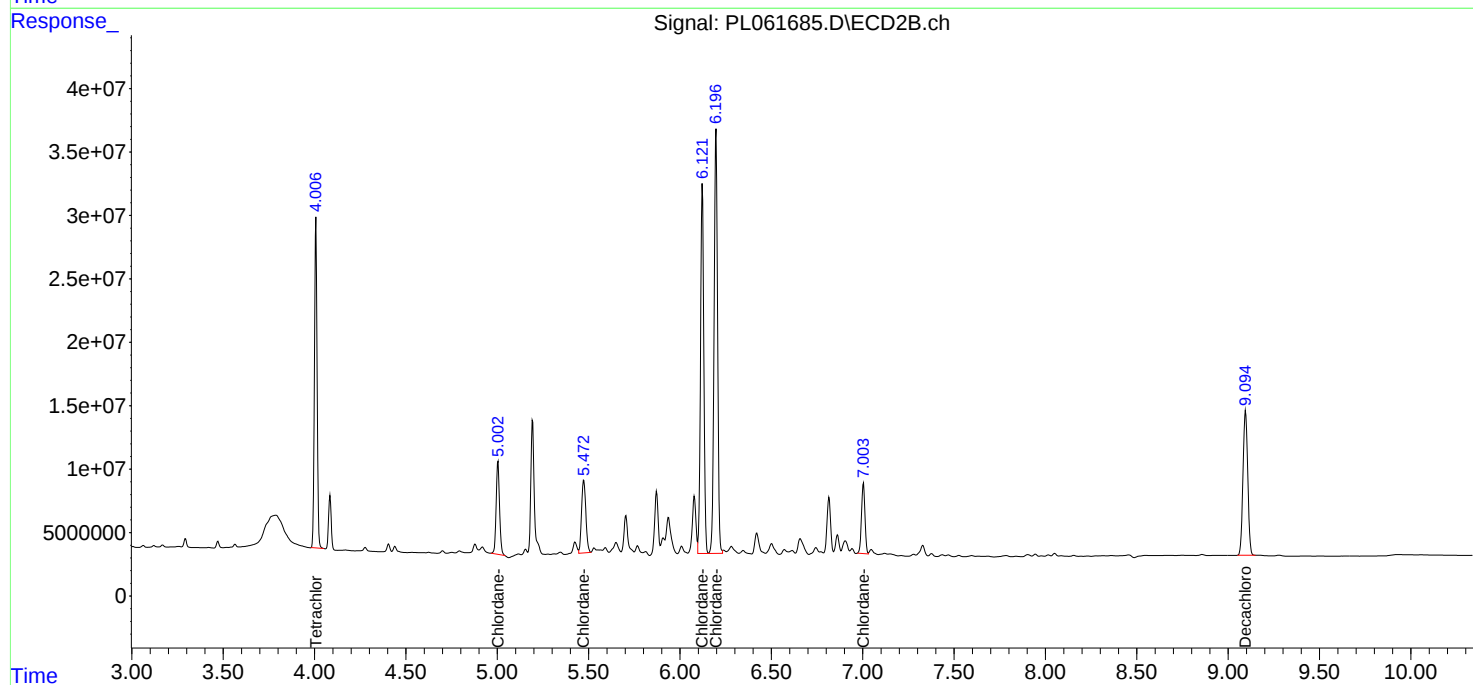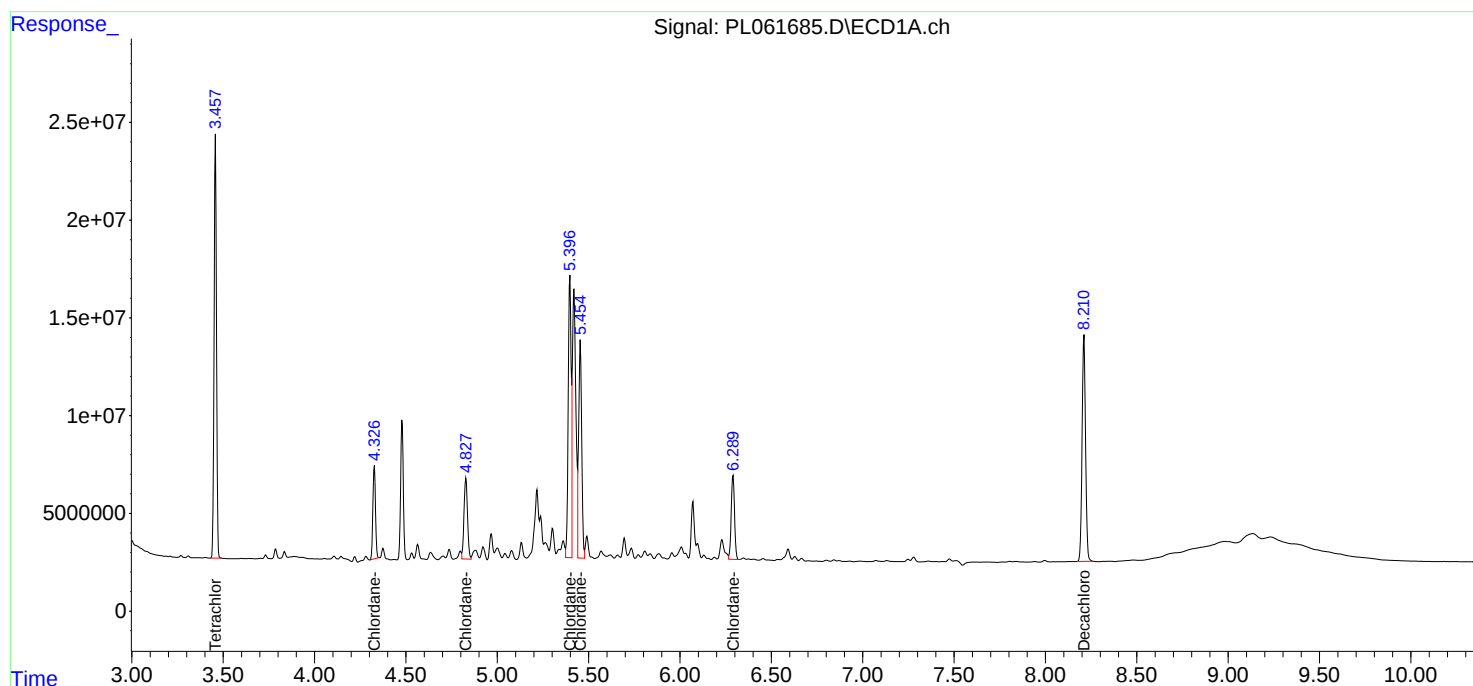


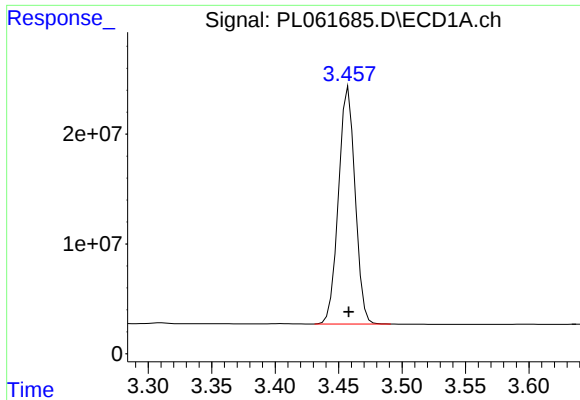

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 196550252
Conc: 97.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

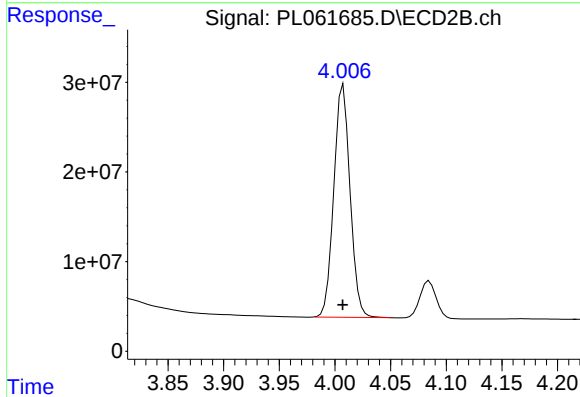


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 263431192
Conc: 99.82 ng/ml

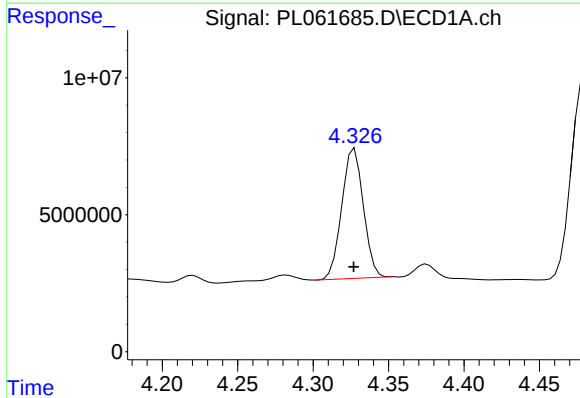


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 47273160
Conc: 932.12 ng/ml

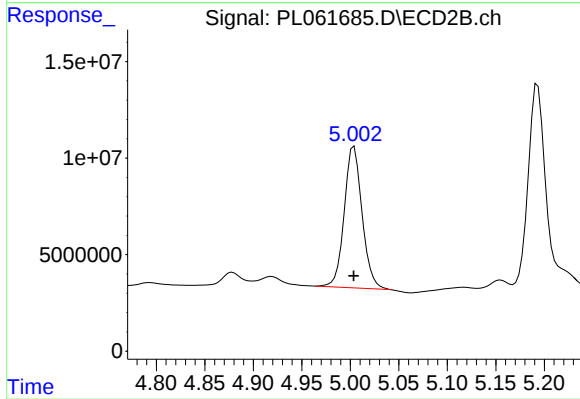

#23 Chlordane-1


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 93295522
Conc: 978.73 ng/ml

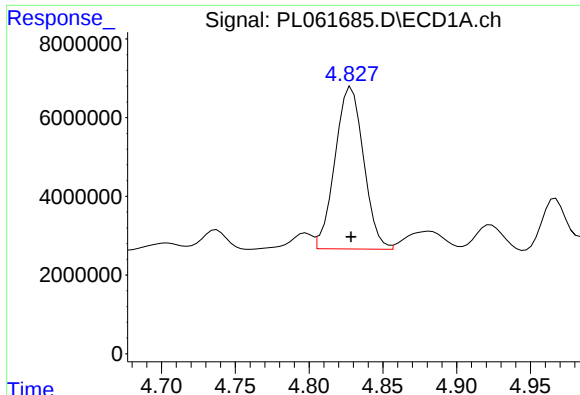

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 55529035
Conc: 910.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

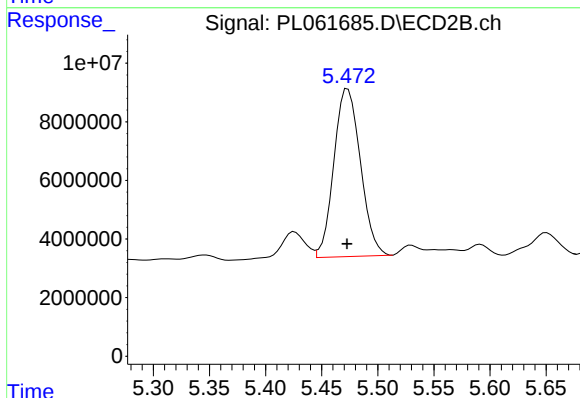


#24 Chlordane-2

R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 94361279
Conc: 947.38 ng/ml

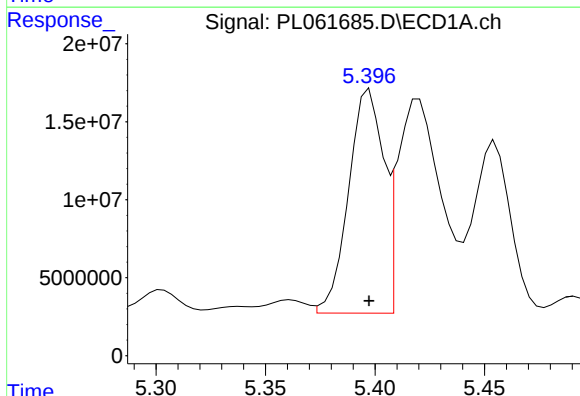


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 158831503
Conc: 989.31 ng/ml

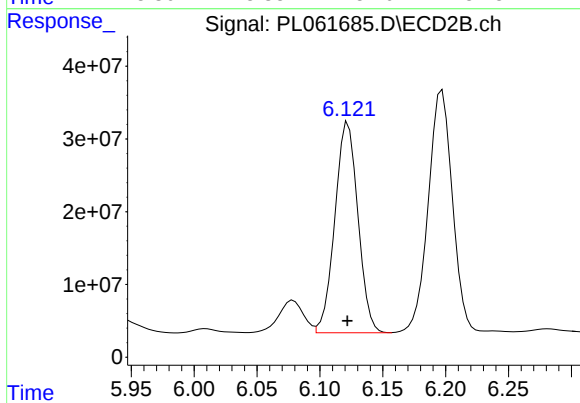

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 370022584
Conc: 994.07 ng/ml

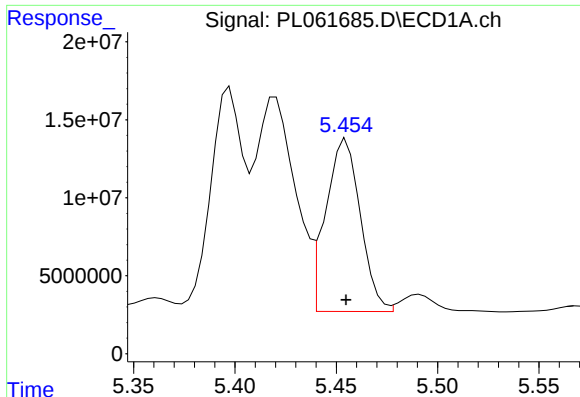

#26 Chlordane-4


R.T.: 5.455 min
Delta R.T.: 0.000 min
Response: 131357670
Conc: 972.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

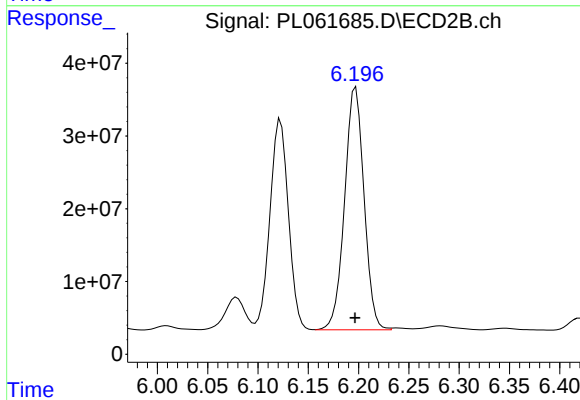


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 447194399
Conc: 982.16 ng/ml

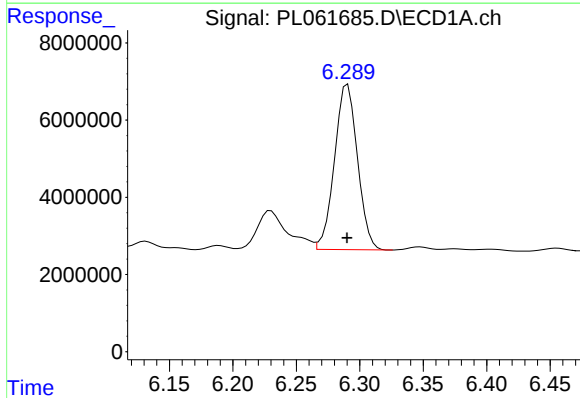


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 53867458
Conc: 979.50 ng/ml

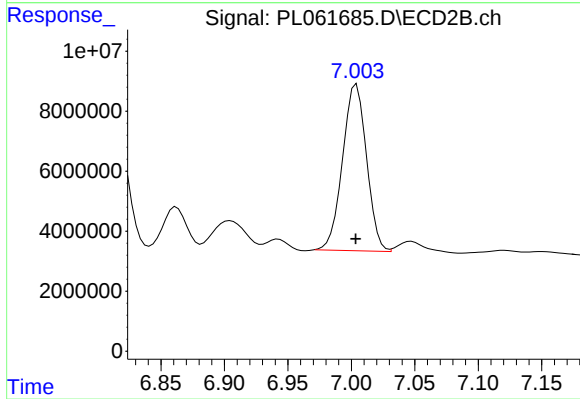

#27 Chlordane-5


R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 72885415
Conc: 1004.80 ng/ml

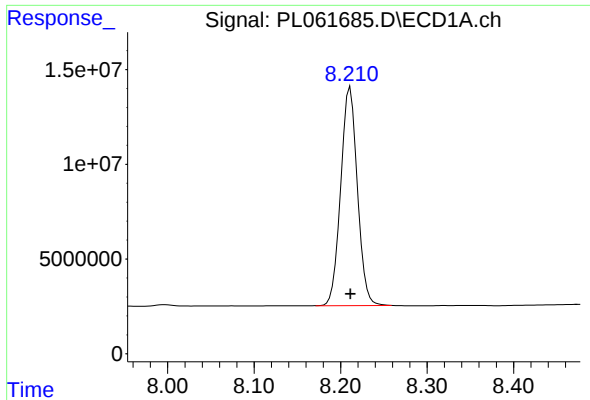

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 153355269
Conc: 92.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

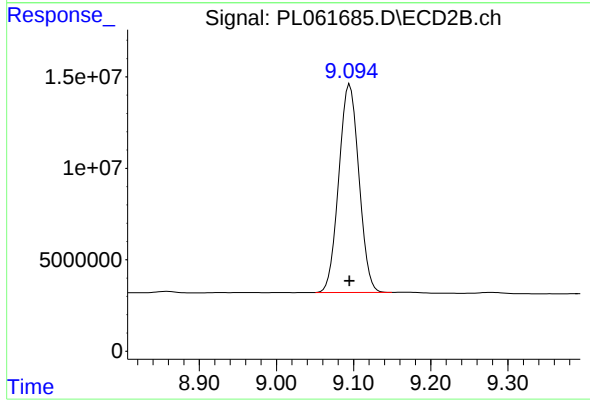

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 205998470
Conc: 96.05 ng/ml