

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 12:58
 Operator : DD\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 13:32:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:32:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	100.8E6	131.9E6	50.000	50.000
28)	SA Decachlor...	8.211	9.095	83178050	107.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.327	5.004	25357842	47661668	500.000	500.000
24)	Chlordane-2	4.829	5.473	30507508	49801149	500.000	500.000
25)	Chlordane-3	5.397	6.122	80273665	186.1E6	500.000	500.000
26)	Chlordane-4	5.455	6.197	67542018	227.7E6	500.000	500.000
27)	Chlordane-5	6.290	7.004	27497559	36268481	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 12:58
Operator : DD\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 13:32:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:32:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

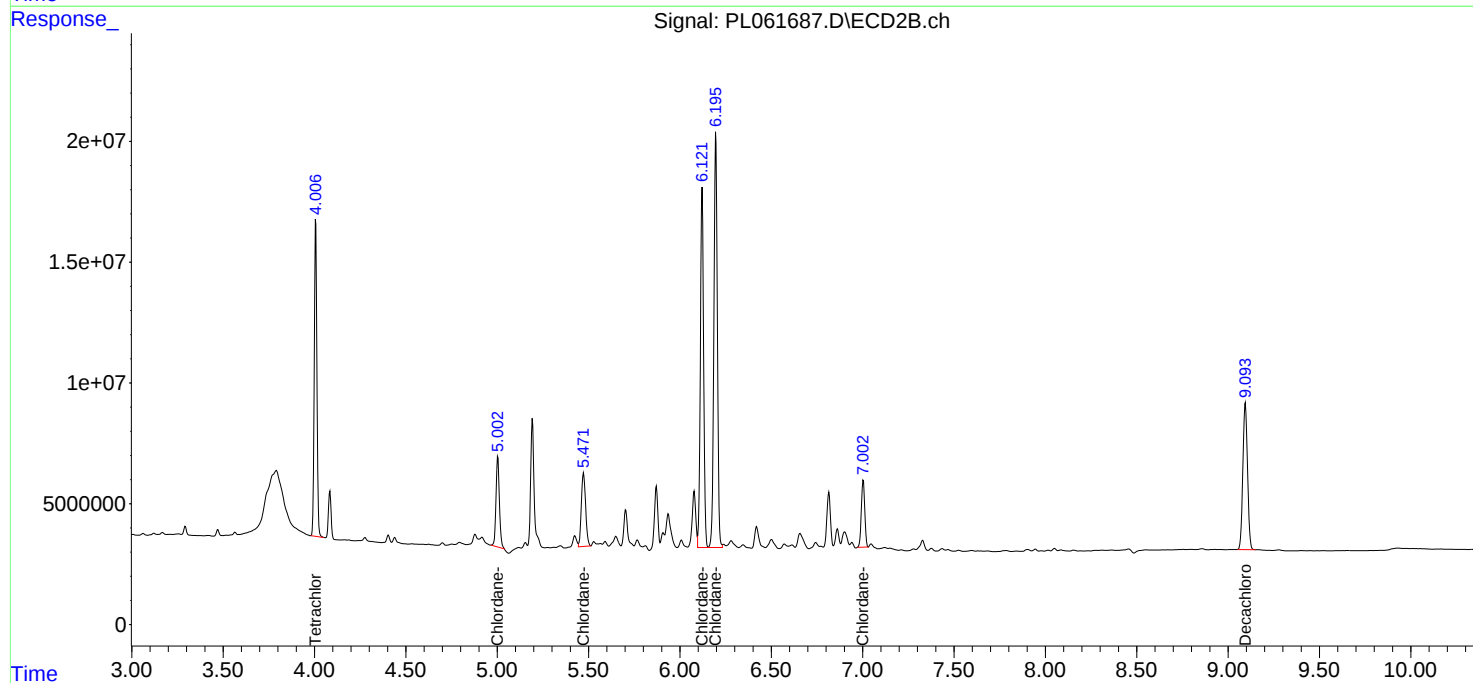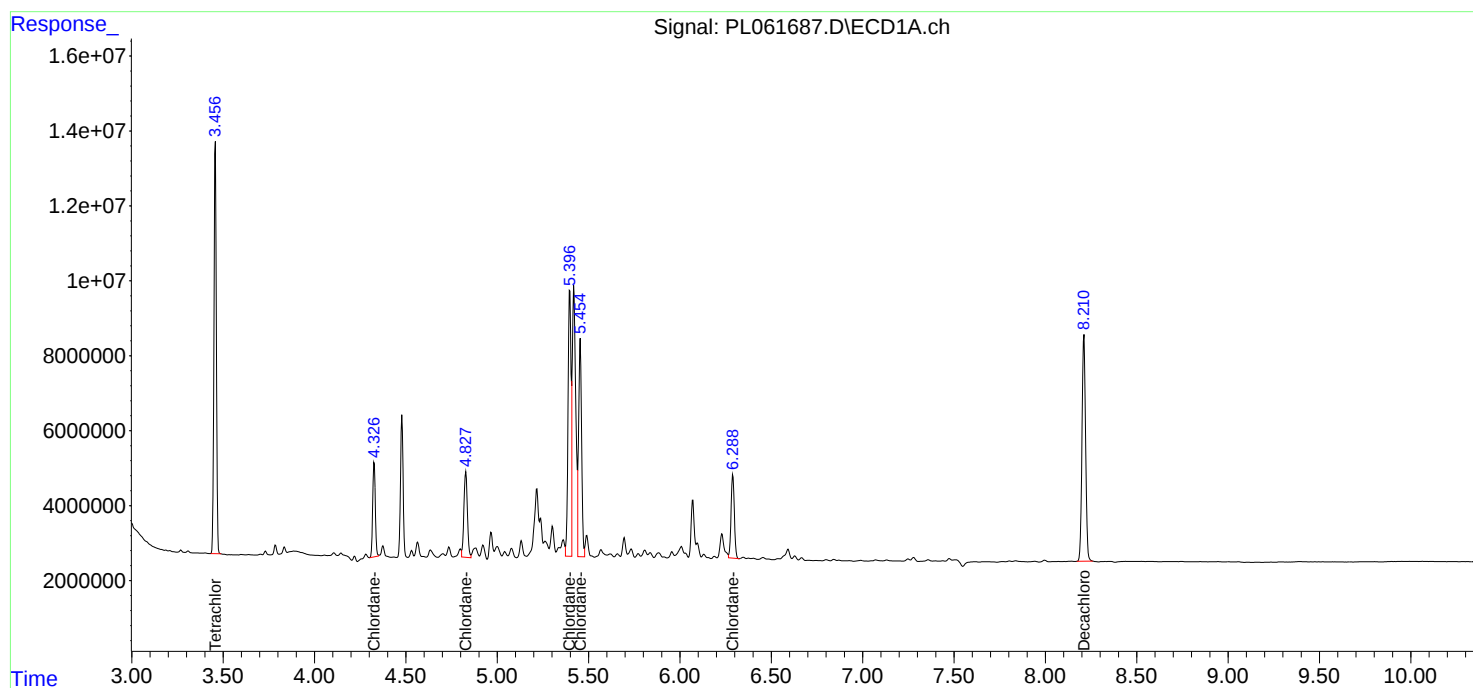


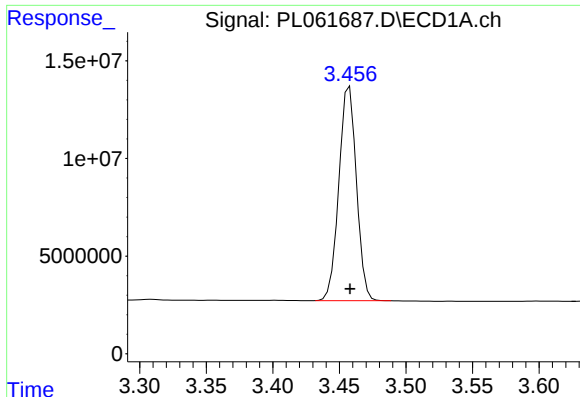

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 100795184
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

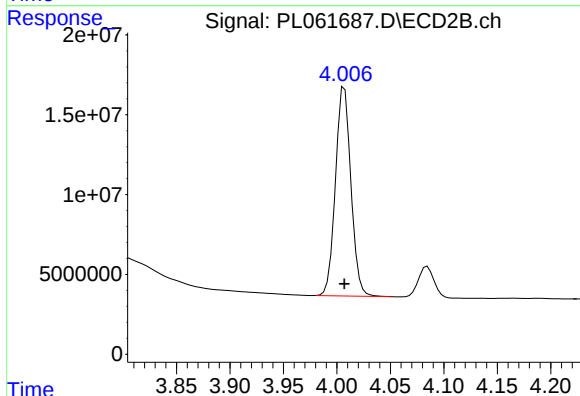


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 131948223
Conc: 50.00 ng/ml

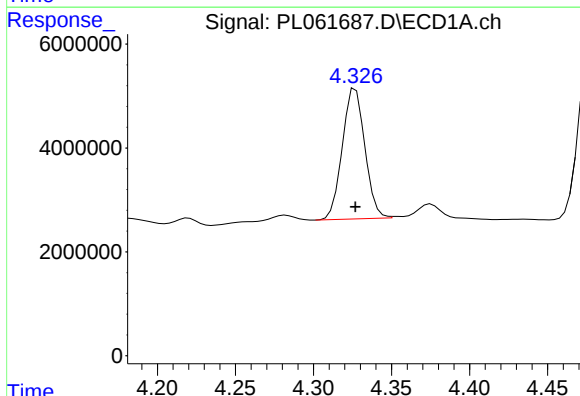


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 25357842
Conc: 500.00 ng/ml

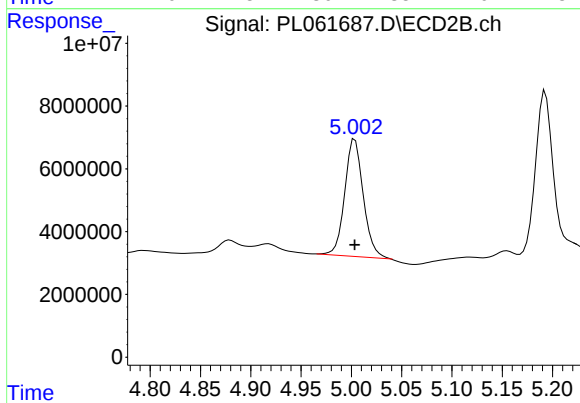

#23 Chlordane-1


R.T.: 5.004 min
Delta R.T.: 0.000 min
Response: 47661668
Conc: 500.00 ng/ml

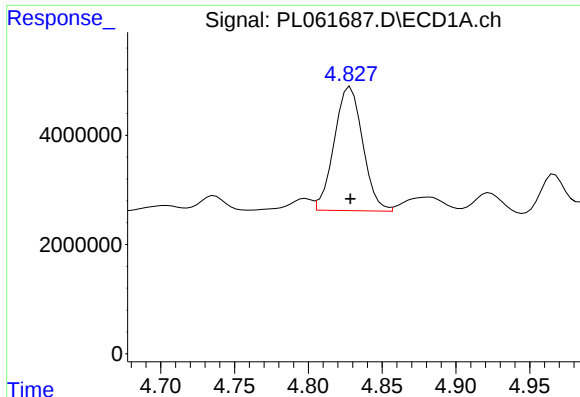

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 30507508
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

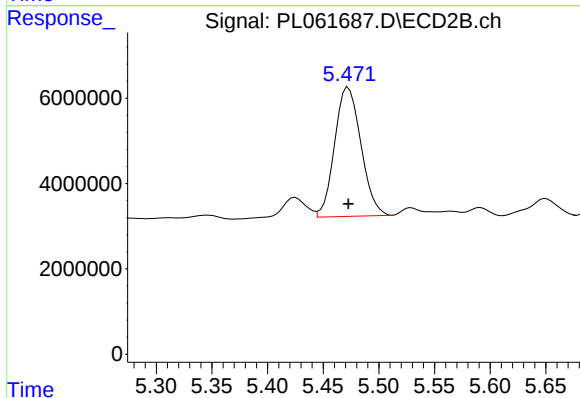


#24 Chlordane-2

R.T.: 5.473 min
Delta R.T.: 0.000 min
Response: 49801149
Conc: 500.00 ng/ml

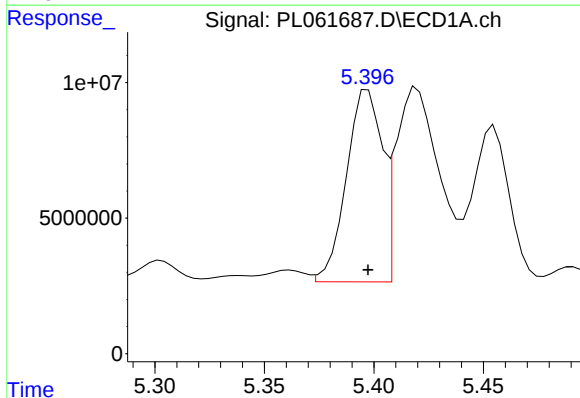


#25 Chlordane-3

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 80273665
Conc: 500.00 ng/ml

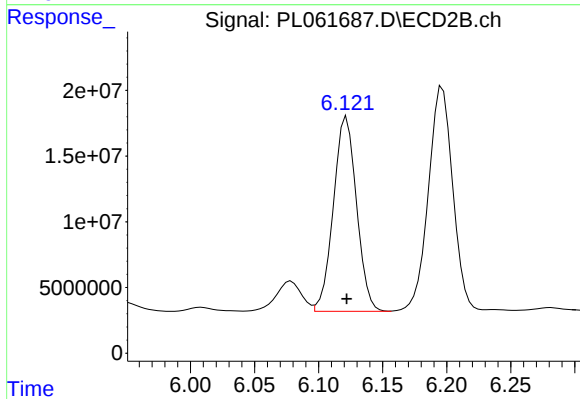

#25 Chlordane-3


R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 186115322
Conc: 500.00 ng/ml

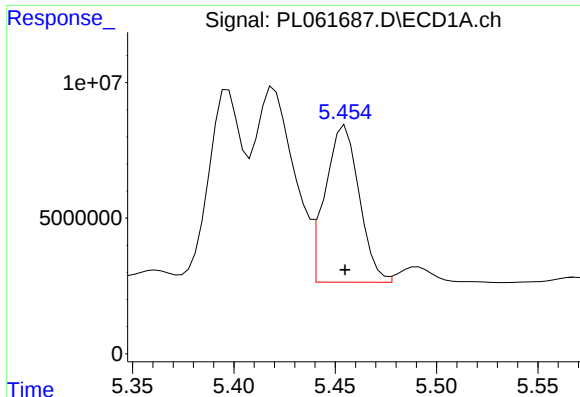

#26 Chlordane-4


R.T.: 5.455 min
Delta R.T.: 0.000 min
Response: 67542018
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

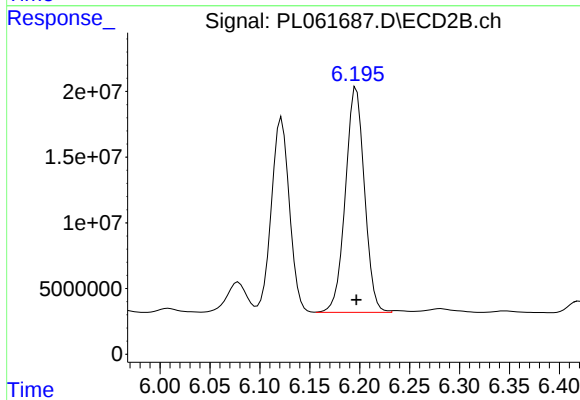


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 227658558
Conc: 500.00 ng/ml

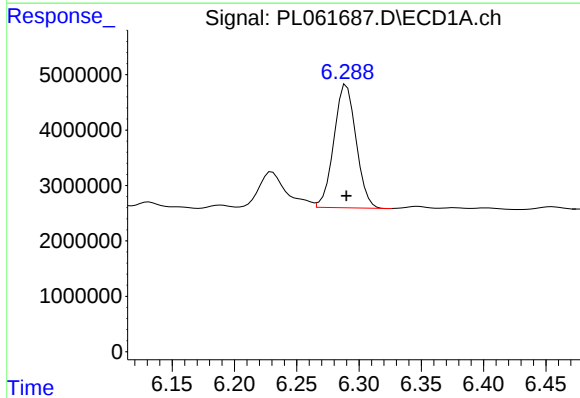


#27 Chlordane-5

R.T.: 6.290 min
Delta R.T.: 0.000 min
Response: 27497559
Conc: 500.00 ng/ml

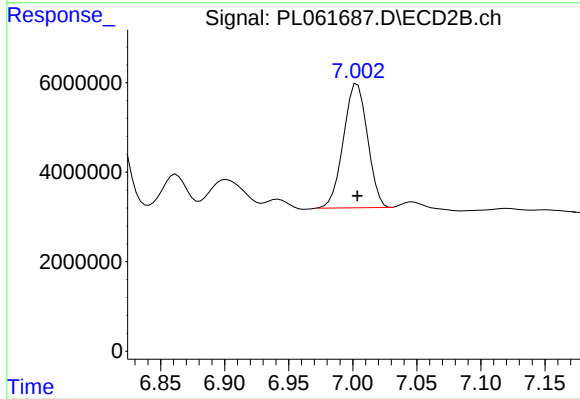

#27 Chlordane-5


R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 36268481
Conc: 500.00 ng/ml

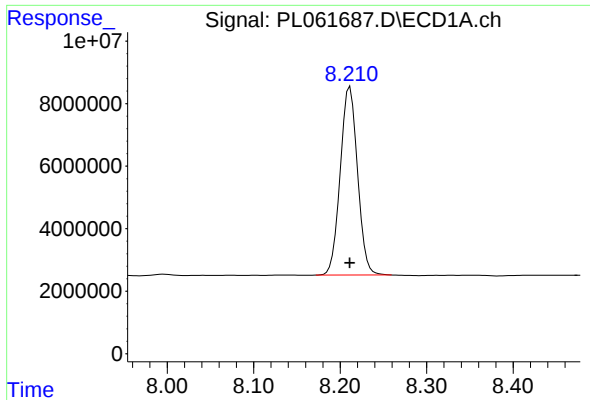

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 83178050
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

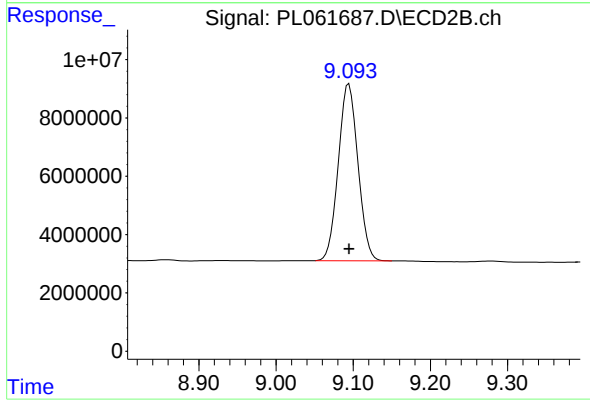

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 107236365
Conc: 50.00 ng/ml