

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 19:08
 Operator : DD\AJ
 Sample : L3971-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PT-CHLR-WP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:12:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	4.008	81002243	60649853	47.482	22.230 #
28)	SA Decachlor...	8.211	9.097	43764006	58719700	26.903	26.674
Target Compounds							
23)	Chlordane-1	4.327	5.005	97391690	193.1E6	1966.877	2050.768
24)	Chlordane-2	4.829	5.475	107.2E6	185.4E6	1823.217	1801.876
25)	Chlordane-3	5.398	6.124	353.5E6	753.1E6	2248.710	2055.317
26)	Chlordane-4	5.456	6.198	292.7E6	864.8E6	2243.264	1926.346
27)	Chlordane-5	6.291	7.005	100.1E6	142.8E6	1835.395	1964.972


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 19:08
Operator : DD\AJ
Sample : L3971-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:12:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

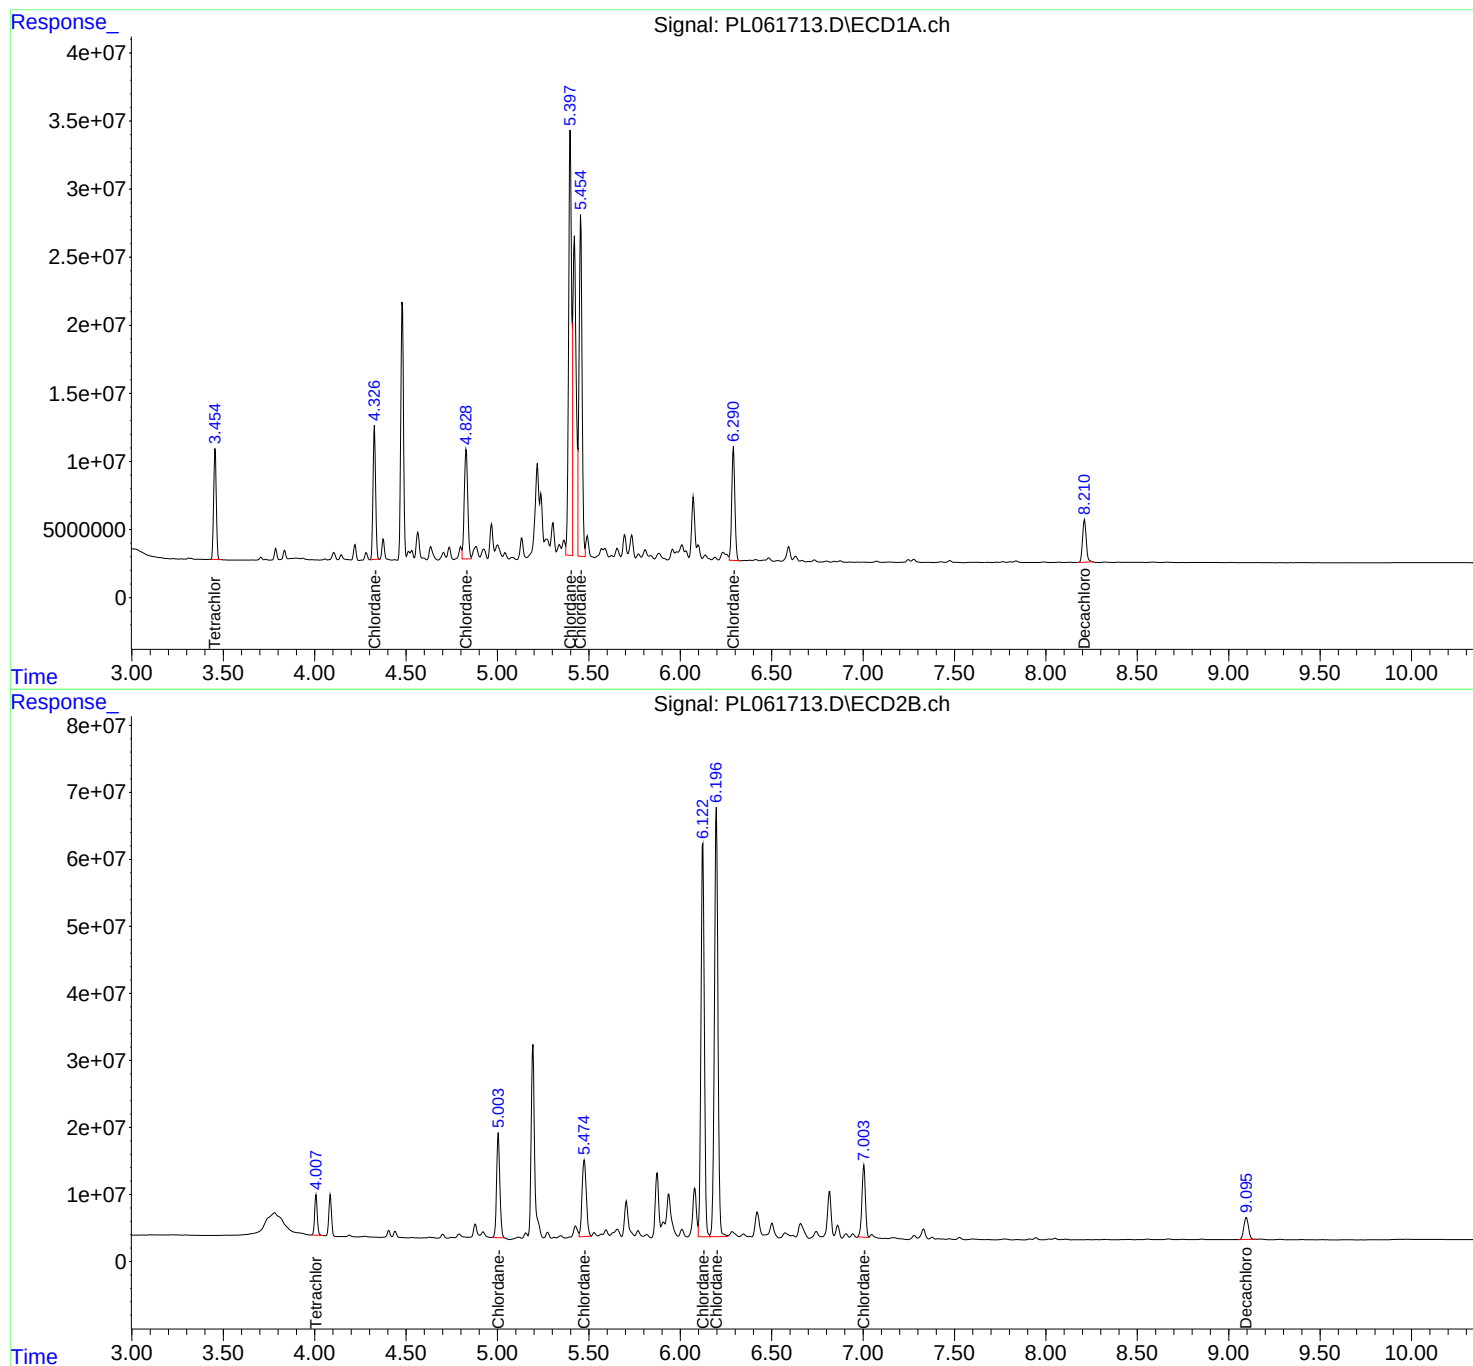


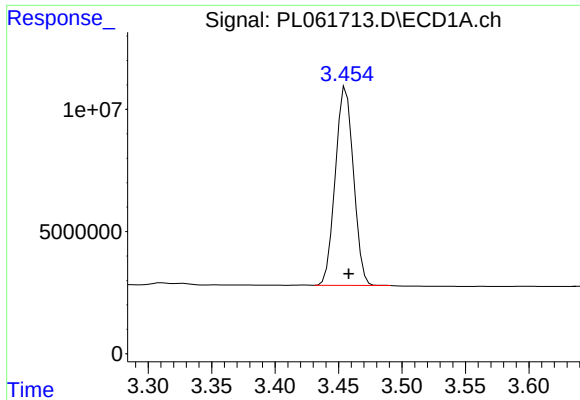

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 81002243
Conc: 47.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

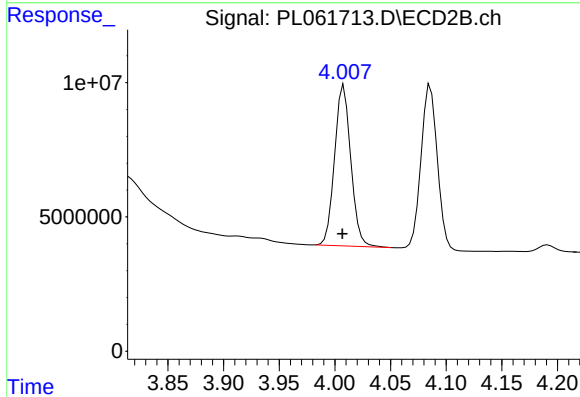


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 60649853
Conc: 22.23 ng/ml

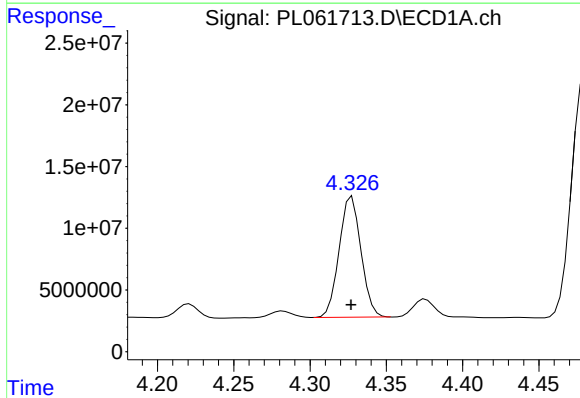


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 97391690
Conc: 1966.88 ng/ml

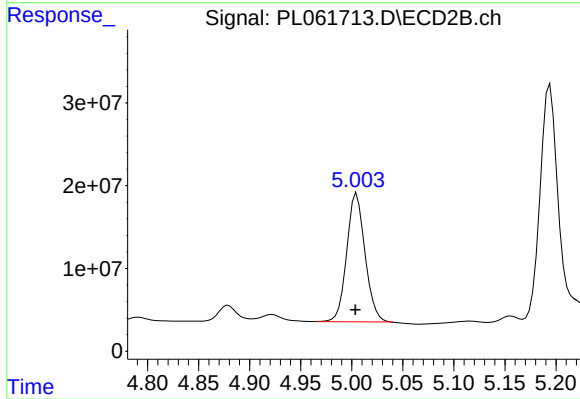

#23 Chlordane-1


R.T.: 5.005 min
Delta R.T.: 0.001 min
Response: 193090991
Conc: 2050.77 ng/ml

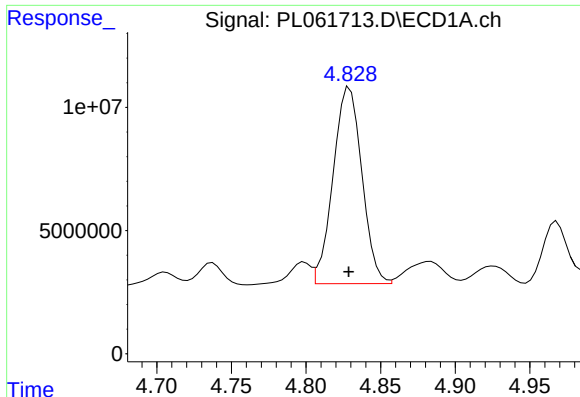

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 107215803
Conc: 1823.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

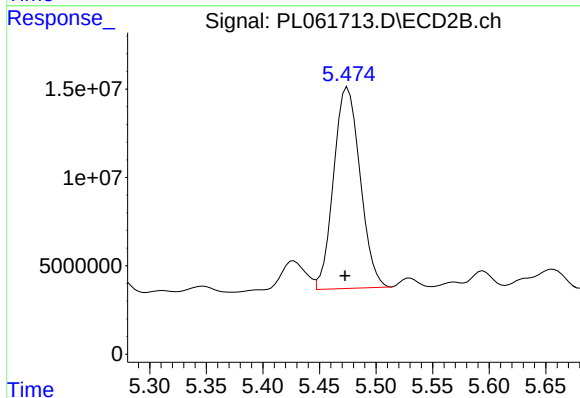


#24 Chlordane-2

R.T.: 5.475 min
Delta R.T.: 0.002 min
Response: 185421745
Conc: 1801.88 ng/ml

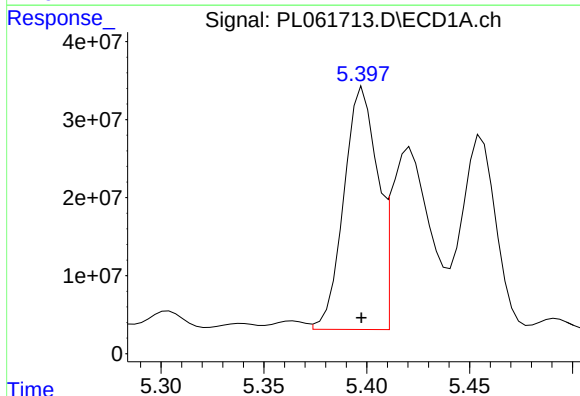


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.001 min
Response: 353456338
Conc: 2248.71 ng/ml

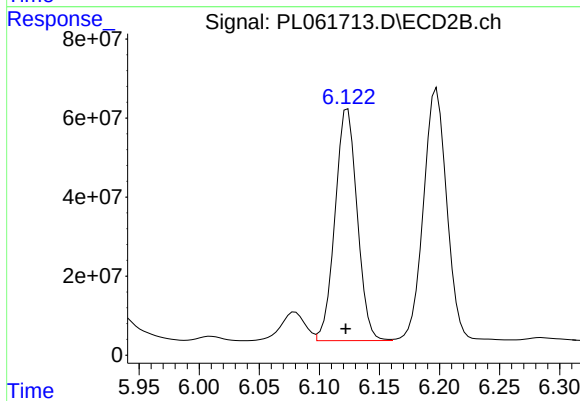

#25 Chlordane-3


R.T.: 6.124 min
Delta R.T.: 0.002 min
Response: 753144939
Conc: 2055.32 ng/ml

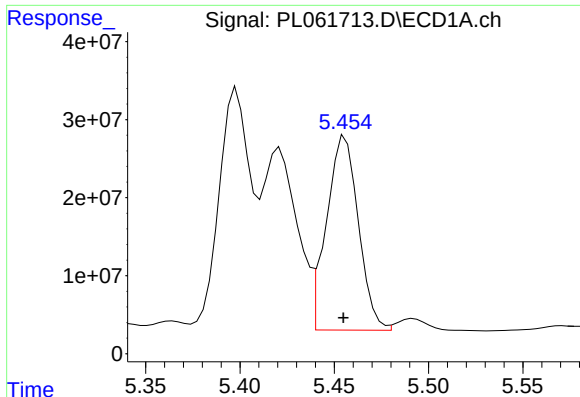

#26 Chlordane-4


R.T.: 5.456 min
Delta R.T.: 0.000 min
Response: 292682133
Conc: 2243.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

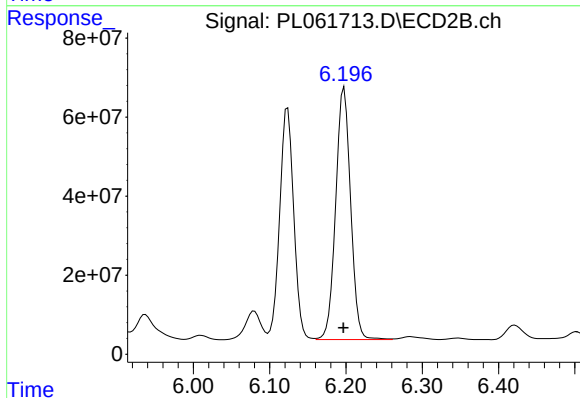


#26 Chlordane-4

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 864768137
Conc: 1926.35 ng/ml

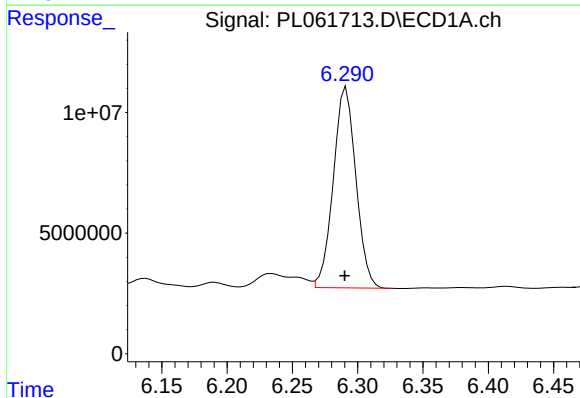


#27 Chlordane-5

R.T.: 6.291 min
Delta R.T.: 0.001 min
Response: 100077438
Conc: 1835.40 ng/ml

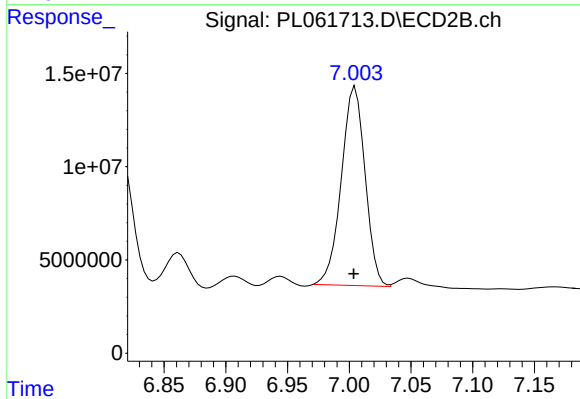

#27 Chlordane-5


R.T.: 7.005 min
Delta R.T.: 0.001 min
Response: 142814923
Conc: 1964.97 ng/ml

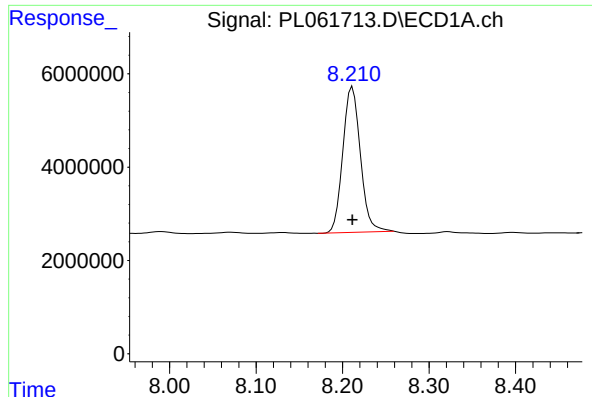

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 43764006
Conc: 26.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PT-CHLR-WP

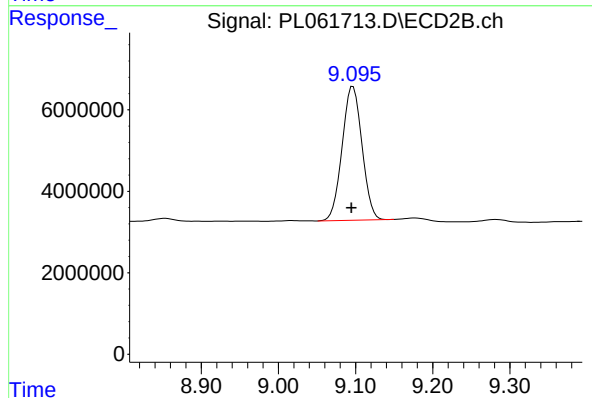

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.002 min
Response: 58719700
Conc: 26.67 ng/ml