

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 20:18
 Operator : DD\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:13:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.009	100.5E6	134.9E6	58.922	49.454
28)	SA Decachlor...	8.212	9.096	87115375	120.1E6	53.552	54.562
Target Compounds							
23)	Chlordane-1	4.327	5.005	26383962	48482842	532.838	514.923
24)	Chlordane-2	4.829	5.474	31014355	51600660	527.403	501.440
25)	Chlordane-3	5.398	6.123	83177570	195.8E6	529.181	534.441
26)	Chlordane-4	5.456	6.197	69486415	238.8E6	532.579	532.002
27)	Chlordane-5	6.291	7.004	28006845	38141690	513.639	524.786



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 20:18
Operator : DD\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:13:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

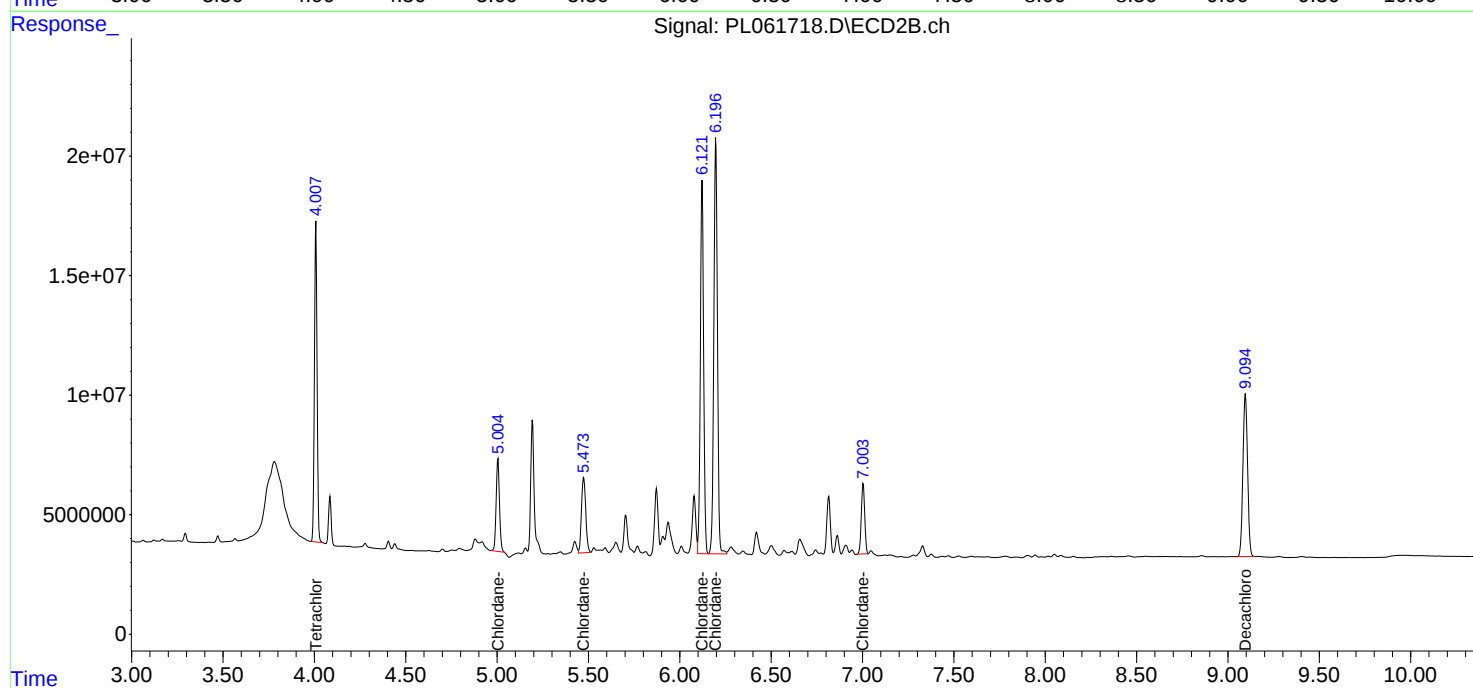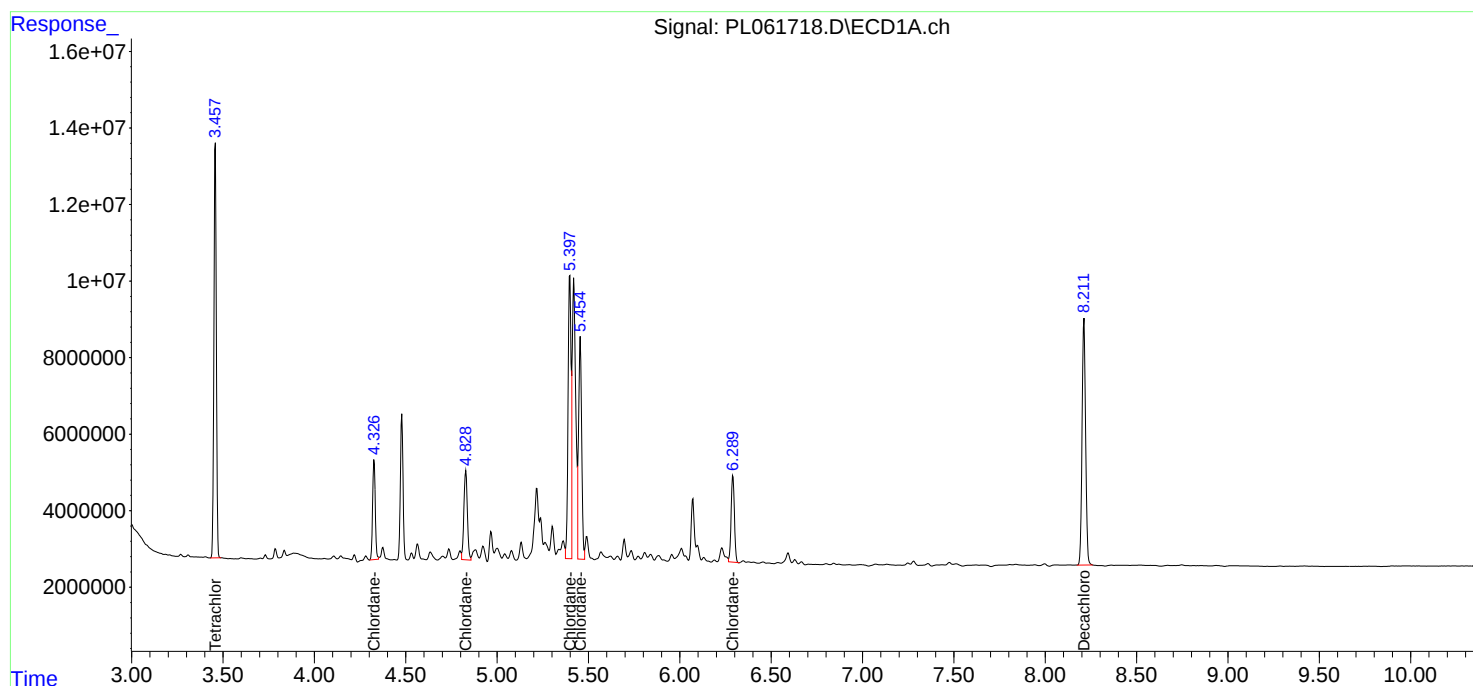


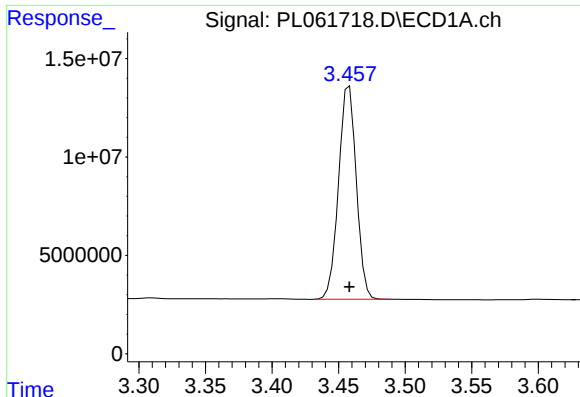

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 100518795
Conc: 58.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

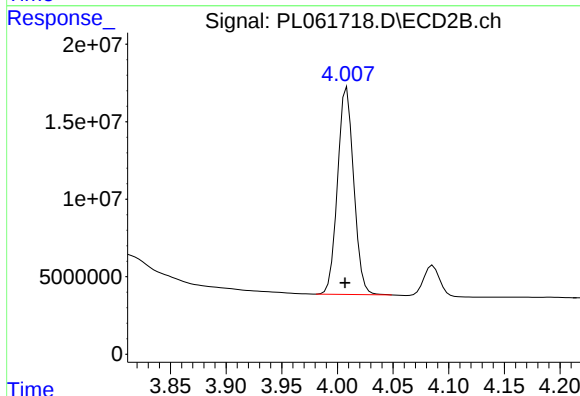


#1 Tetrachloro-m-xylene

R.T.: 4.009 min
Delta R.T.: 0.002 min
Response: 134923175
Conc: 49.45 ng/ml

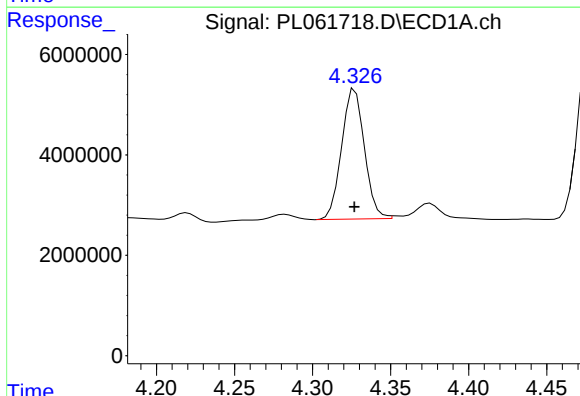


#23 Chlordane-1

R.T.: 4.327 min
Delta R.T.: 0.000 min
Response: 26383962
Conc: 532.84 ng/ml

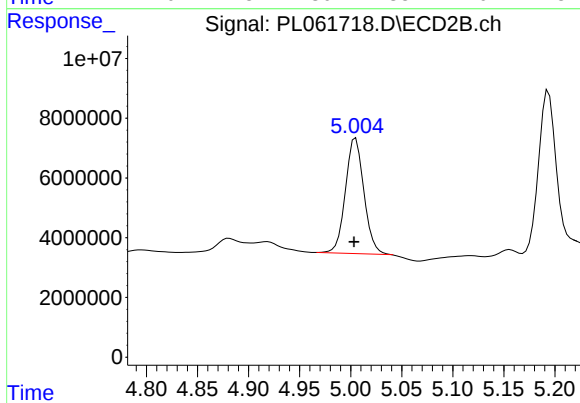

#23 Chlordane-1


R.T.: 5.005 min
Delta R.T.: 0.001 min
Response: 48482842
Conc: 514.92 ng/ml

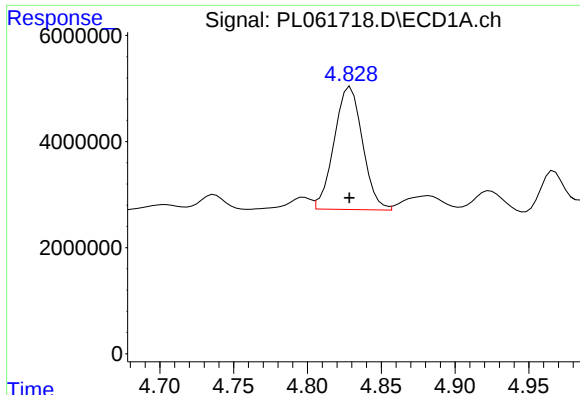

#24 Chlordane-2


R.T.: 4.829 min
Delta R.T.: 0.000 min
Response: 31014355
Conc: 527.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

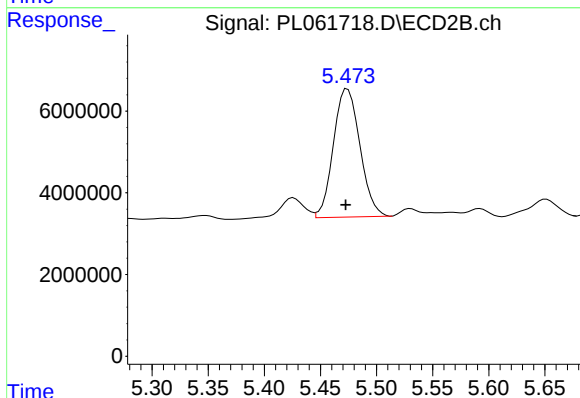


#24 Chlordane-2

R.T.: 5.474 min
Delta R.T.: 0.002 min
Response: 51600660
Conc: 501.44 ng/ml

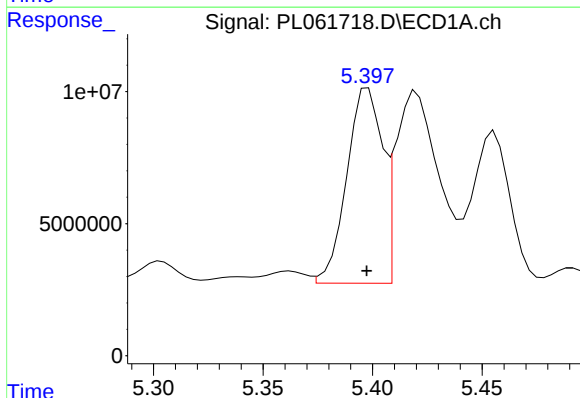


#25 Chlordane-3

R.T.: 5.398 min
Delta R.T.: 0.000 min
Response: 83177570
Conc: 529.18 ng/ml

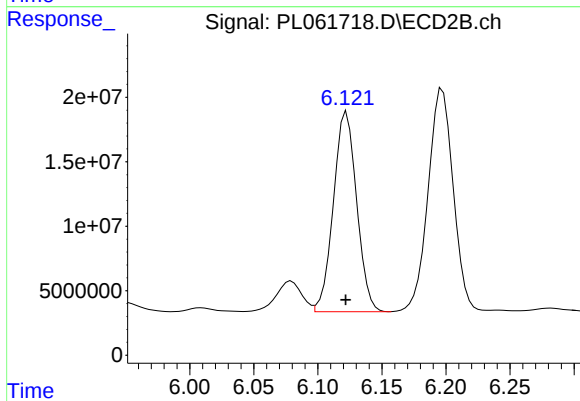

#25 Chlordane-3


R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 195839241
Conc: 534.44 ng/ml

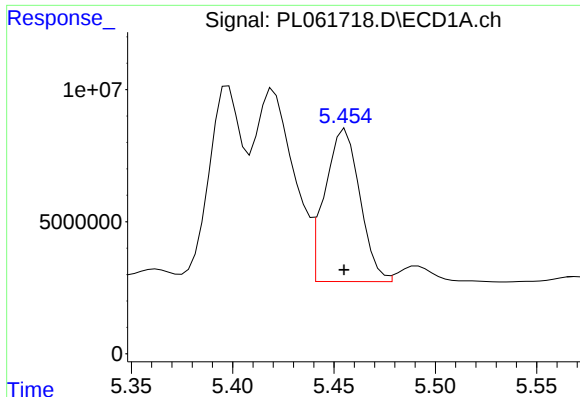

#26 Chlordane-4


R.T.: 5.456 min
Delta R.T.: 0.000 min
Response: 69486415
Conc: 532.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

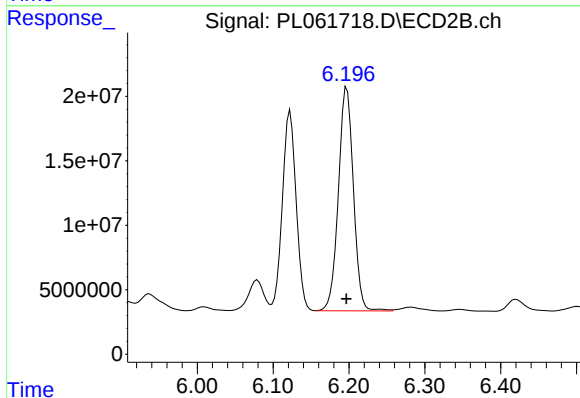


#26 Chlordane-4

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 238824185
Conc: 532.00 ng/ml

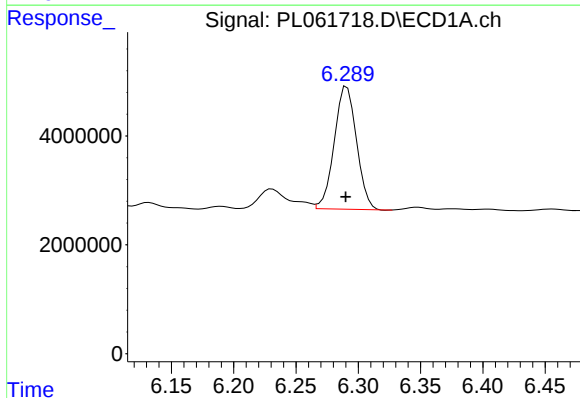


#27 Chlordane-5

R.T.: 6.291 min
Delta R.T.: 0.000 min
Response: 28006845
Conc: 513.64 ng/ml

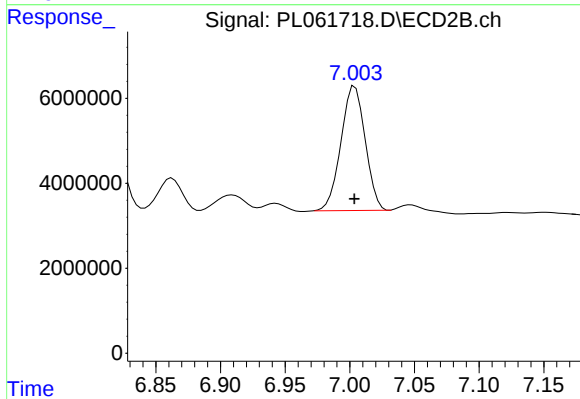

#27 Chlordane-5


R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 38141690
Conc: 524.79 ng/ml

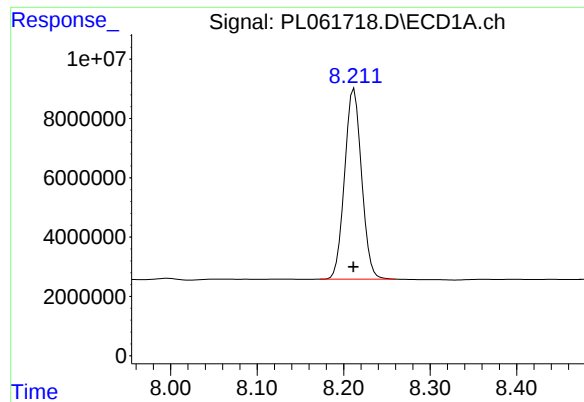

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 87115375
Conc: 53.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

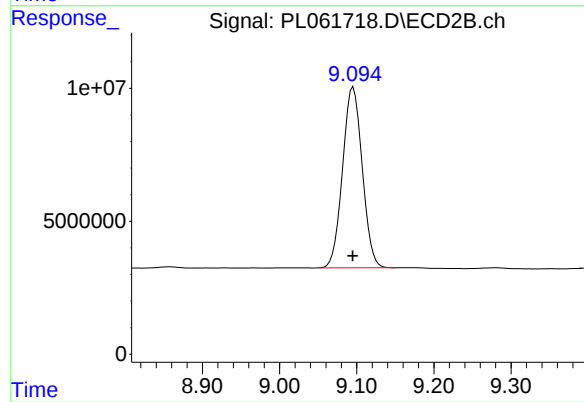

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 120111276
Conc: 54.56 ng/ml