

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2020 22:11
 Operator : DD\AJ
 Sample : L3863-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-01-092220

Manual Integrations
 APPROVED

Ankita
 9/24/2020 3:29:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:15:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	4.008	24138034	36470531	14.149	13.368
28)	SA Decachlor...	8.211	9.096	21701542	32901772	13.340	14.946
Target Compounds							
17)	MA 4,4'-DDT	6.373	7.143	1783991	2127043	1.414m	0.971m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2020 22:11
Operator : DD\AJ
Sample : L3863-05
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HD-01-092220


Manual Integrations
APPROVED

Ankita
9/24/2020 3:29:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:15:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

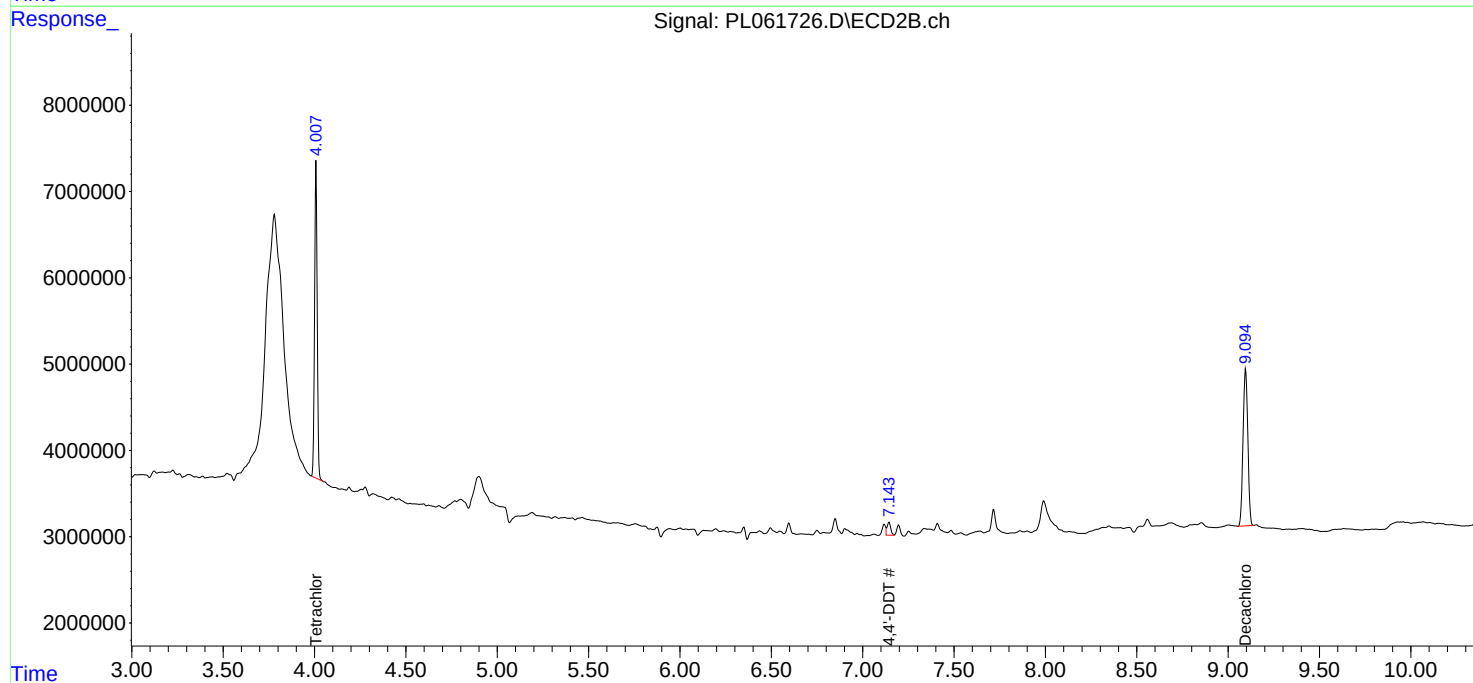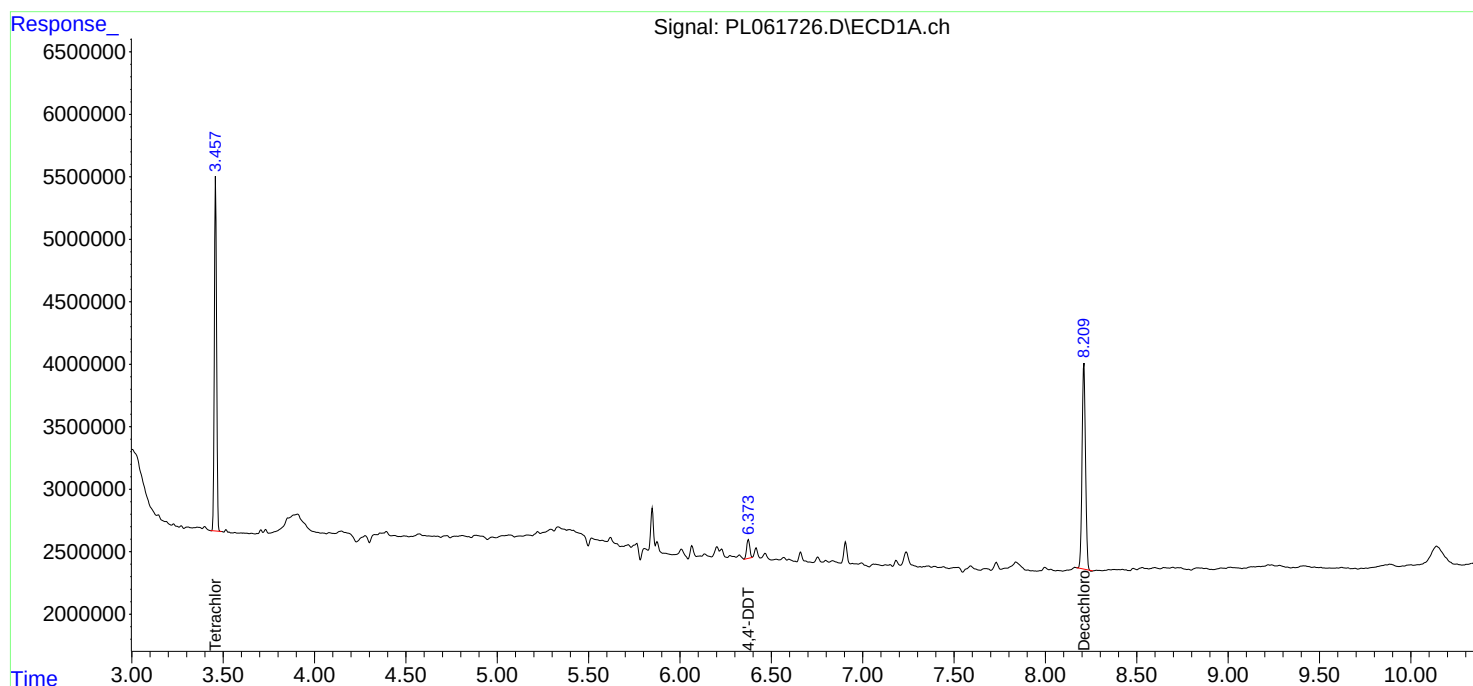

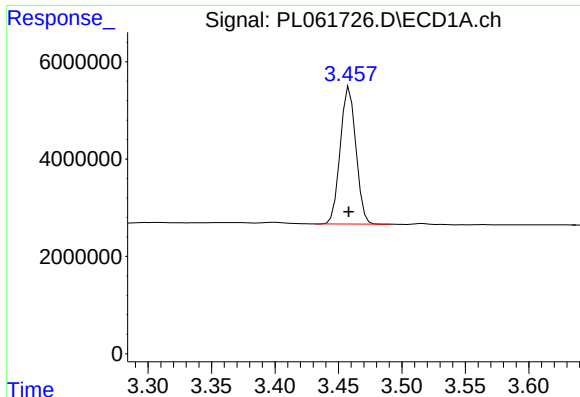


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 24138034
Conc: 14.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-092220


Manual Integrations
APPROVED

Ankita
9/24/2020 3:29:34 PM

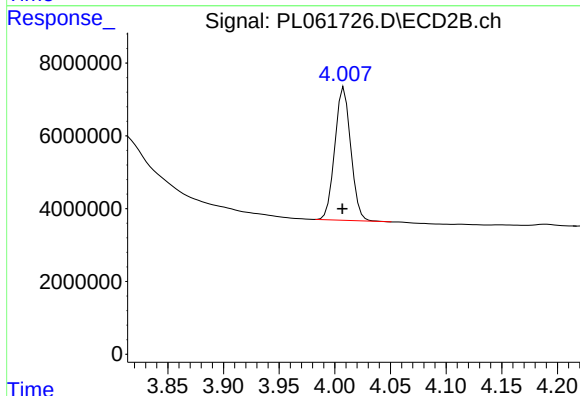


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.002 min
Response: 36470531
Conc: 13.37 ng/ml

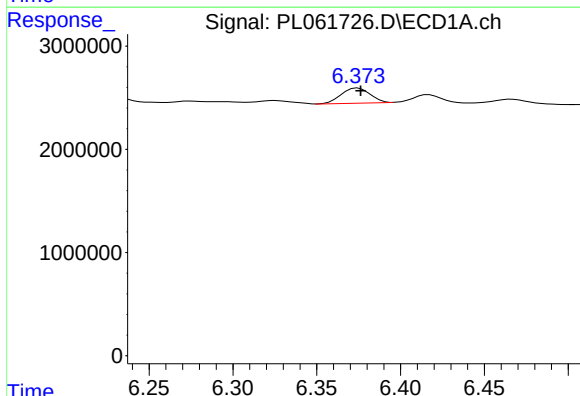


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.003 min
Response: 1783991
Conc: 1.41 ng/ml m

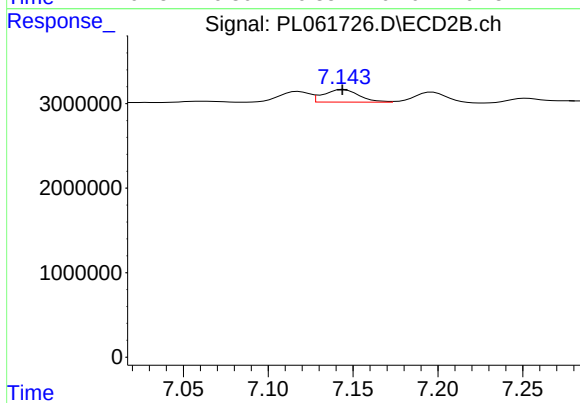

#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: 0.000 min
Response: 2127043
Conc: 0.97 ng/ml m

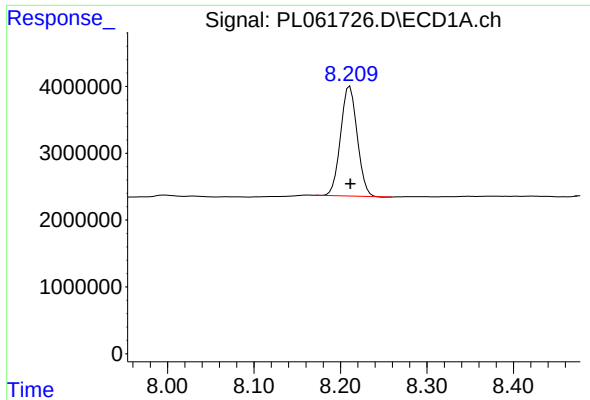


#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 21701542
Conc: 13.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-01-092220

Manual Integrations
APPROVED

Ankita
9/24/2020 3:29:34 PM

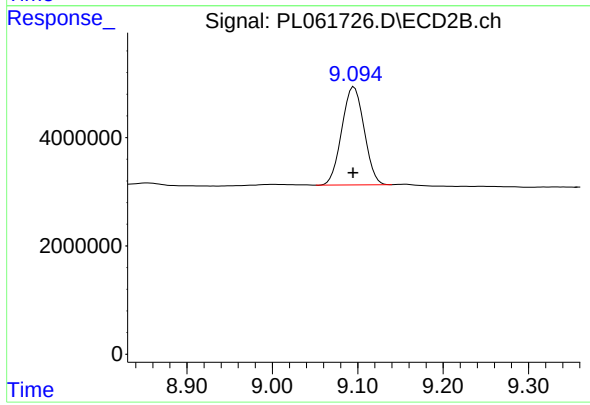

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.001 min
Response: 32901772
Conc: 14.95 ng/ml