

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
 Data File : PL061747.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 03:08
 Operator : DD\AJ
 Sample : L4094-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS-WC-L-01

Manual Integrations
 APPROVED

Ankita
 9/24/2020 3:29:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 07:21:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.459	4.008	27116774	36662463	15.895	13.438
28) SA Decachlor...	8.211	9.094	15956922	22864048	9.809	10.386m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092320\
Data File : PL061747.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 03:08
Operator : DD\AJ
Sample : L4094-01
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01


Manual Integrations
APPROVED

Ankita
9/24/2020 3:29:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 07:21:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

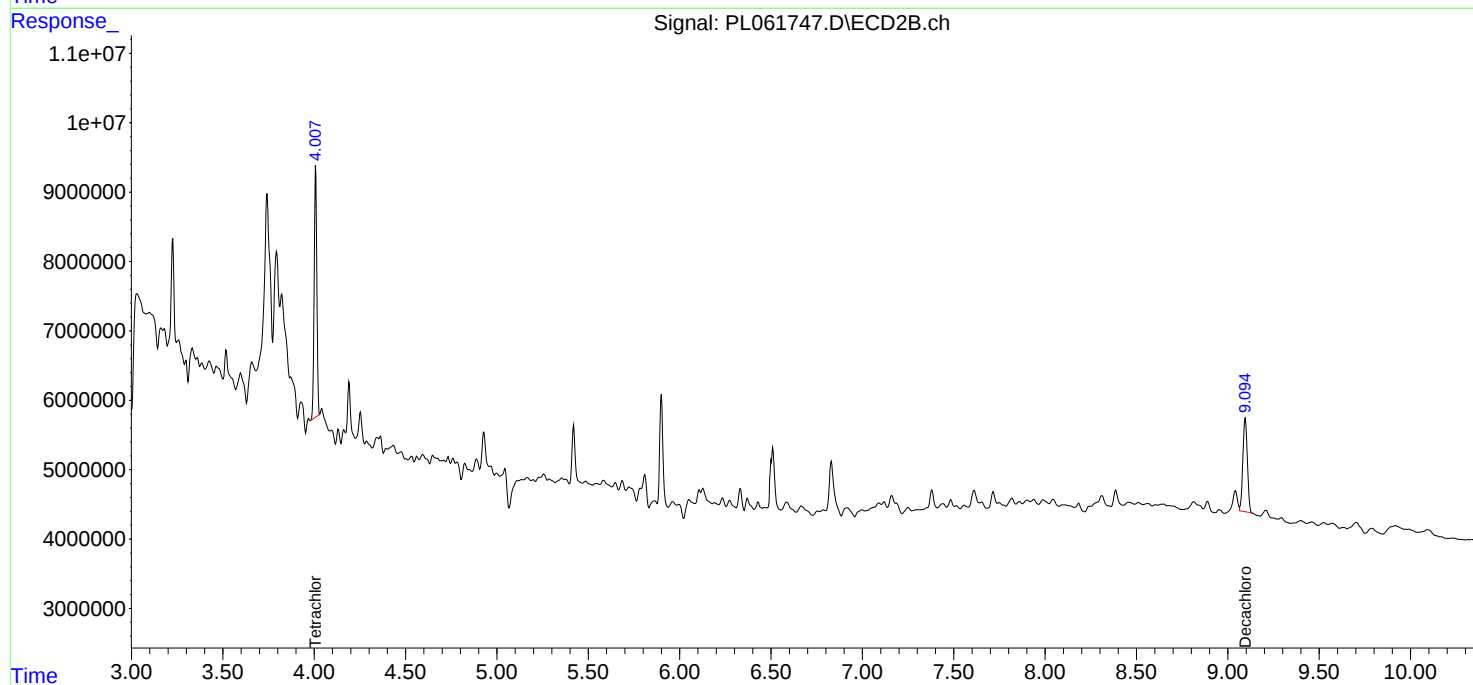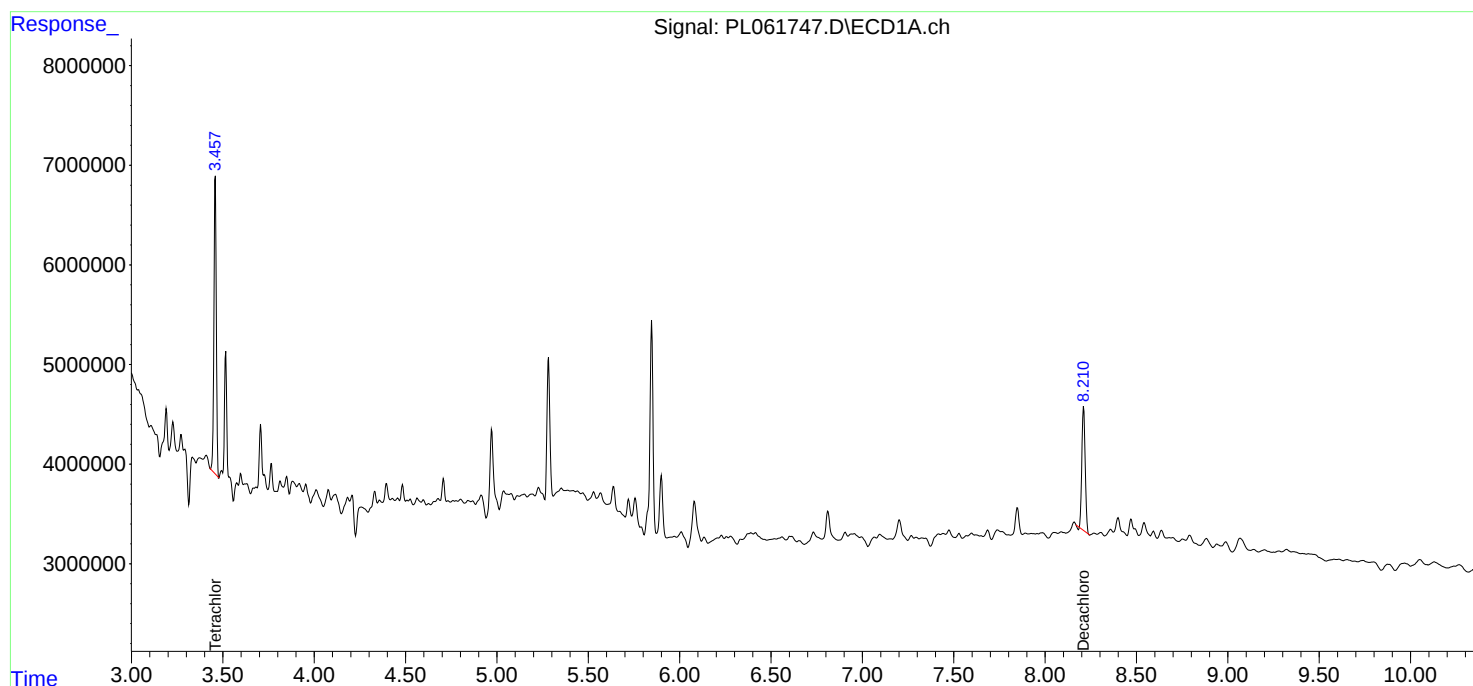

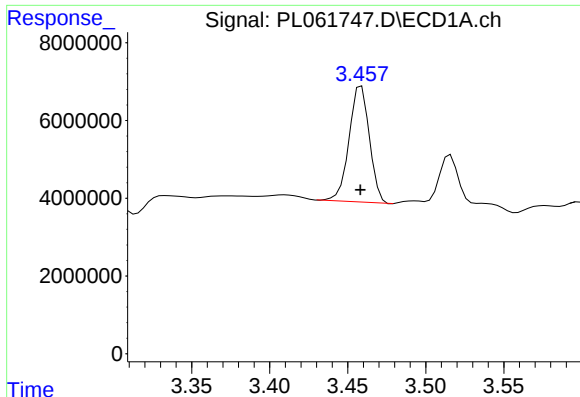


#1 Tetrachloro-m-xylene

R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 27116774
Conc: 15.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS-WC-L-01


Manual Integrations
APPROVED

Ankita
9/24/2020 3:29:50 PM

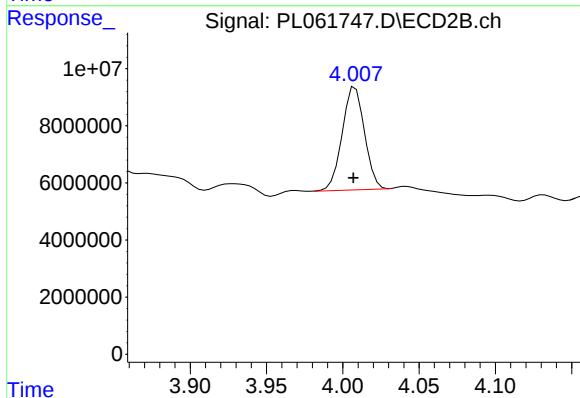


#1 Tetrachloro-m-xylene

R.T.: 4.008 min
Delta R.T.: 0.001 min
Response: 36662463
Conc: 13.44 ng/ml

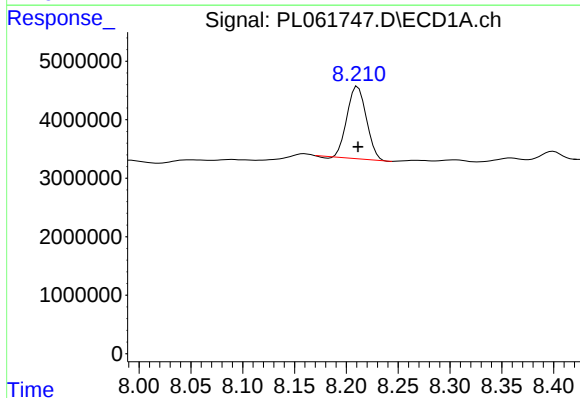

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 15956922
Conc: 9.81 ng/ml

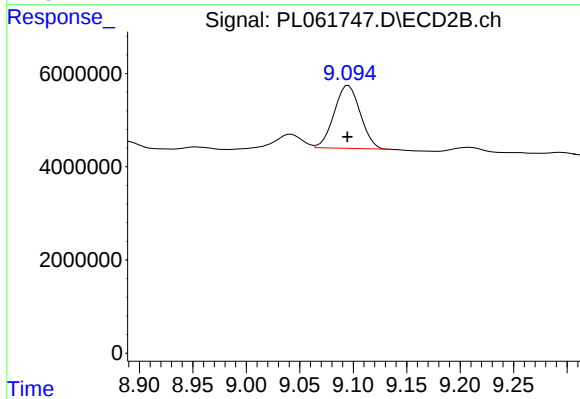

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 22864048
Conc: 10.39 ng/ml m