

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091963.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 13:06
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 13:20:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 13:20:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.782	105.7E6	151.2E6	50.000	50.000
28)	SA Decachlor...	9.061	7.924	78626748	121.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.706	3.781	49457629	49048818	500.000	500.000
24)	Chlordane-2	5.236	4.358	51426580	54655467	500.000	500.000
25)	Chlordane-3	5.946	4.989	177.7E6	164.8E6	500.000	500.000
26)	Chlordane-4	6.028	5.051	216.0E6	157.8E6	500.000	500.000
27)	Chlordane-5	6.877	5.947	42070403	54145786	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091963.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 13:06
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 13:20:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 13:20:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

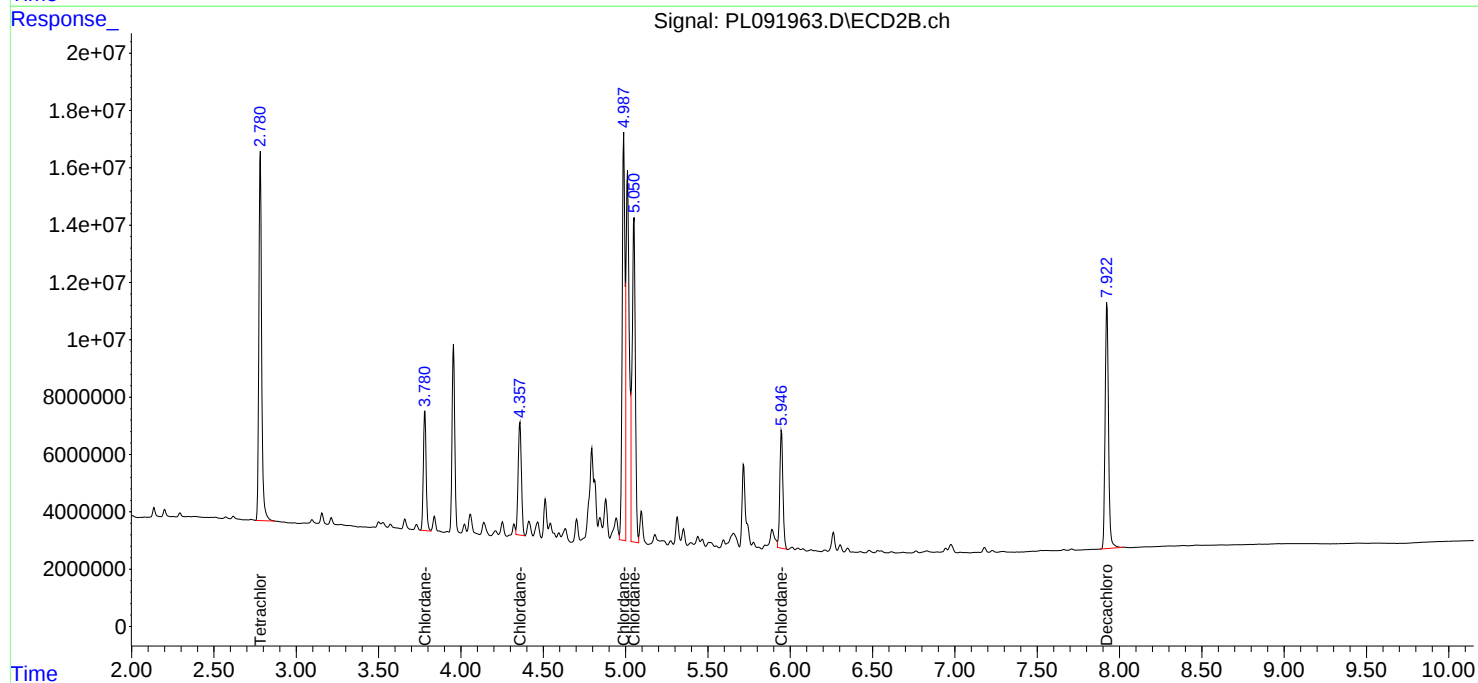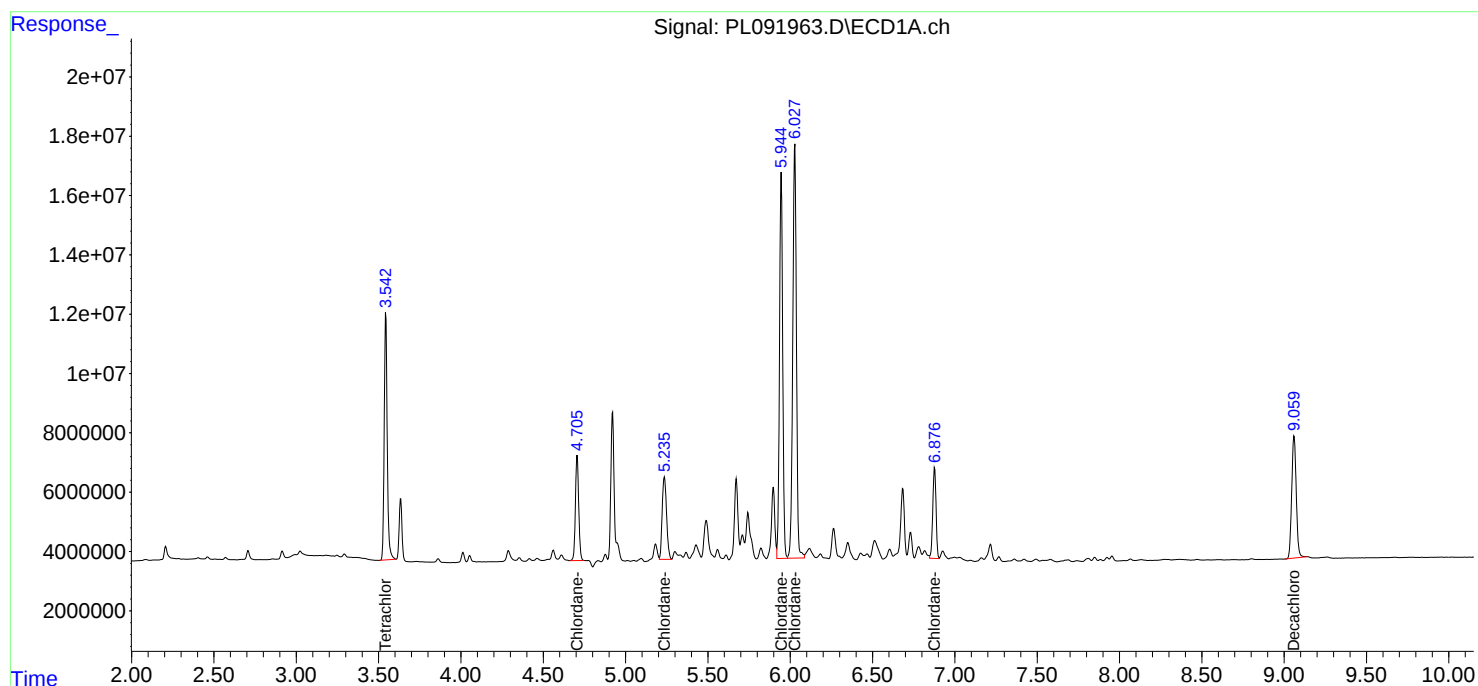


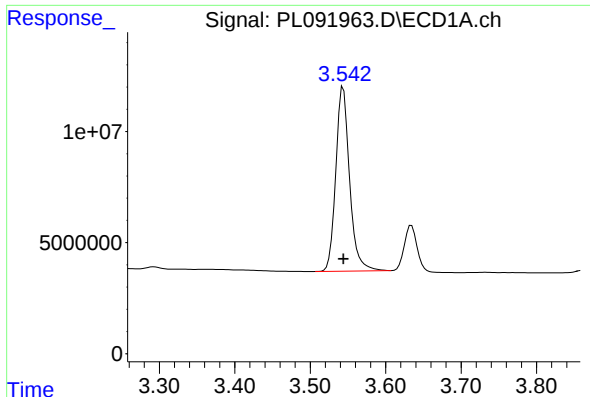

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 105675393
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

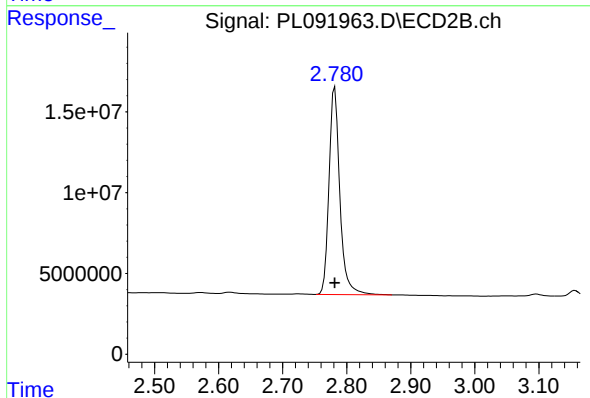


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 151157034
Conc: 50.00 ng/ml

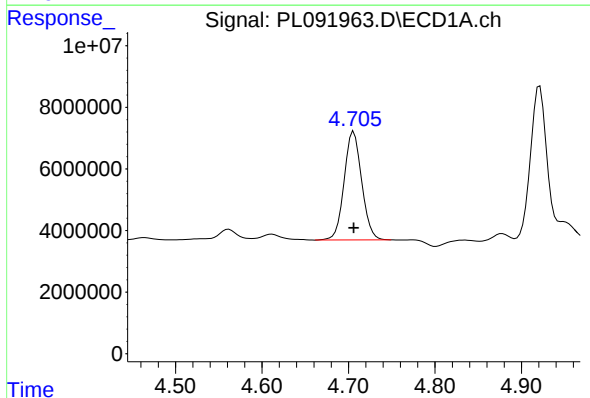


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 49457629
Conc: 500.00 ng/ml

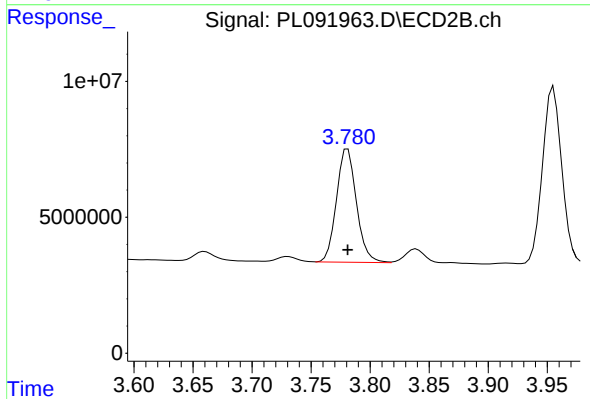

#23 Chlordane-1


R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 49048818
Conc: 500.00 ng/ml

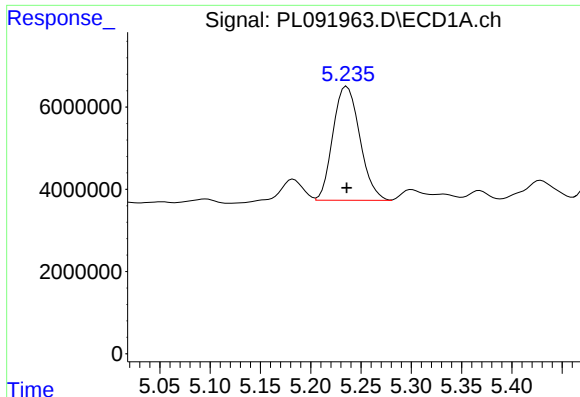

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 51426580
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

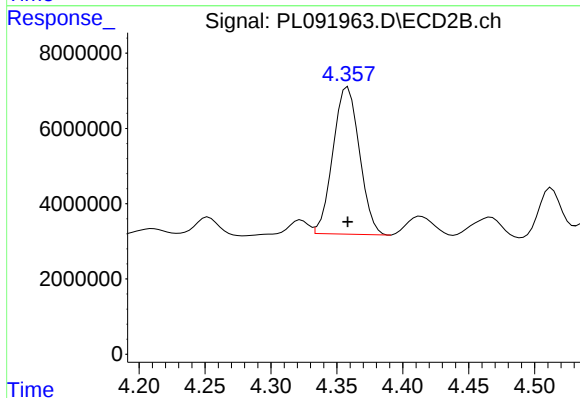


#24 Chlordane-2

R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 54655467
Conc: 500.00 ng/ml

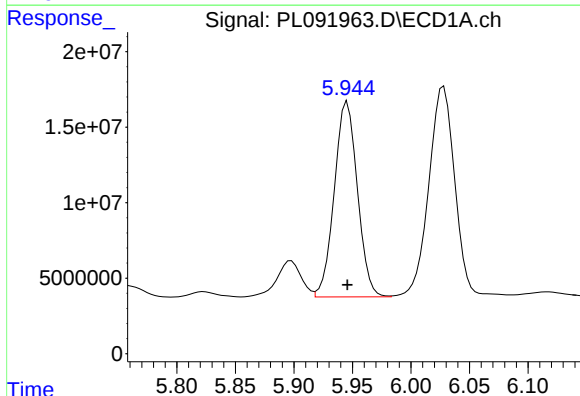


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 177668269
Conc: 500.00 ng/ml

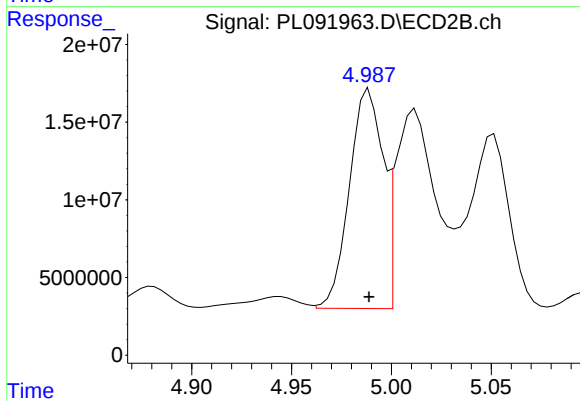

#25 Chlordane-3


R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 164767709
Conc: 500.00 ng/ml

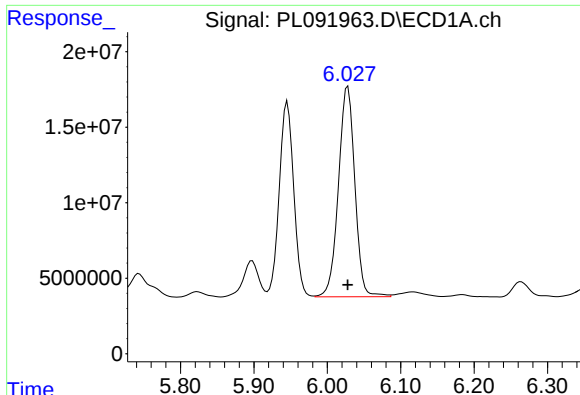

#26 Chlordane-4


R.T.: 6.028 min
Delta R.T.: 0.000 min
Response: 216031706
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

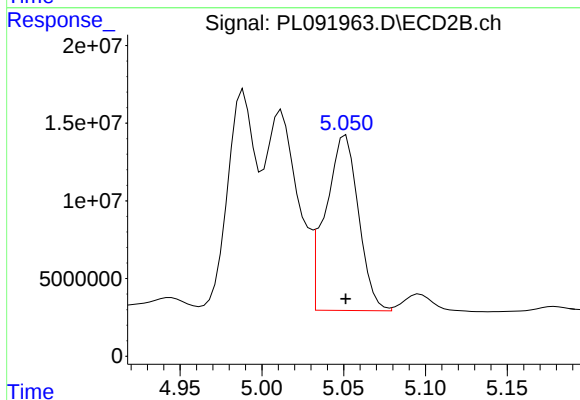


#26 Chlordane-4

R.T.: 5.051 min
Delta R.T.: 0.000 min
Response: 157779752
Conc: 500.00 ng/ml

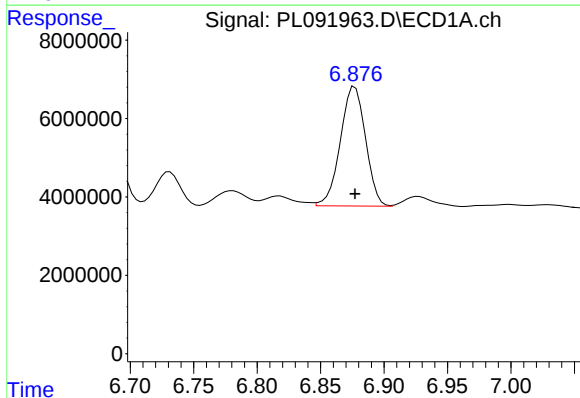


#27 Chlordane-5

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 42070403
Conc: 500.00 ng/ml

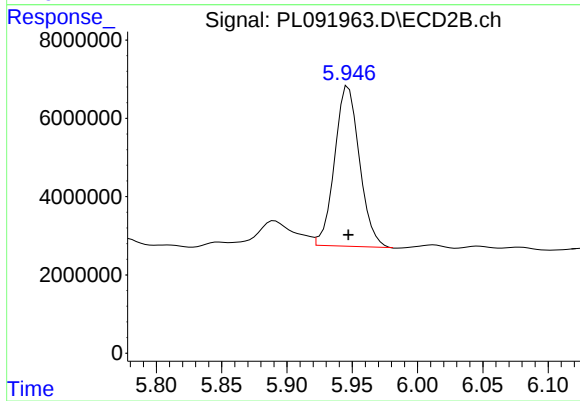

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 54145786
Conc: 500.00 ng/ml

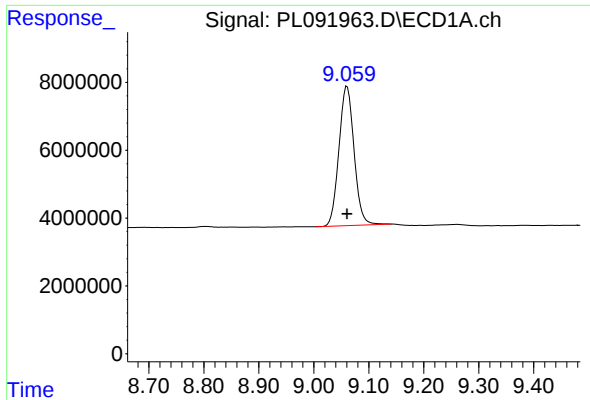

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 78626748
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

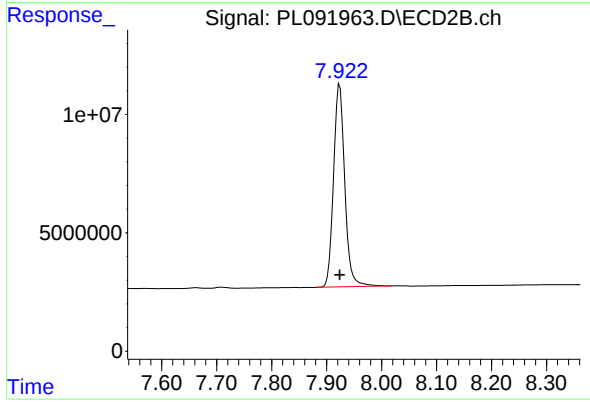

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.000 min
Response: 121336825
Conc: 50.00 ng/ml