

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 18:55
 Operator : AR\AJ
 Sample : P4103-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:11:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.783	35698468	51102339	16.047	20.375 #
28)	SA Decachlor...	9.060	7.923	33159014	50987576	20.241	20.379
Target Compounds							
2)	A alpha-BHC	0.000	3.293	0	1408404	N.D.	0.387 #
4)	MA Heptachlor	0.000	3.950	0	4000636	N.D.	1.159 #
7)	B delta-BHC	4.772	4.142	12644185	-246471	4.384	N.D. #
14)	MA Endrin	0.000	5.666f	0	273917	N.D.	0.104 #
15)	B Endosulfa...	0.000	5.938	0	49430	N.D.	0.020 #
17)	MA 4,4'-DDT	0.000	6.037	0	265257	N.D.	0.115 #
22)	Mirex	0.000	7.033	0	292370	N.D.	0.120 #
23)	Chlordane-1	0.000	3.795	0	70345	N.D.	0.704 #
27)	Chlordane-5	0.000	5.938	0	49430	N.D.	0.456 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 18:55
Operator : AR\AJ
Sample : P4103-17
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:11:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

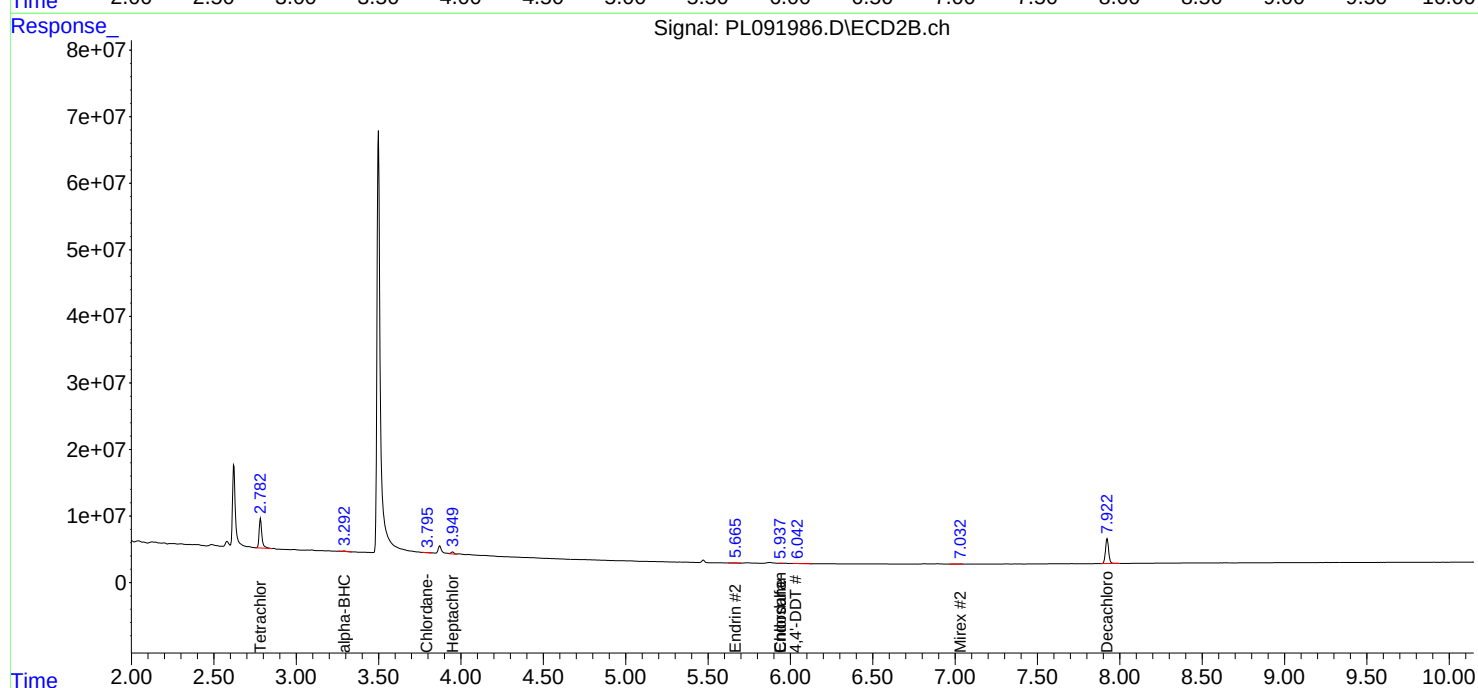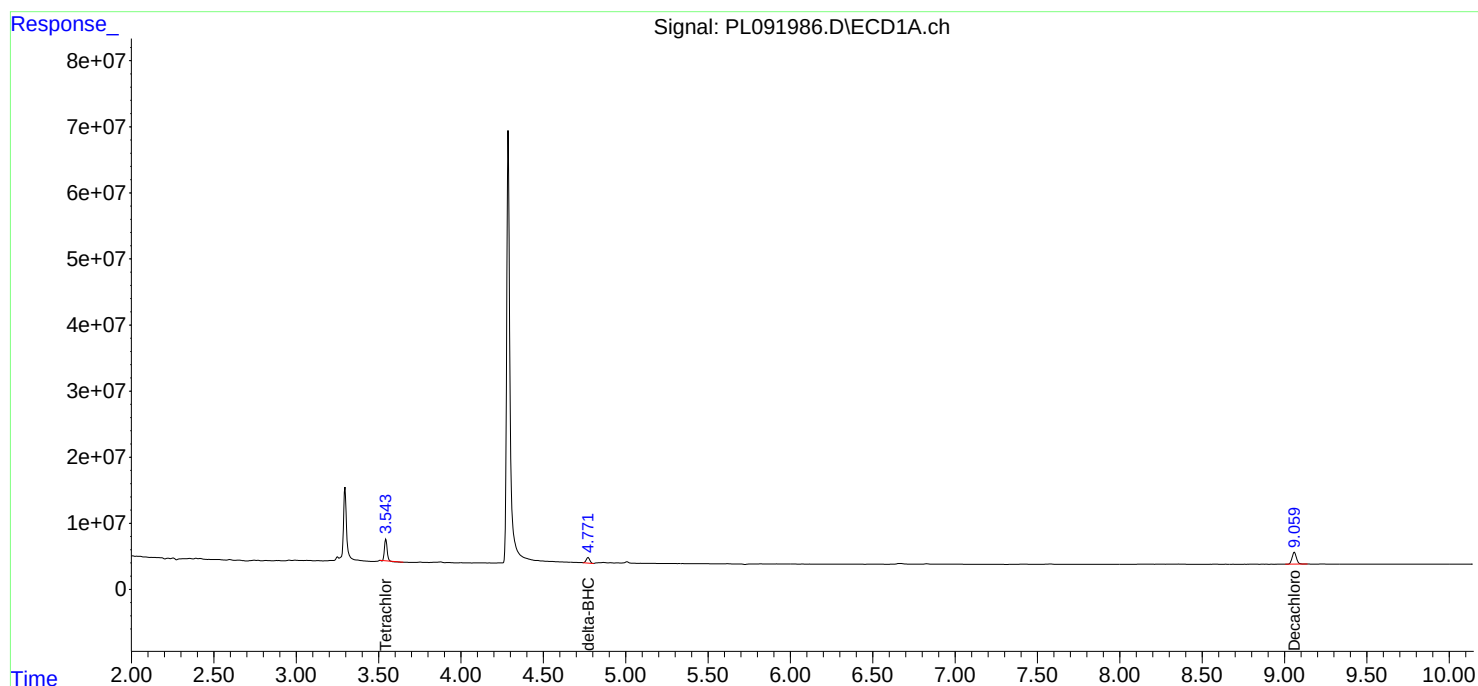


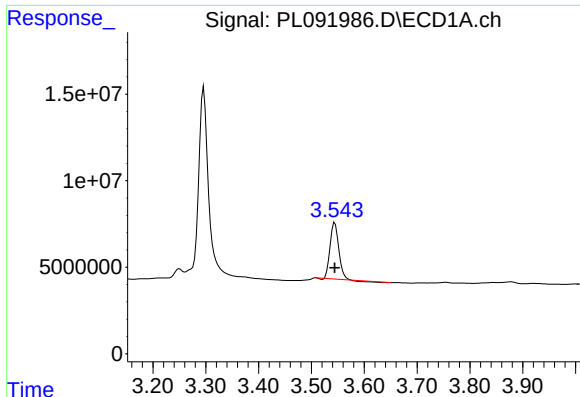

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 35698468
Conc: 16.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

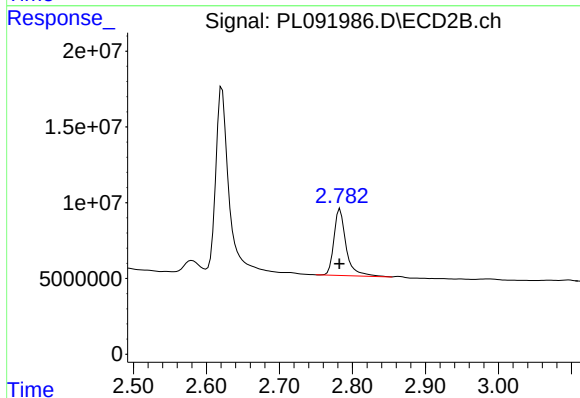


#1 Tetrachloro-m-xylene

R.T.: 2.783 min
Delta R.T.: 0.000 min
Response: 51102339
Conc: 20.38 ng/ml

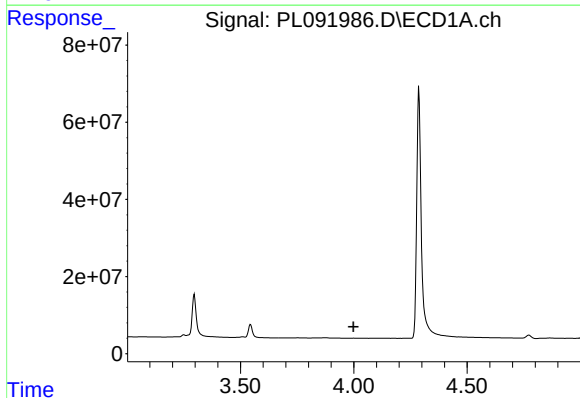


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.999 min
Response: 0
Conc: N.D.

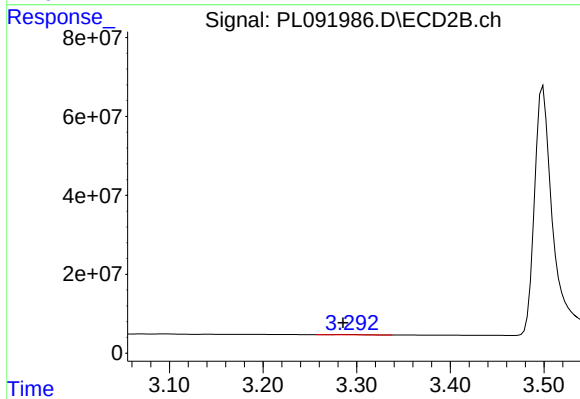

#2 alpha-BHC


R.T.: 3.293 min
Delta R.T.: 0.007 min
Response: 1408404
Conc: 0.39 ng/ml

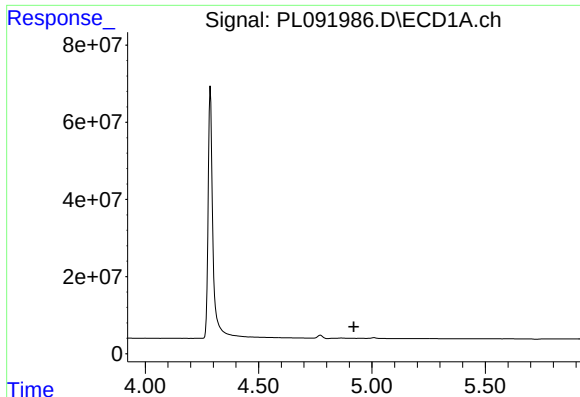

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.920 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

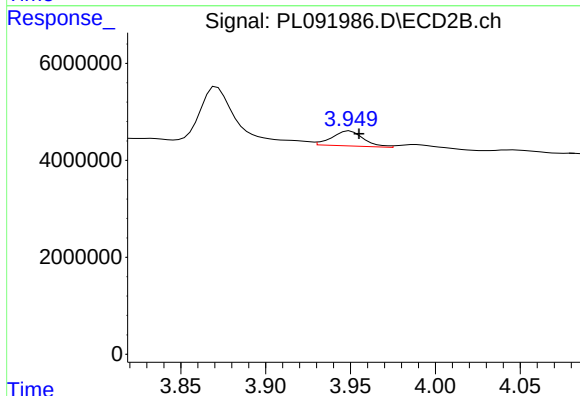


#4 Heptachlor

R.T.: 3.950 min
Delta R.T.: -0.005 min
Response: 4000636
Conc: 1.16 ng/ml

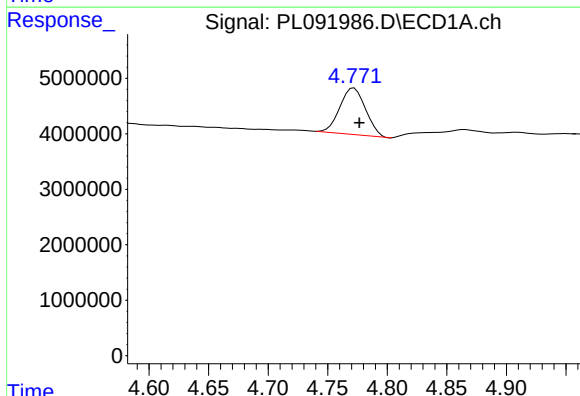


#7 delta-BHC

R.T.: 4.772 min
Delta R.T.: -0.004 min
Response: 12644185
Conc: 4.38 ng/ml

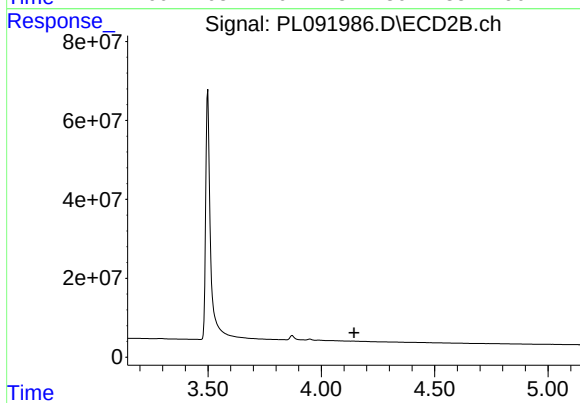

#7 delta-BHC


R.T.: 4.142 min
Delta R.T.: -0.003 min
Response: -246471
Conc: N.D.

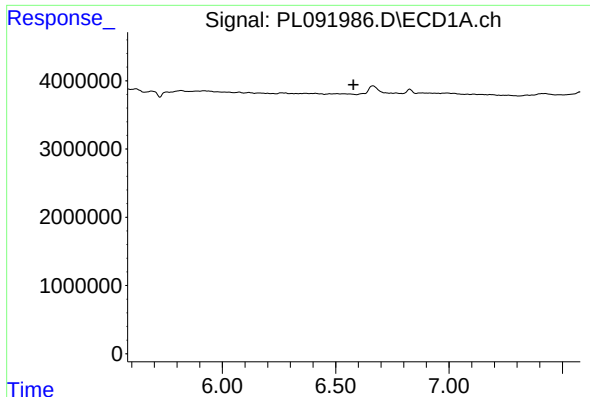

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.579 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

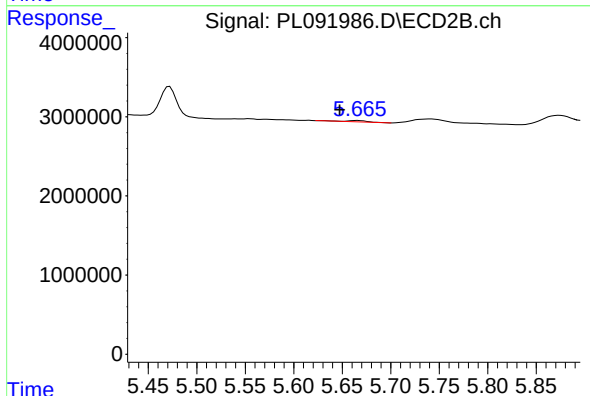


#14 Endrin

R.T.: 5.666 min
Delta R.T.: 0.018 min
Response: 273917
Conc: 0.10 ng/ml

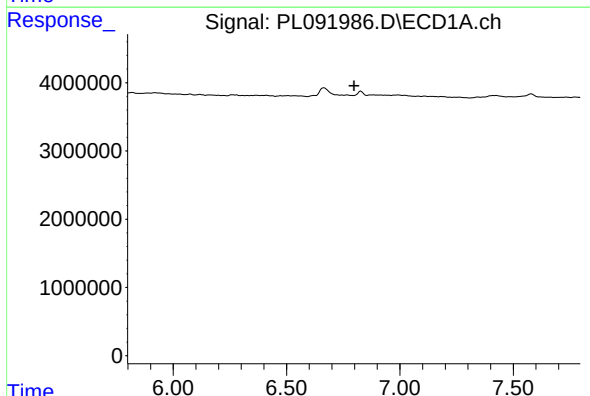


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.798 min
Response: 0
Conc: N.D.

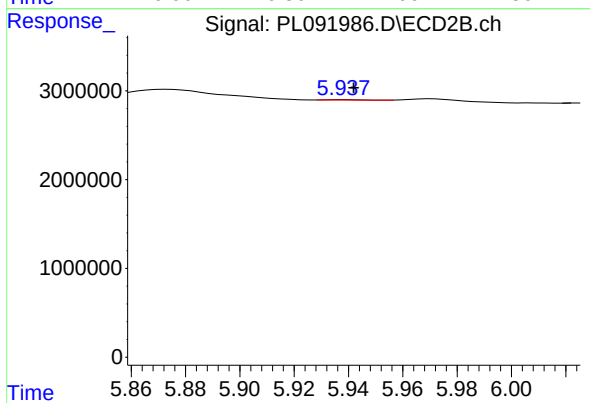

#15 Endosulfan II


R.T.: 5.938 min
Delta R.T.: -0.004 min
Response: 49430
Conc: 0.02 ng/ml

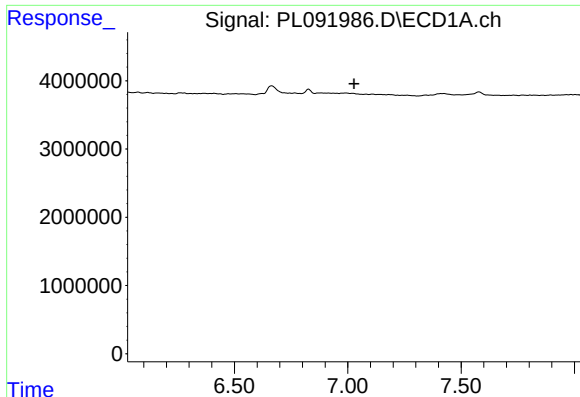

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.028 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

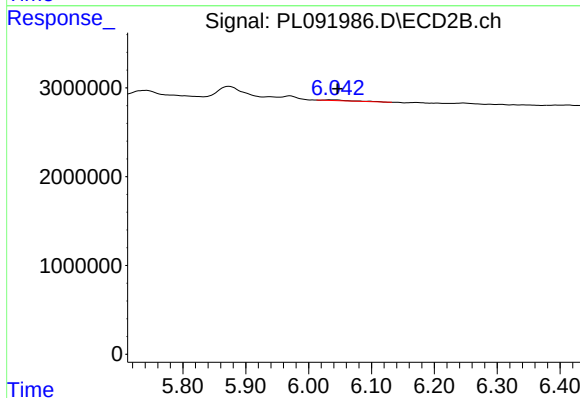


#17 4,4'-DDT

R.T.: 6.037 min
Delta R.T.: -0.009 min
Response: 265257
Conc: 0.11 ng/ml

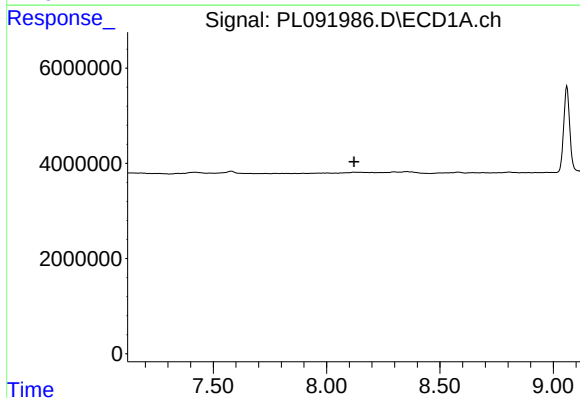


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

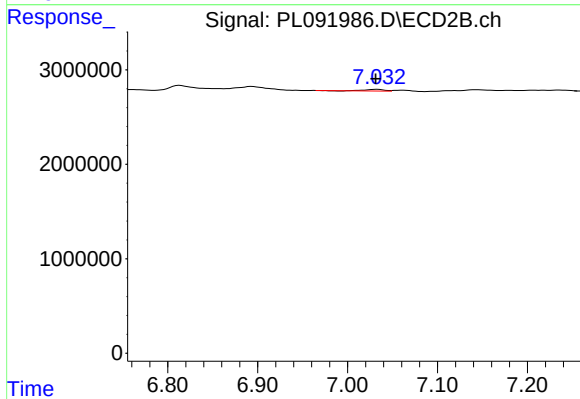

#22 Mirex


R.T.: 7.033 min
Delta R.T.: 0.002 min
Response: 292370
Conc: 0.12 ng/ml

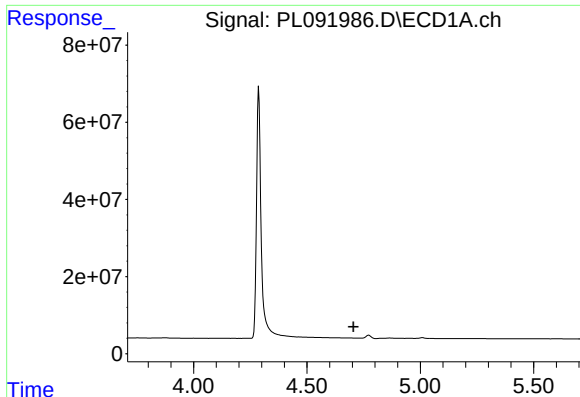

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

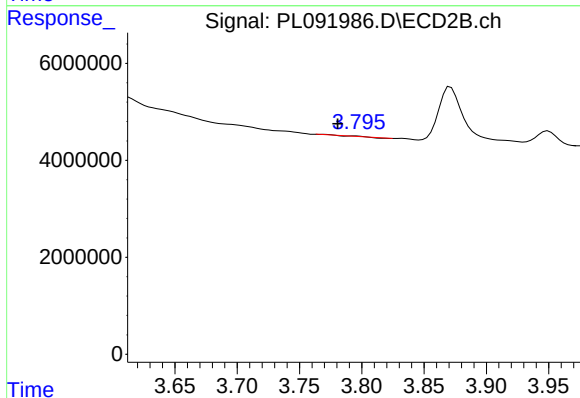


#23 Chlordane-1

R.T.: 3.795 min
Delta R.T.: 0.014 min
Response: 70345
Conc: 0.70 ng/ml

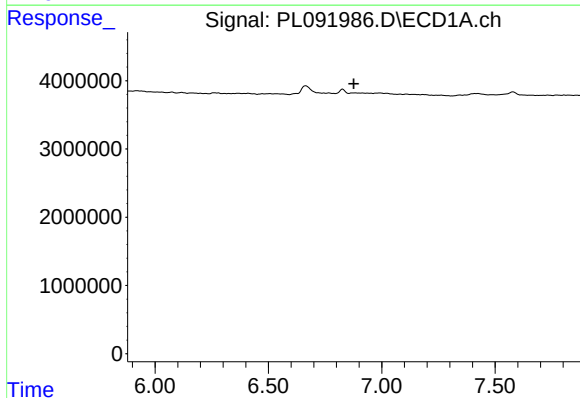


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.876 min
Response: 0
Conc: N.D.

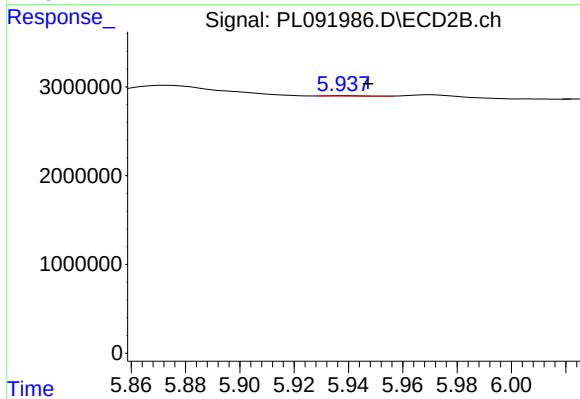

#27 Chlordane-5


R.T.: 5.938 min
Delta R.T.: -0.009 min
Response: 49430
Conc: 0.46 ng/ml

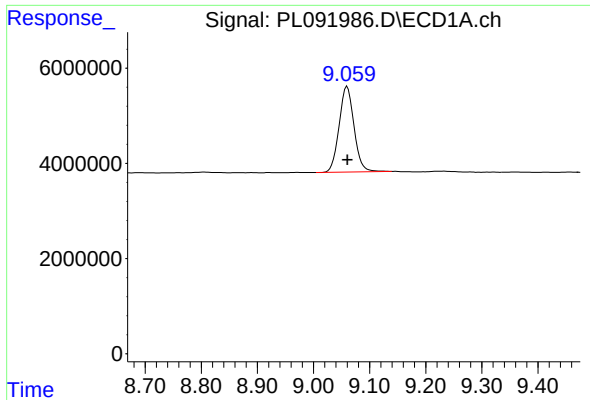

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 33159014
Conc: 20.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

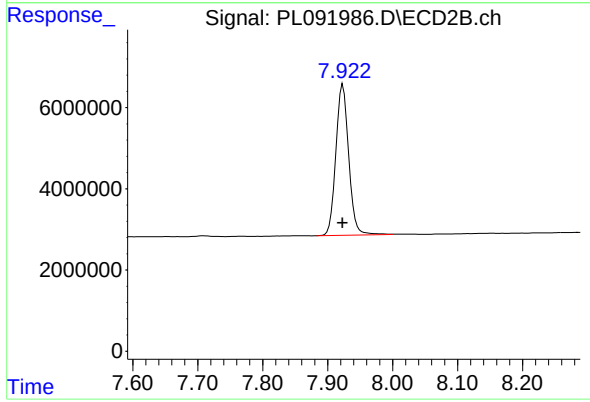

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 50987576
Conc: 20.38 ng/ml