

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 11:19
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 14:09:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 14:03:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.782	45060464	48406382	20.255	19.300
28) SA Decachlor...	9.060	7.923	33098954	49691998	20.204	19.861
Target Compounds						
9) A Endosulfan I	6.074	5.108	24134272	25750637	10.432	9.382
10) B gamma-Chl...	5.944	4.988	26576974	30002831	10.755	9.972
12) B 4,4'-DDE	6.196	5.241	43461118	52985590	20.080	19.067
13) MA Dieldrin	6.349	5.372	48004708	54324325	19.683	18.529
19) B Endosulfa...	7.162	6.344	37460879	49592805	18.898	20.556
20) A Methoxychlor	7.503	6.621	89545919	118.8E6	91.214	95.016
21) B Endrin ke...	7.647	6.850	43132114	52293680	19.627	18.886



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 11:19
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 14:09:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 14:03:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

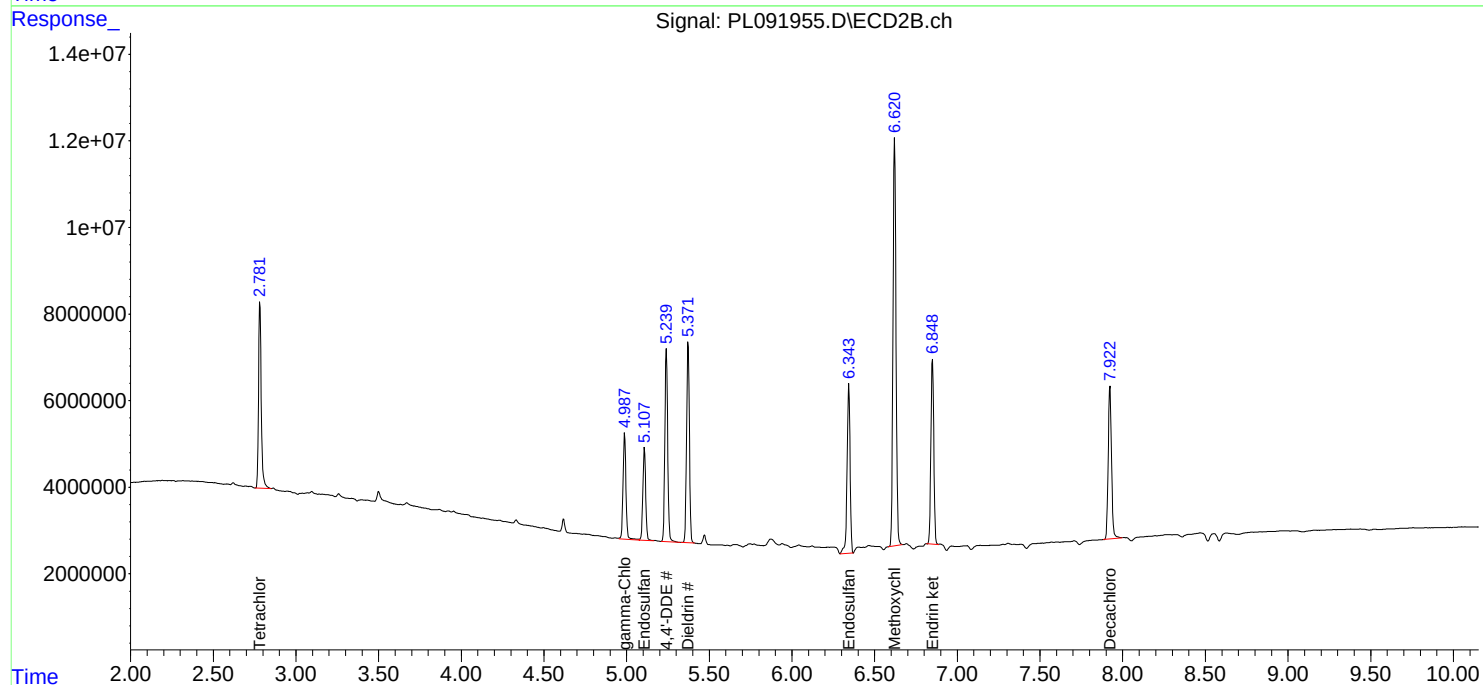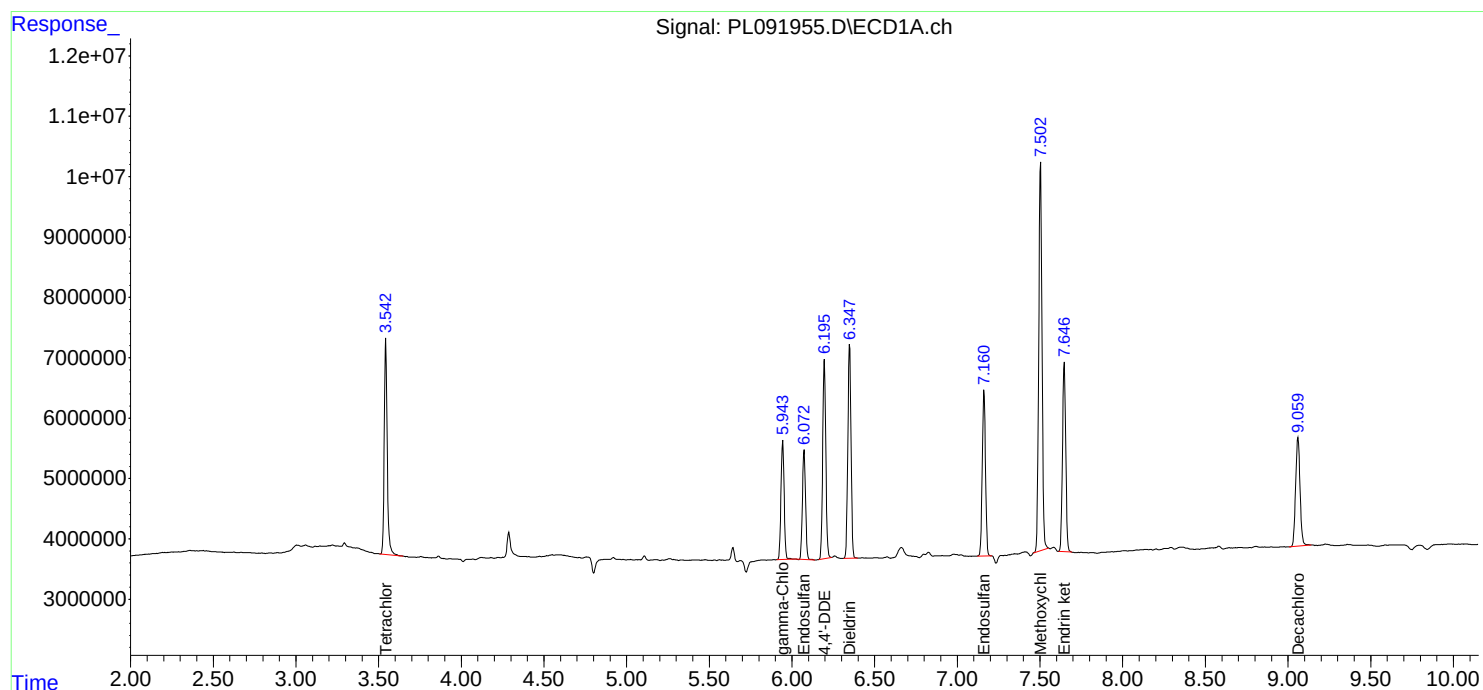


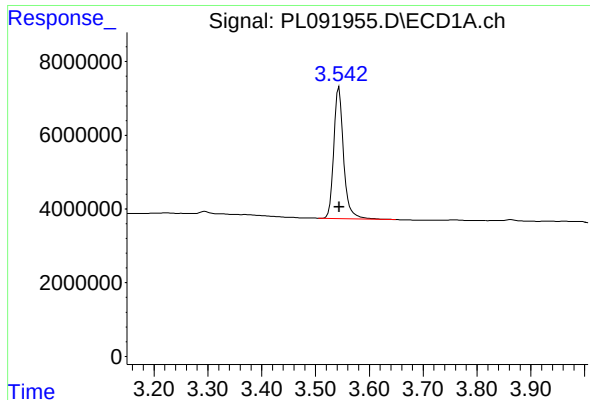

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 45060464
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

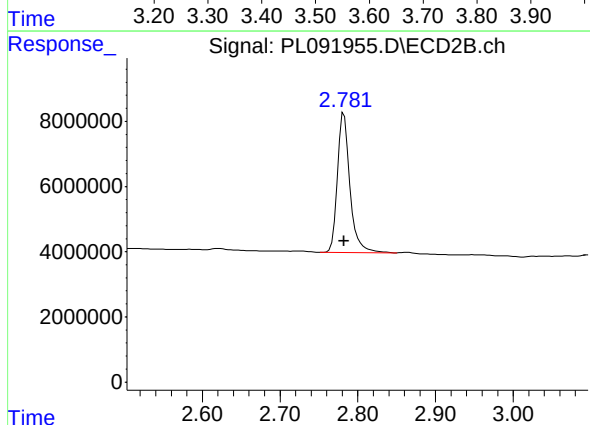


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 48406382
Conc: 19.30 ng/ml

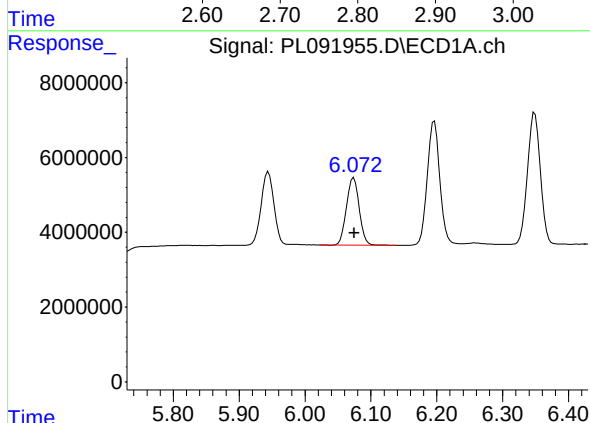


#9 Endosulfan I

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 24134272
Conc: 10.43 ng/ml

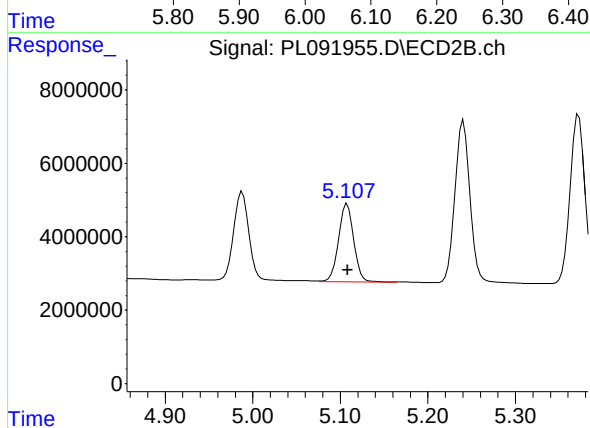

#9 Endosulfan I


R.T.: 5.108 min
Delta R.T.: 0.000 min
Response: 25750637
Conc: 9.38 ng/ml

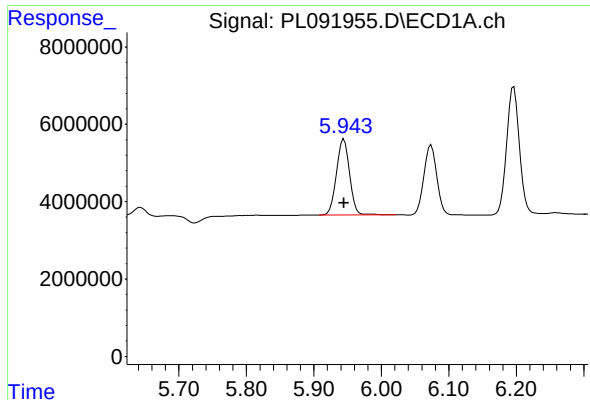

#10 gamma-Chlordane


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 26576974
Conc: 10.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

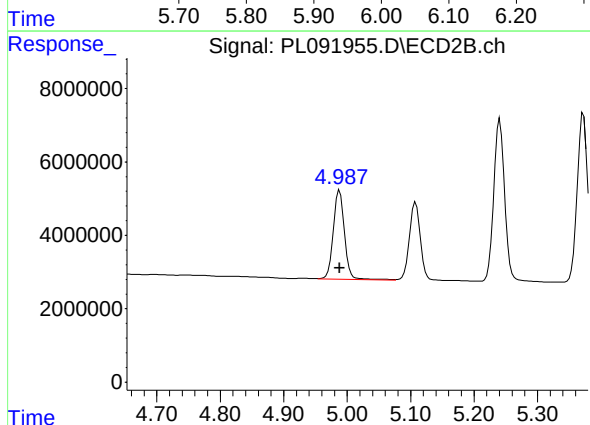


#10 gamma-Chlordane

R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 30002831
Conc: 9.97 ng/ml

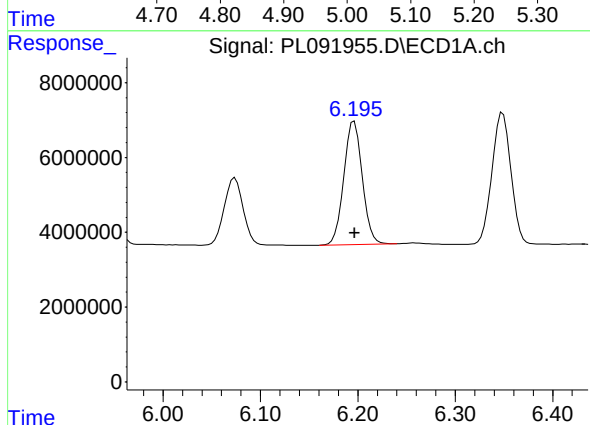


#12 4,4'-DDE

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 43461118
Conc: 20.08 ng/ml

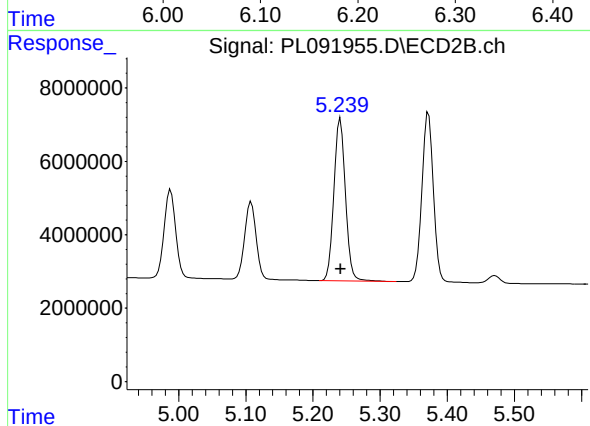

#12 4,4'-DDE


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 52985590
Conc: 19.07 ng/ml

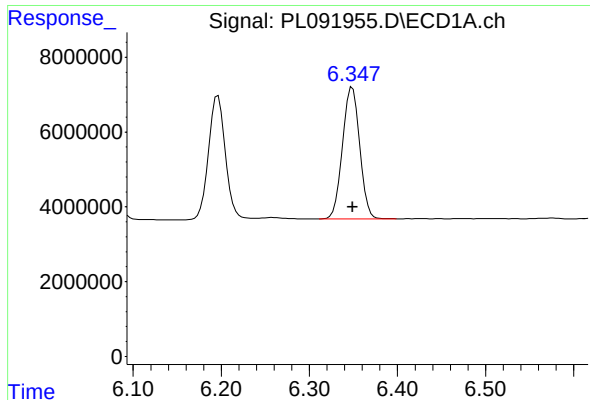

#13 Dieldrin


R.T.: 6.349 min
Delta R.T.: 0.000 min
Response: 48004708
Conc: 19.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

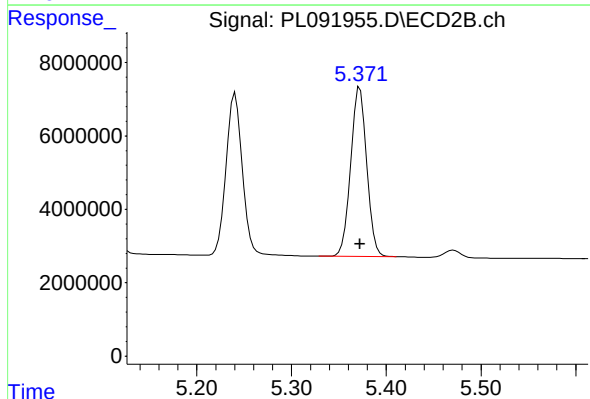


#13 Dieldrin

R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 54324325
Conc: 18.53 ng/ml

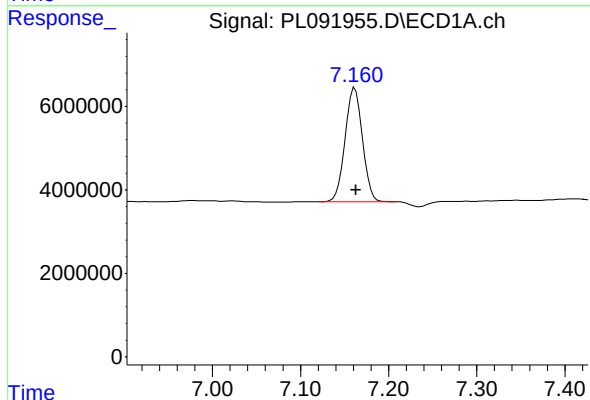


#19 Endosulfan Sulfate

R.T.: 7.162 min
Delta R.T.: -0.001 min
Response: 37460879
Conc: 18.90 ng/ml

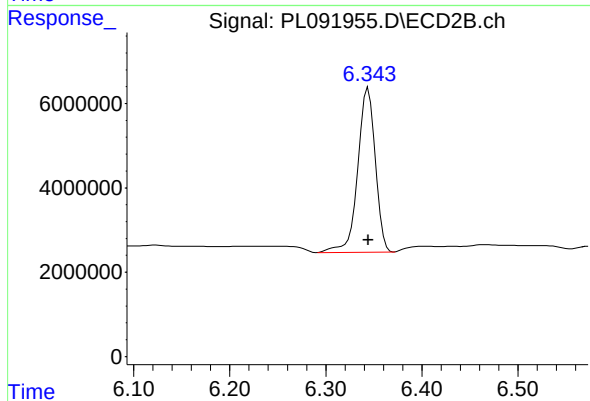

#19 Endosulfan Sulfate


R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 49592805
Conc: 20.56 ng/ml

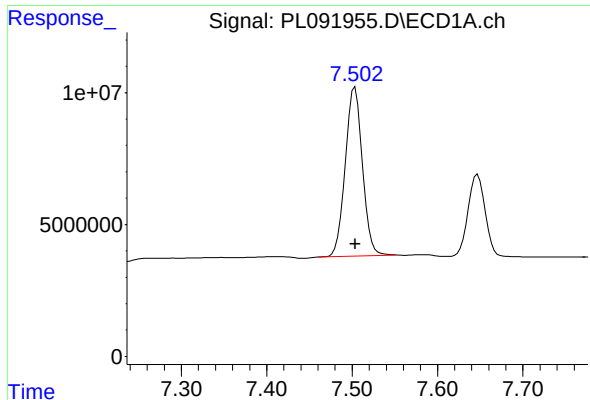

#20 Methoxychlor


R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 89545919
Conc: 91.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

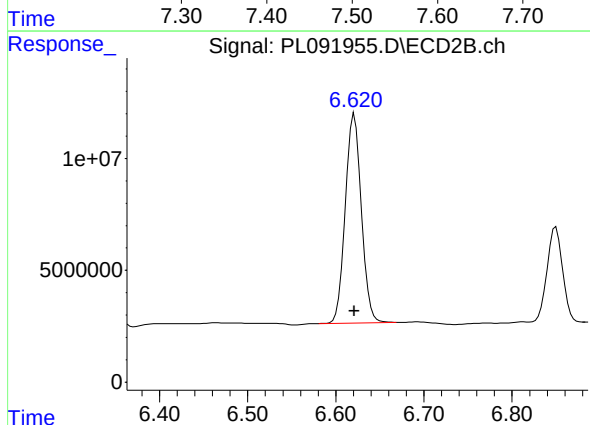


#20 Methoxychlor

R.T.: 6.621 min
Delta R.T.: 0.000 min
Response: 118802961
Conc: 95.02 ng/ml

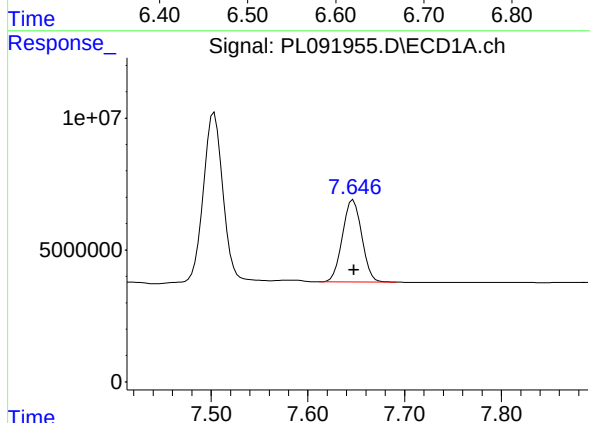


#21 Endrin ketone

R.T.: 7.647 min
Delta R.T.: 0.000 min
Response: 43132114
Conc: 19.63 ng/ml

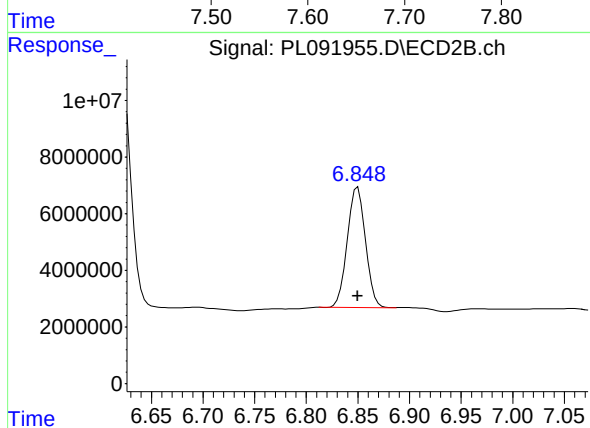

#21 Endrin ketone


R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 52293680
Conc: 18.89 ng/ml

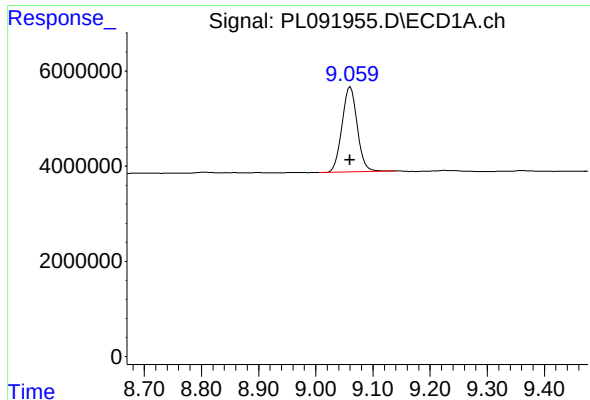

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 33098954
Conc: 20.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

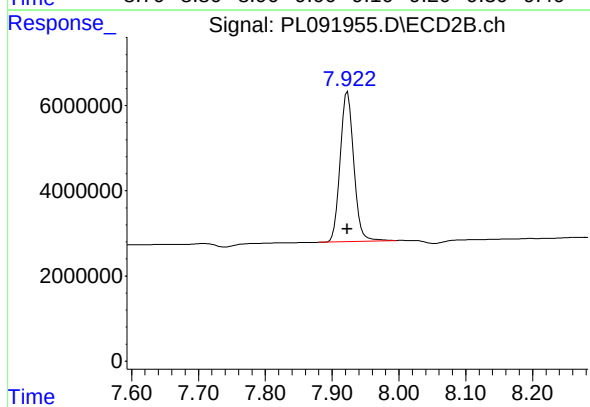

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 49691998
Conc: 19.86 ng/ml