

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 12:52
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 13:24:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 13:20:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	2.781	154.0E6	226.5E6	74.044	74.357
28) SA Decachlor...	9.060	7.923	112.0E6	175.4E6	73.260	73.126
Target Compounds						
23) Chlordane-1	4.706	3.781	72049361	73625516	741.962	744.739
24) Chlordane-2	5.235	4.358	73316499	78800619	737.480	735.627
25) Chlordane-3	5.945	4.988	260.9E6	246.8E6	737.373	740.927
26) Chlordane-4	6.027	5.051	315.0E6	235.5E6	735.890	737.999
27) Chlordane-5	6.876	5.947	60646959	81542348	734.818	740.556



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 12:52
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 13:24:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 13:20:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

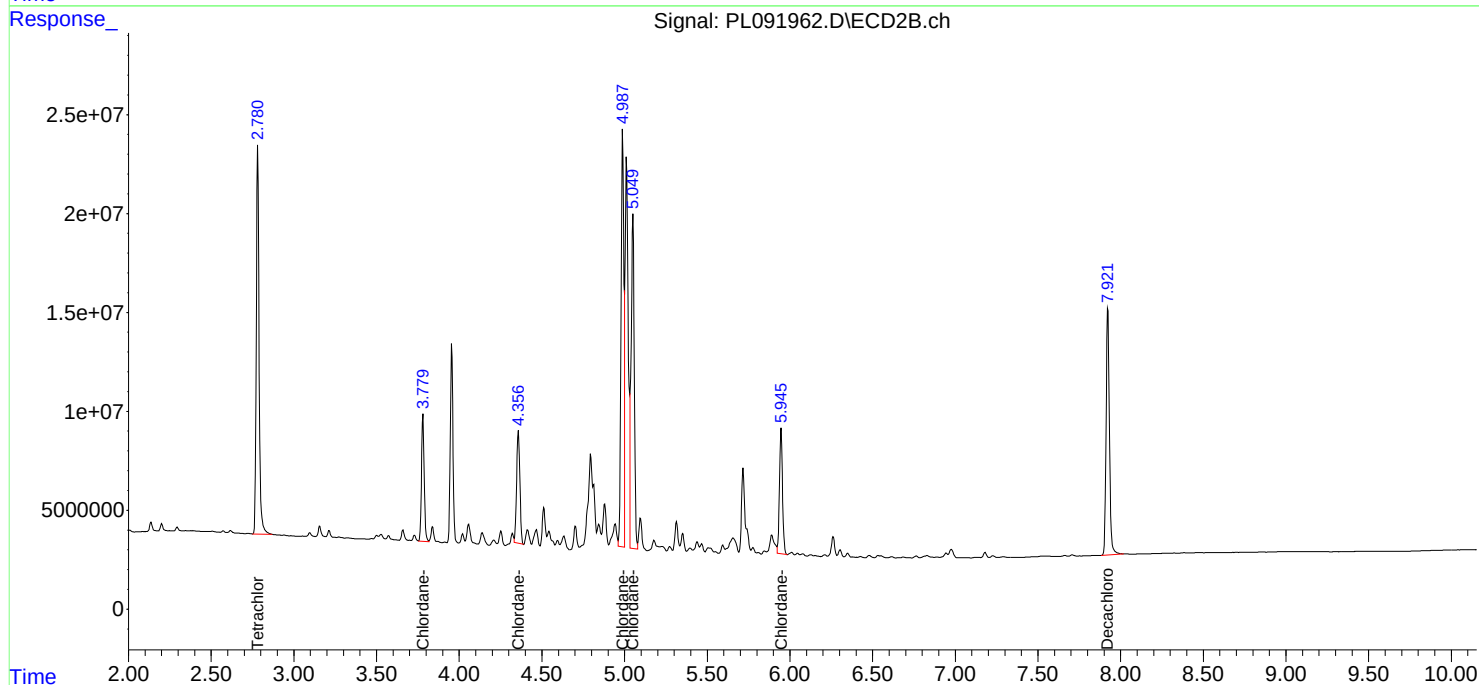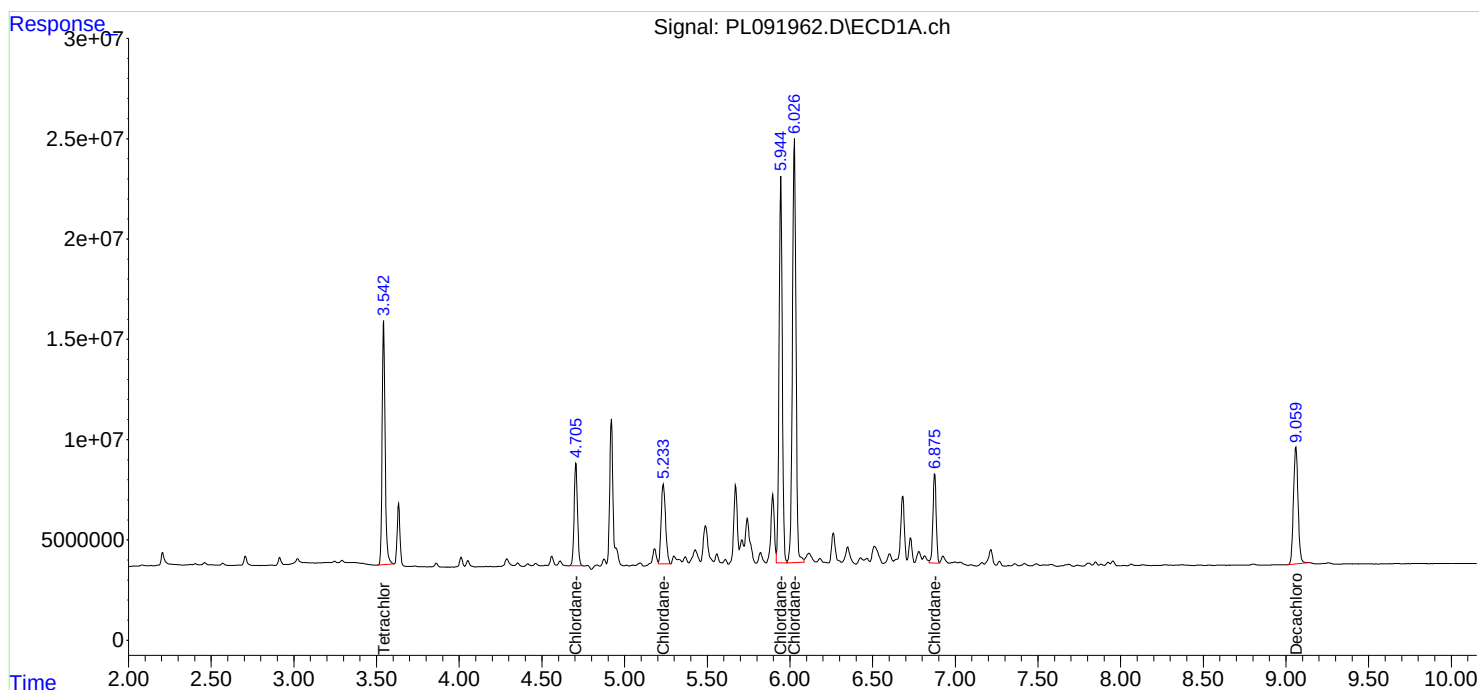


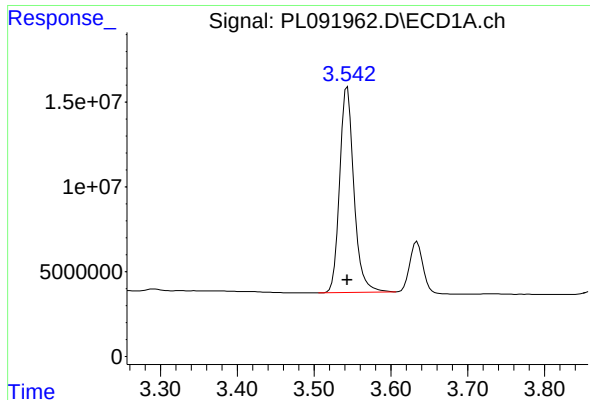

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 154014047
Conc: 74.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

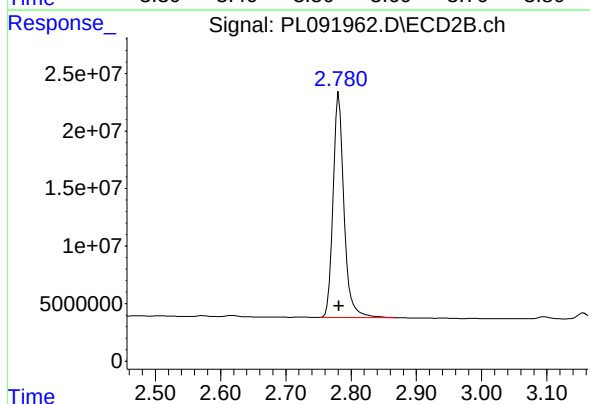


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: 0.000 min
Response: 226493399
Conc: 74.36 ng/ml

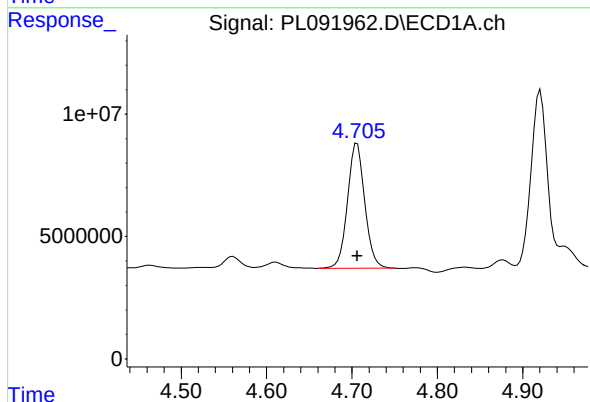


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 72049361
Conc: 741.96 ng/ml

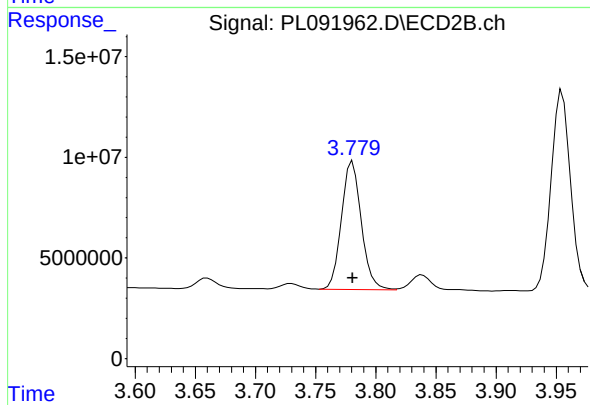

#23 Chlordane-1


R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 73625516
Conc: 744.74 ng/ml

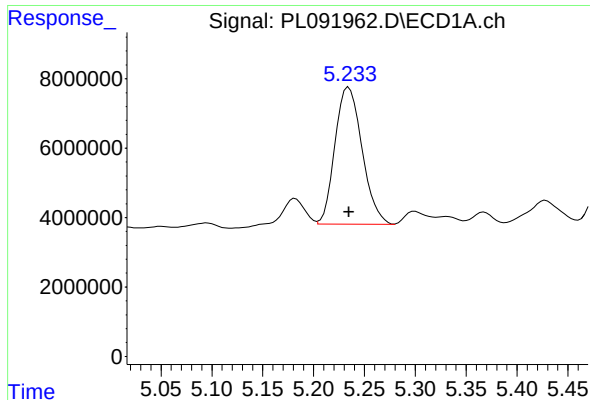

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 73316499
Conc: 737.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

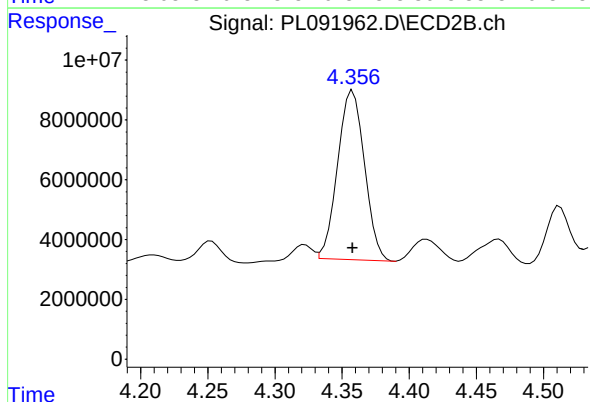


#24 Chlordane-2

R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 78800619
Conc: 735.63 ng/ml

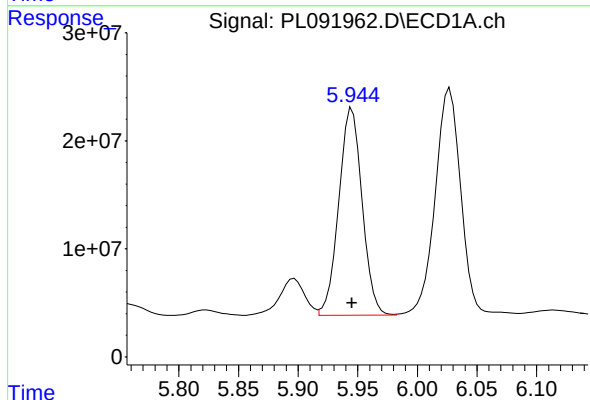


#25 Chlordane-3

R.T.: 5.945 min
Delta R.T.: 0.000 min
Response: 260887975
Conc: 737.37 ng/ml

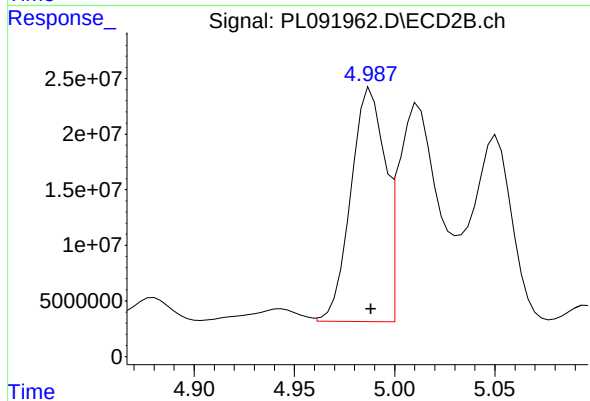

#25 Chlordane-3


R.T.: 4.988 min
Delta R.T.: 0.000 min
Response: 246754754
Conc: 740.93 ng/ml

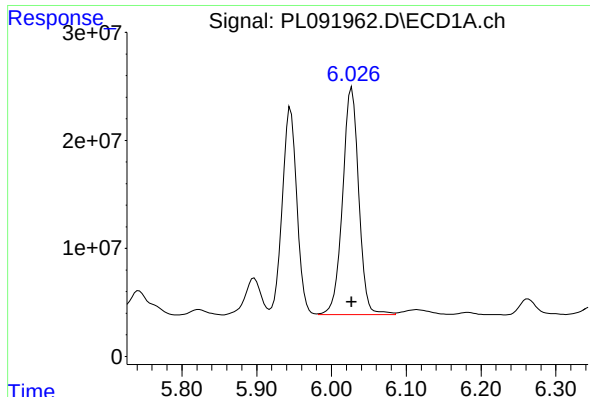

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 315028906
Conc: 735.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

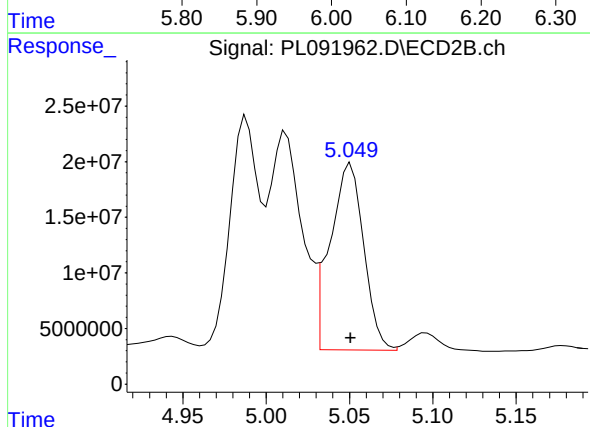


#26 Chlordane-4

R.T.: 5.051 min
Delta R.T.: 0.000 min
Response: 235522405
Conc: 738.00 ng/ml

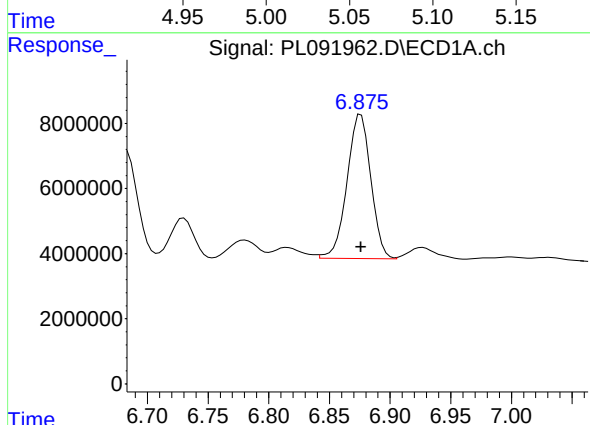


#27 Chlordane-5

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 60646959
Conc: 734.82 ng/ml

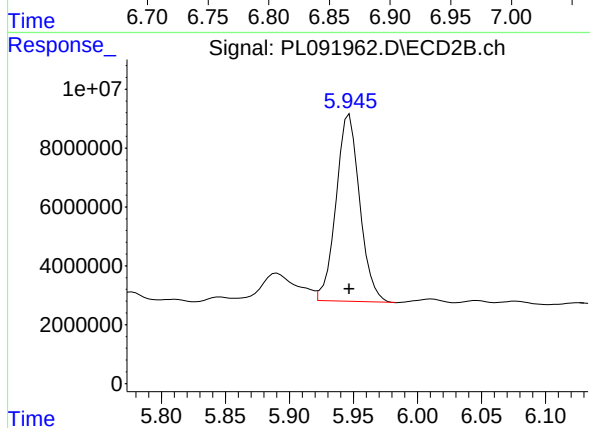

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 81542348
Conc: 740.56 ng/ml

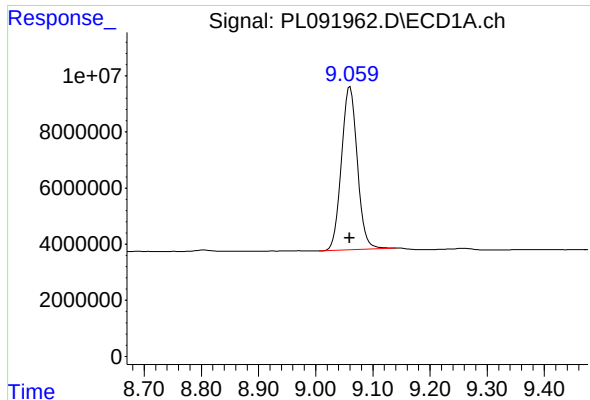

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 112019666
Conc: 73.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

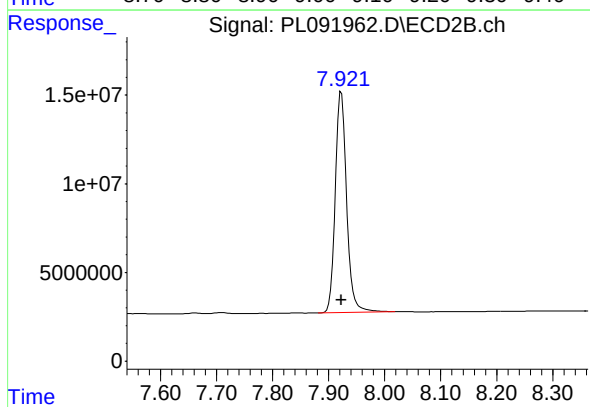

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 175442109
Conc: 73.13 ng/ml