

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 13:19
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 13:59:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 13:58:59 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.782	55649362	76418777	26.293	25.066
28) SA Decachlor...	9.061	7.923	40996191	63515556	26.334	26.089
Target Compounds						
23) Chlordane-1	4.706	3.781	26612873	25182916	267.620	253.532
24) Chlordane-2	5.235	4.359	27705732	28764449	270.916	263.641
25) Chlordane-3	5.945	4.989	93344435	81883907	260.230	246.891
26) Chlordane-4	6.027	5.052	113.8E6	79198691	261.772	248.622
27) Chlordane-5	6.876	5.947	22279405	27334257	264.666	248.682



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 13:19
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 13:59:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 13:58:59 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

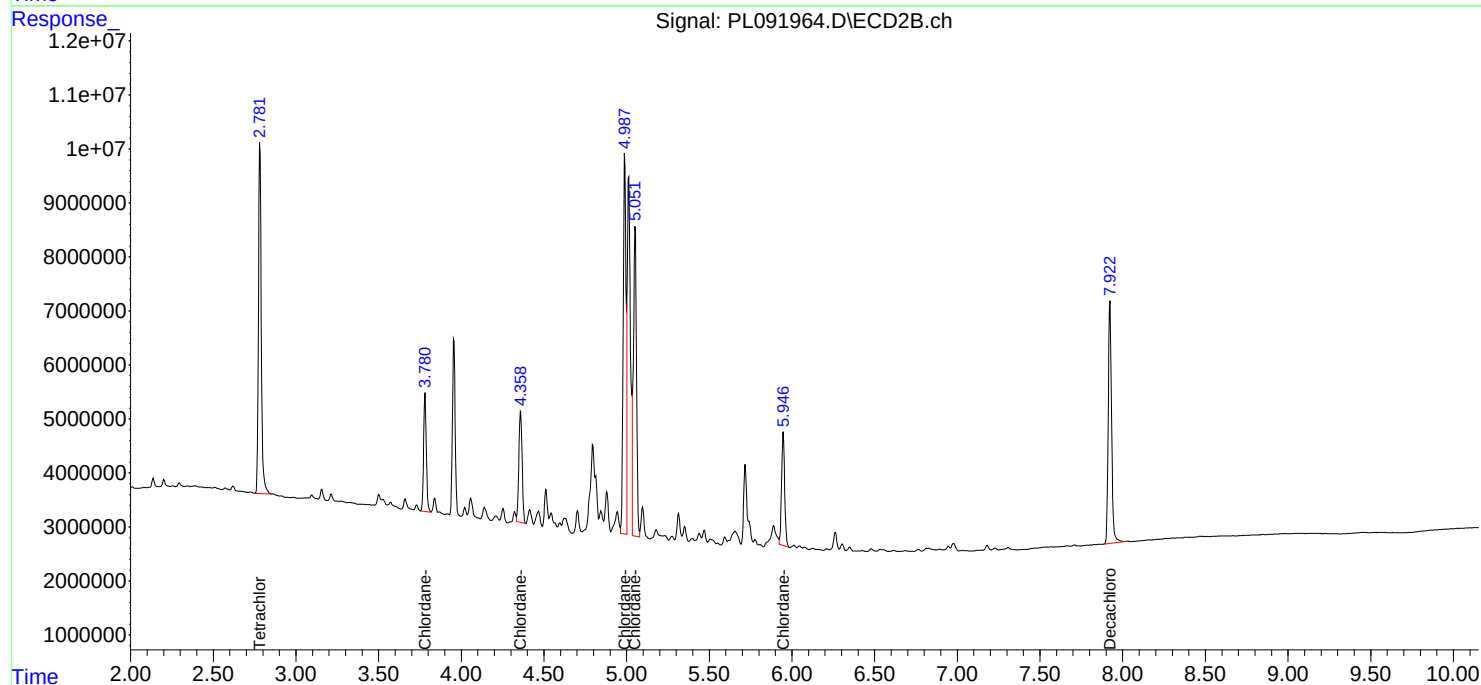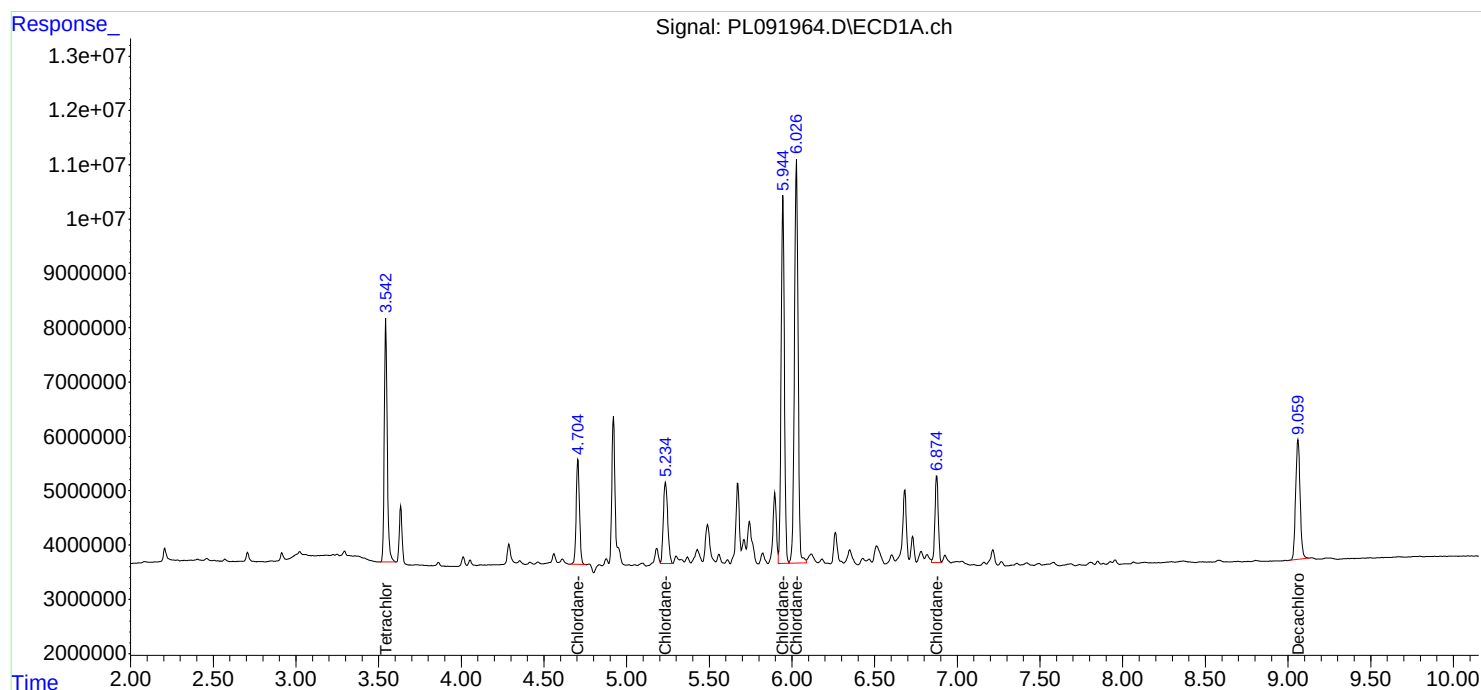


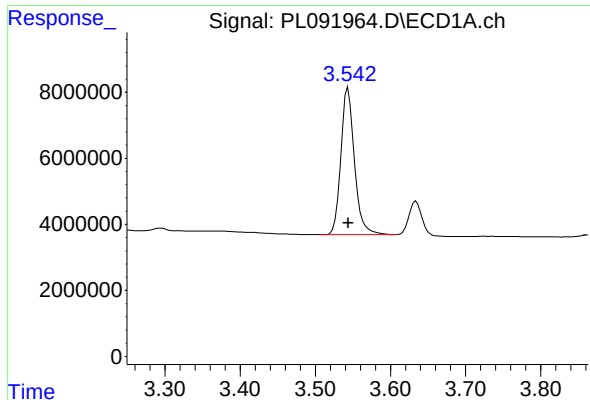

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 55649362
Conc: 26.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

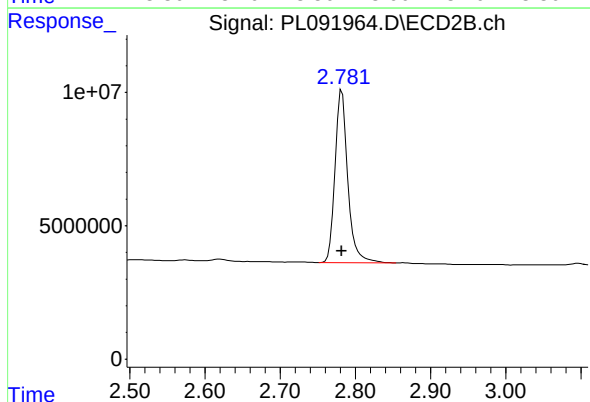


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 76418777
Conc: 25.07 ng/ml

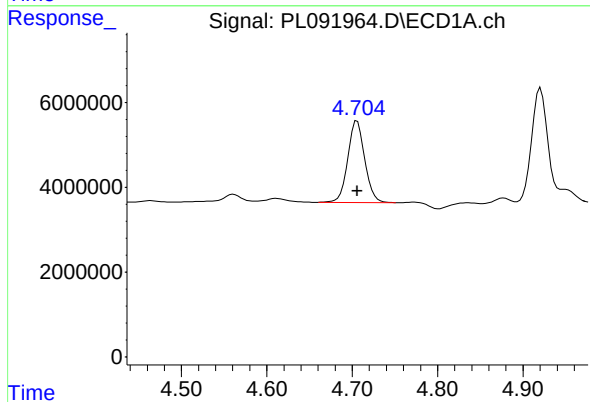


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 26612873
Conc: 267.62 ng/ml

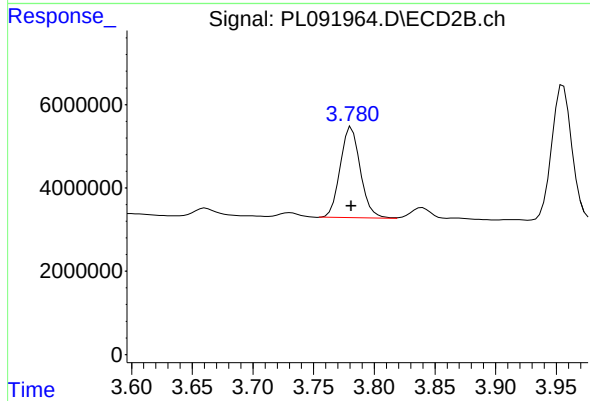

#23 Chlordane-1


R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 25182916
Conc: 253.53 ng/ml

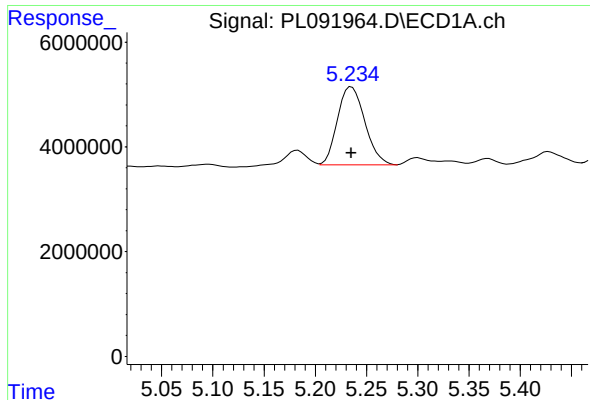

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 27705732
Conc: 270.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

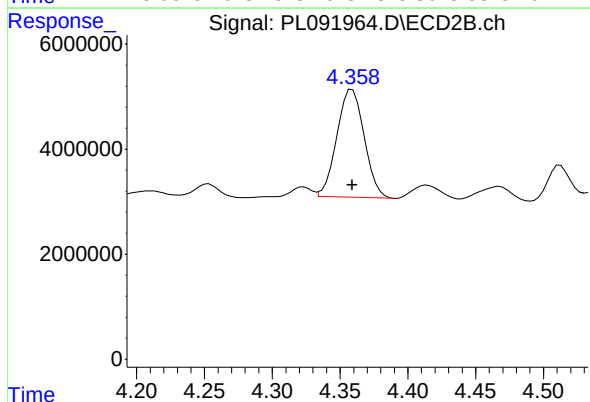


#24 Chlordane-2

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 28764449
Conc: 263.64 ng/ml

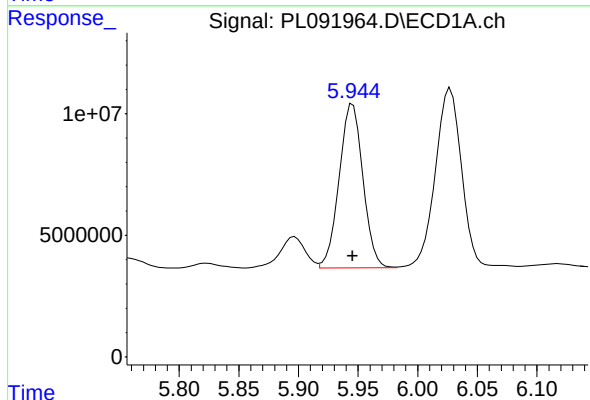


#25 Chlordane-3

R.T.: 5.945 min
Delta R.T.: 0.000 min
Response: 93344435
Conc: 260.23 ng/ml

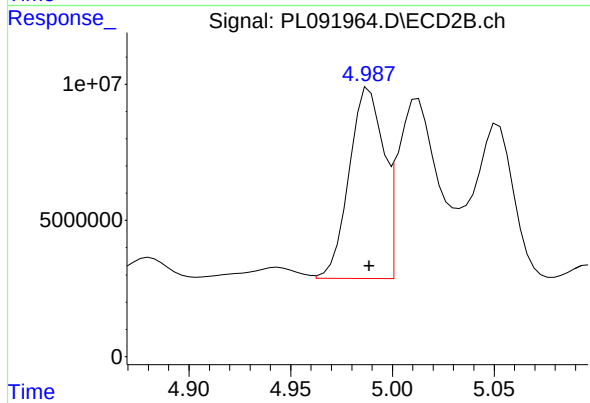

#25 Chlordane-3


R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 81883907
Conc: 246.89 ng/ml

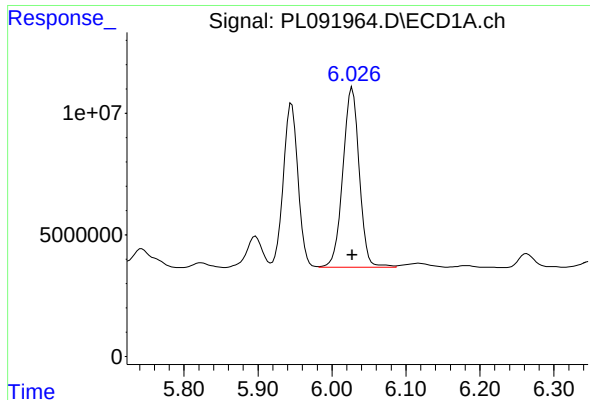

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 113849651
Conc: 261.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

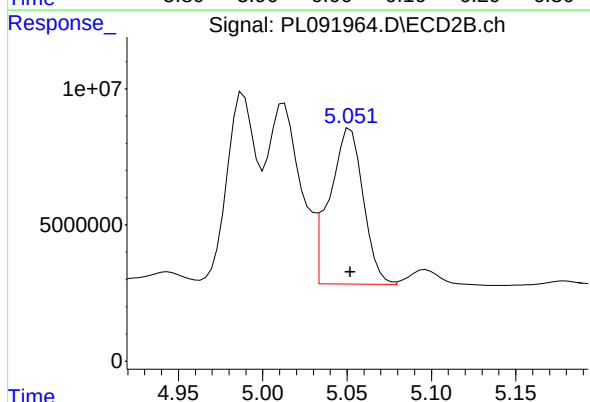


#26 Chlordane-4

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 79198691
Conc: 248.62 ng/ml

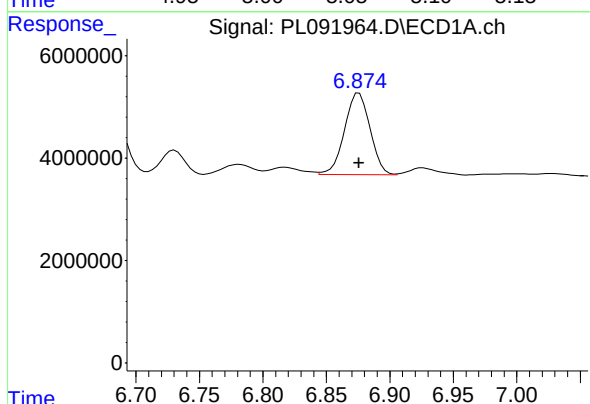


#27 Chlordane-5

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 22279405
Conc: 264.67 ng/ml

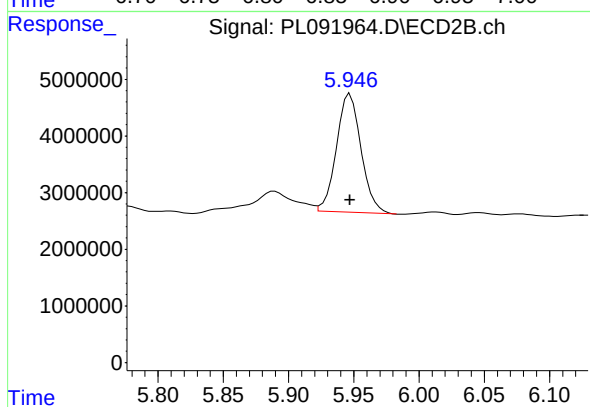

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 27334257
Conc: 248.68 ng/ml

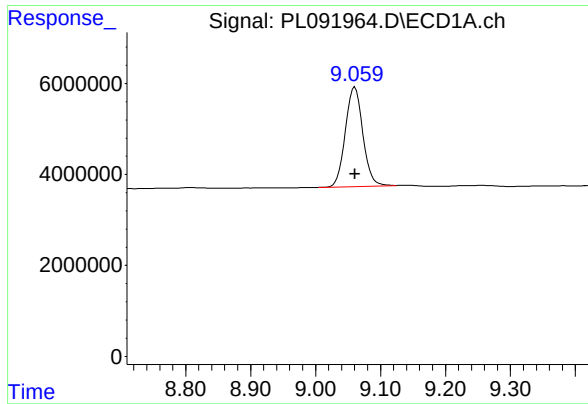

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 40996191
Conc: 26.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

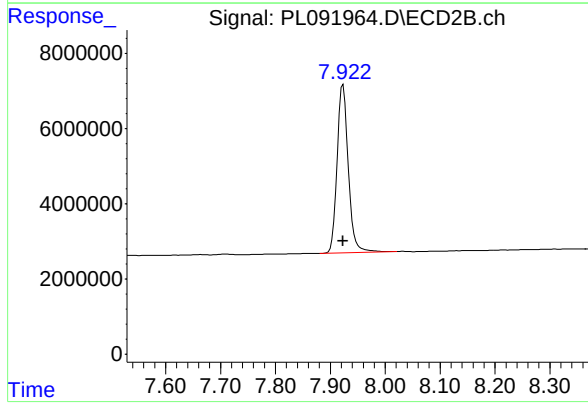

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 63515556
Conc: 26.09 ng/ml