

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 15:20
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL092324

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 23 16:42:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:41:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.782	106.0E6	152.5E6	48.293	49.786
28) SA Decachlor...	9.061	7.924	78307449	122.8E6	48.429	49.154
Target Compounds						
23) Chlordane-1	4.706	3.781	48433111	49506810	472.544	495.163
24) Chlordane-2	5.236	4.359	51223526	55177128	477.624	491.661
25) Chlordane-3	5.946	4.989	177.0E6	165.6E6	472.503	499.985
26) Chlordane-4	6.028	5.052	215.1E6	156.2E6	474.993	492.258
27) Chlordane-5	6.877	5.948	42165256	54383336	483.464	501.463



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 15:20
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL092324

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 23 16:42:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:41:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

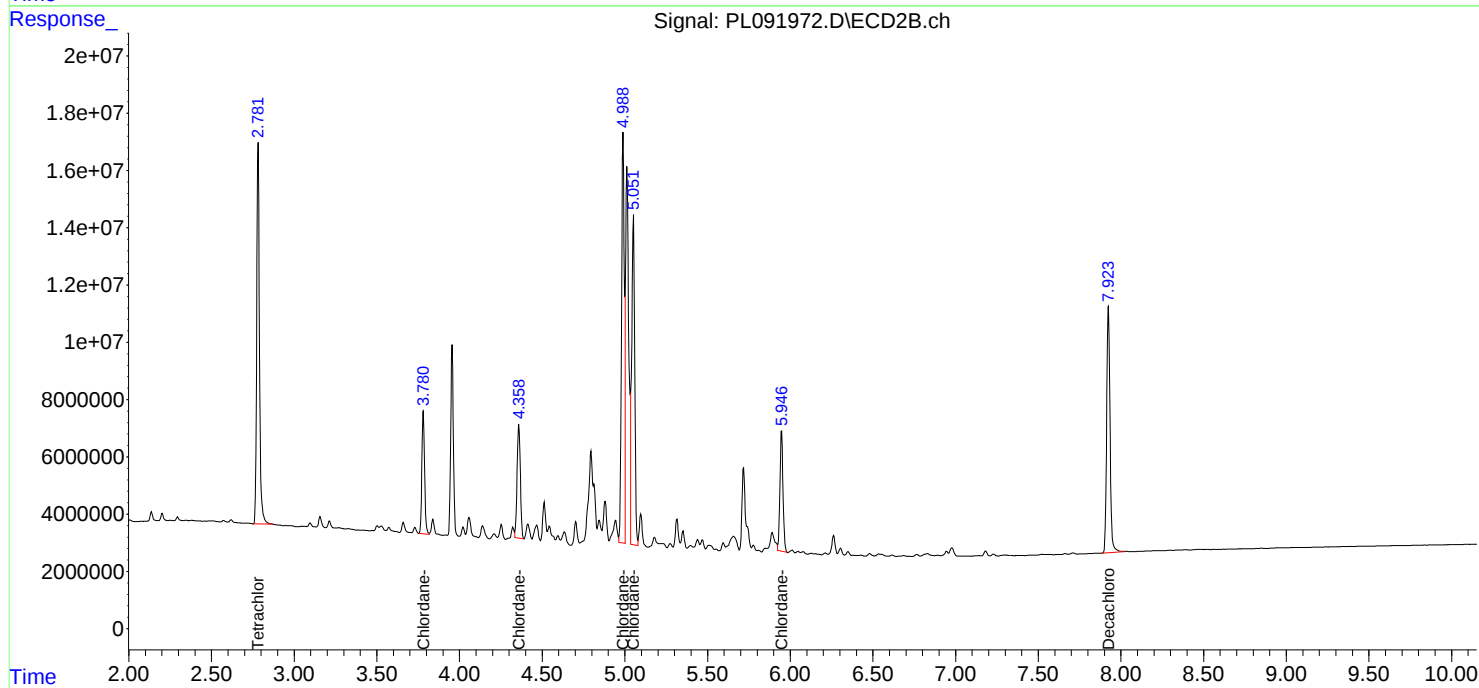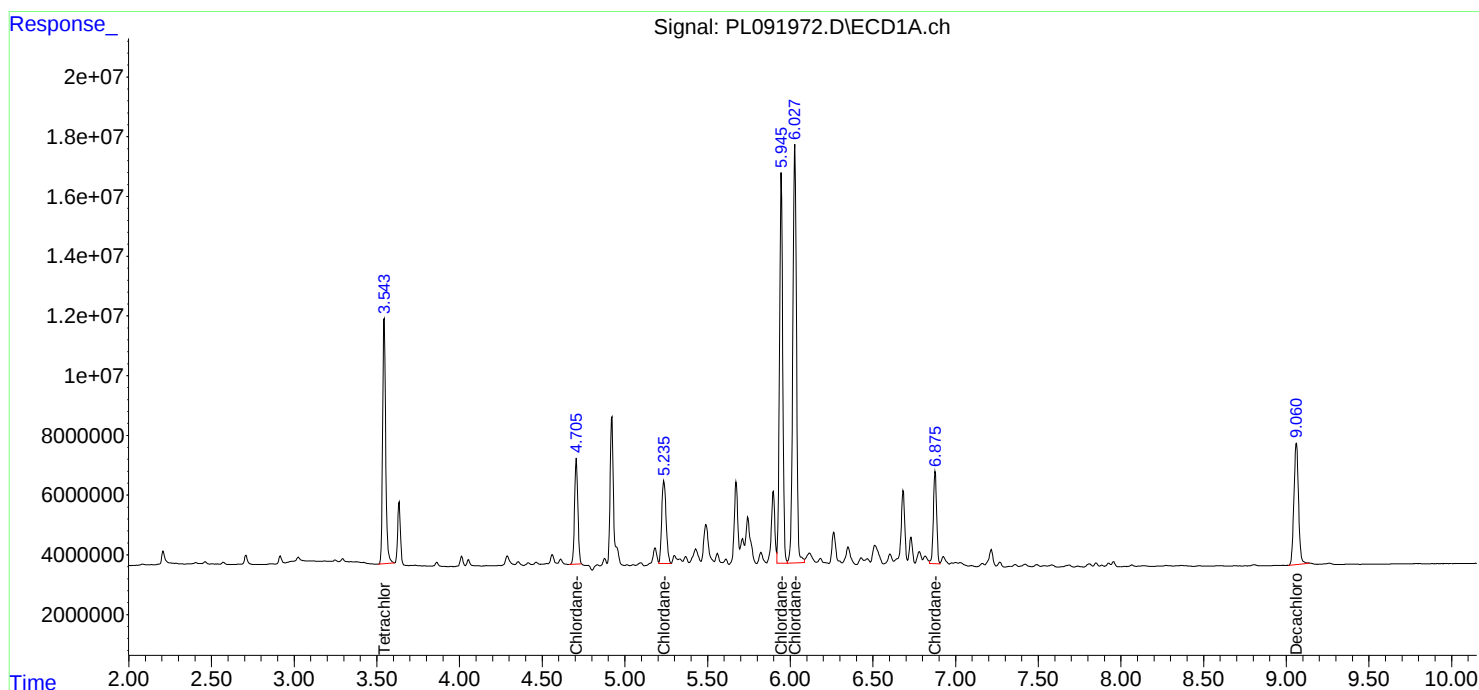


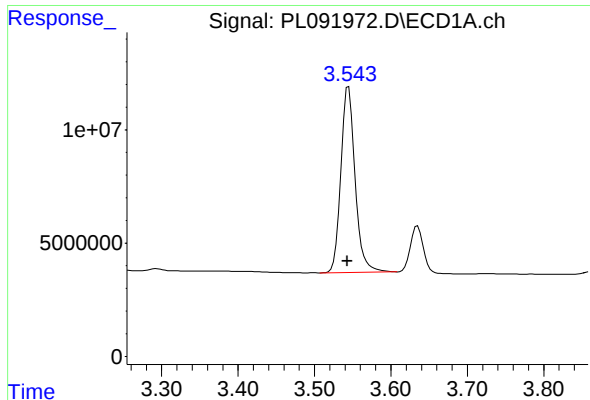

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.001 min
Response: 106020958
Conc: 48.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092324

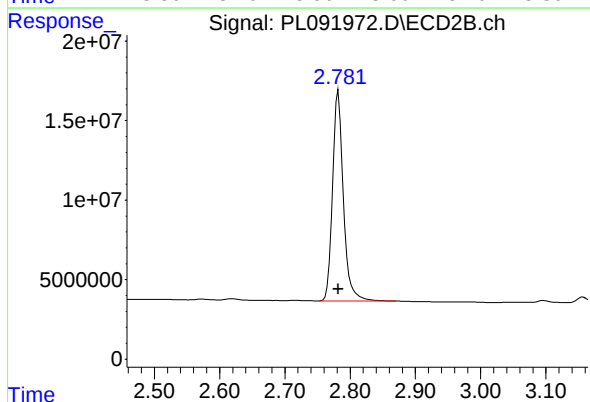


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 152495345
Conc: 49.79 ng/ml

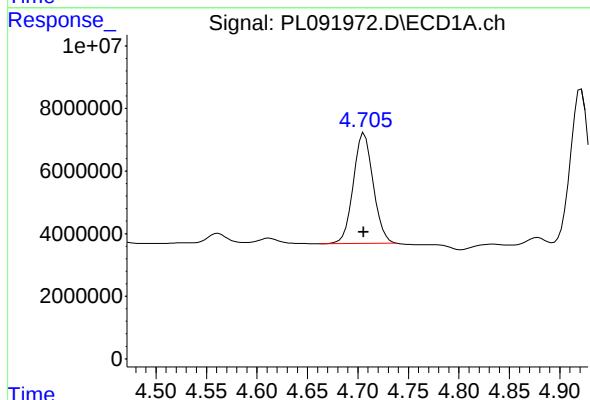


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 48433111
Conc: 472.54 ng/ml

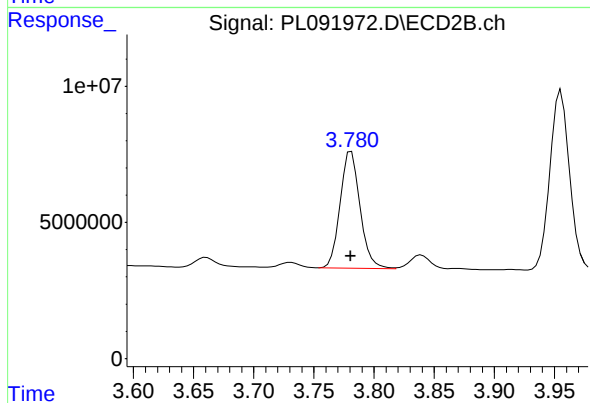

#23 Chlordane-1


R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 49506810
Conc: 495.16 ng/ml

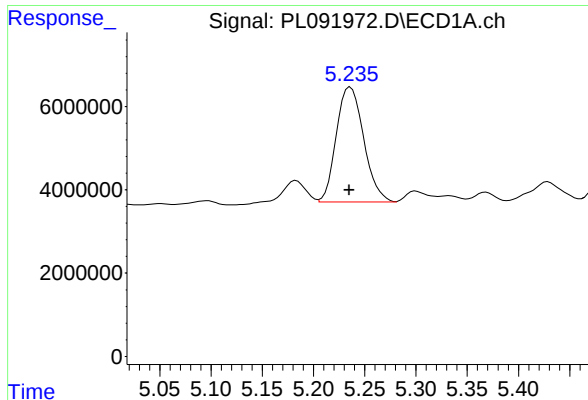

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 51223526
Conc: 477.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092324

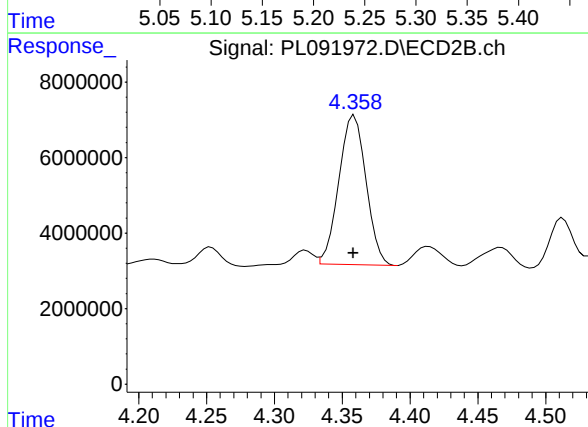


#24 Chlordane-2

R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 55177128
Conc: 491.66 ng/ml

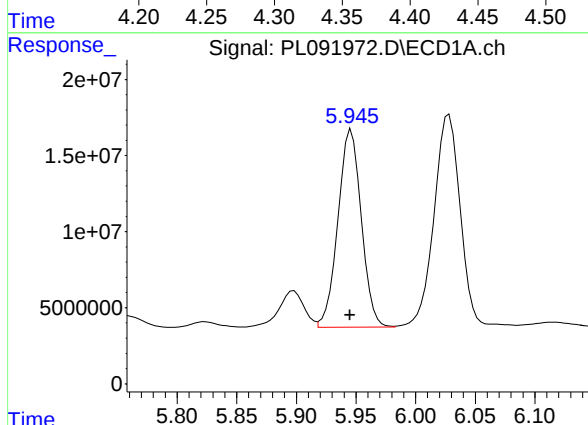


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 176988585
Conc: 472.50 ng/ml

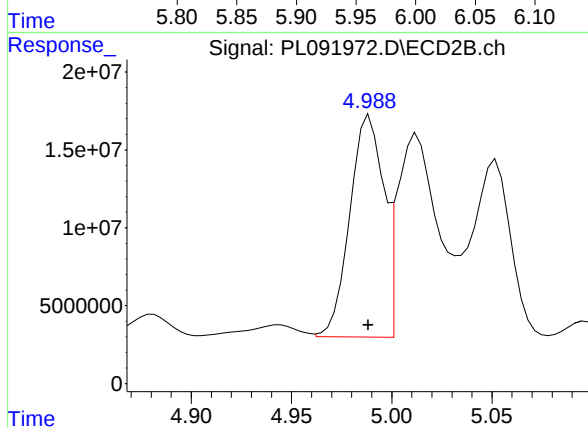

#25 Chlordane-3


R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 165609265
Conc: 499.99 ng/ml

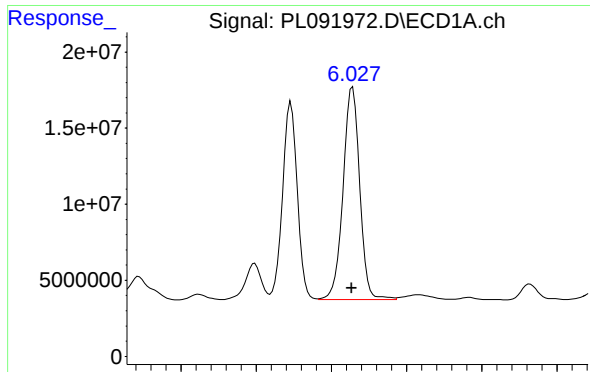

#26 Chlordane-4


R.T.: 6.028 min
Delta R.T.: 0.001 min
Response: 215098949
Conc: 474.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092324

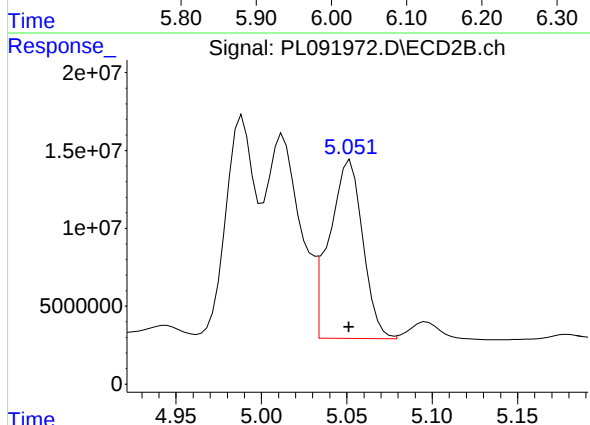


#26 Chlordane-4

R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 156184672
Conc: 492.26 ng/ml

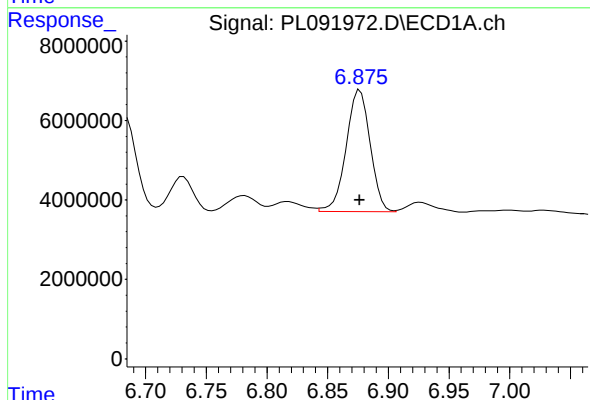


#27 Chlordane-5

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 42165256
Conc: 483.46 ng/ml

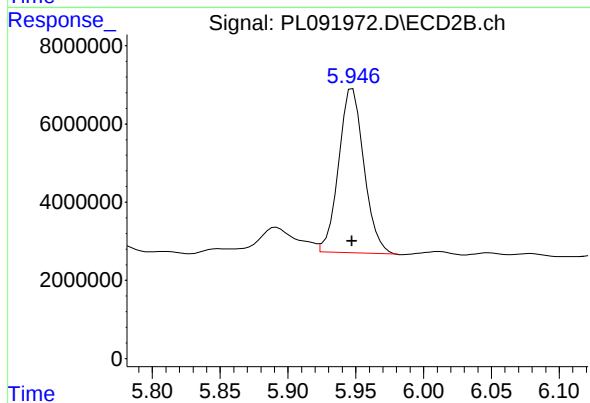

#27 Chlordane-5


R.T.: 5.948 min
Delta R.T.: 0.000 min
Response: 54383336
Conc: 501.46 ng/ml

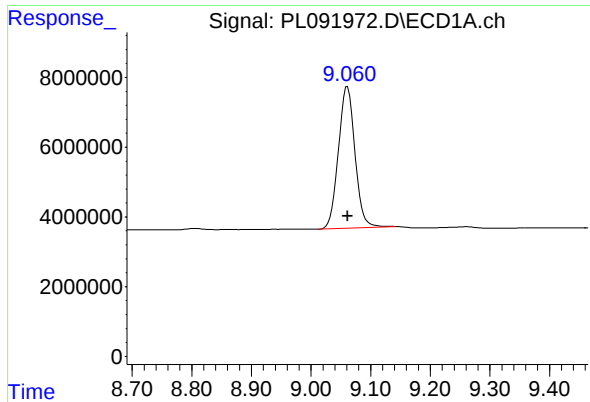

#28 Decachlorobiphenyl

R.T.: 9.061 min
Delta R.T.: 0.000 min
Response: 78307449
Conc: 48.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092324

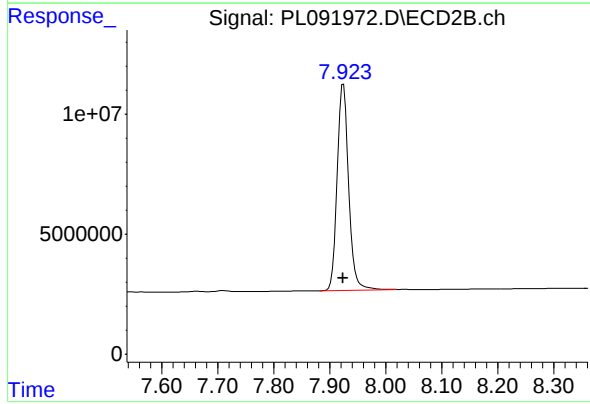

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.000 min
Response: 122848008
Conc: 49.15 ng/ml