

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 18:14
 Operator : AR\AJ
 Sample : P4103-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-14-5-7.5B

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:09:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.782	38364016	45304227	17.245	18.063m
28) SA Decachlor...	9.059	7.923	22900593	35903266	13.979m	14.350

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 18:14
Operator : AR\AJ
Sample : P4103-08
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-14-5-7.5B


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/24/2024
Supervised By : Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:09:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

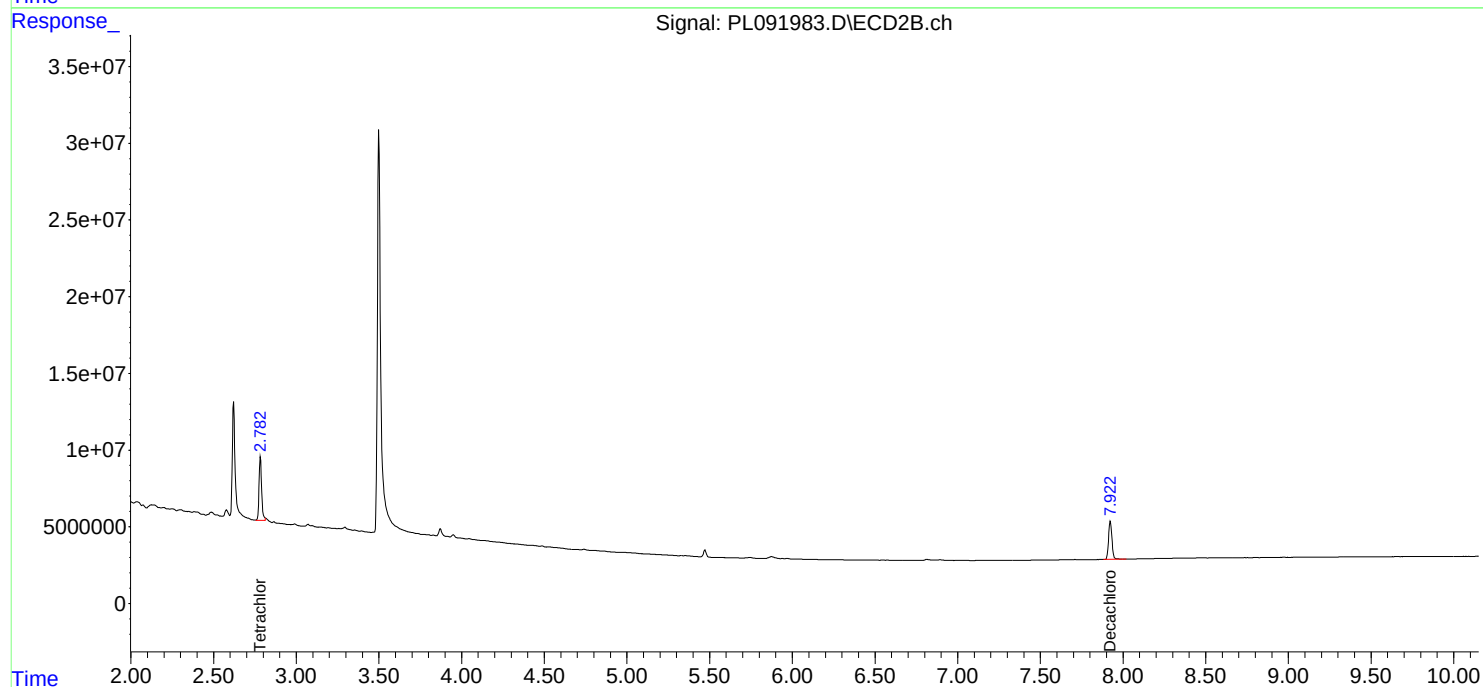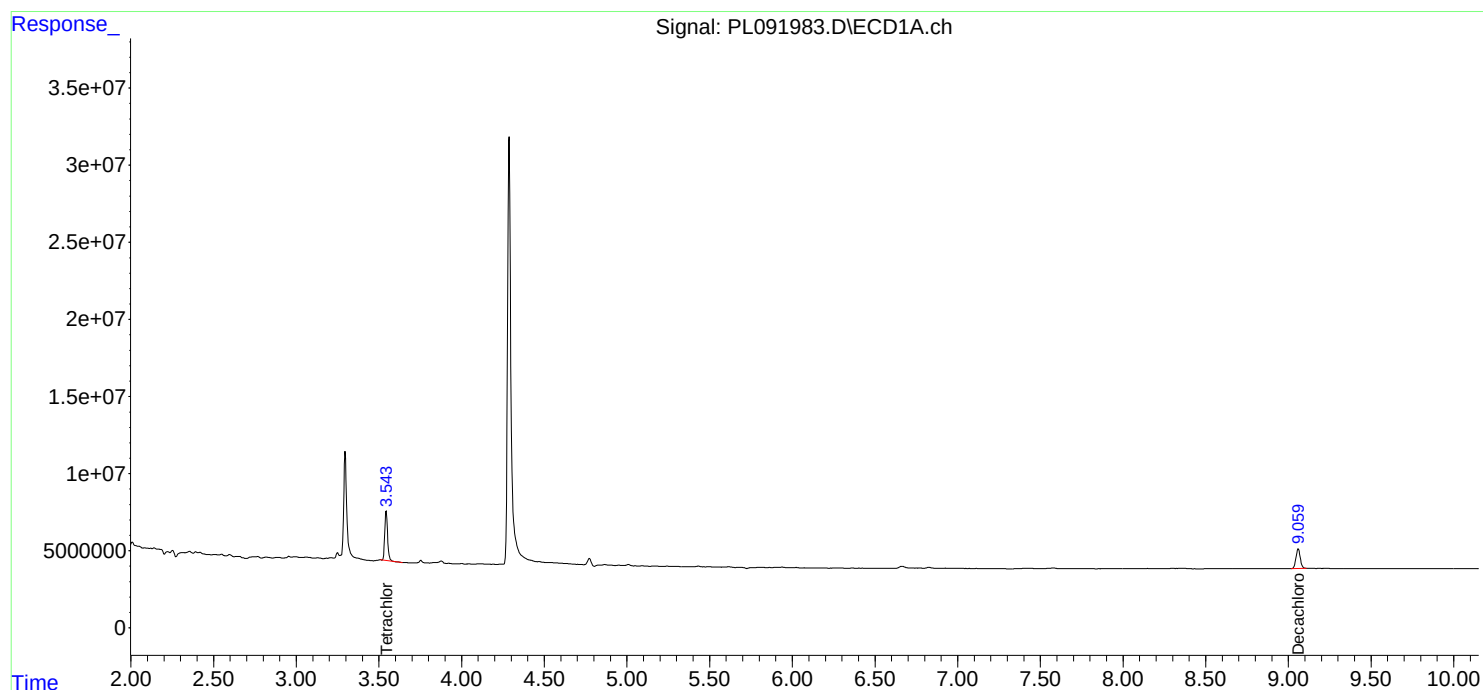

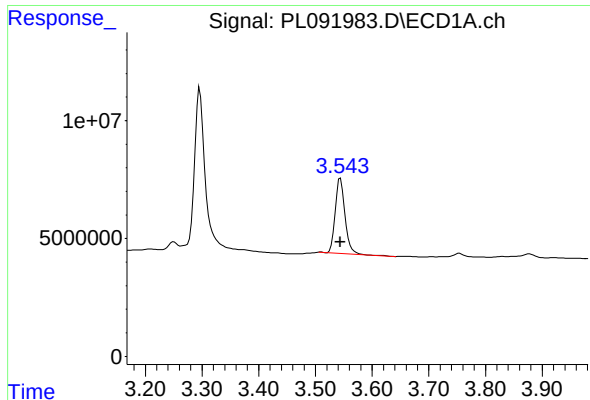

#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 38364016
Conc: 17.24 ng/ml

Instrument :


ECD_L

ClientSampleId :

WC-14-5-7.5B


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

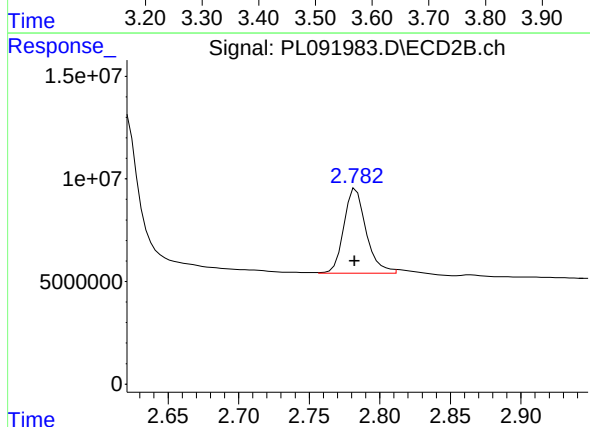


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 45304227
Conc: 18.06 ng/ml m

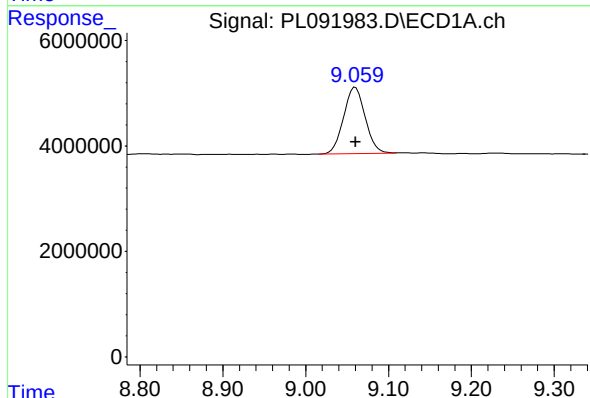

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.002 min
Response: 22900593
Conc: 13.98 ng/ml m

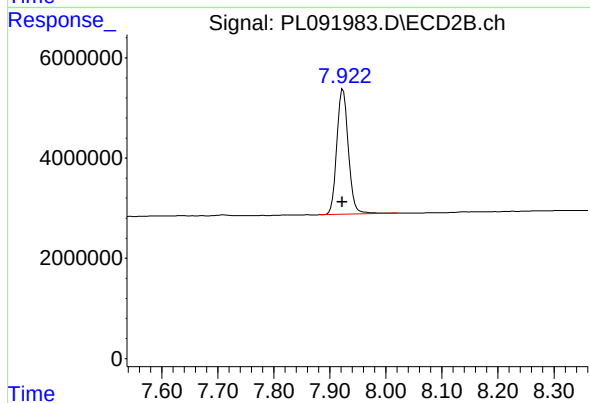

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 35903266
Conc: 14.35 ng/ml