

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
 Data File : PL091984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Sep 2024 18:28
 Operator : AR\AJ
 Sample : P4103-11
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-14-7.5-10A

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/24/2024
 Supervised By :Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 24 02:10:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	2.782	35965652	52673585	16.167m	21.002m#
28) SA Decachlor...	9.059	7.924	23590804	36237948	14.400m	14.484

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092324\
Data File : PL091984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Sep 2024 18:28
Operator : AR\AJ
Sample : P4103-11
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-14-7.5-10A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/24/2024
Supervised By : Ankita Jodhani 09/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 24 02:10:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

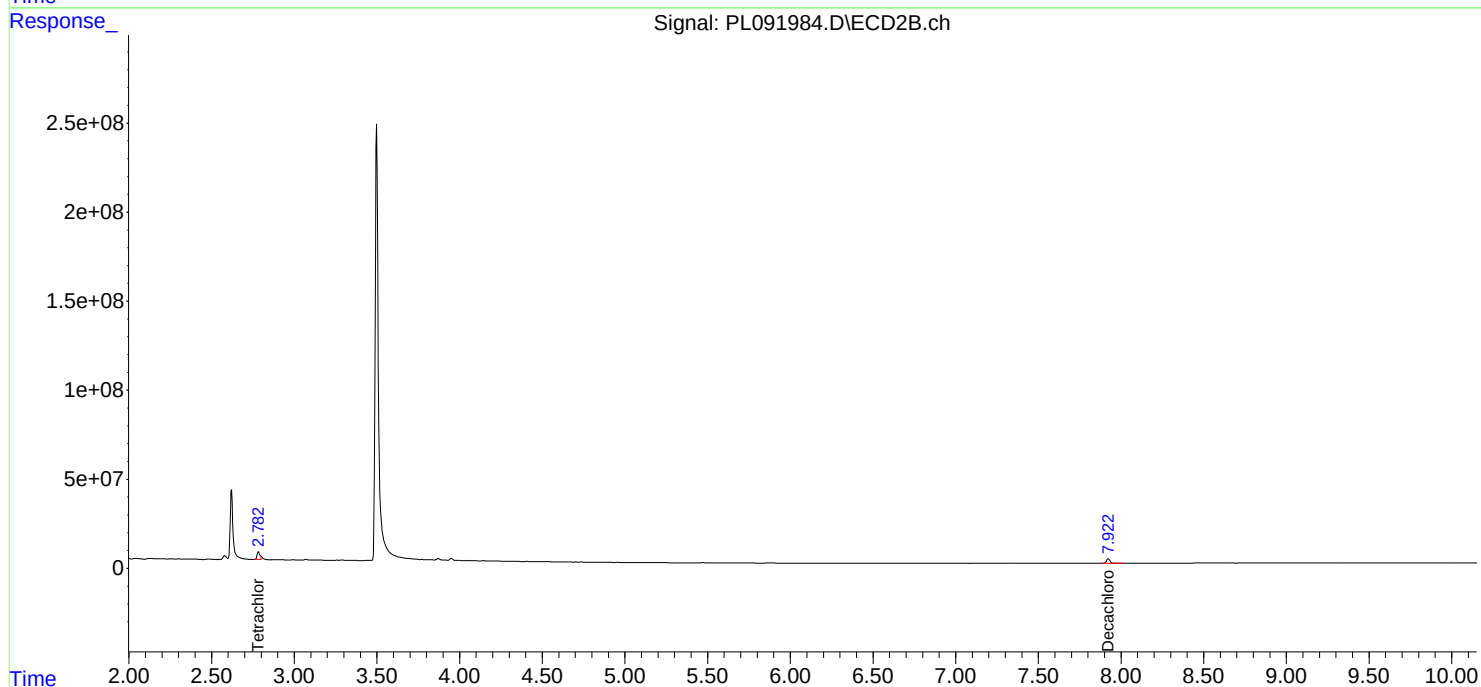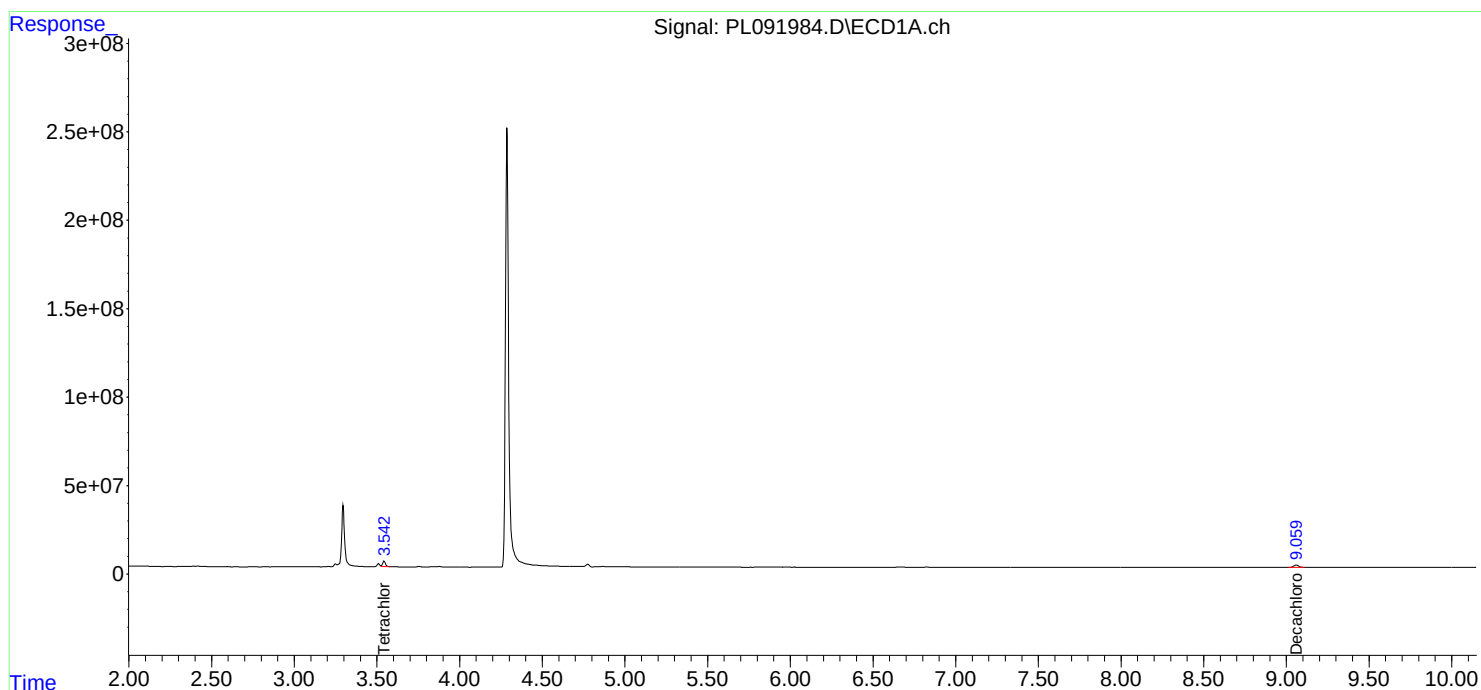

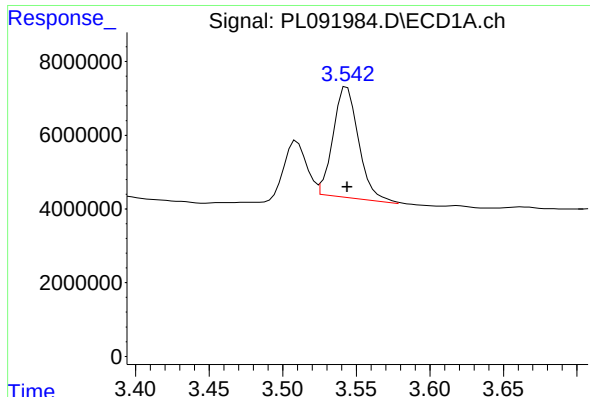


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 35965652
Conc: 16.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-14-7.5-10A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/24/2024
Supervised By :Ankita Jodhani 09/24/2024

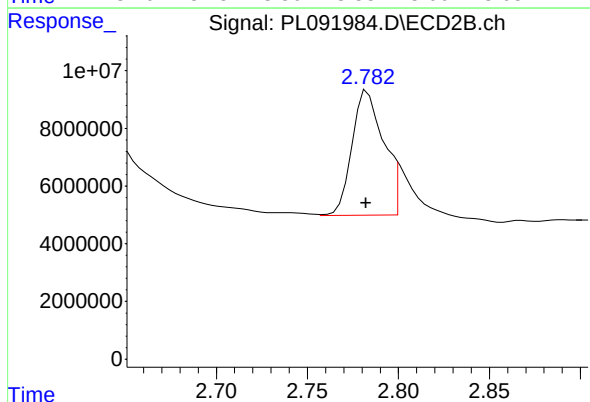


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 52673585
Conc: 21.00 ng/ml m

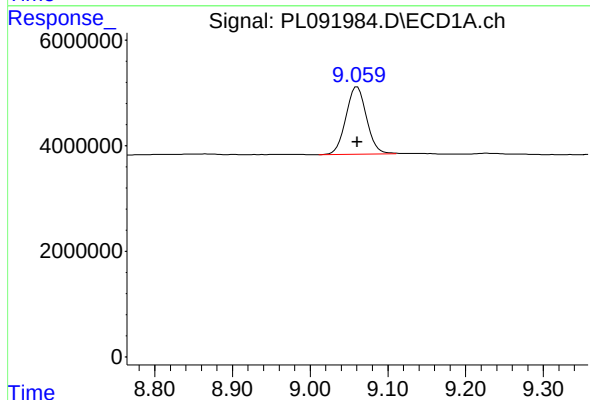

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.001 min
Response: 23590804
Conc: 14.40 ng/ml m

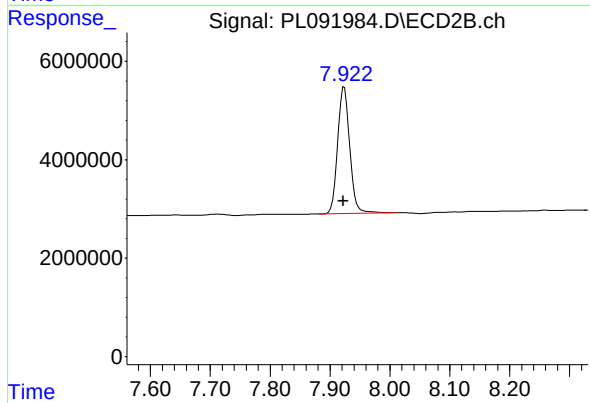

#28 Decachlorobiphenyl

R.T.: 7.924 min
Delta R.T.: 0.001 min
Response: 36237948
Conc: 14.48 ng/ml