

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092418\
 Data File : PL040254.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2018 17:04
 Operator : AJ\SJ
 Sample : J5021-17DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 00:53:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.842	0	5976857	N.D.	1.830 #
28)	SA Decachlor...	0.000	8.793	0	7780508	N.D.	2.432 #
Target Compounds							
3)	MA gamma-BHC...	3.993f	0.000	51502865	0	4.666	N.D. #
10)	B gamma-Chl...	5.054f	0.000	15441572	0	1.430	N.D. #
12)	B 4,4'-DDE	5.333	6.132	176.8E6	70468023	16.773	18.595
14)	MA Endrin	5.711	6.521f	86107145	30219994	8.746	9.467
15)	B Endosulfa...	5.921f	0.000	64087465	0	6.169	N.D. #
16)	A 4,4'-DDD	5.842	6.612	18458842	9793277	2.136	3.058 #
17)	MA 4,4'-DDT	6.073	6.908	301.3E6	112.8E6	35.642	39.484
25)	Chlordane-3	5.054	0.000	15441572	0	12.596	N.D. #
27)	Chlordane-5	5.921	0.000	64087465	0	154.522	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092418\
Data File : PL040254.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2018 17:04
Operator : AJ\SJ
Sample : J5021-17DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 00:53:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

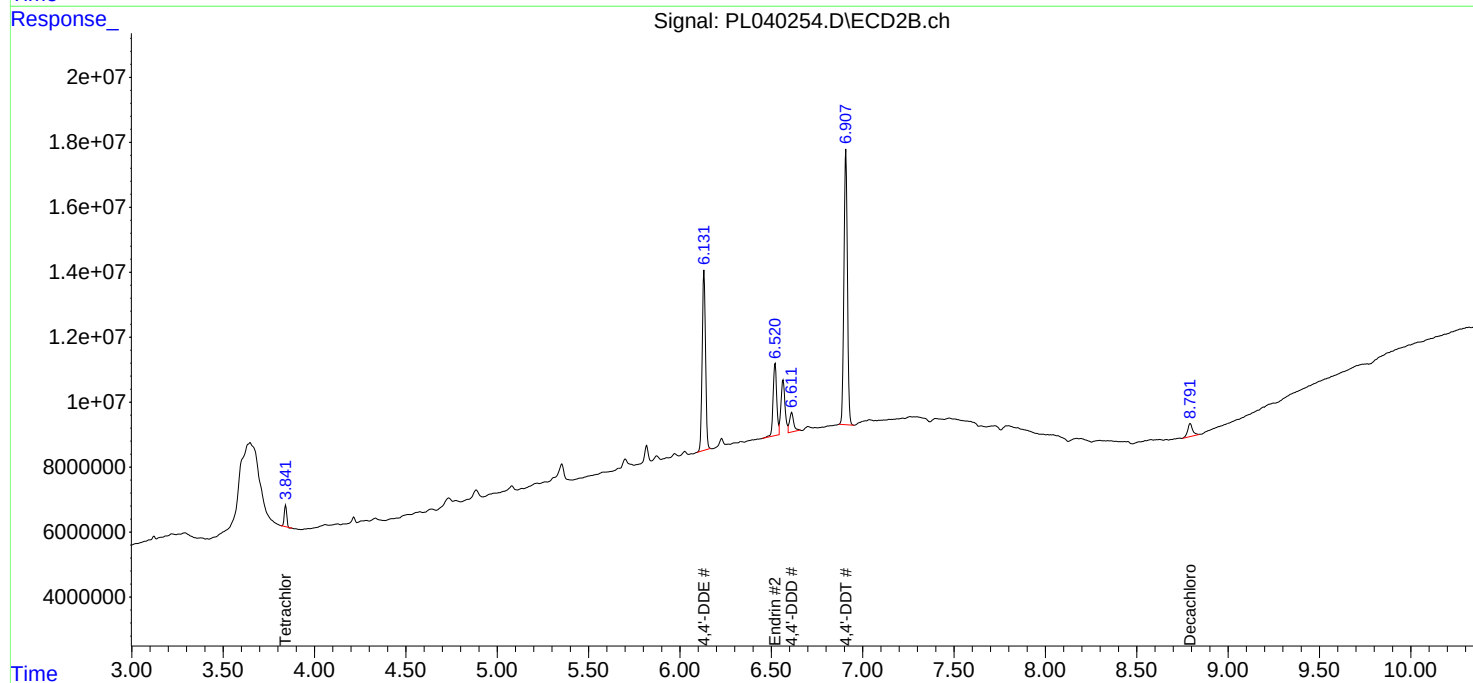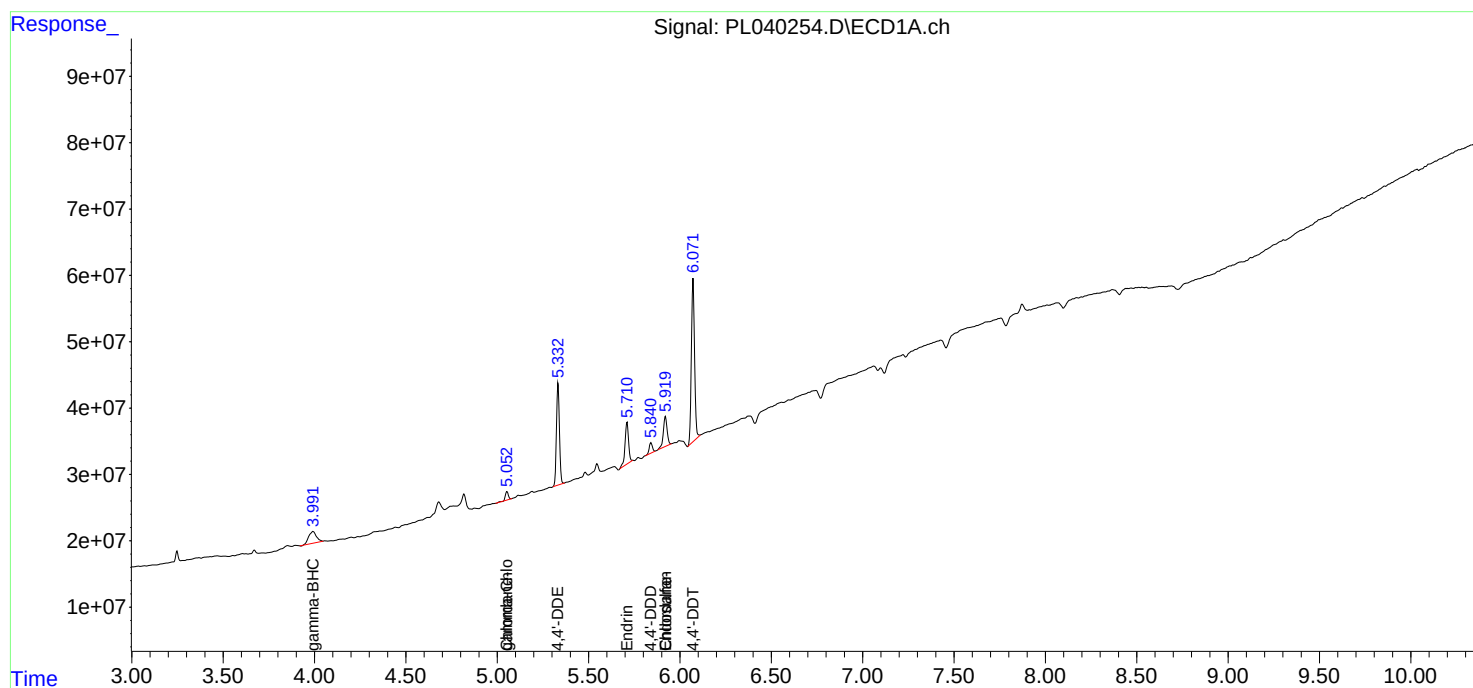


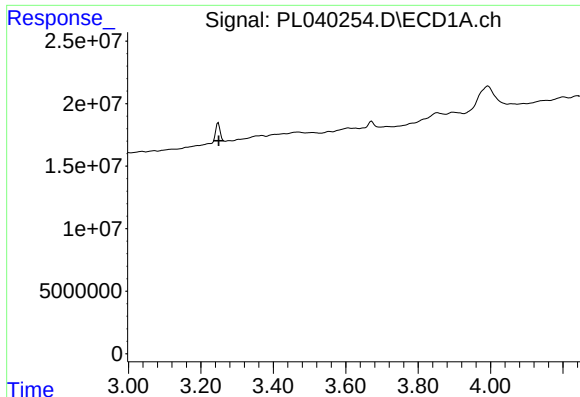

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.249 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

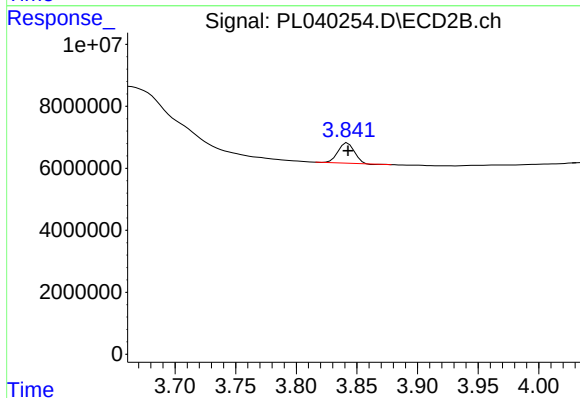


#1 Tetrachloro-m-xylene

R.T.: 3.842 min
Delta R.T.: 0.000 min
Response: 5976857
Conc: 1.83 ng/ml

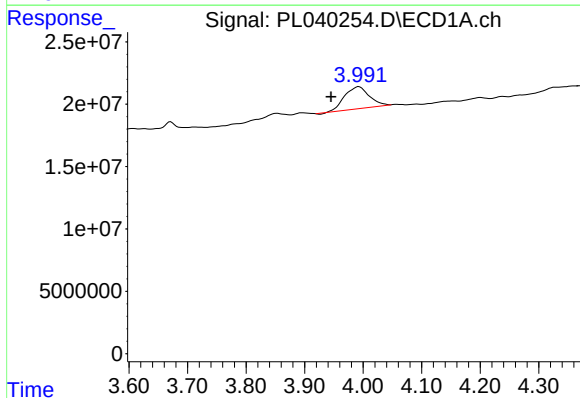


#3 gamma-BHC (Lindane)

R.T.: 3.993 min
Delta R.T.: 0.047 min
Response: 51502865
Conc: 4.67 ng/ml

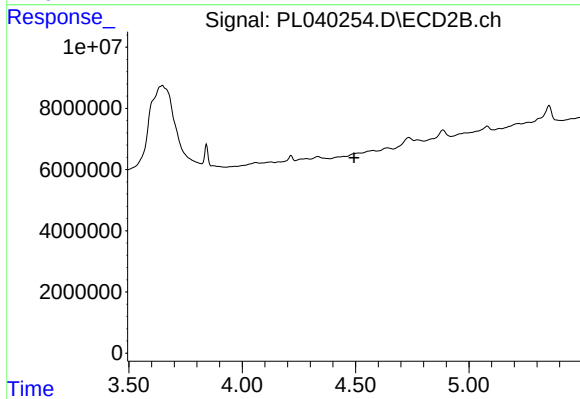

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.493 min
Response: 0
Conc: N.D.

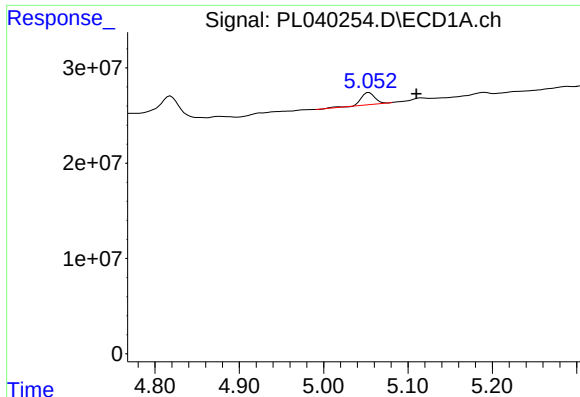

#10 gamma-Chlordane


R.T.: 5.054 min
Delta R.T.: -0.056 min
Response: 15441572
Conc: 1.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

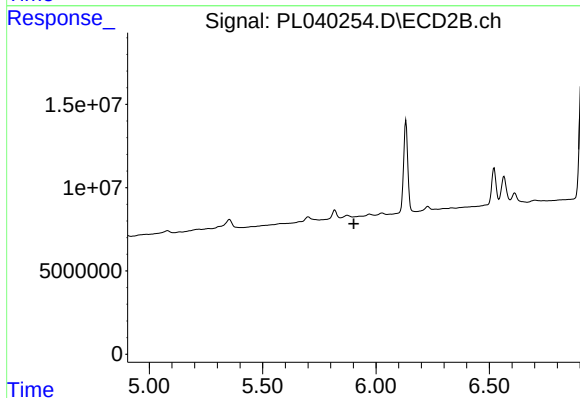


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.902 min
Response: 0
Conc: N.D.

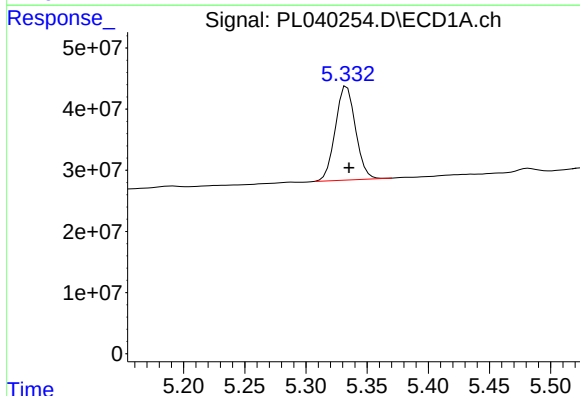


#12 4,4'-DDE

R.T.: 5.333 min
Delta R.T.: -0.002 min
Response: 176768579
Conc: 16.77 ng/ml

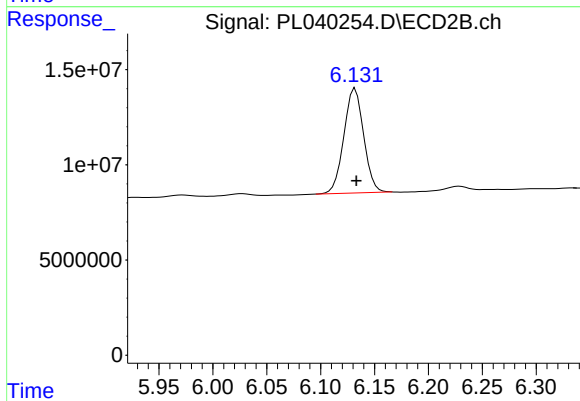

#12 4,4'-DDE


R.T.: 6.132 min
Delta R.T.: -0.001 min
Response: 70468023
Conc: 18.60 ng/ml

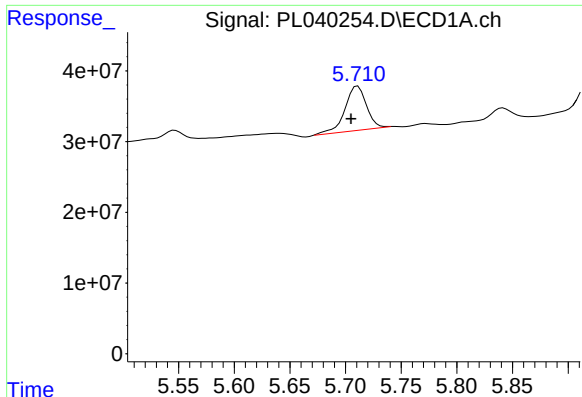

#14 Endrin


R.T.: 5.711 min
Delta R.T.: 0.006 min
Response: 86107145
Conc: 8.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

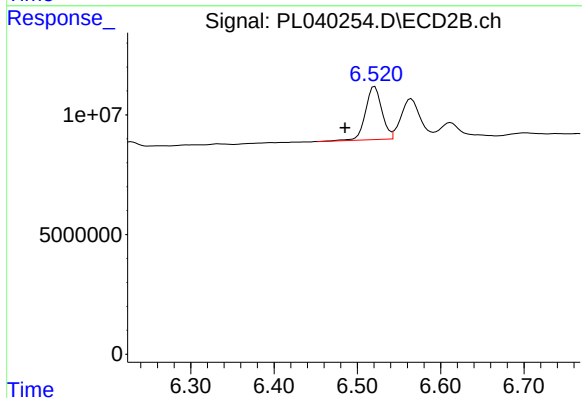


#14 Endrin

R.T.: 6.521 min
Delta R.T.: 0.036 min
Response: 30219994
Conc: 9.47 ng/ml

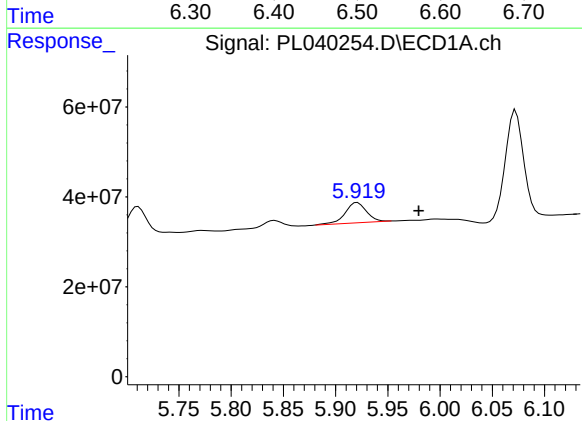


#15 Endosulfan II

R.T.: 5.921 min
Delta R.T.: -0.059 min
Response: 64087465
Conc: 6.17 ng/ml

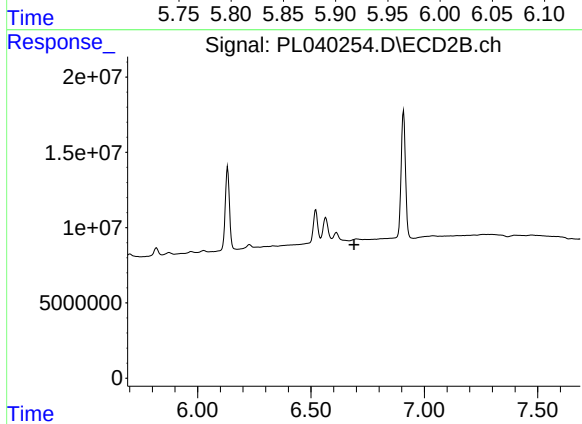

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.690 min
Response: 0
Conc: N.D.

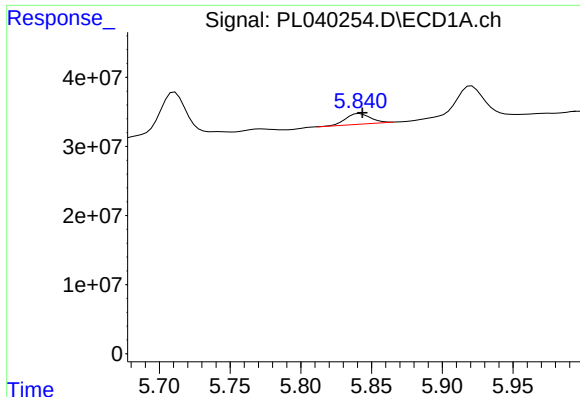

#16 4,4'-DDD


R.T.: 5.842 min
Delta R.T.: -0.002 min
Response: 18458842
Conc: 2.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

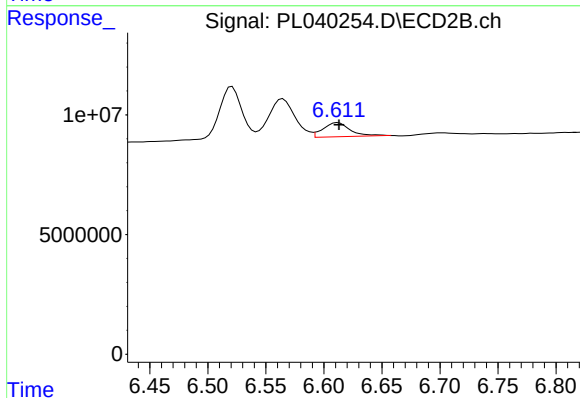


#16 4,4'-DDD

R.T.: 6.612 min
Delta R.T.: 0.000 min
Response: 9793277
Conc: 3.06 ng/ml

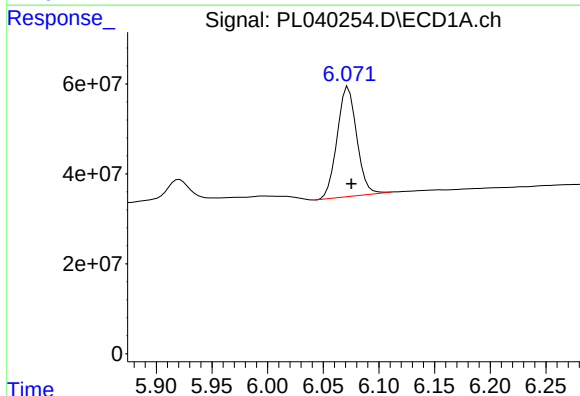


#17 4,4'-DDT

R.T.: 6.073 min
Delta R.T.: -0.003 min
Response: 301308358
Conc: 35.64 ng/ml

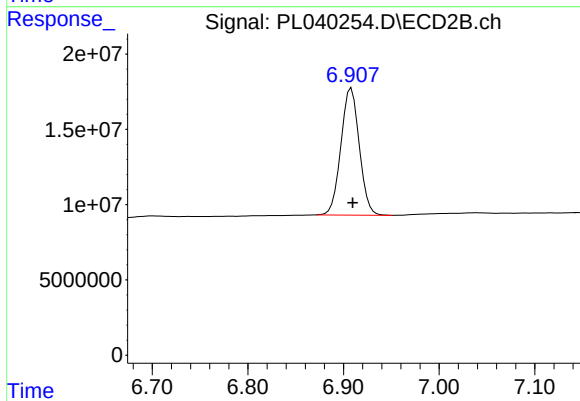

#17 4,4'-DDT


R.T.: 6.908 min
Delta R.T.: -0.002 min
Response: 112778265
Conc: 39.48 ng/ml

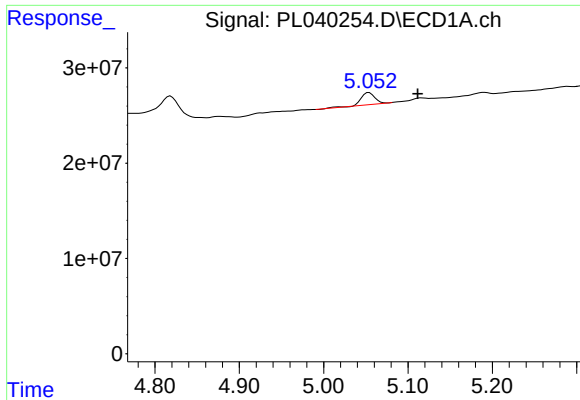

#25 Chlordane-3


R.T.: 5.054 min
Delta R.T.: -0.058 min
Response: 15441572
Conc: 12.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

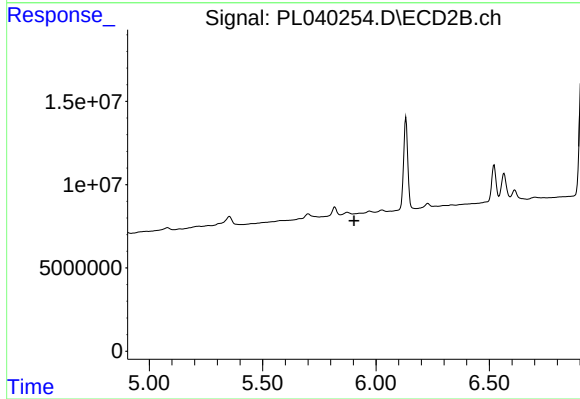


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.904 min
Response: 0
Conc: N.D.

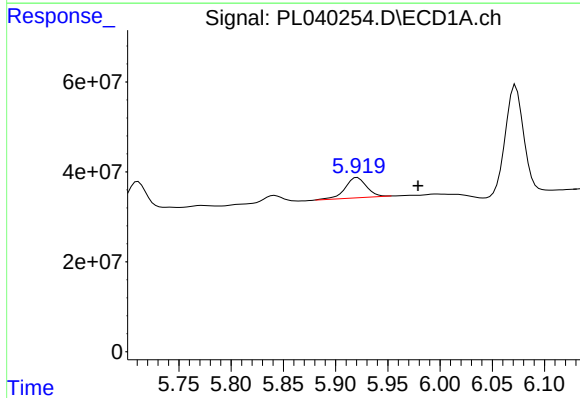


#27 Chlordane-5

R.T.: 5.921 min
Delta R.T.: -0.058 min
Response: 64087465
Conc: 154.52 ng/ml

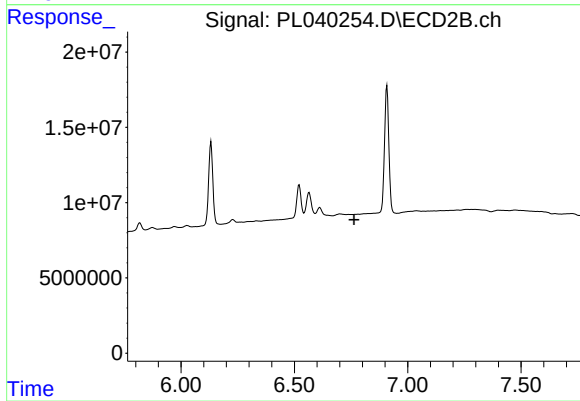

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

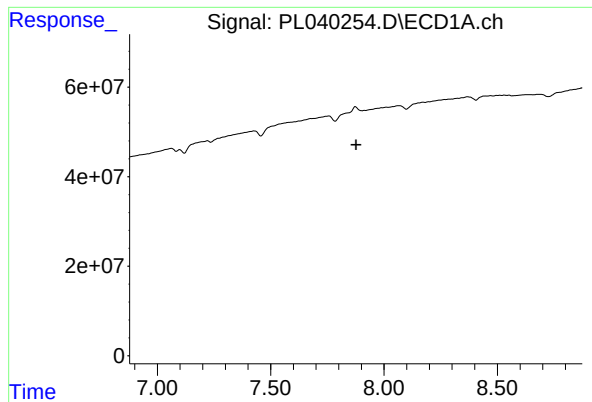

#28 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T.: 7.876 min

Response: 0

Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

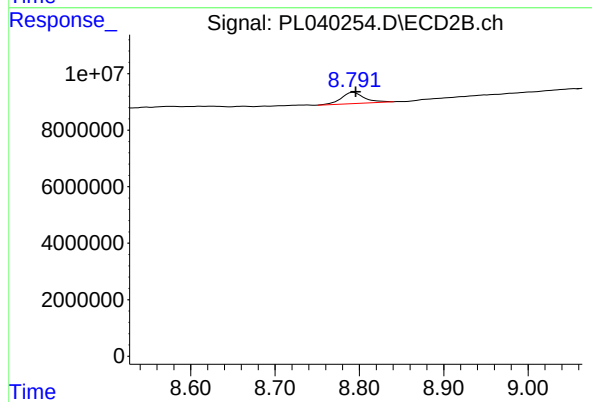

#28 Decachlorobiphenyl

R.T.: 8.793 min

Delta R.T.: -0.003 min

Response: 7780508

Conc: 2.43 ng/ml