

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092418\
 Data File : PL040259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2018 18:43
 Operator : AJ\SJ
 Sample : J5056-01 (Sig #1); J5056-11 (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RA-BASELINE-WATER

Manual Integrations
 APPROVED

Sohil
 9/25/2018 3:49:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 00:54:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.247	3.843	124.3E6	47334315	16.342m	14.495
28)	SA Decachlor...	7.875	8.794	102.1E6	39964132	11.528	12.490

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092418\
Data File : PL040259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2018 18:43
Operator : AJ\SJ
Sample : J5056-01 (Sig #1); J5056-11 (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RA-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
9/25/2018 3:49:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 00:54:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

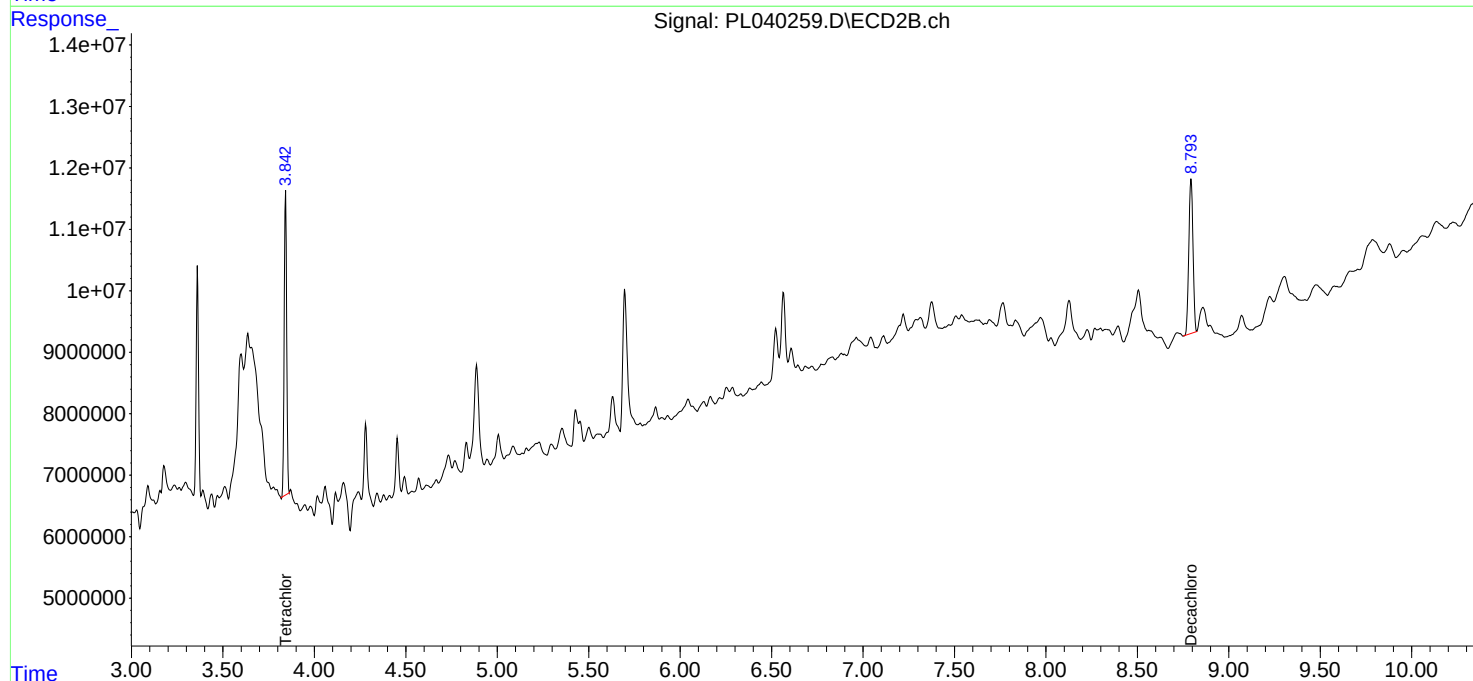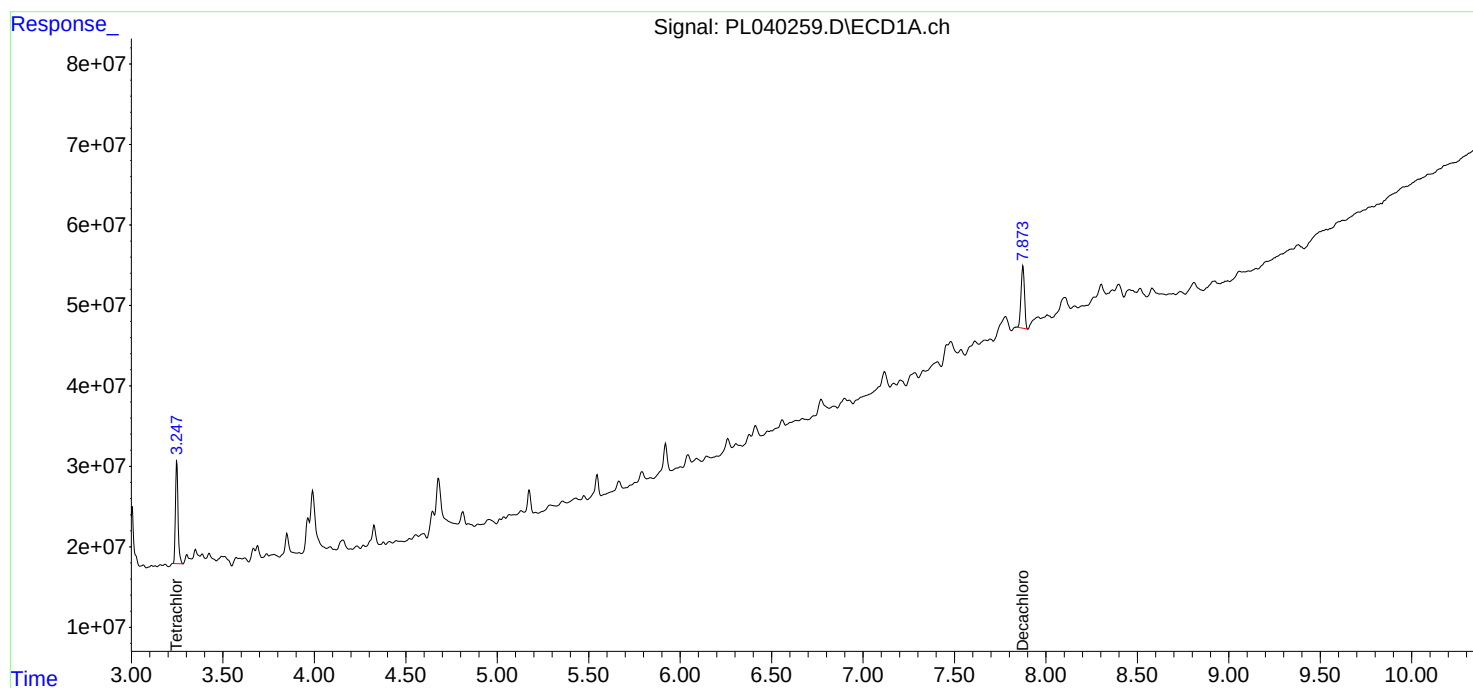

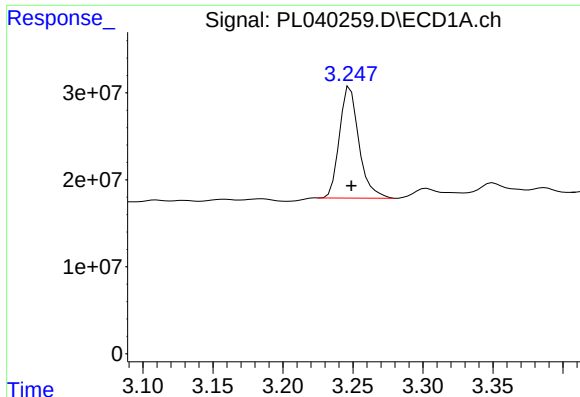


#1 Tetrachloro-m-xylene

R.T.: 3.247 min
Delta R.T.: -0.002 min
Response: 124332085
Conc: 16.34 ng/ml m

Instrument :
ECD_L
ClientSampleId :
RA-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
9/25/2018 3:49:55 PM

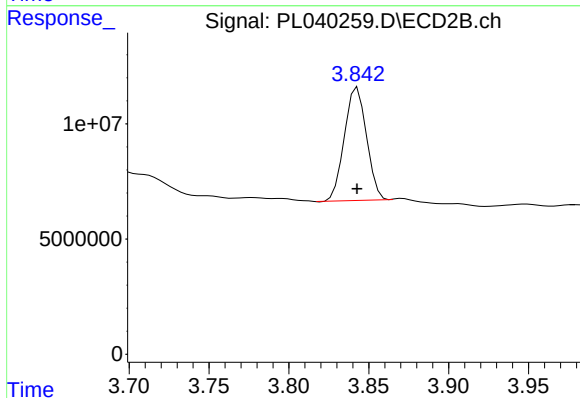


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 47334315
Conc: 14.49 ng/ml

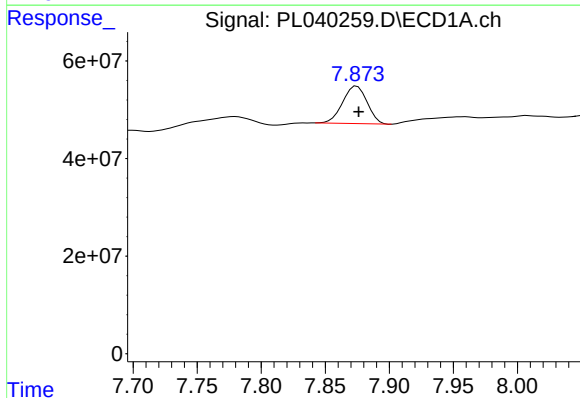

#28 Decachlorobiphenyl

R.T.: 7.875 min
Delta R.T.: -0.002 min
Response: 102093389
Conc: 11.53 ng/ml

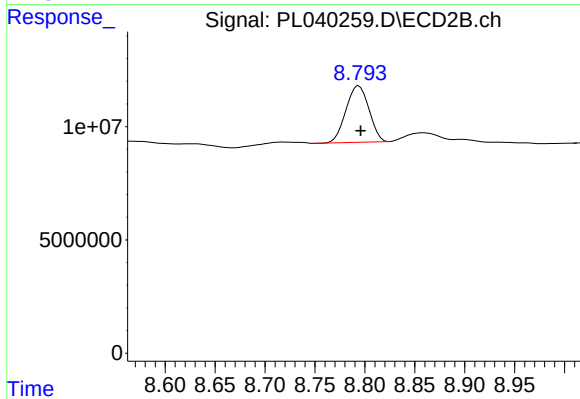

#28 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: -0.002 min
Response: 39964132
Conc: 12.49 ng/ml