

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
 Data File : PL052700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2019 17:57
 Operator : SG\AJ
 Sample : K4997-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-08-091919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:16:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.048	136.5E6	44305884	17.504	20.334
28)	SA Decachlor...	8.351	9.125	153.3E6	50021697	17.531	20.889
Target Compounds							
2)	A alpha-BHC	4.005	0.000	57006129	0	4.742	N.D. #
5)	MB Aldrin	4.833	0.000	1915003	0	0.177	N.D. #
6)	B beta-BHC	0.000	4.864f	0	382964	N.D.	0.287 #
7)	B delta-BHC	0.000	5.087f	0	3396376	N.D.	1.186 #
13)	MA Dieldrin	0.000	6.557f	0	1955422	N.D.	0.801 #
15)	B Endosulfa...	0.000	6.975	0	1569847	N.D.	0.703 #
16)	A 4,4'-DDD	6.259	0.000	2622780	0	0.342	N.D. #
23)	Chlordane-1	4.466f	5.029	1812949	1199150	6.739	15.444 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
Data File : PL052700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2019 17:57
Operator : SG\AJ
Sample : K4997-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-08-091919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:16:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

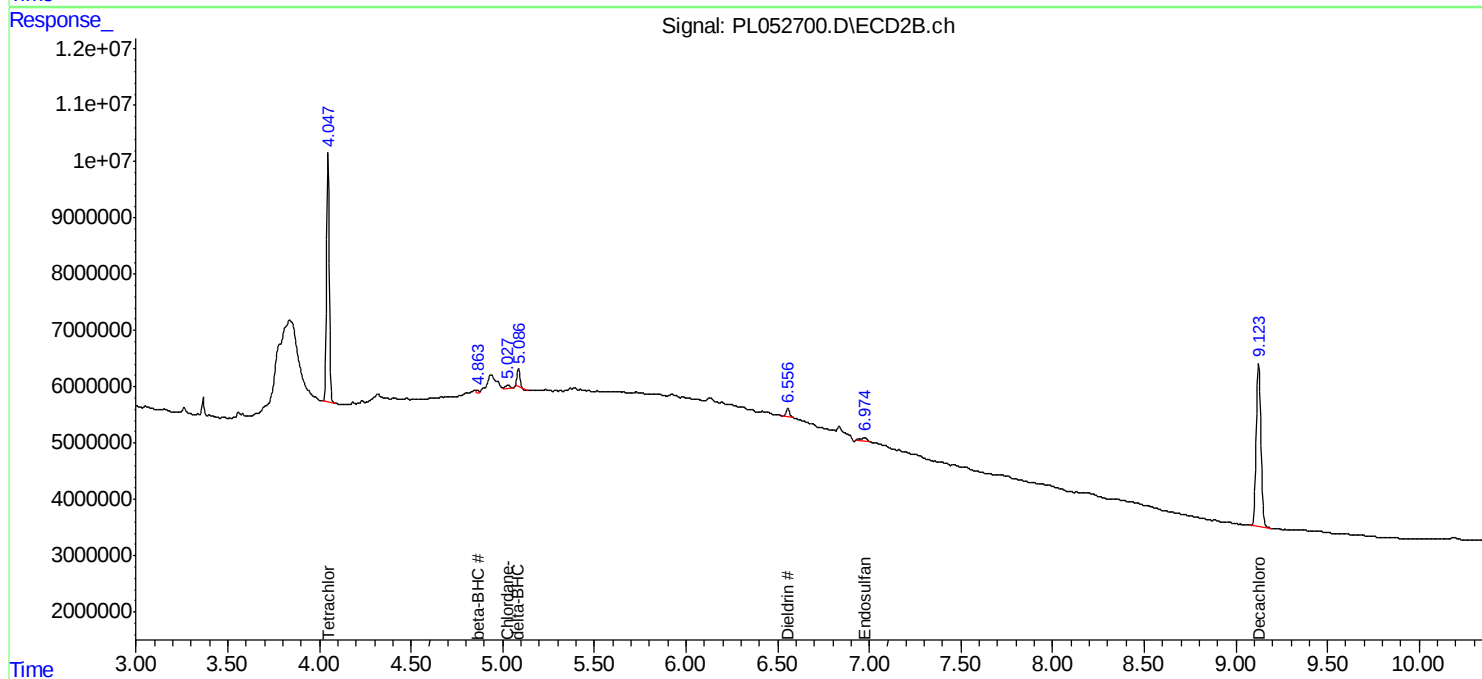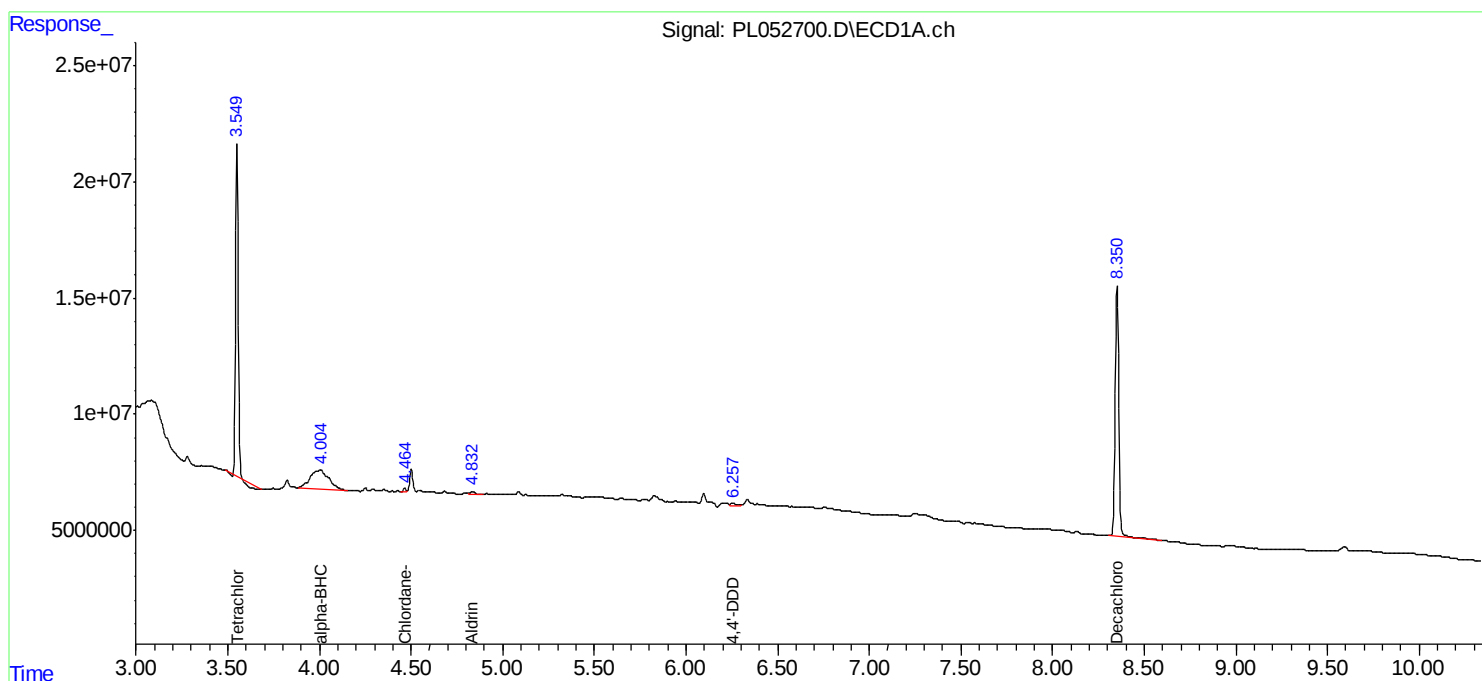


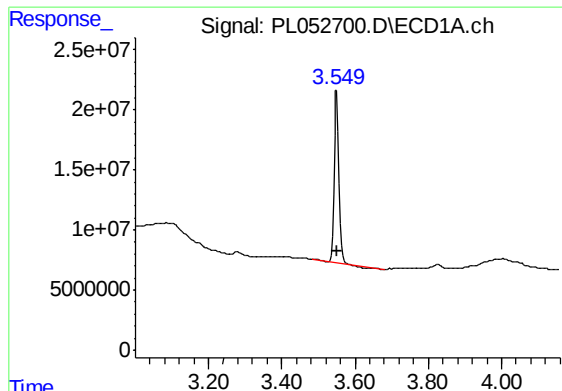

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 136494259
Conc: 17.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-08-091919

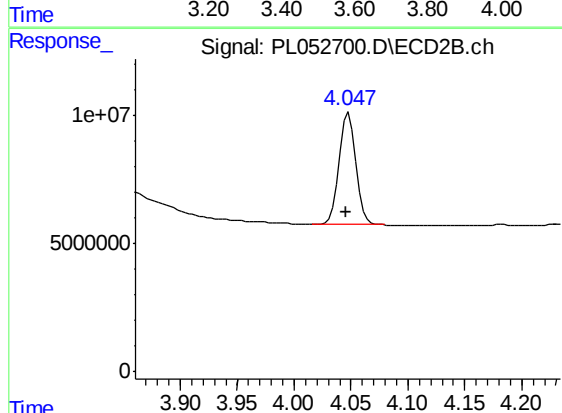


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.003 min
Response: 44305884
Conc: 20.33 ng/ml

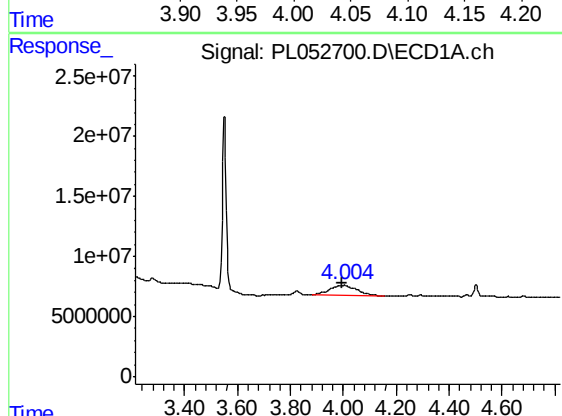


#2 alpha-BHC

R.T.: 4.005 min
Delta R.T.: 0.008 min
Response: 57006129
Conc: 4.74 ng/ml

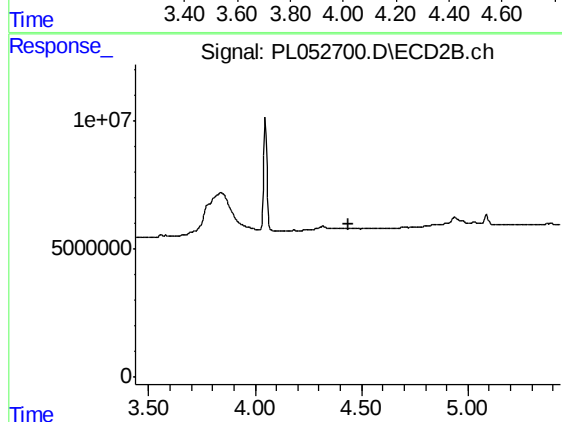

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.437 min
Response: 0
Conc: N.D.

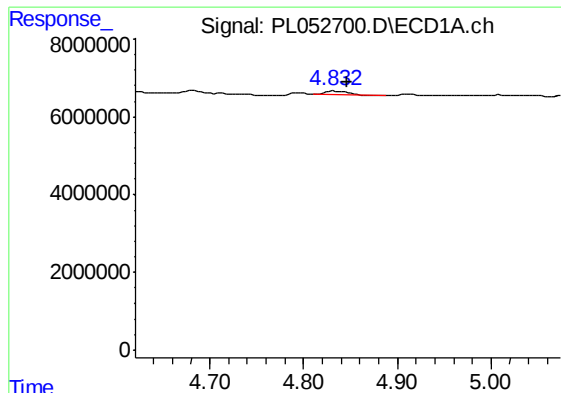

#5 Aldrin


R.T.: 4.833 min
Delta R.T.: -0.014 min
Response: 1915003
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-08-091919

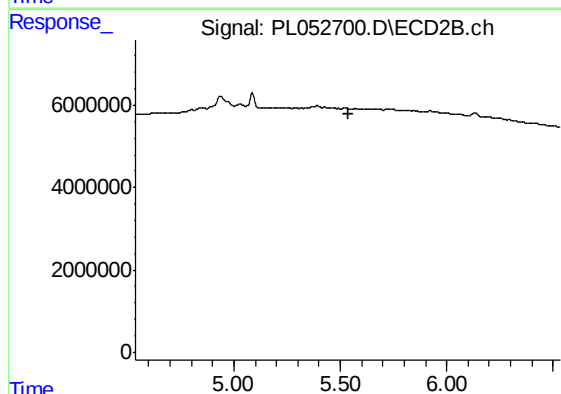


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.537 min
Response: 0
Conc: N.D.

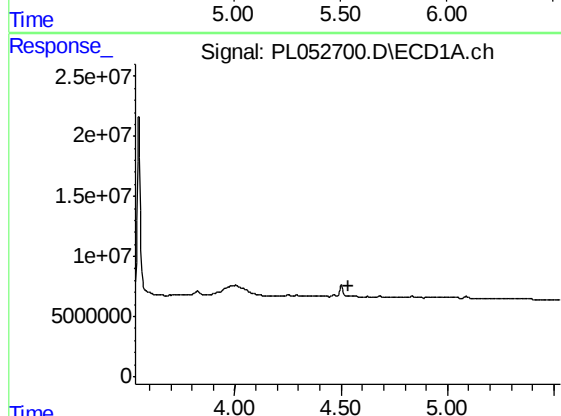


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.534 min
Response: 0
Conc: N.D.

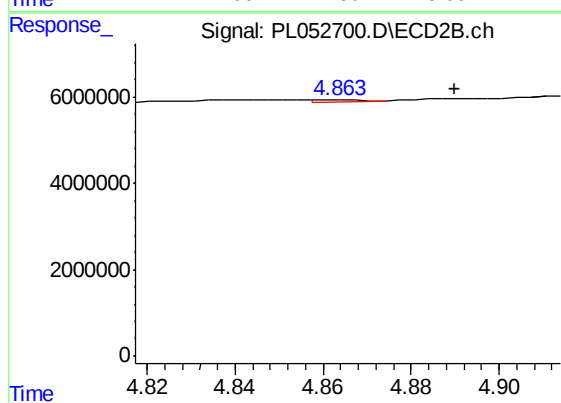

#6 beta-BHC


R.T.: 4.864 min
Delta R.T.: -0.026 min
Response: 382964
Conc: 0.29 ng/ml

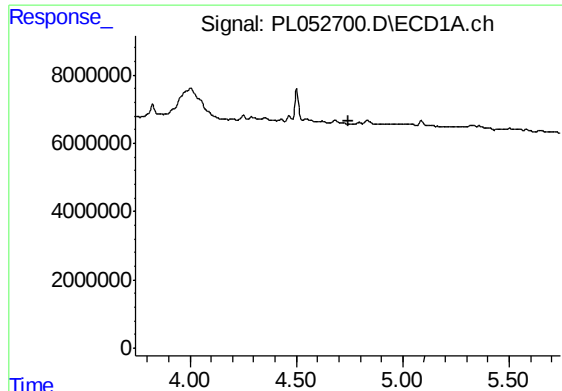

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-08-091919

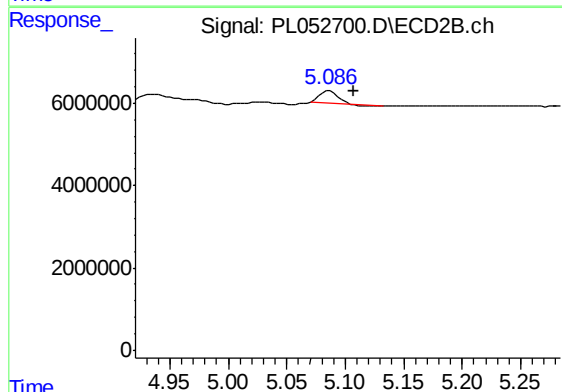


#7 delta-BHC

R.T.: 5.087 min
Delta R.T.: -0.021 min
Response: 3396376
Conc: 1.19 ng/ml

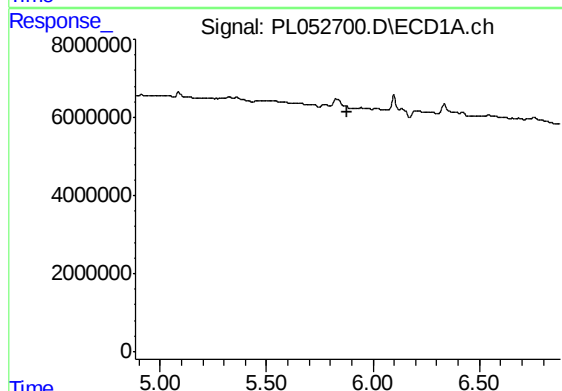


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.882 min
Response: 0
Conc: N.D.

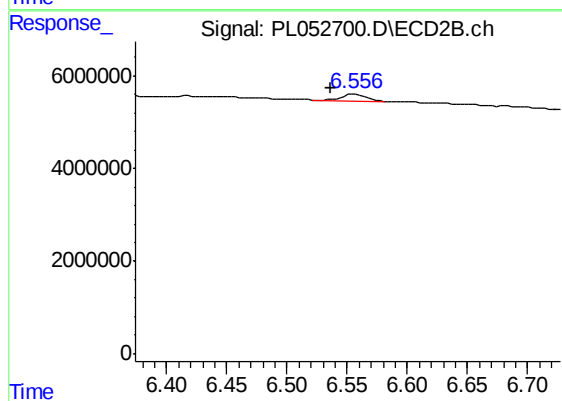

#13 Dieldrin


R.T.: 6.557 min
Delta R.T.: 0.021 min
Response: 1955422
Conc: 0.80 ng/ml

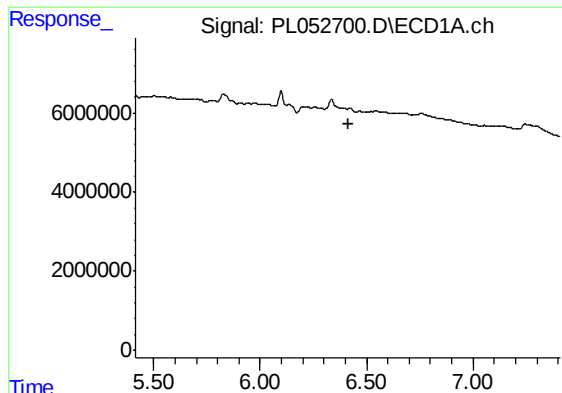

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-08-091919

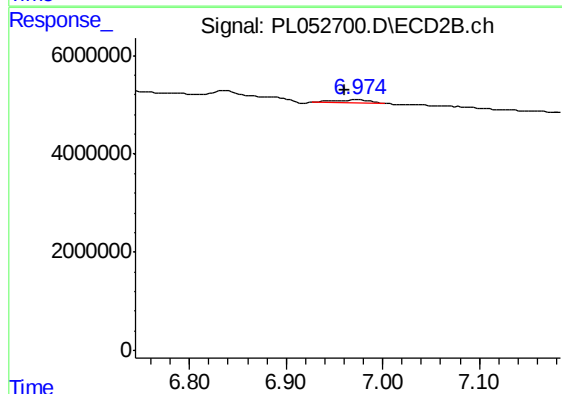


#15 Endosulfan II

R.T.: 6.975 min
Delta R.T.: 0.014 min
Response: 1569847
Conc: 0.70 ng/ml

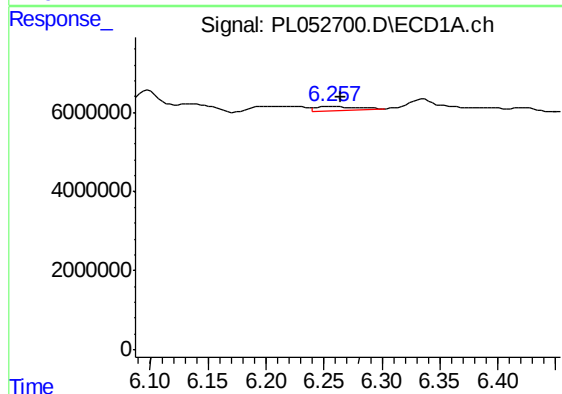


#16 4,4'-DDD

R.T.: 6.259 min
Delta R.T.: -0.006 min
Response: 2622780
Conc: 0.34 ng/ml

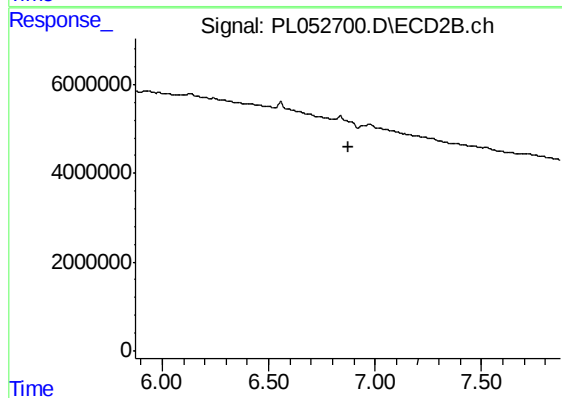

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.873 min
Response: 0
Conc: N.D.

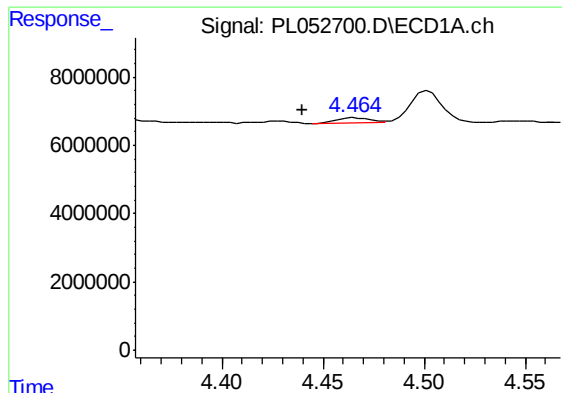

#23 Chlordane-1


R.T.: 4.466 min
Delta R.T.: 0.026 min
Response: 1812949
Conc: 6.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-08-091919

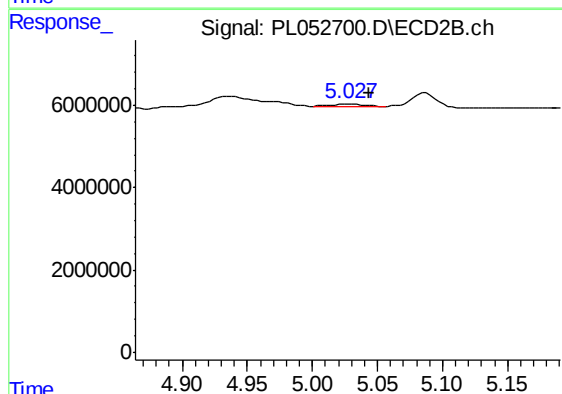


#23 Chlordane-1

R.T.: 5.029 min
Delta R.T.: -0.014 min
Response: 1199150
Conc: 15.44 ng/ml

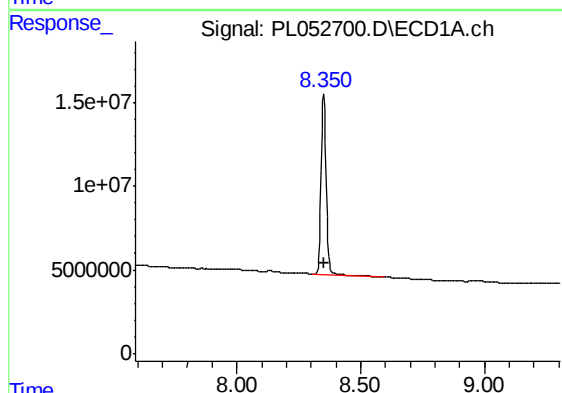

#28 Decachlorobiphenyl

R.T.: 8.351 min
Delta R.T.: -0.003 min
Response: 153301287
Conc: 17.53 ng/ml

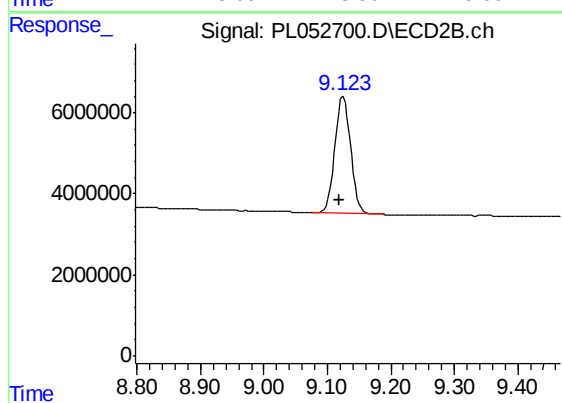

#28 Decachlorobiphenyl

R.T.: 9.125 min
Delta R.T.: 0.006 min
Response: 50021697
Conc: 20.89 ng/ml