

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
 Data File : PL052716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2019 21:42
 Operator : SG\AJ
 Sample : K5008-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:22:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	4.048	114.3E6	33089550	14.655	15.186
28)	SA Decachlor...	8.350	9.126	115.7E6	37564720	13.230	15.687
Target Compounds							
2)	A alpha-BHC	4.007	0.000	90572337	0	7.534	N.D. #
3)	MA gamma-BHC...	4.306f	0.000	4689772	0	0.414	N.D. #
7)	B delta-BHC	0.000	5.087f	0	869536	N.D.	0.304 #
9)	A Endosulfan I	5.641	0.000	968023	0	0.099	N.D. #
10)	B gamma-Chl...	0.000	6.166	0	493407	N.D.	0.194 #
17)	MA 4,4'-DDT	6.503	0.000	1778055	0	0.229	N.D. #
23)	Chlordane-1	0.000	5.027f	0	1217828	N.D.	15.684 #
25)	Chlordane-3	0.000	6.166	0	493407	N.D.	1.613 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
Data File : PL052716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2019 21:42
Operator : SG\AJ
Sample : K5008-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:22:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

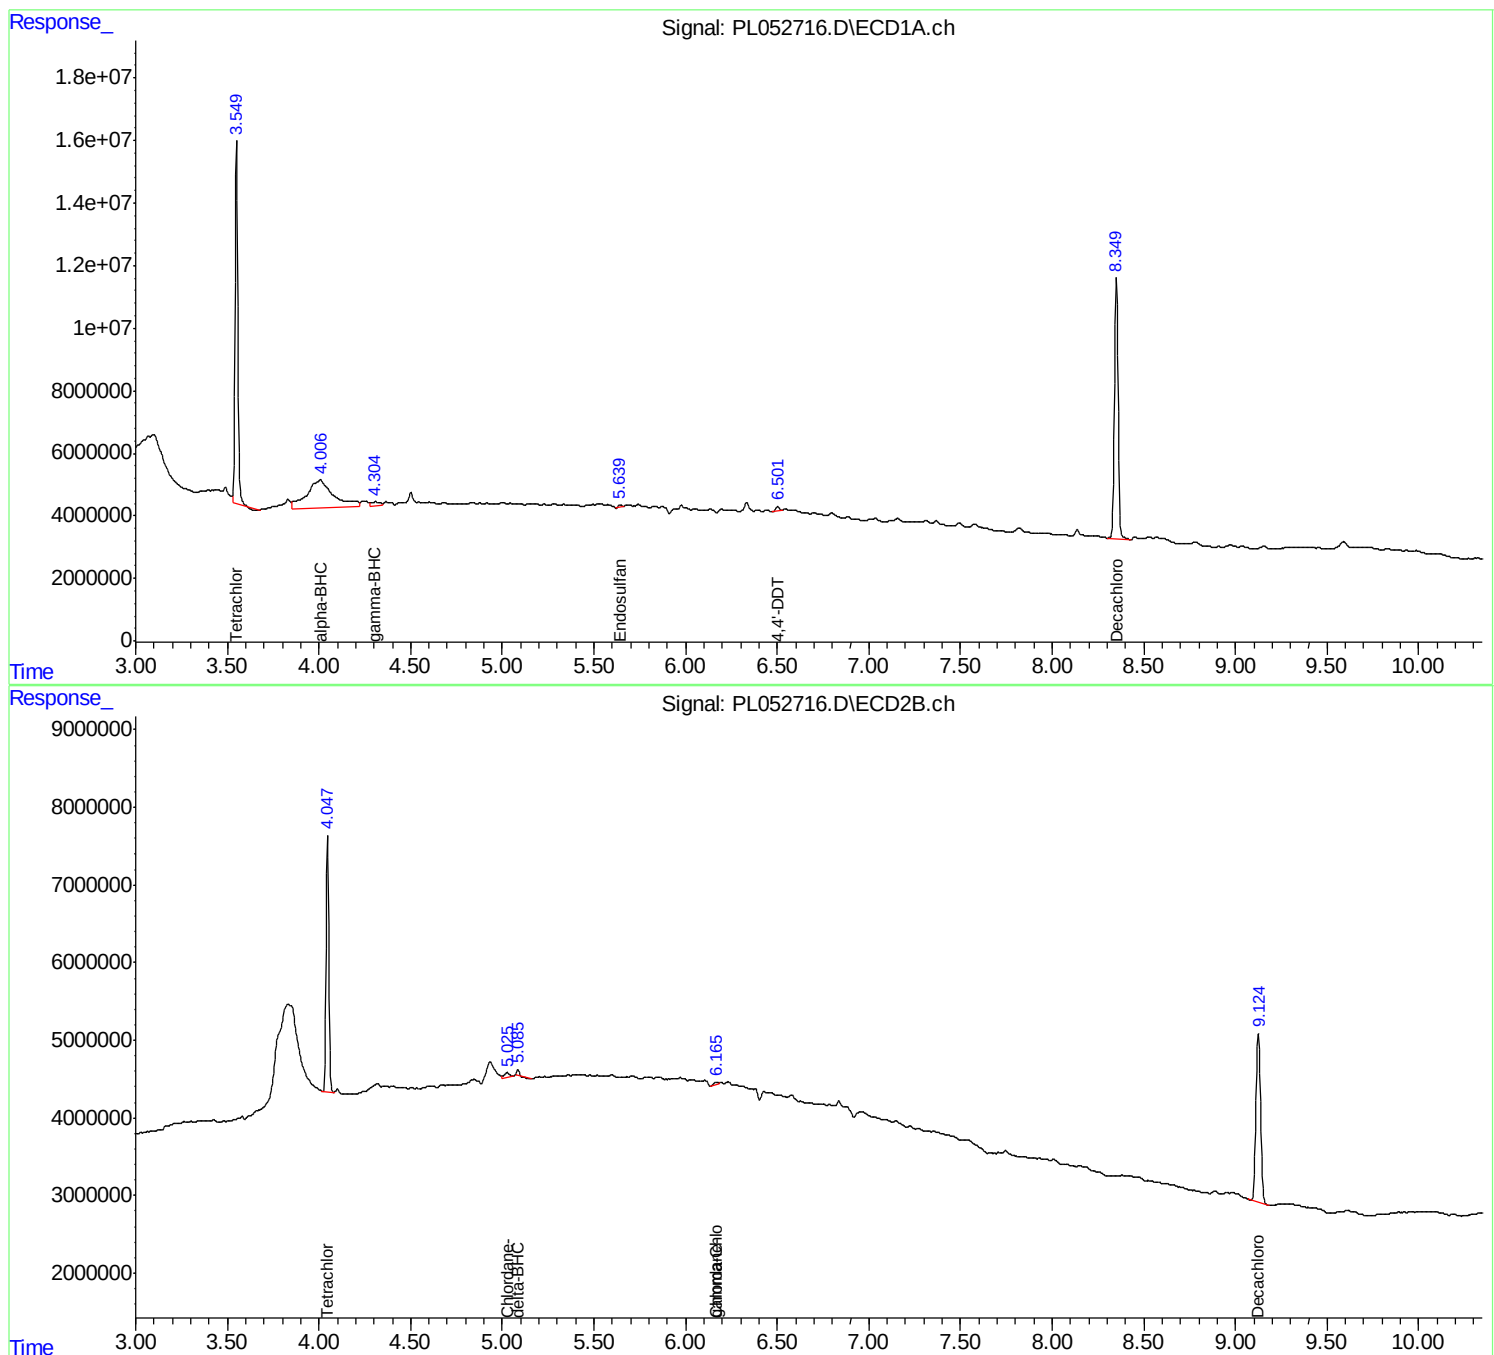


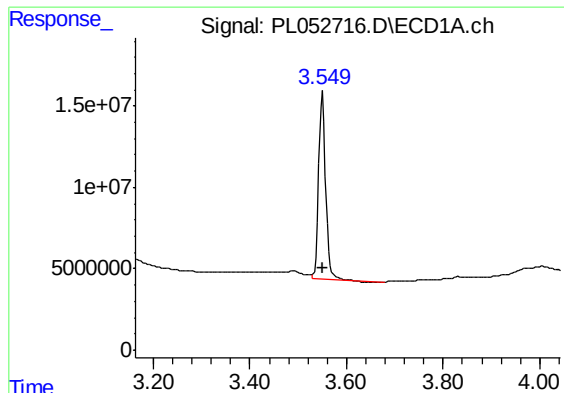

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 114279303
Conc: 14.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6

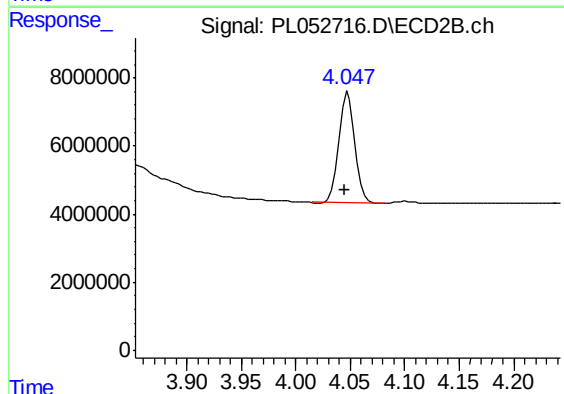


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.003 min
Response: 33089550
Conc: 15.19 ng/ml

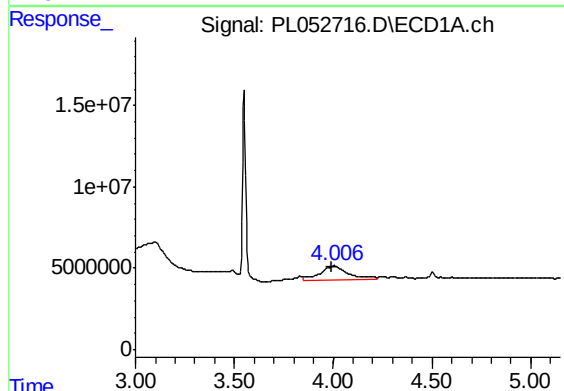


#2 alpha-BHC

R.T.: 4.007 min
Delta R.T.: 0.010 min
Response: 90572337
Conc: 7.53 ng/ml

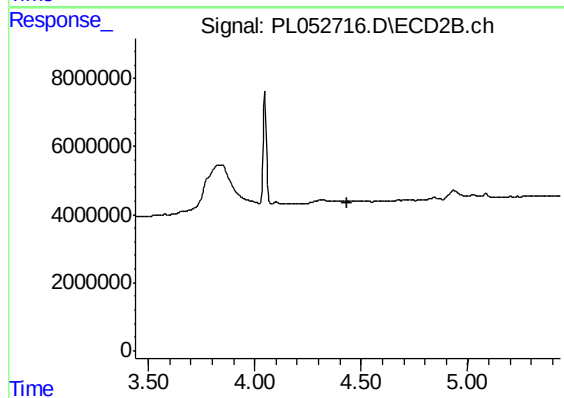

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.437 min
Response: 0
Conc: N.D.

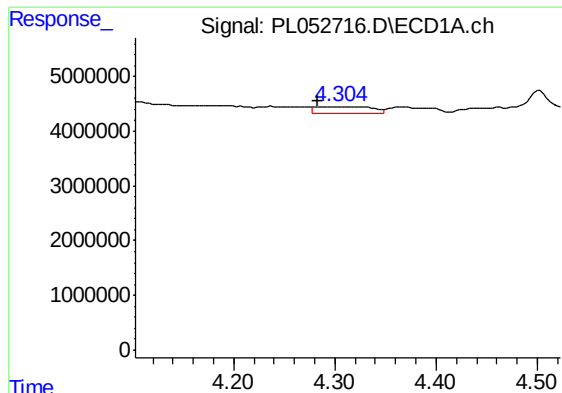

#3 gamma-BHC (Lindane)


R.T.: 4.306 min
Delta R.T.: 0.023 min
Response: 4689772
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6

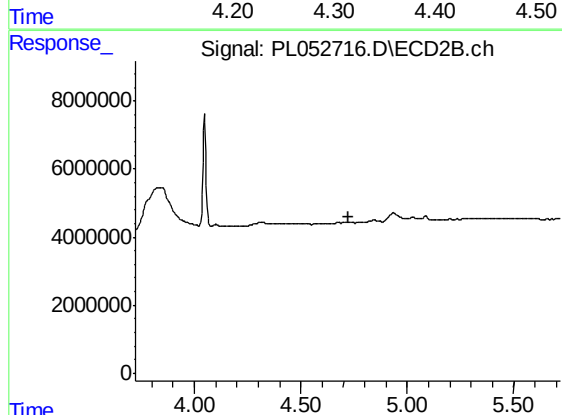


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.722 min
Response: 0
Conc: N.D.

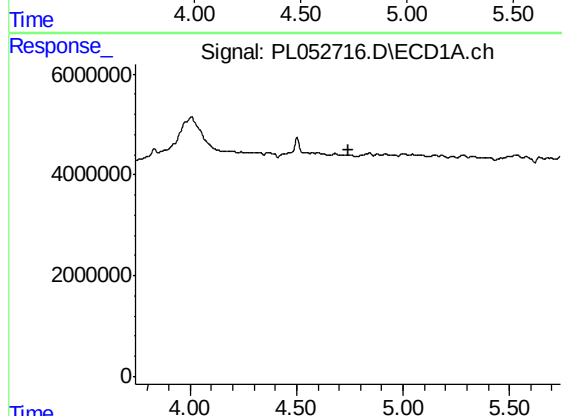


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.743 min
Response: 0
Conc: N.D.

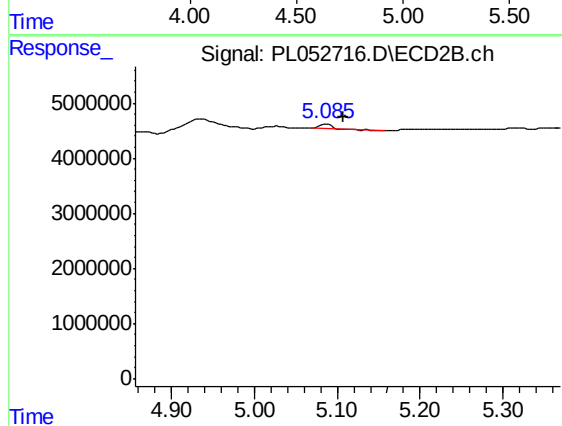

#7 delta-BHC


R.T.: 5.087 min
Delta R.T.: -0.021 min
Response: 869536
Conc: 0.30 ng/ml

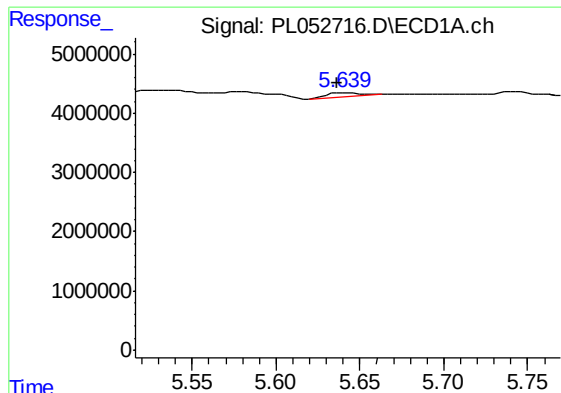

#9 Endosulfan I


R.T.: 5.641 min
Delta R.T.: 0.005 min
Response: 968023
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6

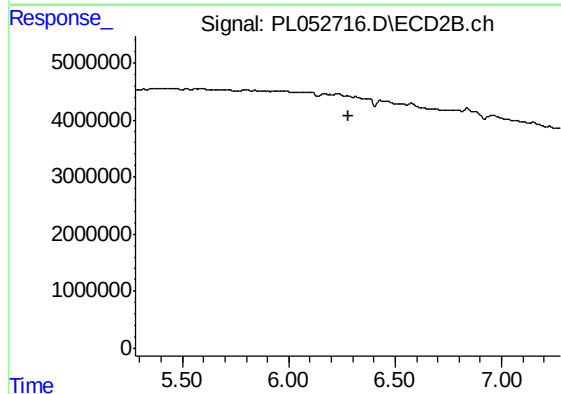


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

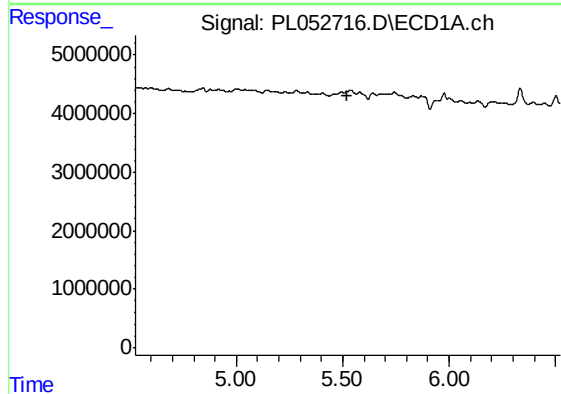


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.523 min
Response: 0
Conc: N.D.

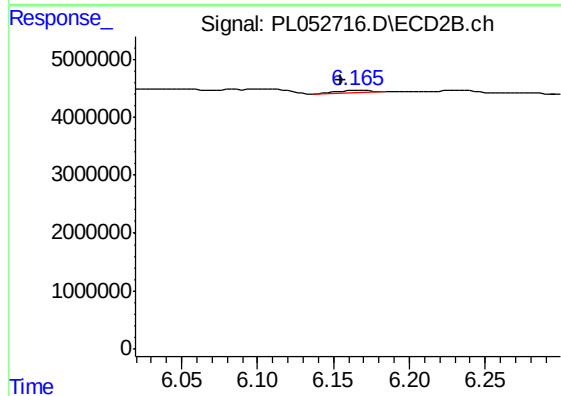

#10 gamma-Chlordane


R.T.: 6.166 min
Delta R.T.: 0.011 min
Response: 493407
Conc: 0.19 ng/ml

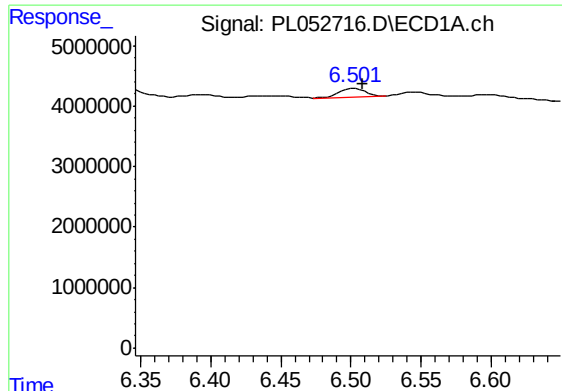

#17 4,4'-DDT


R.T.: 6.503 min
Delta R.T.: -0.006 min
Response: 1778055
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6

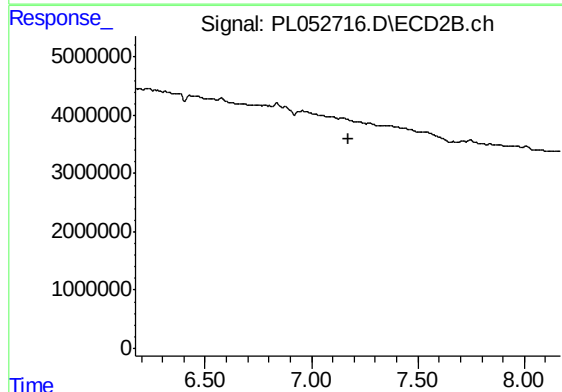


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

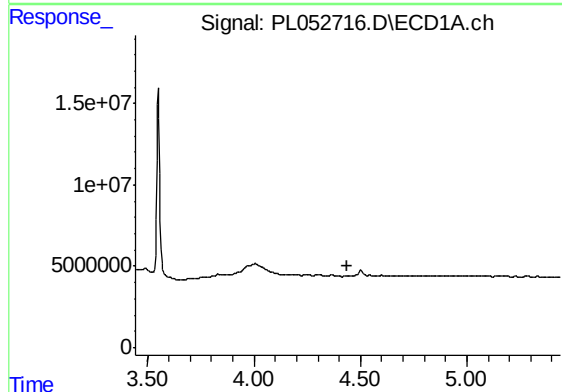


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.440 min
Response: 0
Conc: N.D.

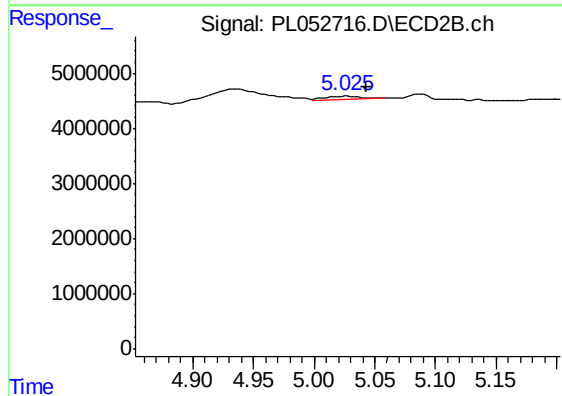

#23 Chlordane-1


R.T.: 5.027 min
Delta R.T.: -0.016 min
Response: 1217828
Conc: 15.68 ng/ml

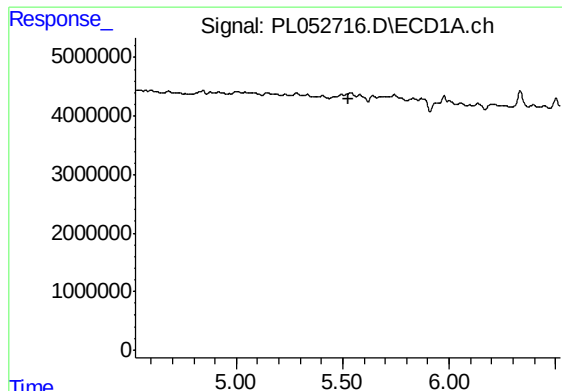

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.525 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-6

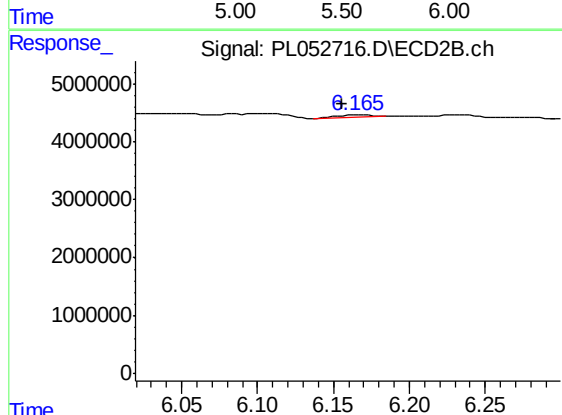


#25 Chlordane-3

R.T.: 6.166 min
Delta R.T.: 0.010 min
Response: 493407
Conc: 1.61 ng/ml

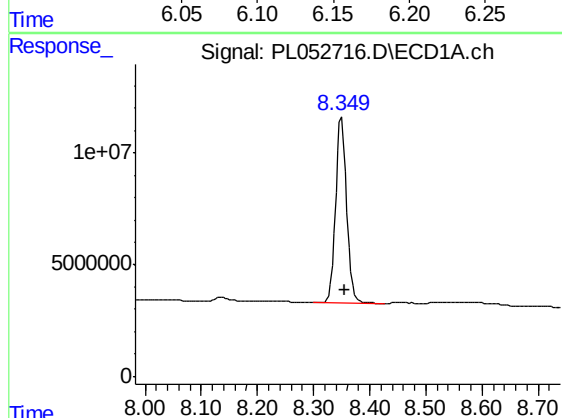

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.004 min
Response: 115694962
Conc: 13.23 ng/ml

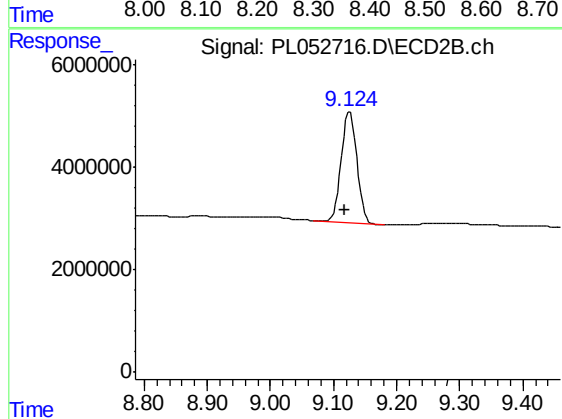

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.007 min
Response: 37564720
Conc: 15.69 ng/ml