

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
 Data File : PL052716.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2019 21:42
 Operator : SG\AJ
 Sample : K5008-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6

Manual Integrations
 APPROVED

Ankita
 9/26/2019 8:36:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:22:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	4.048	112.2E6	33089550	14.390m	15.186
28)	SA Decachlor...	8.350	9.126	115.7E6	37564720	13.230	15.687

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
Data File : PL052716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2019 21:42
Operator : SG\AJ
Sample : K5008-06
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-6


Manual Integrations
APPROVED

Ankita
9/26/2019 8:36:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:22:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

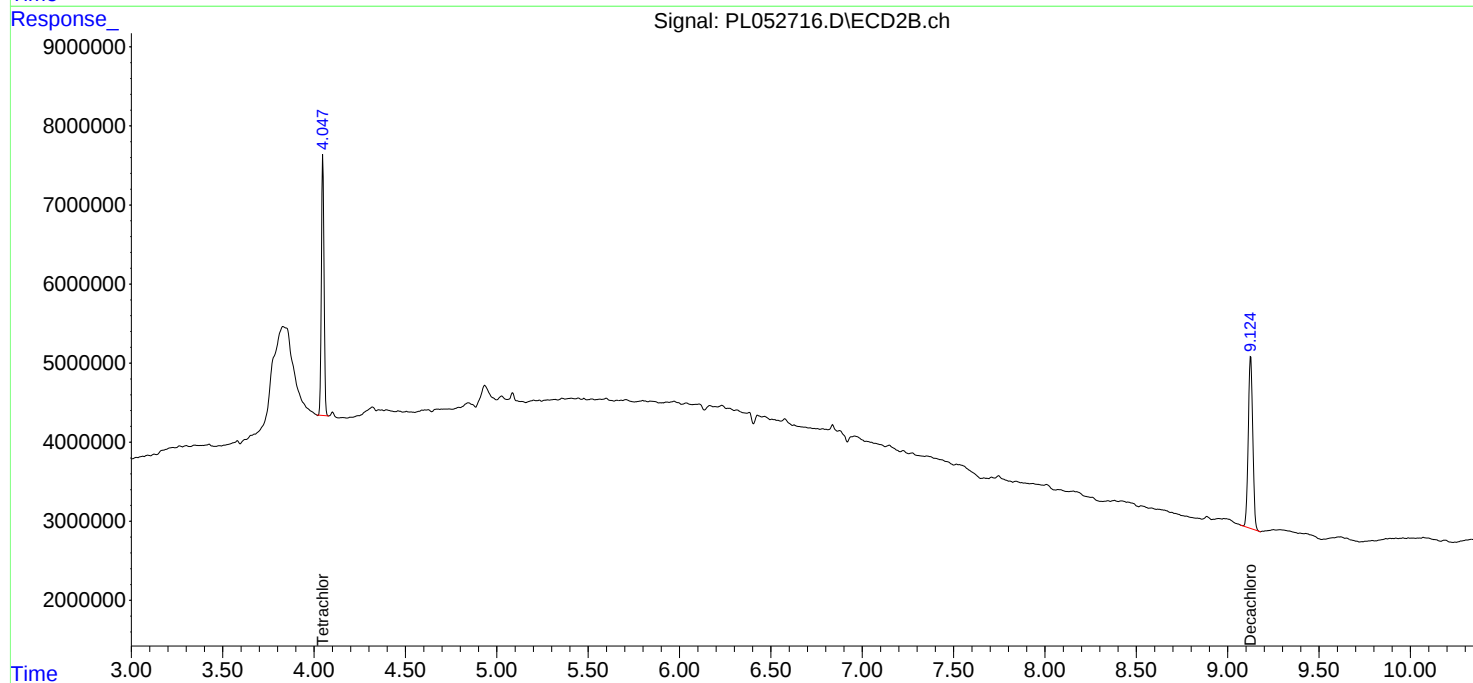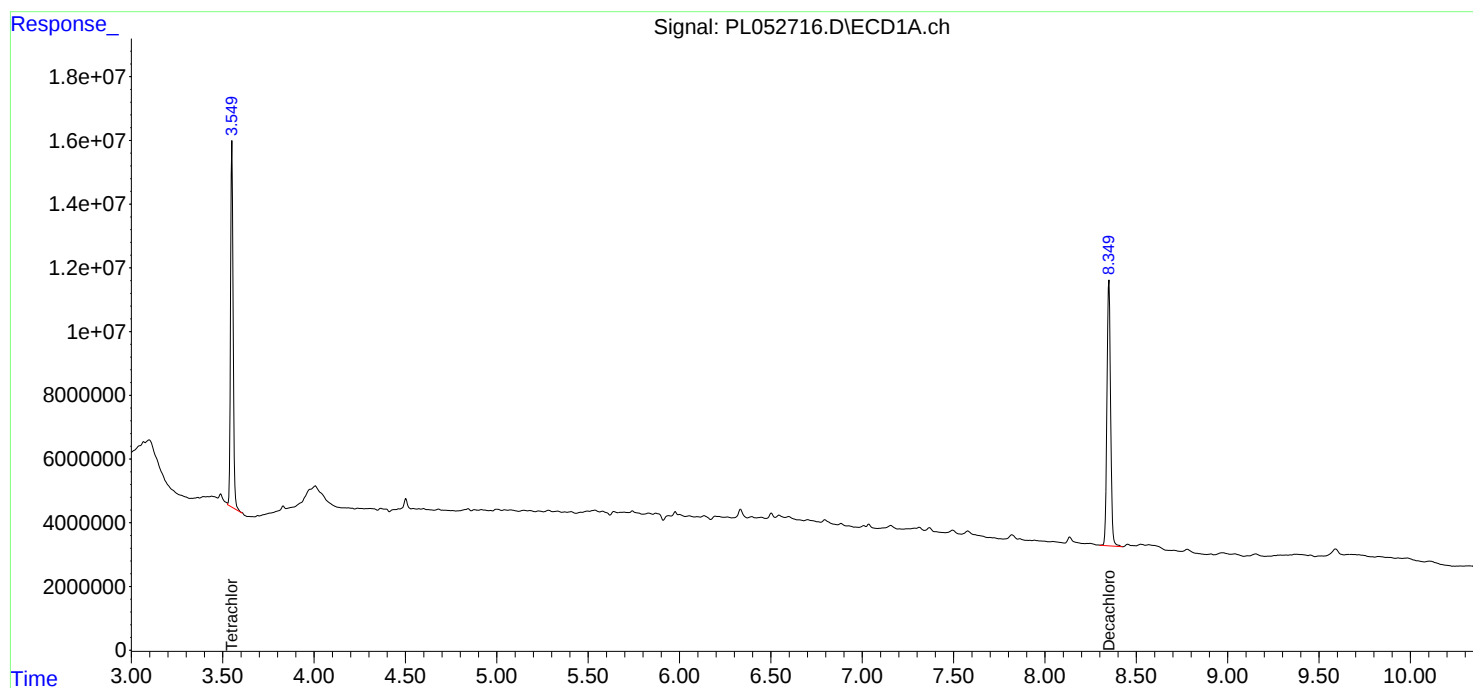

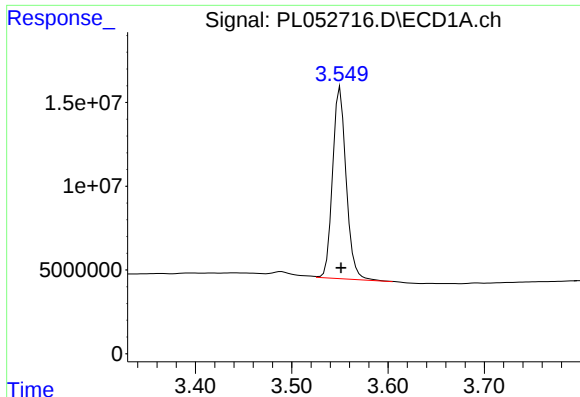


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.002 min
Response: 112206241
Conc: 14.39 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SB-6


Manual Integrations
APPROVED

Ankita
9/26/2019 8:36:21 AM

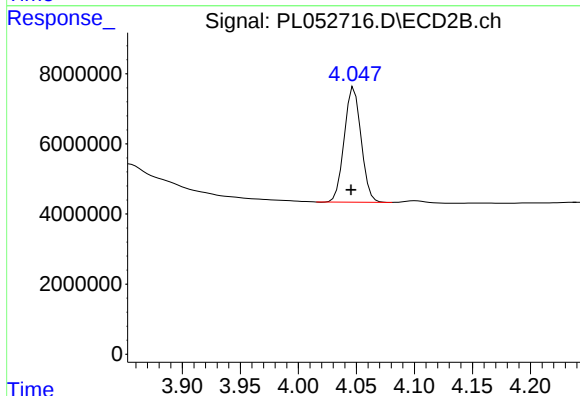


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.003 min
Response: 33089550
Conc: 15.19 ng/ml

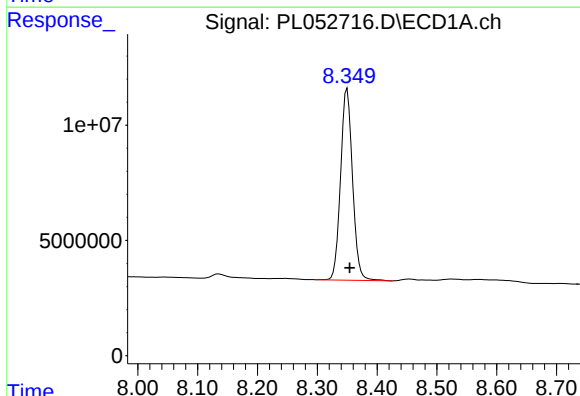

#28 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.004 min
Response: 115694962
Conc: 13.23 ng/ml

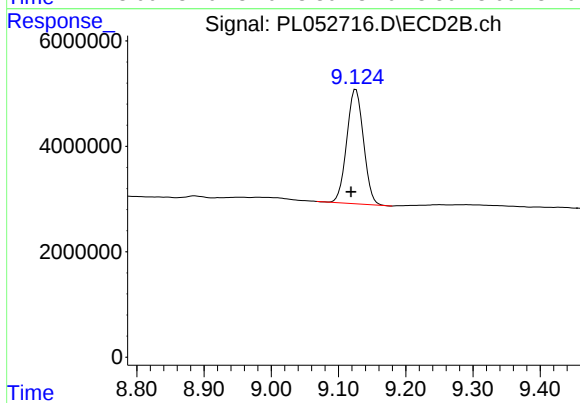

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.007 min
Response: 37564720
Conc: 15.69 ng/ml