

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
 Data File : PL052724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2019 23:35
 Operator : SG\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Ankita
 9/26/2019 8:37:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:25:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 11:25:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.551	4.048	404.0E6	115.1E6	51.804	52.805
28)	SA Decachlor...	8.348	9.126	374.0E6	122.4E6	42.766m	51.105
Target Compounds							
2)	A alpha-BHC	3.994	4.439	648.8E6	167.9E6	53.970m	54.928
3)	MA gamma-BHC...	4.281	4.724	585.6E6	157.7E6	51.755m	54.605
4)	MA Heptachlor	4.591	5.234	578.4E6	162.4E6	51.191m	55.324
5)	MB Aldrin	4.845	5.540	574.0E6	151.7E6	53.156	57.260
6)	B beta-BHC	4.532	4.893	255.9E6	72906050	52.299	54.666
7)	B delta-BHC	4.741	5.110	603.0E6	157.0E6	53.357	54.833
8)	B Heptachlo...	5.291	5.926	541.1E6	154.1E6	52.956	58.776
9)	A Endosulfan I	5.633	6.283	465.3E6	130.0E6	47.696m	55.779
10)	B gamma-Chl...	5.519	6.159	533.4E6	142.5E6	50.222m	56.018
11)	B alpha-Chl...	5.580	6.232	530.8E6	139.5E6	51.350	55.830
12)	B 4,4'-DDE	5.742	6.388	395.7E6	138.3E6	42.402m	56.714 #
13)	MA Dieldrin	5.878	6.540	510.3E6	137.5E6	49.230m	56.301
14)	MA Endrin	6.137	6.757	397.1E6	102.2E6	48.026m	52.794
15)	B Endosulfa...	6.409	6.965	437.8E6	120.2E6	45.136m	53.841
16)	A 4,4'-DDD	6.260	6.877	385.3E6	106.9E6	50.301m	58.046
17)	MA 4,4'-DDT	6.505	7.176	371.4E6	97901984	47.852	53.525
18)	B Endrin al...	6.578	7.089	370.4E6	103.4E6	47.902m	55.764
19)	B Endosulfa...	6.792	7.311	386.2E6	109.4E6	46.557m	53.271
20)	A Methoxychlor	7.050	7.633	177.3E6	50348498	43.849m	49.687
21)	B Endrin ke...	7.288	7.783	506.7E6	119.5E6	48.802	53.804
22)	Mirex	7.484	8.239	335.3E6	91275854	43.844	53.333

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092419\
Data File : PL052724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2019 23:35
Operator : SG\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:25:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL091719.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 11:25:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

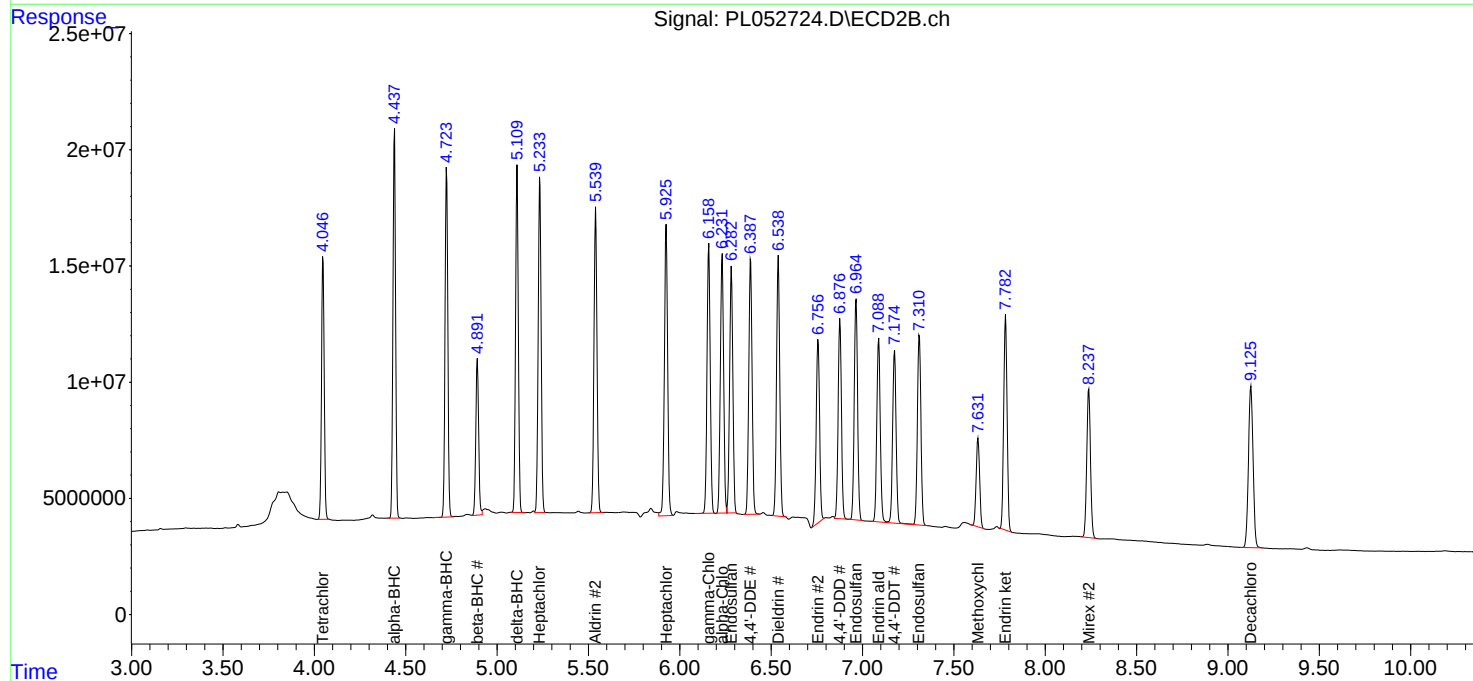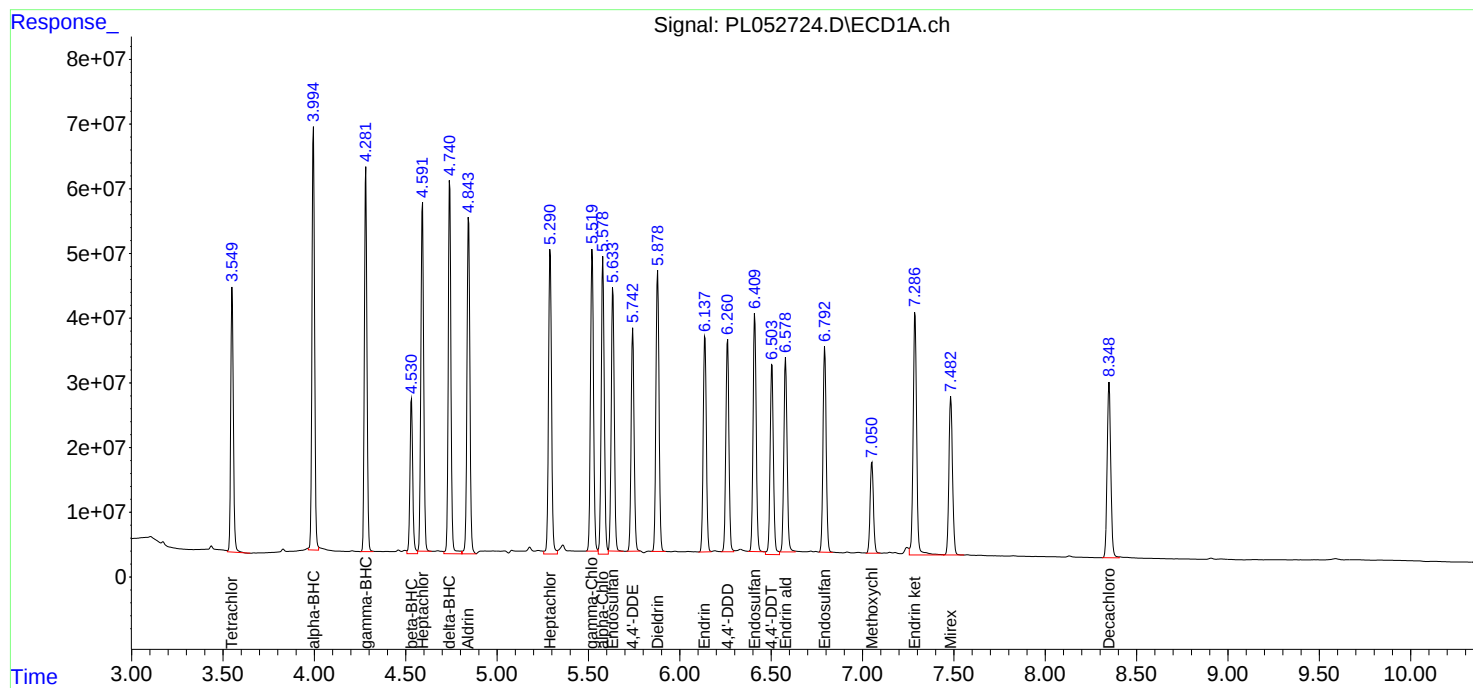

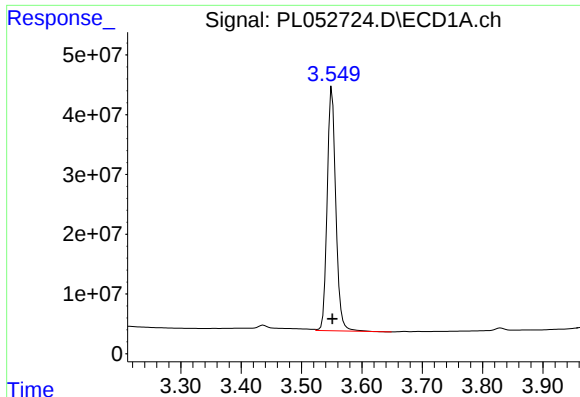


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: 0.000 min
Response: 403950559
Conc: 51.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

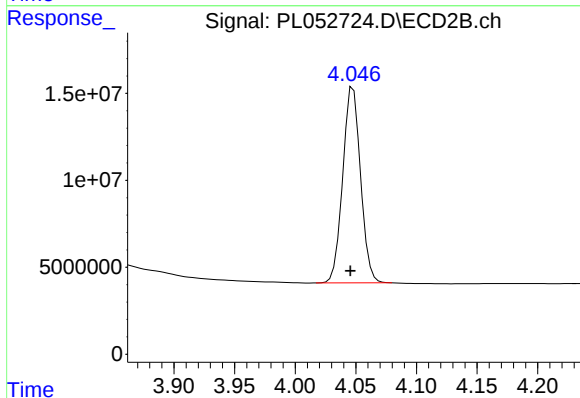


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: 0.002 min
Response: 115058083
Conc: 52.80 ng/ml

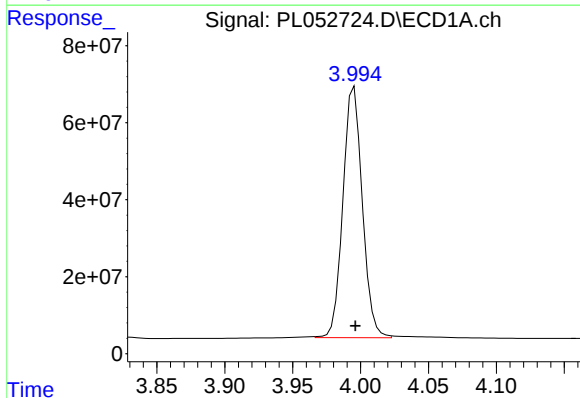


#2 alpha-BHC

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 648847777
Conc: 53.97 ng/ml m

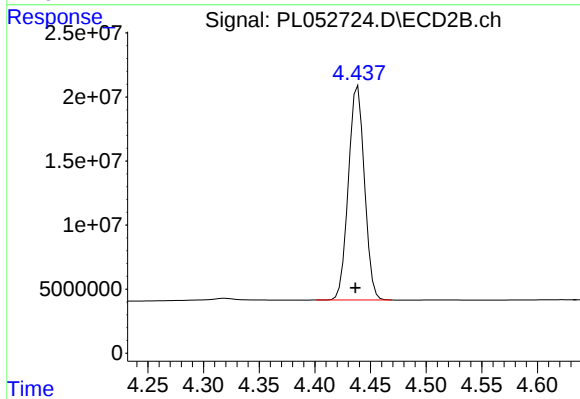

#2 alpha-BHC

R.T.: 4.439 min
Delta R.T.: 0.002 min
Response: 167892493
Conc: 54.93 ng/ml

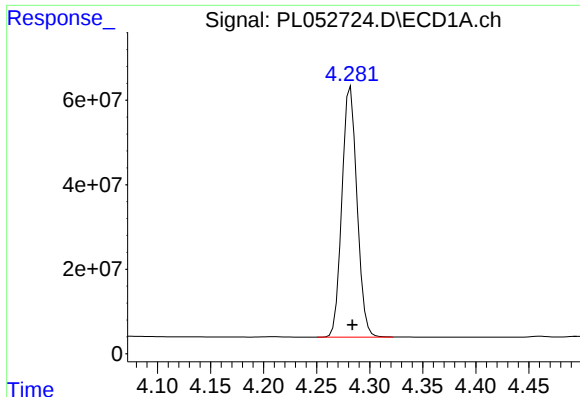


#3 gamma-BHC (Lindane)

R.T.: 4.281 min
Delta R.T.: -0.003 min
Response: 585575274
Conc: 51.76 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

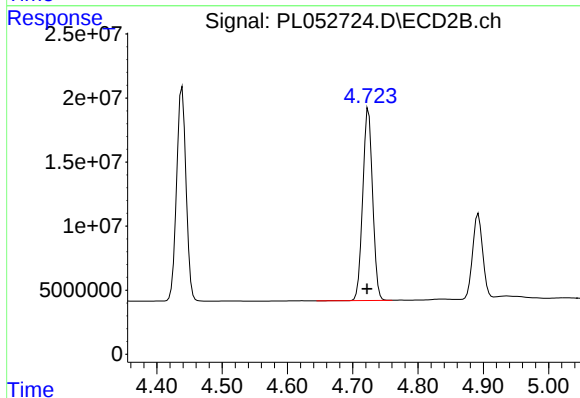


#3 gamma-BHC (Lindane)

R.T.: 4.724 min
Delta R.T.: 0.002 min
Response: 157670917
Conc: 54.60 ng/ml

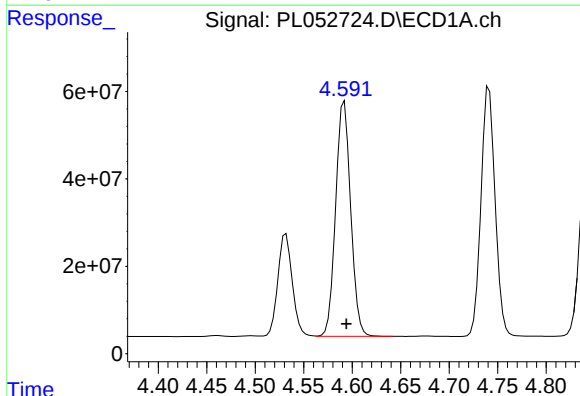


#4 Heptachlor

R.T.: 4.591 min
Delta R.T.: -0.004 min
Response: 578411449
Conc: 51.19 ng/ml m

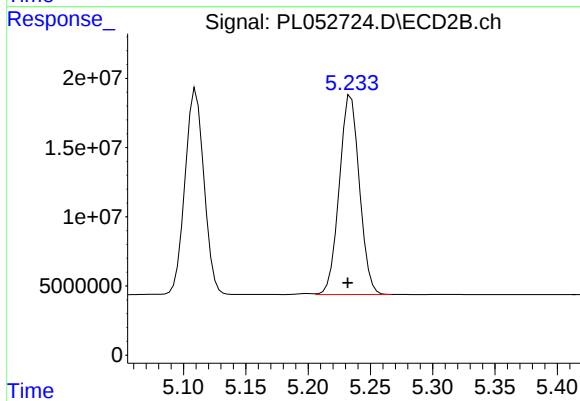

#4 Heptachlor

R.T.: 5.234 min
Delta R.T.: 0.003 min
Response: 162365776
Conc: 55.32 ng/ml

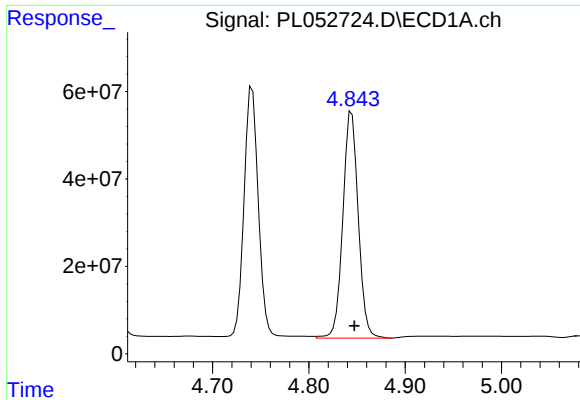


#5 Aldrin

R.T.: 4.845 min
Delta R.T.: -0.003 min
Response: 574001875
Conc: 53.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

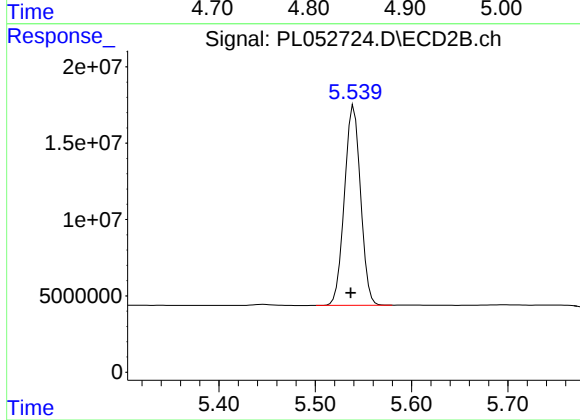


#5 Aldrin

R.T.: 5.540 min
Delta R.T.: 0.003 min
Response: 151667062
Conc: 57.26 ng/ml

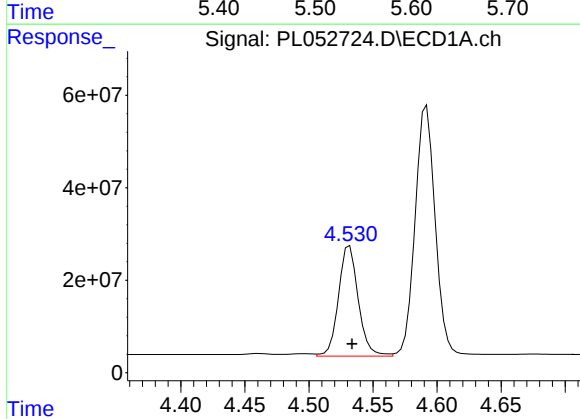


#6 beta-BHC

R.T.: 4.532 min
Delta R.T.: -0.002 min
Response: 255942806
Conc: 52.30 ng/ml

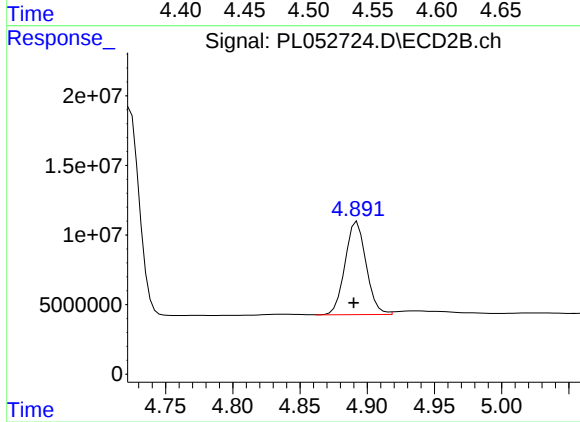

#6 beta-BHC

R.T.: 4.893 min
Delta R.T.: 0.003 min
Response: 72906050
Conc: 54.67 ng/ml

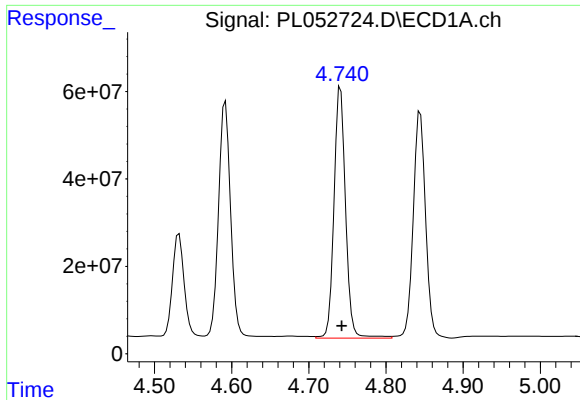


#7 delta-BHC

R.T.: 4.741 min
Delta R.T.: -0.002 min
Response: 602957623
Conc: 53.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

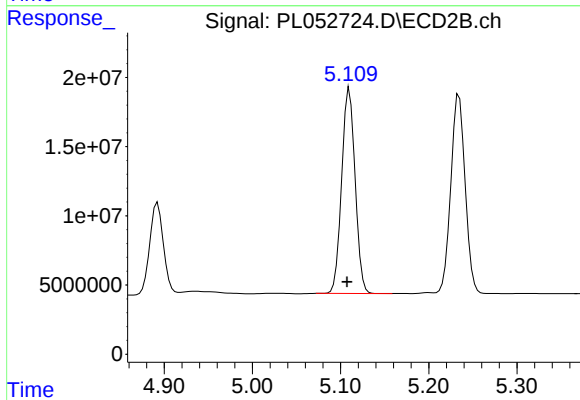


#7 delta-BHC

R.T.: 5.110 min
Delta R.T.: 0.003 min
Response: 156979086
Conc: 54.83 ng/ml

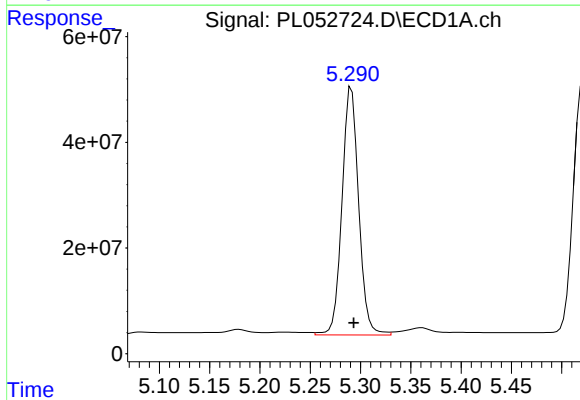


#8 Heptachlor epoxide

R.T.: 5.291 min
Delta R.T.: -0.002 min
Response: 541065809
Conc: 52.96 ng/ml

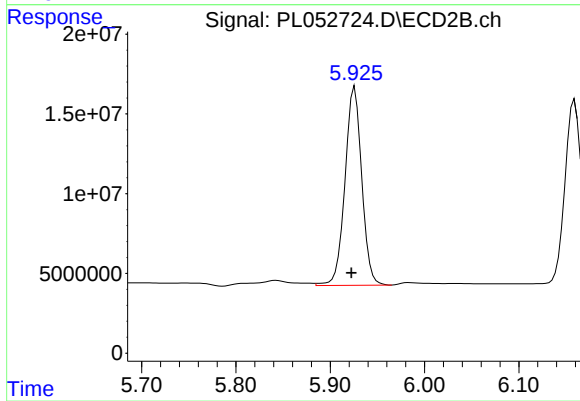

#8 Heptachlor epoxide

R.T.: 5.926 min
Delta R.T.: 0.004 min
Response: 154137868
Conc: 58.78 ng/ml

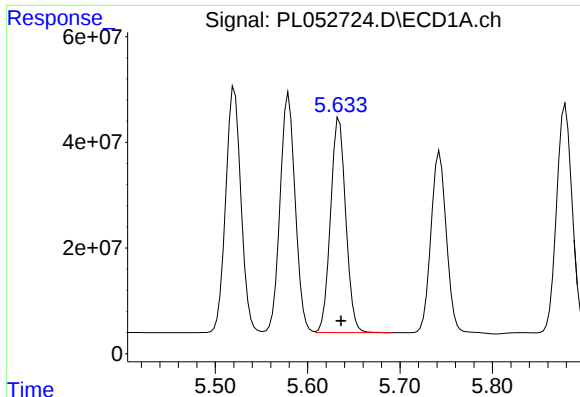


#9 Endosulfan I

R.T.: 5.633 min
Delta R.T.: -0.003 min
Response: 465308917
Conc: 47.70 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

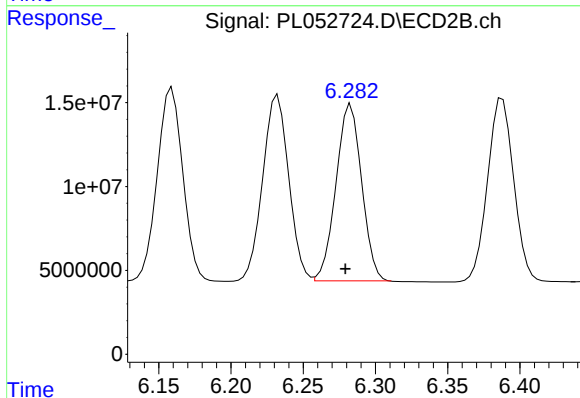


#9 Endosulfan I

R.T.: 6.283 min
Delta R.T.: 0.004 min
Response: 130033139
Conc: 55.78 ng/ml

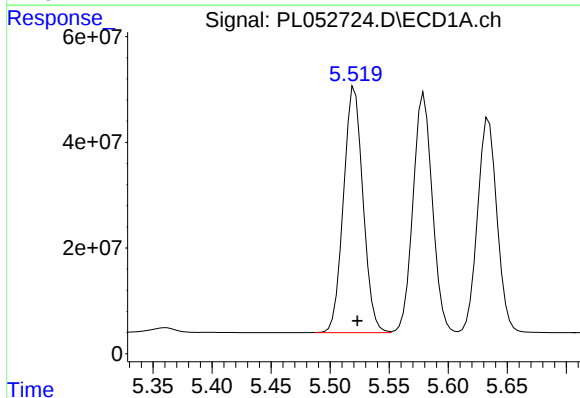


#10 gamma-Chlordane

R.T.: 5.519 min
Delta R.T.: -0.004 min
Response: 533364599
Conc: 50.22 ng/ml m

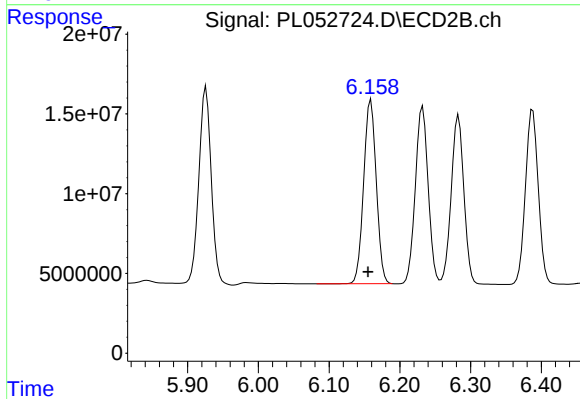

#10 gamma-Chlordane

R.T.: 6.159 min
Delta R.T.: 0.004 min
Response: 142509184
Conc: 56.02 ng/ml

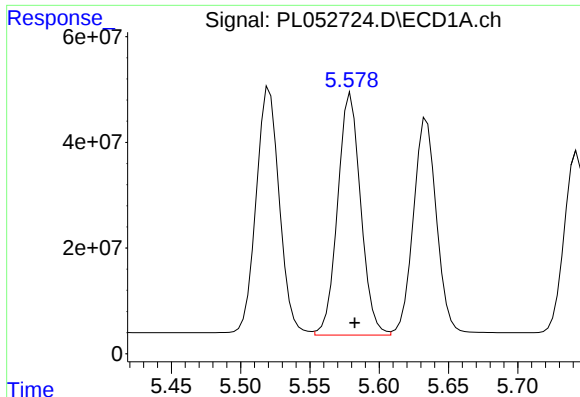


#11 alpha-Chlordane

R.T.: 5.580 min
Delta R.T.: -0.003 min
Response: 530821005
Conc: 51.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

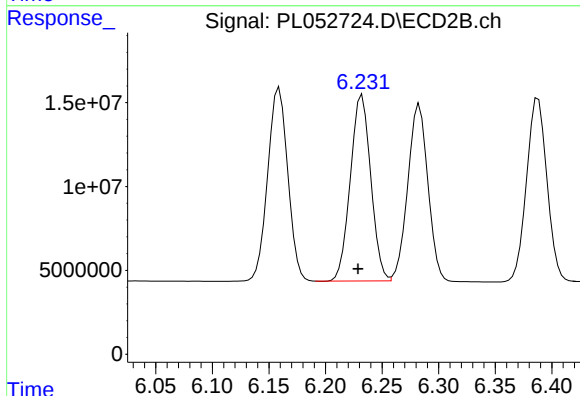


#11 alpha-Chlordane

R.T.: 6.232 min
Delta R.T.: 0.004 min
Response: 139465691
Conc: 55.83 ng/ml

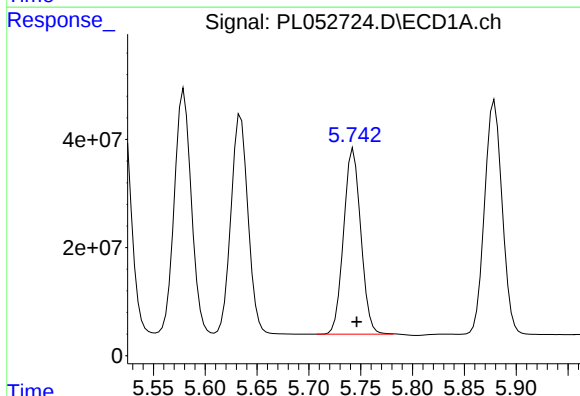


#12 4,4'-DDE

R.T.: 5.742 min
Delta R.T.: -0.005 min
Response: 395659844
Conc: 42.40 ng/ml m

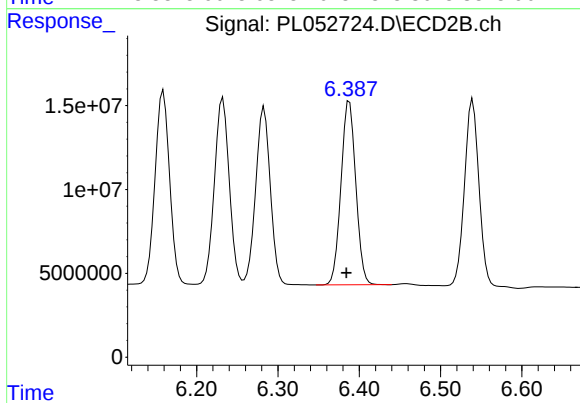

#12 4,4'-DDE

R.T.: 6.388 min
Delta R.T.: 0.004 min
Response: 138269387
Conc: 56.71 ng/ml

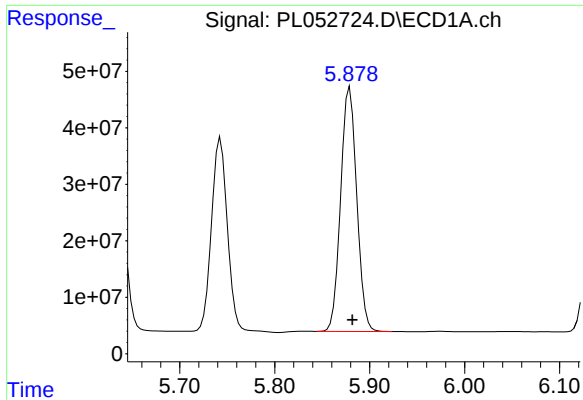


#13 Dieldrin

R.T.: 5.878 min
Delta R.T.: -0.004 min
Response: 510324551
Conc: 49.23 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

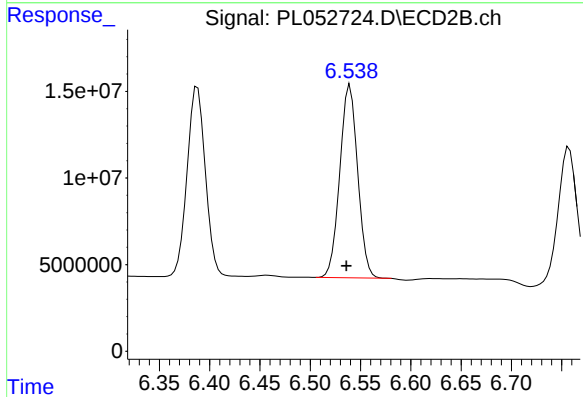


#13 Dieldrin

R.T.: 6.540 min
Delta R.T.: 0.003 min
Response: 137492818
Conc: 56.30 ng/ml

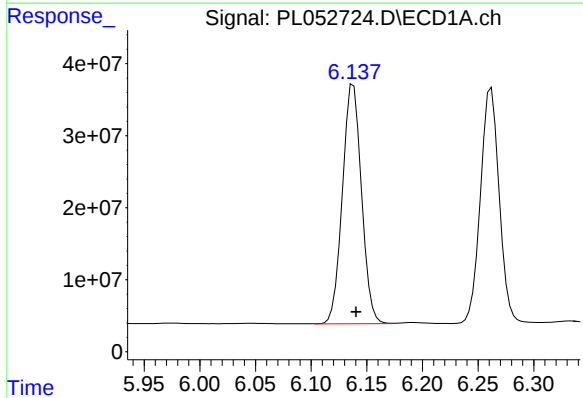


#14 Endrin

R.T.: 6.137 min
Delta R.T.: -0.004 min
Response: 397067382
Conc: 48.03 ng/ml m

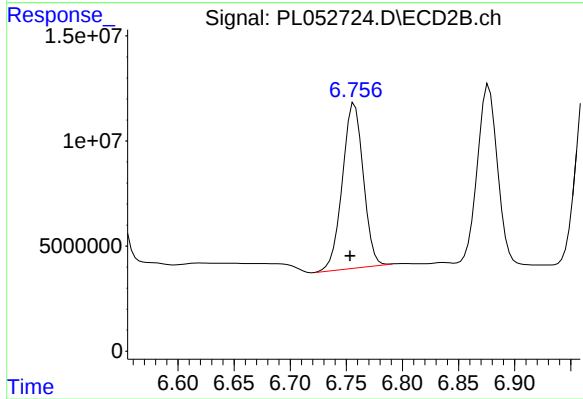

#14 Endrin

R.T.: 6.757 min
Delta R.T.: 0.004 min
Response: 102187243
Conc: 52.79 ng/ml

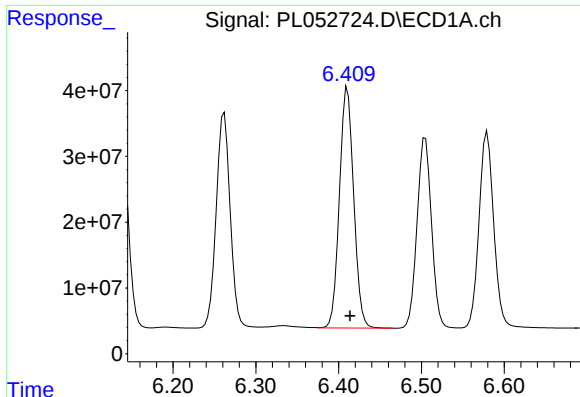


#15 Endosulfan II

R.T.: 6.409 min
Delta R.T.: -0.005 min
Response: 437811309
Conc: 45.14 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

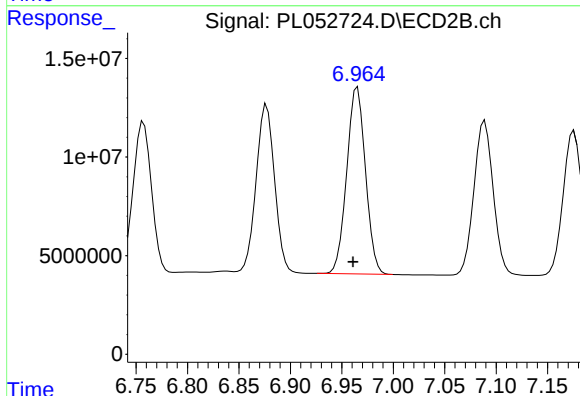


#15 Endosulfan II

R.T.: 6.965 min
Delta R.T.: 0.004 min
Response: 120182937
Conc: 53.84 ng/ml

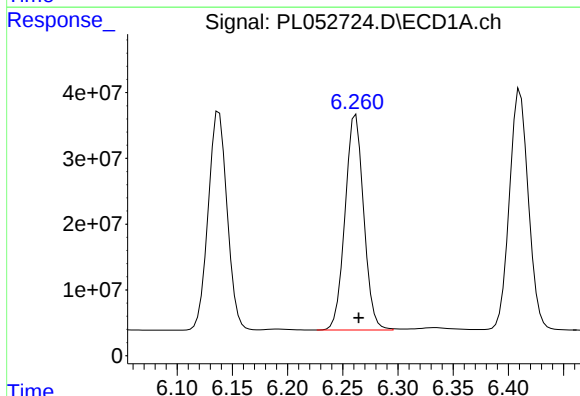


#16 4,4'-DDD

R.T.: 6.260 min
Delta R.T.: -0.004 min
Response: 385252198
Conc: 50.30 ng/ml m

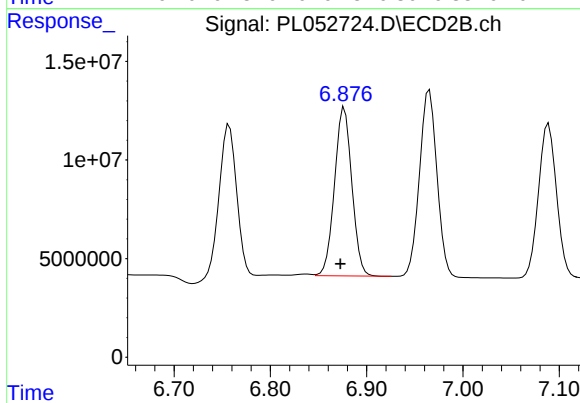

#16 4,4'-DDD

R.T.: 6.877 min
Delta R.T.: 0.004 min
Response: 106908601
Conc: 58.05 ng/ml

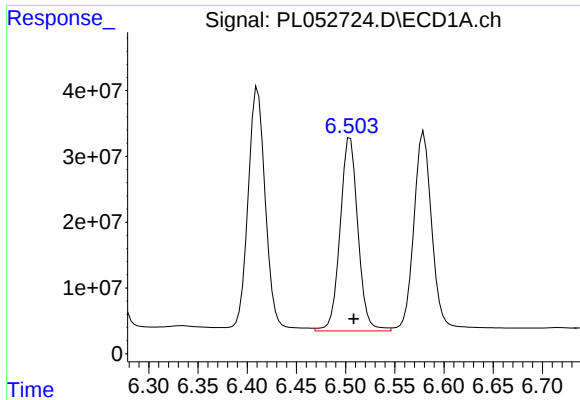


#17 4,4'-DDT

R.T.: 6.505 min
Delta R.T.: -0.004 min
Response: 371394694
Conc: 47.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

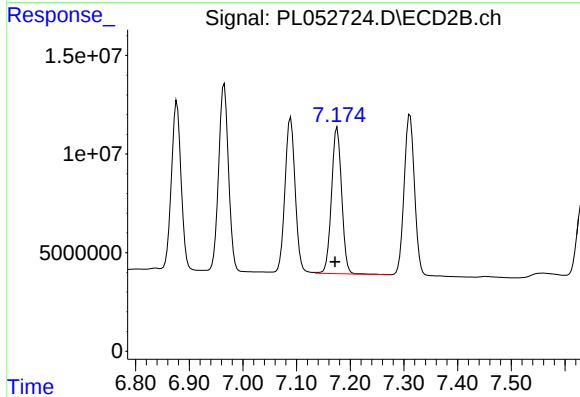


#17 4,4'-DDT

R.T.: 7.176 min
Delta R.T.: 0.004 min
Response: 97901984
Conc: 53.53 ng/ml

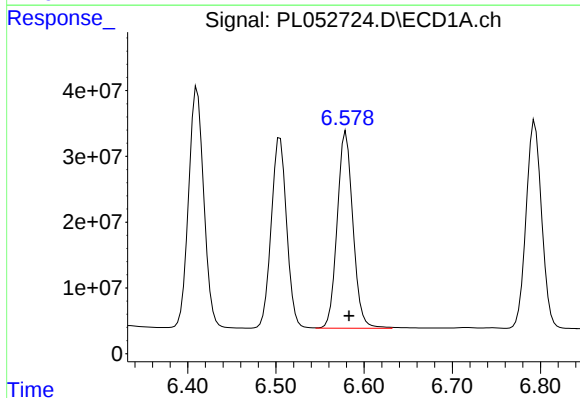


#18 Endrin aldehyde

R.T.: 6.578 min
Delta R.T.: -0.005 min
Response: 370363639
Conc: 47.90 ng/ml m

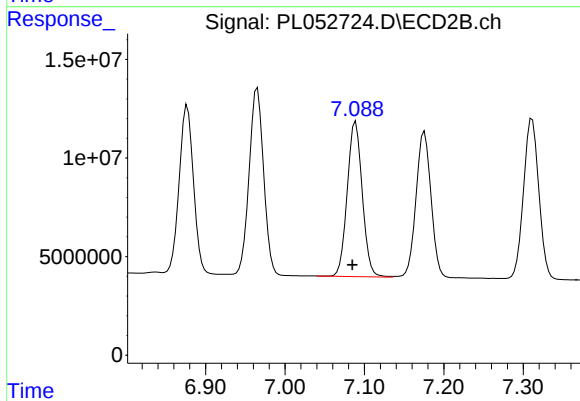

#18 Endrin aldehyde

R.T.: 7.089 min
Delta R.T.: 0.004 min
Response: 103445089
Conc: 55.76 ng/ml

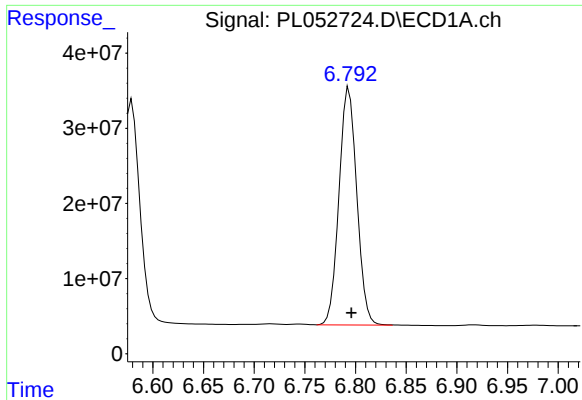


#19 Endosulfan Sulfate

R.T.: 6.792 min
Delta R.T.: -0.004 min
Response: 386186575
Conc: 46.56 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

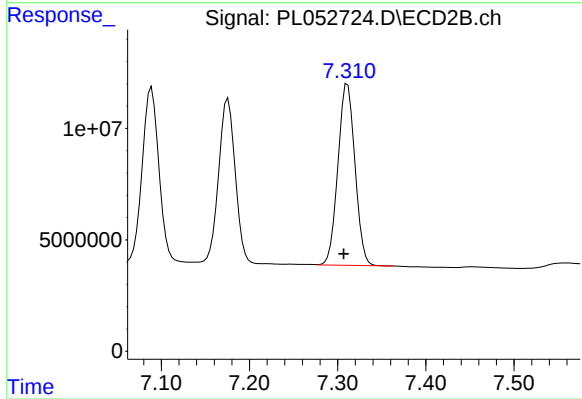


#19 Endosulfan Sulfate

R.T.: 7.311 min
Delta R.T.: 0.004 min
Response: 109412738
Conc: 53.27 ng/ml

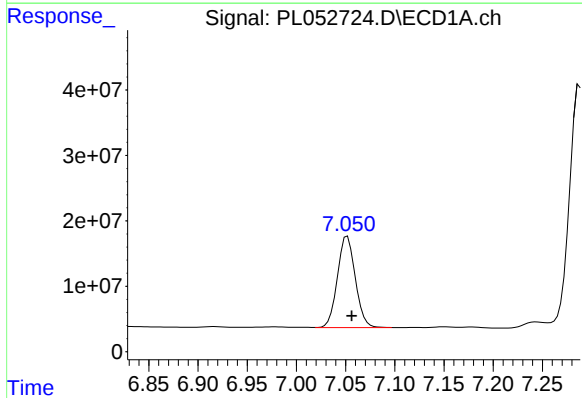


#20 Methoxychlor

R.T.: 7.050 min
Delta R.T.: -0.006 min
Response: 177281348
Conc: 43.85 ng/ml m

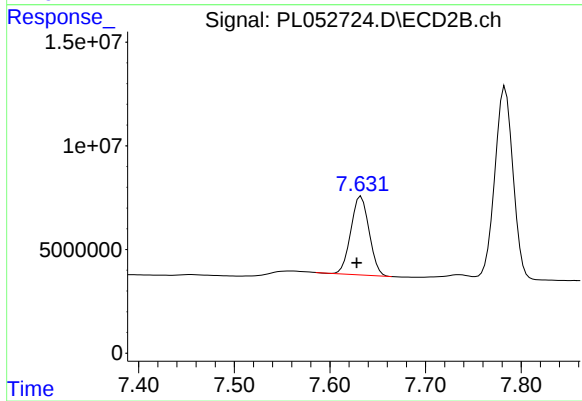

#20 Methoxychlor

R.T.: 7.633 min
Delta R.T.: 0.004 min
Response: 50348498
Conc: 49.69 ng/ml

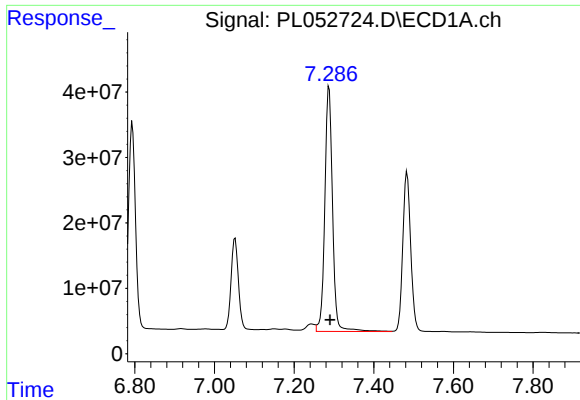


#21 Endrin ketone

R.T.: 7.288 min
Delta R.T.: -0.003 min
Response: 506725641
Conc: 48.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

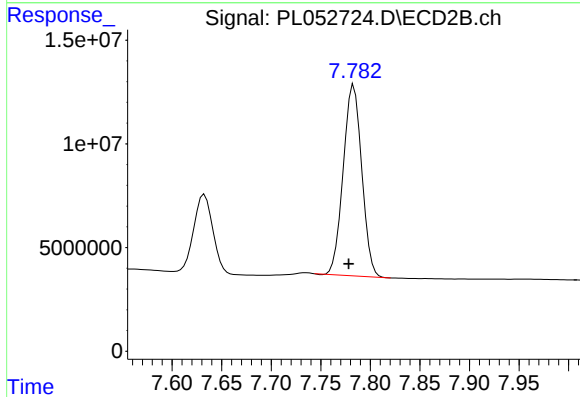


#21 Endrin ketone

R.T.: 7.783 min
Delta R.T.: 0.005 min
Response: 119482872
Conc: 53.80 ng/ml

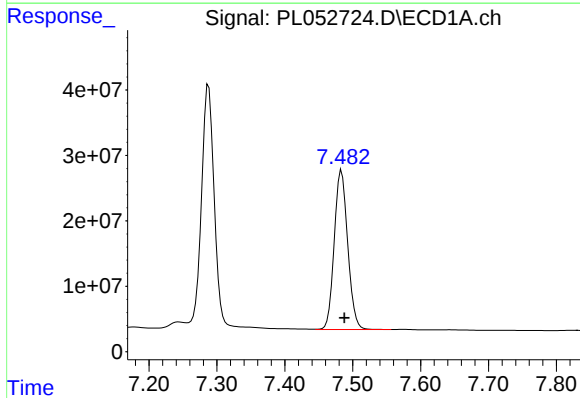


#22 Mirex

R.T.: 7.484 min
Delta R.T.: -0.004 min
Response: 335305376
Conc: 43.84 ng/ml

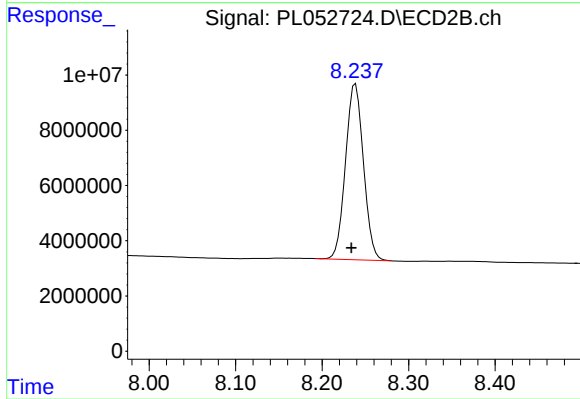

#22 Mirex

R.T.: 8.239 min
Delta R.T.: 0.005 min
Response: 91275854
Conc: 53.33 ng/ml

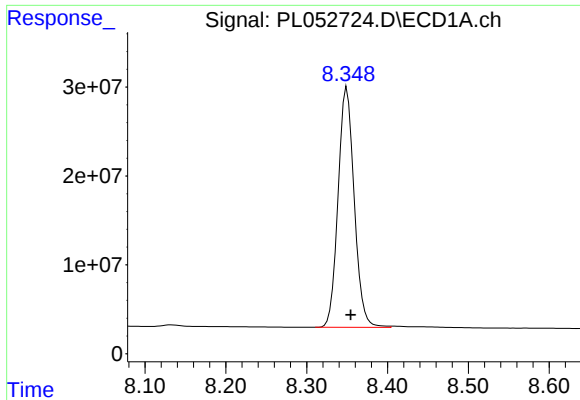


#28 Decachlorobiphenyl

R.T.: 8.348 min
Delta R.T.: -0.006 min
Response: 373970208
Conc: 42.77 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Manual Integrations
APPROVED

Ankita
9/26/2019 8:37:08 AM

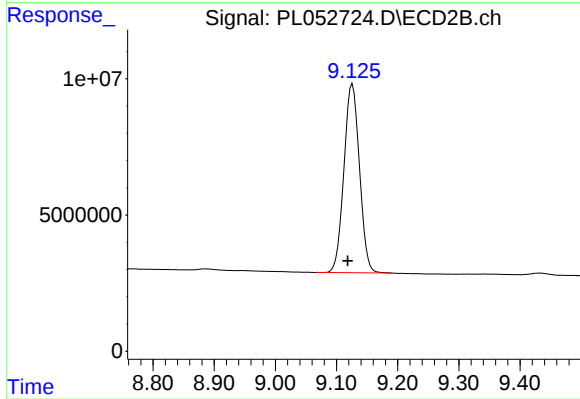

#28 Decachlorobiphenyl

R.T.: 9.126 min
Delta R.T.: 0.008 min
Response: 122377539
Conc: 51.10 ng/ml