

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092420\
 Data File : PL061764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 13:22
 Operator : DD\AJ
 Sample : L4124-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:50:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	39298311	56878145	23.036	20.848
28)	SA Decachlor...	8.209	9.093	31019668	37598405	19.068	17.080
Target Compounds							
9)	A Endosulfan I	5.529f	0.000	4432973	0	2.736	N.D. #
10)	B gamma-Chl...	0.000	6.107	0	2442680	N.D.	0.832 #
11)	B alpha-Chl...	0.000	6.199	0	5904229	N.D.	1.966 #
14)	MA Endrin	0.000	6.746f	0	3634121	N.D.	1.490 #
15)	B Endosulfa...	0.000	6.946f	0	1370566	N.D.	0.530 #
19)	B Endosulfa...	0.000	7.285	0	6416928	N.D.	2.740 #
20)	A Methoxychlor	0.000	7.613	0	3803623	N.D.	3.019 #
21)	B Endrin ke...	0.000	7.750	0	3839080	N.D.	1.636 #
25)	Chlordane-3	0.000	6.107	0	2442680	N.D.	6.666 #
26)	Chlordane-4	0.000	6.199	0	5904229	N.D.	13.152 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092420\
Data File : PL061764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 13:22
Operator : DD\AJ
Sample : L4124-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:50:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

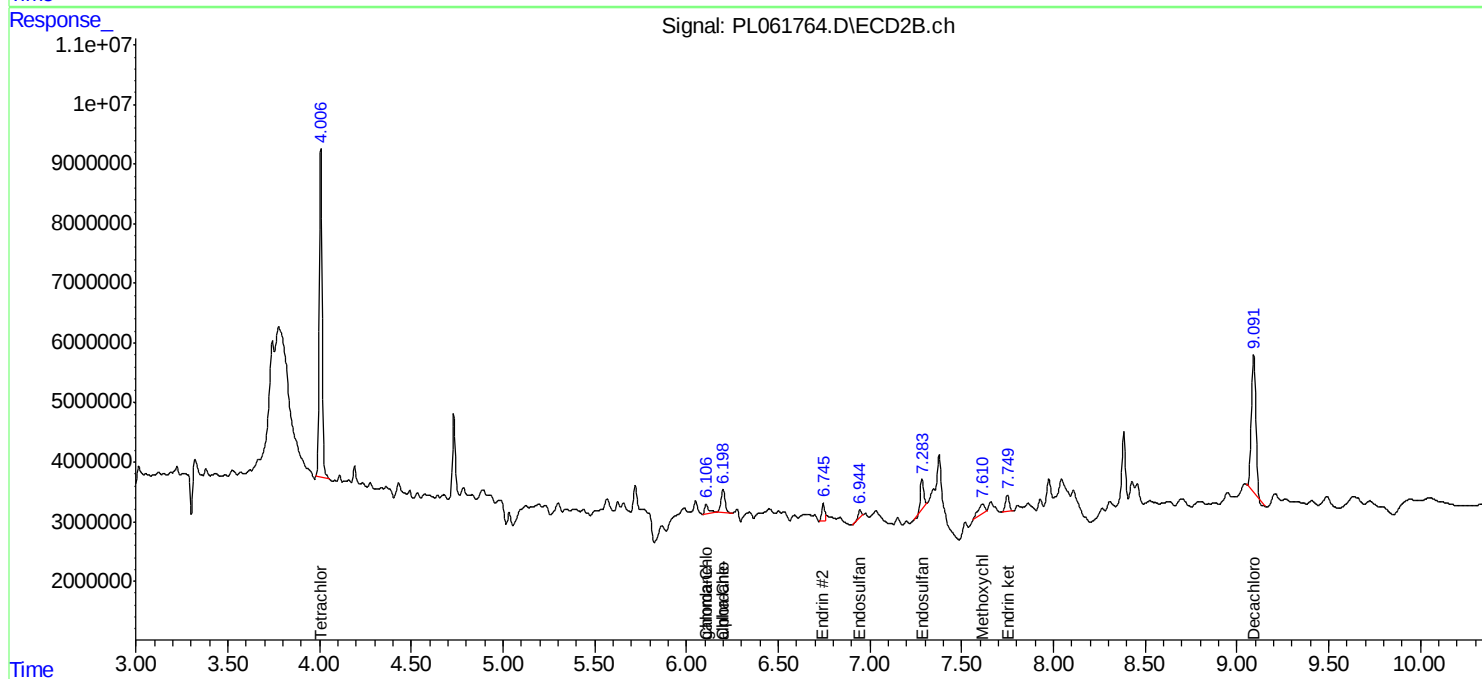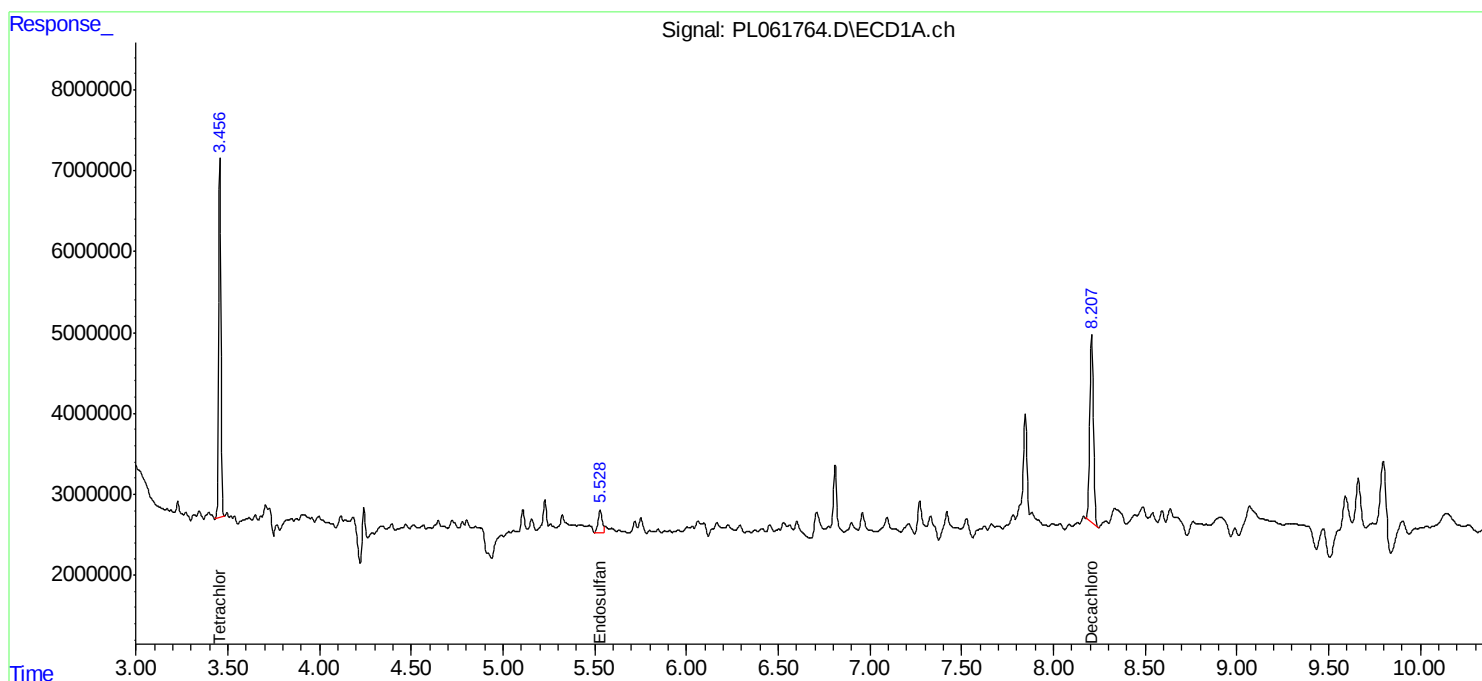


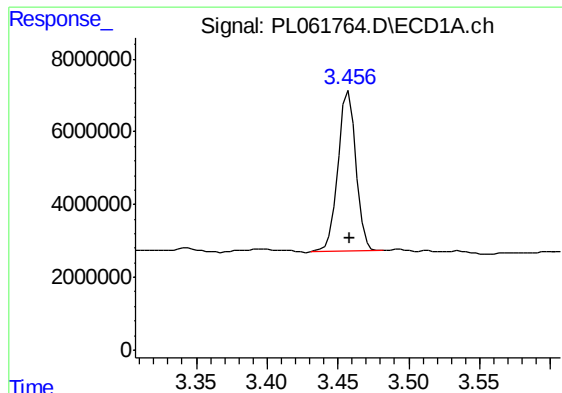

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 39298311
Conc: 23.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-2

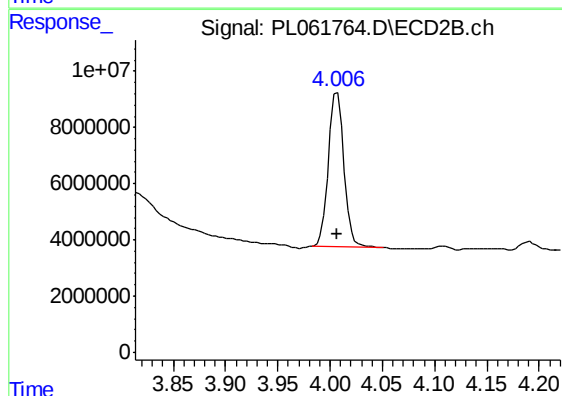


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 56878145
Conc: 20.85 ng/ml

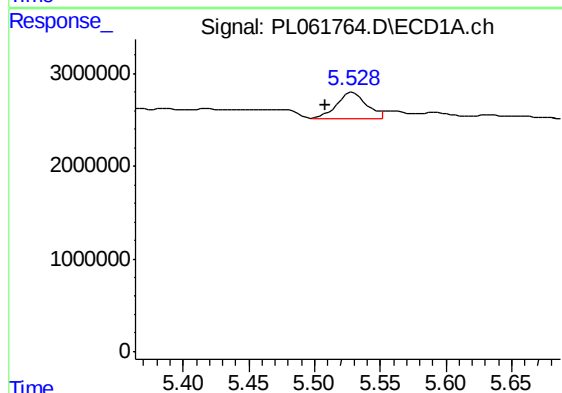


#9 Endosulfan I

R.T.: 5.529 min
Delta R.T.: 0.021 min
Response: 4432973
Conc: 2.74 ng/ml

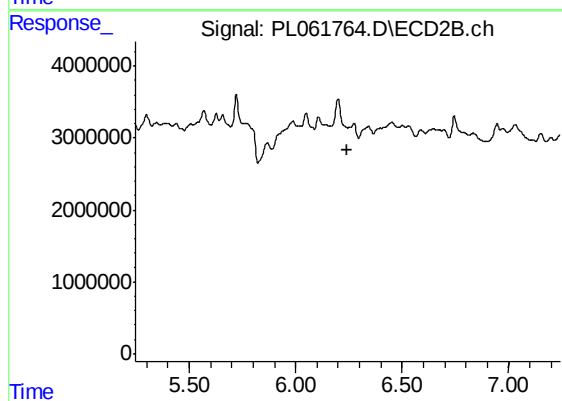

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.245 min
Response: 0
Conc: N.D.

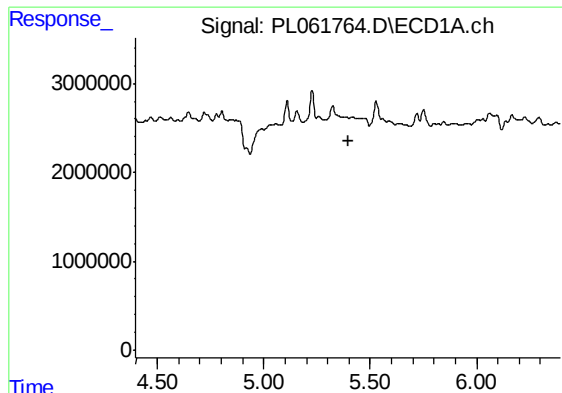

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-2

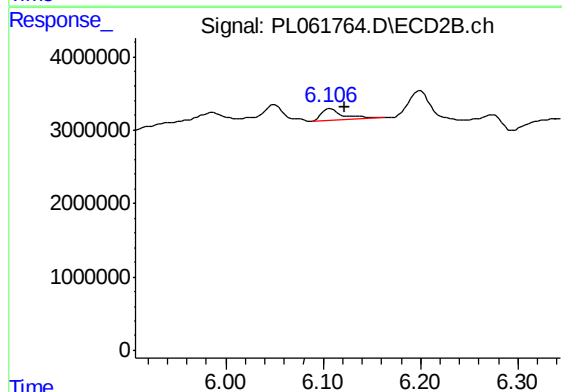


#10 gamma-Chlordane

R.T.: 6.107 min
Delta R.T.: -0.015 min
Response: 2442680
Conc: 0.83 ng/ml

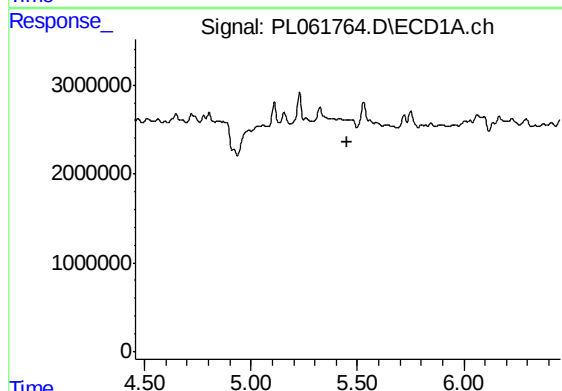


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

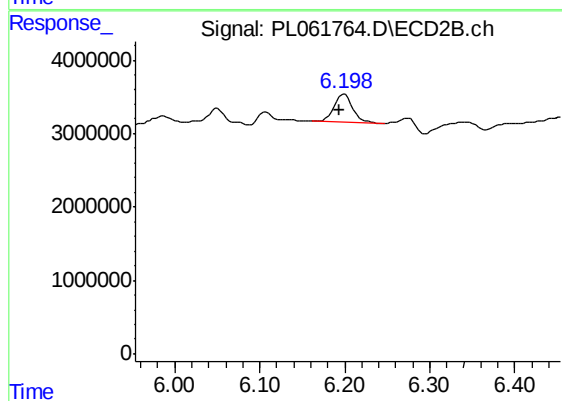

#11 alpha-Chlordane


R.T.: 6.199 min
Delta R.T.: 0.005 min
Response: 5904229
Conc: 1.97 ng/ml

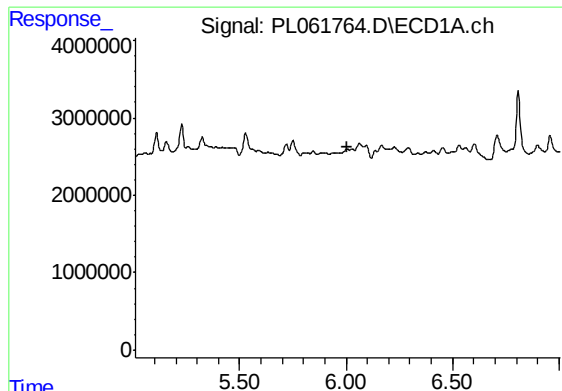

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-2

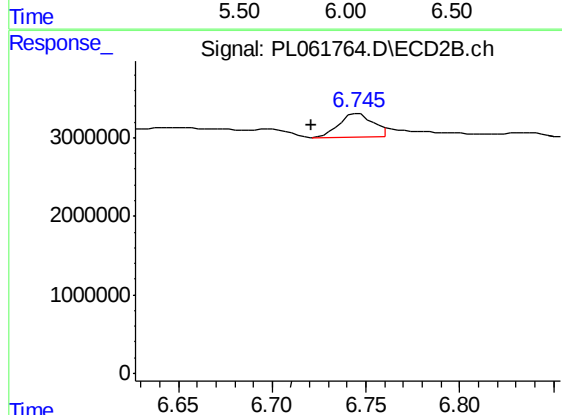


#14 Endrin

R.T.: 6.746 min
Delta R.T.: 0.025 min
Response: 3634121
Conc: 1.49 ng/ml

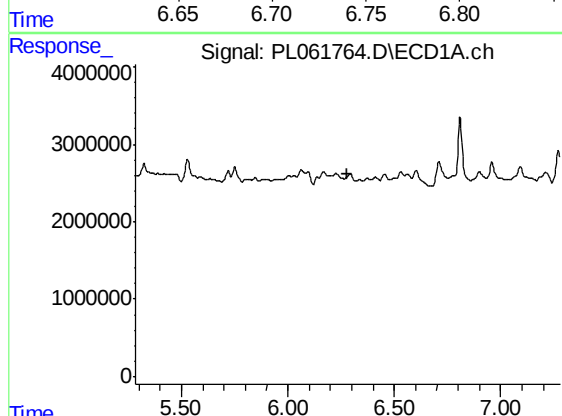


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.281 min
Response: 0
Conc: N.D.

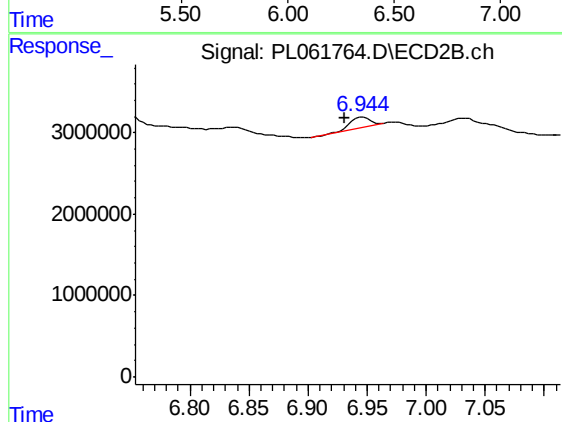

#15 Endosulfan II


R.T.: 6.946 min
Delta R.T.: 0.016 min
Response: 1370566
Conc: 0.53 ng/ml

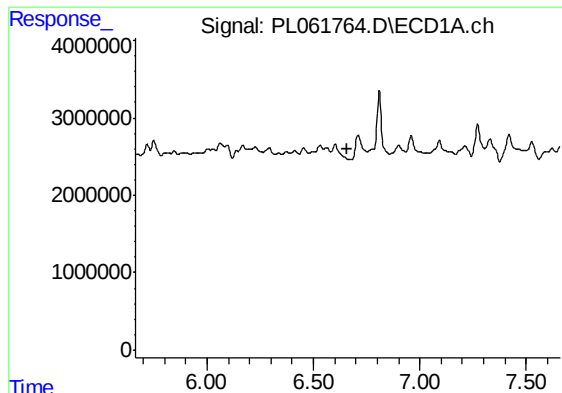

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-2

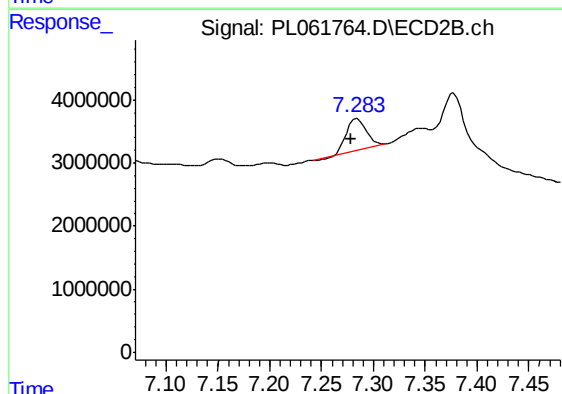


#19 Endosulfan Sulfate

R.T.: 7.285 min
Delta R.T.: 0.006 min
Response: 6416928
Conc: 2.74 ng/ml

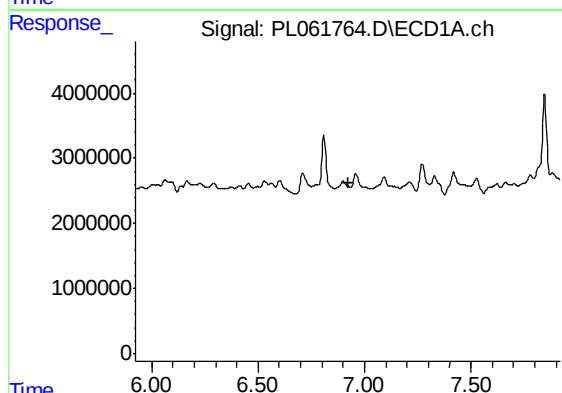


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

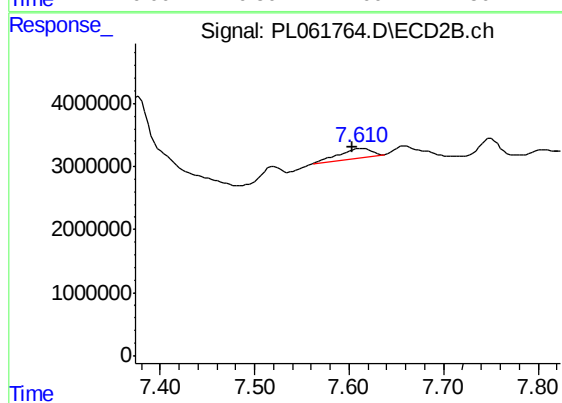

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.009 min
Response: 3803623
Conc: 3.02 ng/ml

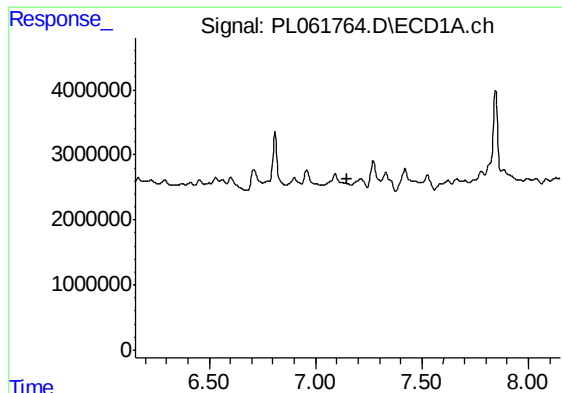

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-2

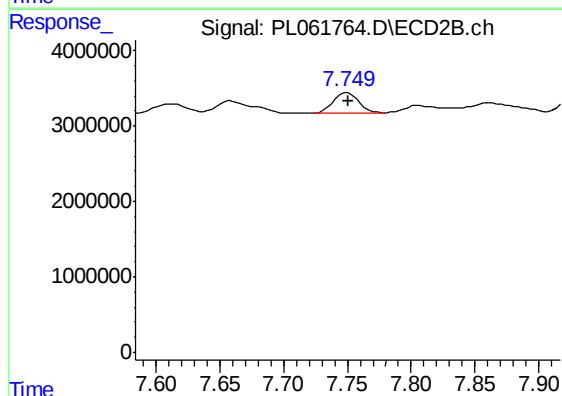


#21 Endrin ketone

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 3839080
Conc: 1.64 ng/ml

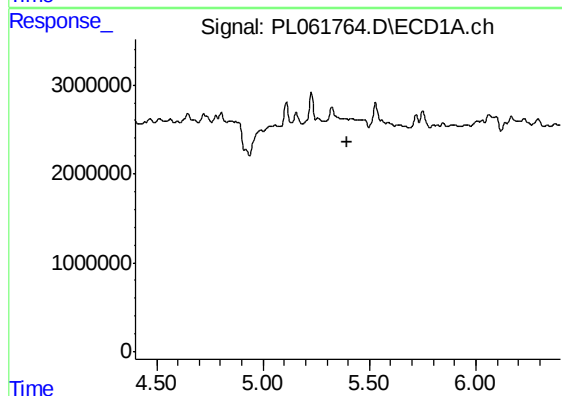


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.397 min
Response: 0
Conc: N.D.

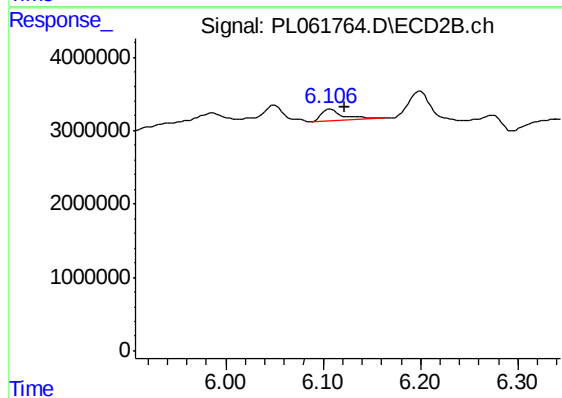

#25 Chlordane-3


R.T.: 6.107 min
Delta R.T.: -0.015 min
Response: 2442680
Conc: 6.67 ng/ml

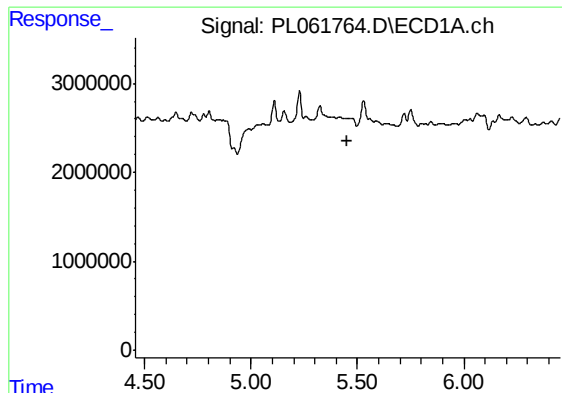

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S-2

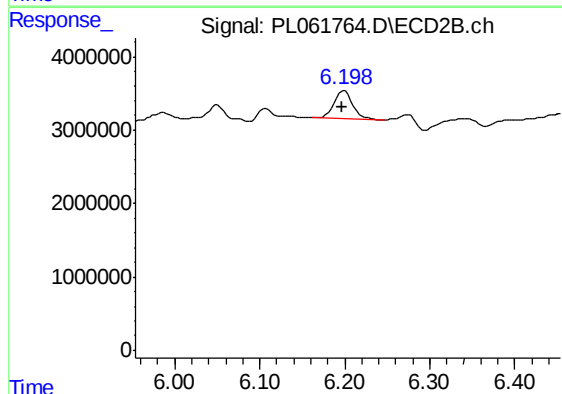


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.003 min
Response: 5904229
Conc: 13.15 ng/ml

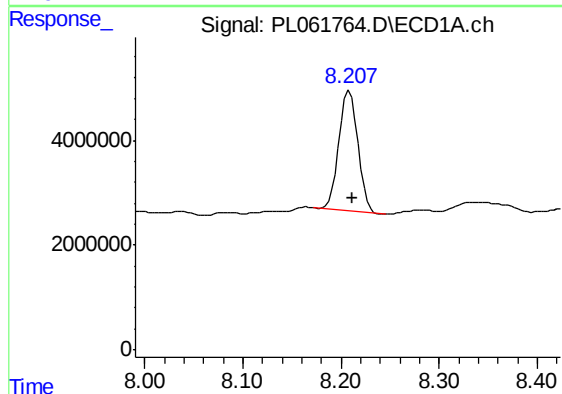

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.003 min
Response: 31019668
Conc: 19.07 ng/ml

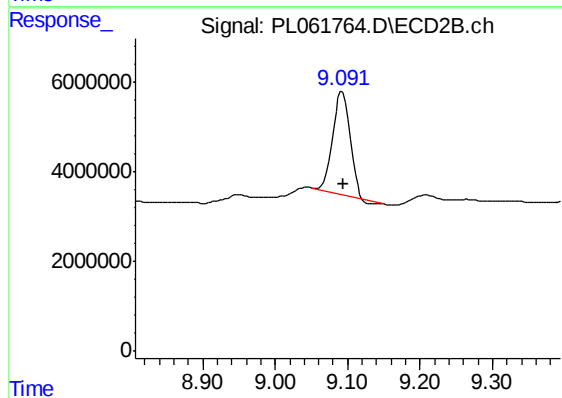

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.002 min
Response: 37598405
Conc: 17.08 ng/ml