

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092420\
 Data File : PL061769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2020 14:33
 Operator : DD\AJ
 Sample : L4125-13
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-31

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:52:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	37299221	53707084	21.864	19.686
28)	SA Decachlor...	8.209	9.093	35496044	49402757	21.820	22.442
Target Compounds							
12)	B 4,4'-DDE	5.638f	0.000	2374408	0	1.511	N.D. #
15)	B Endosulfa...	0.000	6.947f	0	1160250	N.D.	0.449 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092420\
Data File : PL061769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2020 14:33
Operator : DD\AJ
Sample : L4125-13
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-31

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:52:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

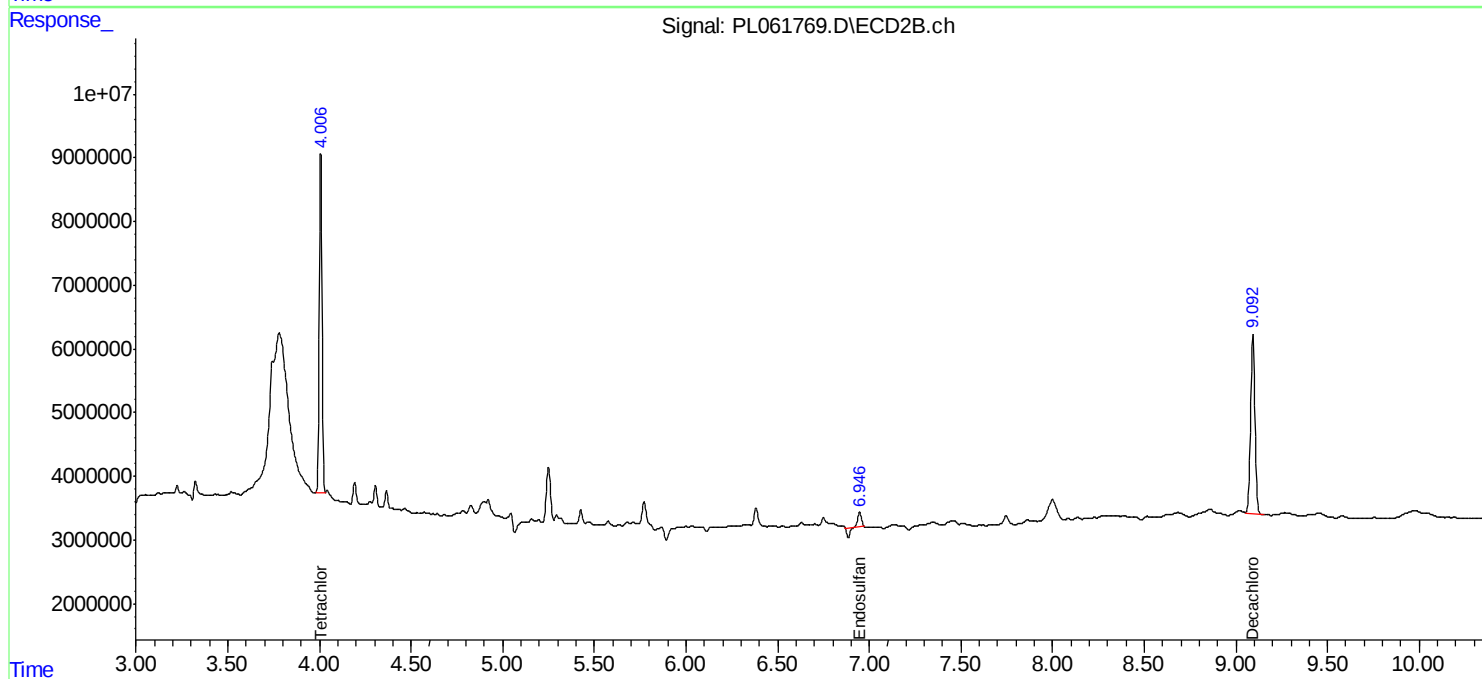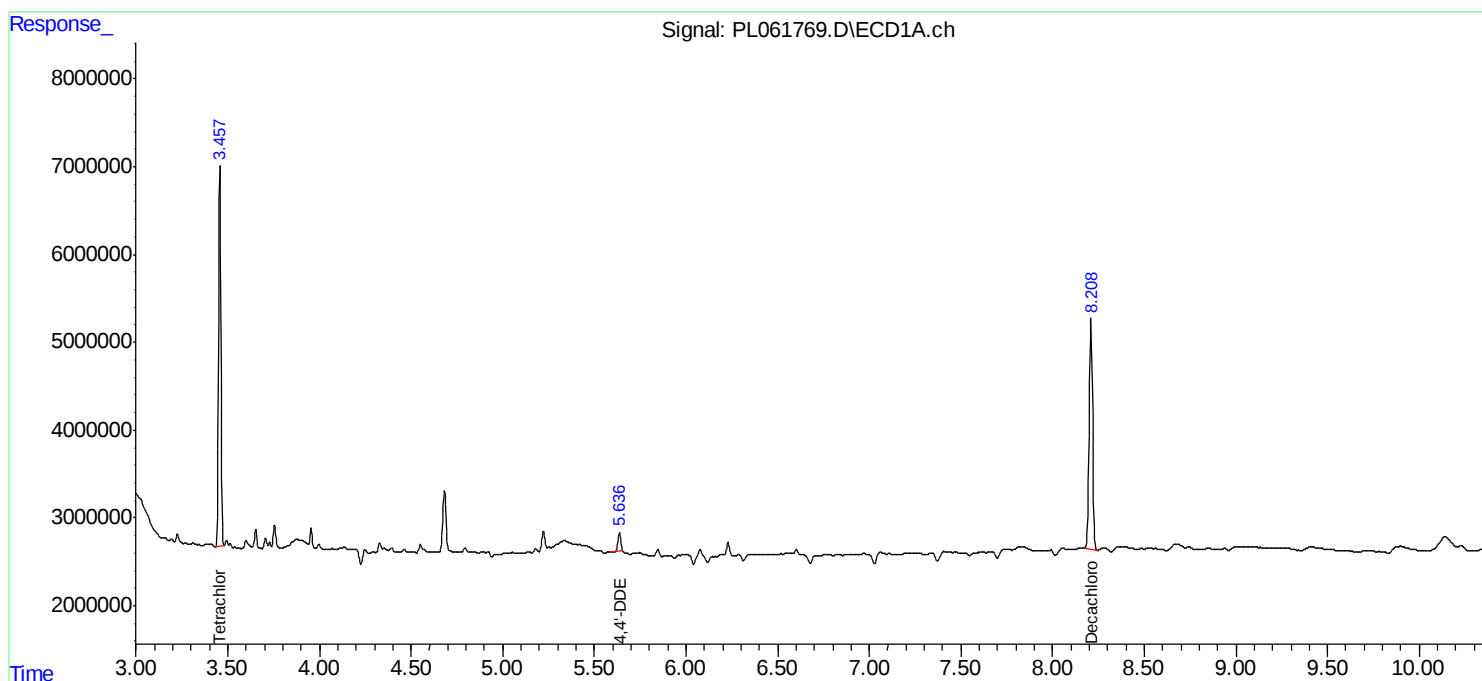


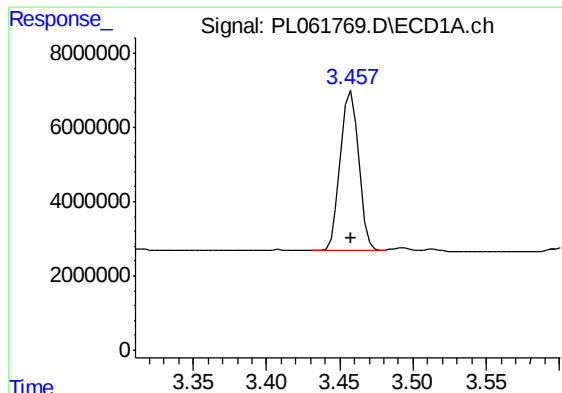

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 37299221
Conc: 21.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-31

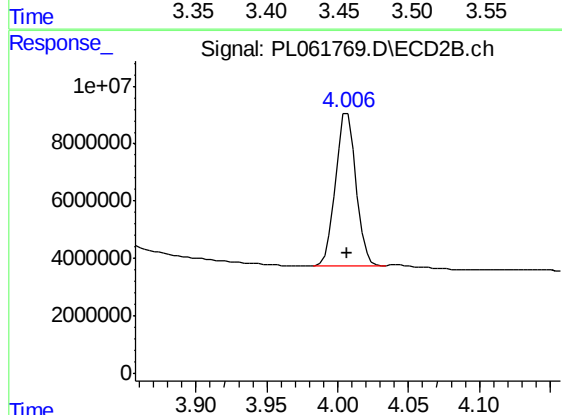


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 53707084
Conc: 19.69 ng/ml

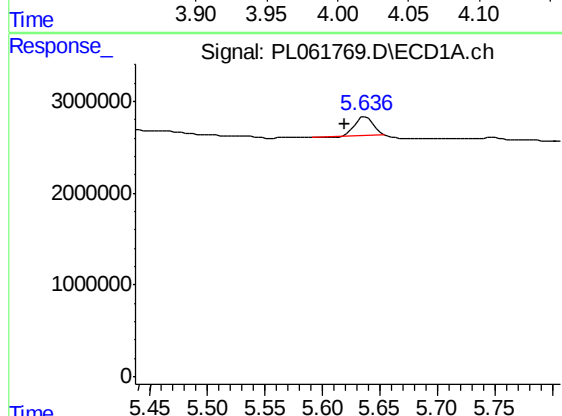


#12 4,4'-DDE

R.T.: 5.638 min
Delta R.T.: 0.018 min
Response: 2374408
Conc: 1.51 ng/ml

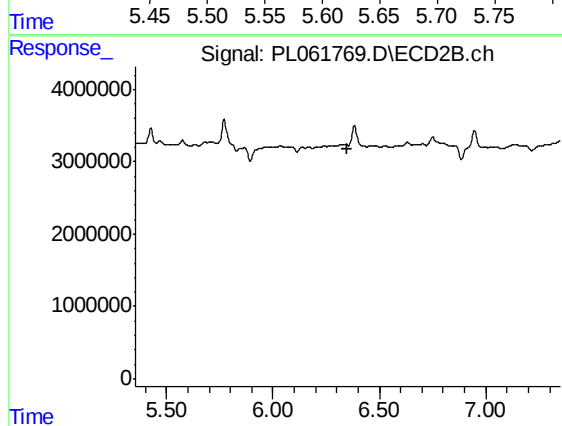

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.352 min
Response: 0
Conc: N.D.

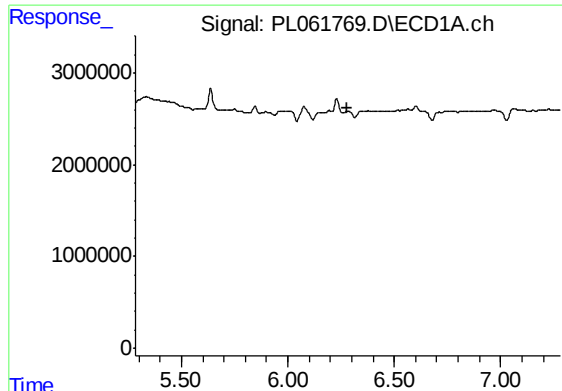

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-31

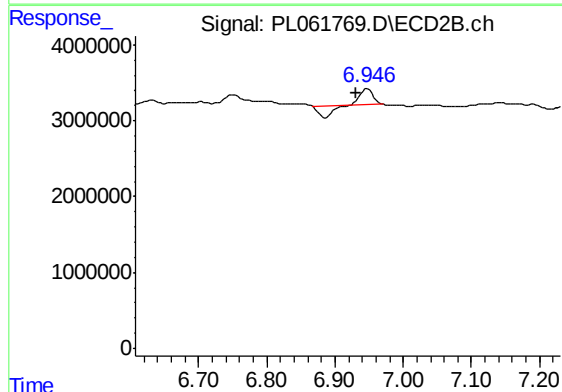


#15 Endosulfan II

R.T.: 6.947 min
Delta R.T.: 0.016 min
Response: 1160250
Conc: 0.45 ng/ml

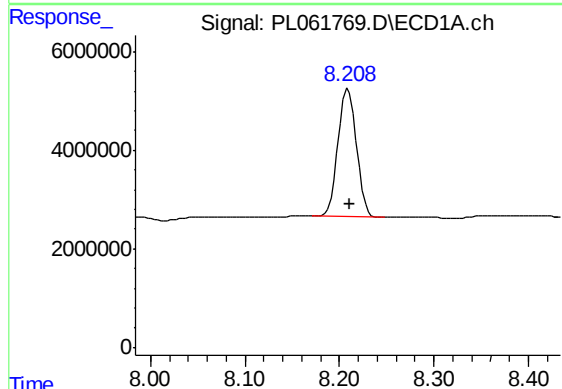

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 35496044
Conc: 21.82 ng/ml

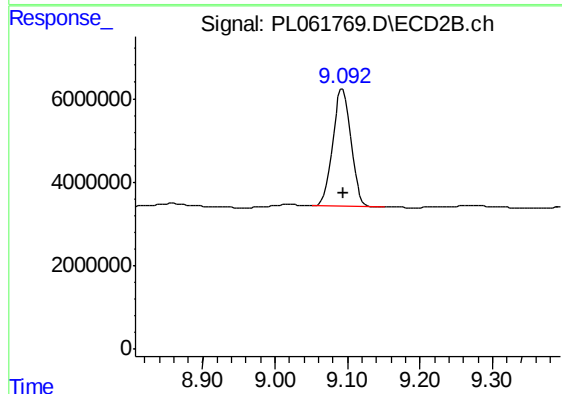

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.001 min
Response: 49402757
Conc: 22.44 ng/ml