

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092424\
 Data File : PL092004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Sep 2024 14:35
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 01:18:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 23 16:44:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.782	98225428	140.7E6	44.153	56.089 #
28)	SA Decachlor...	9.060	7.923	73319861	113.0E6	44.756	45.172
Target Compounds							
23)	Chlordane-1	4.706	3.781	45186114	45572058	440.864	455.808
24)	Chlordane-2	5.235	4.358	47245210	51014589	440.529	454.570
25)	Chlordane-3	5.946	4.989	165.1E6	153.0E6	440.743	461.976
26)	Chlordane-4	6.027	5.051	200.3E6	145.8E6	442.260	459.421
27)	Chlordane-5	6.876	5.947	39006794	49726991	447.249	458.527



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092424\
Data File : PL092004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Sep 2024 14:35
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 01:18:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092324.M
Quant Title : GC Extractables
QLast Update : Mon Sep 23 16:44:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

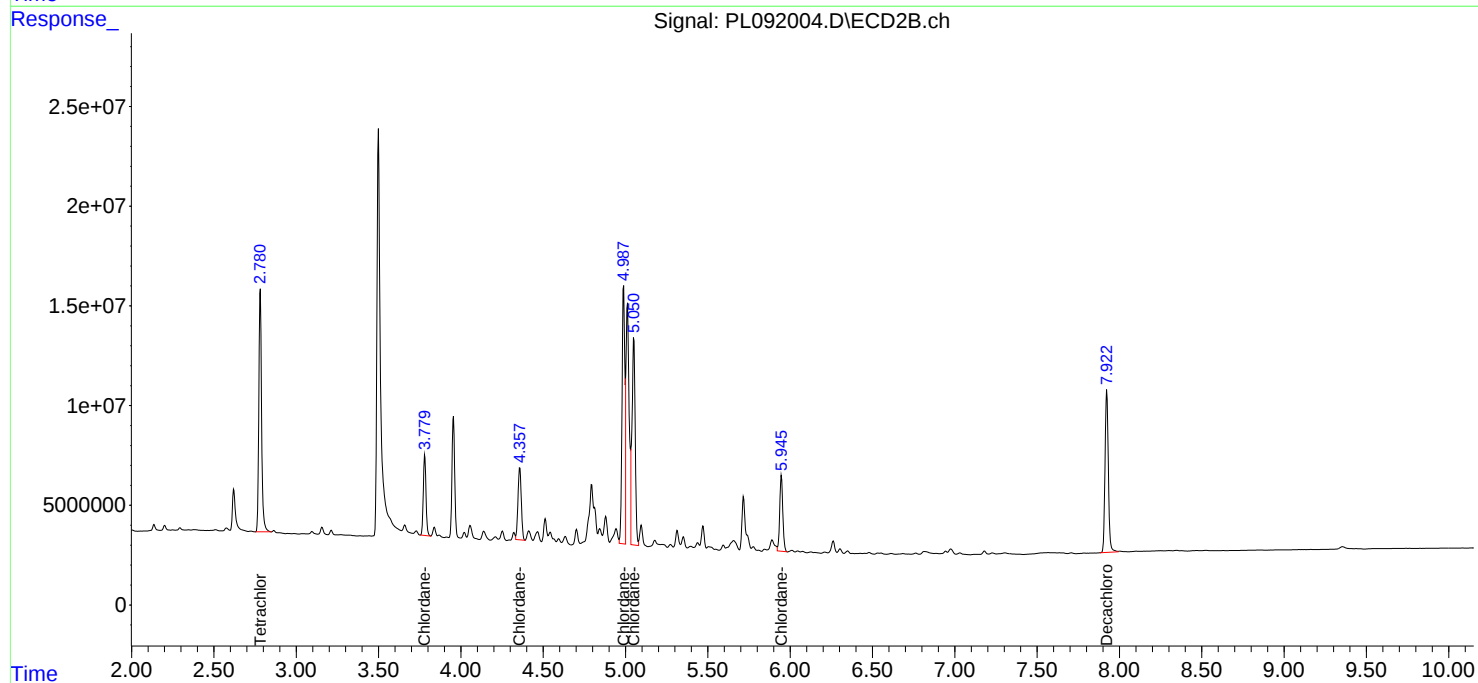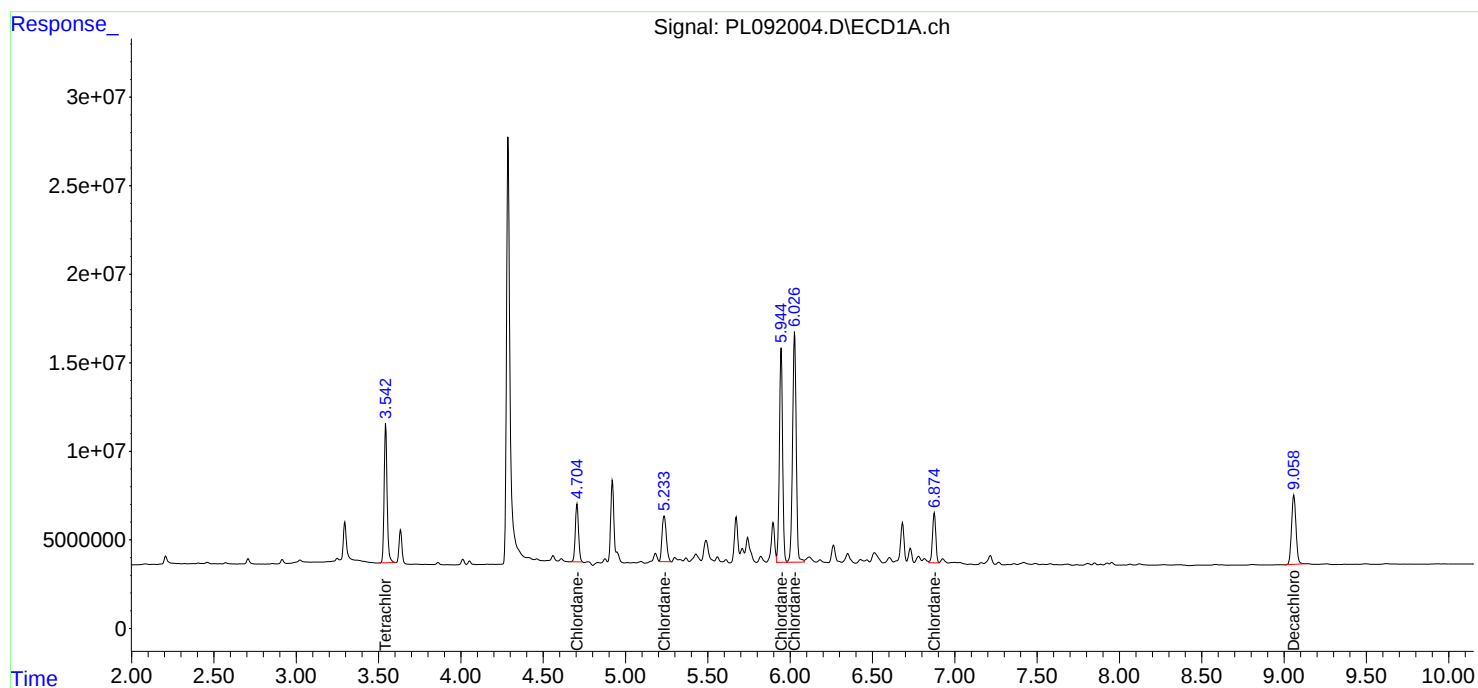


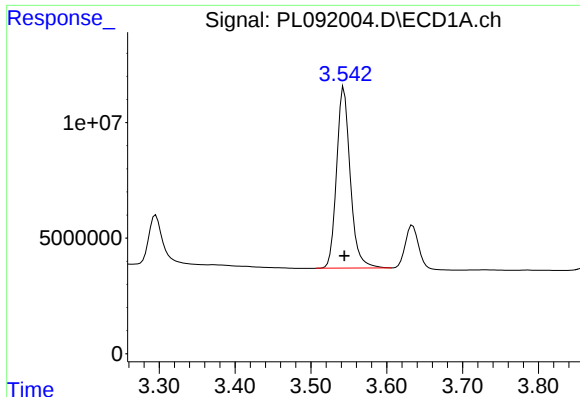

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.000 min
Response: 98225428
Conc: 44.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

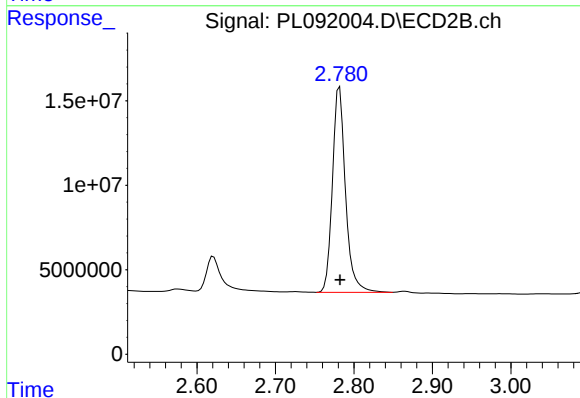


#1 Tetrachloro-m-xylene

R.T.: 2.782 min
Delta R.T.: 0.000 min
Response: 140674561
Conc: 56.09 ng/ml

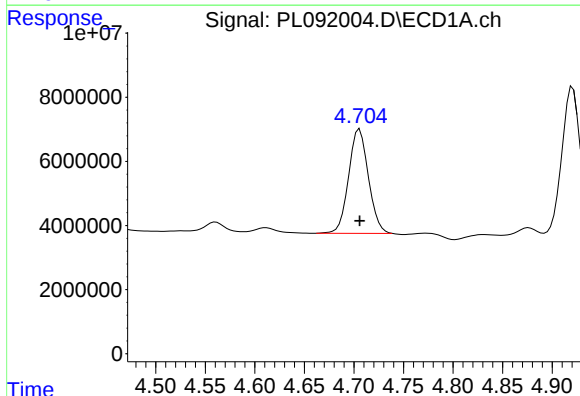


#23 Chlordane-1

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 45186114
Conc: 440.86 ng/ml

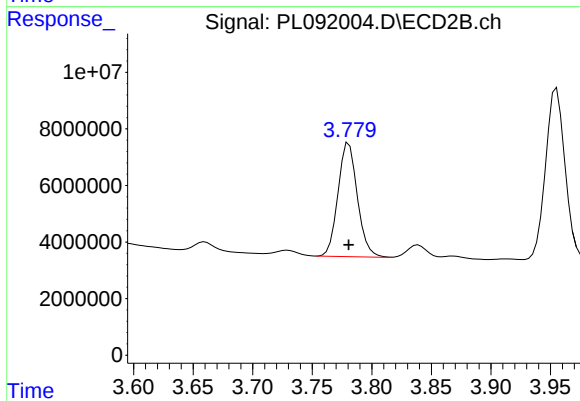

#23 Chlordane-1


R.T.: 3.781 min
Delta R.T.: 0.000 min
Response: 45572058
Conc: 455.81 ng/ml

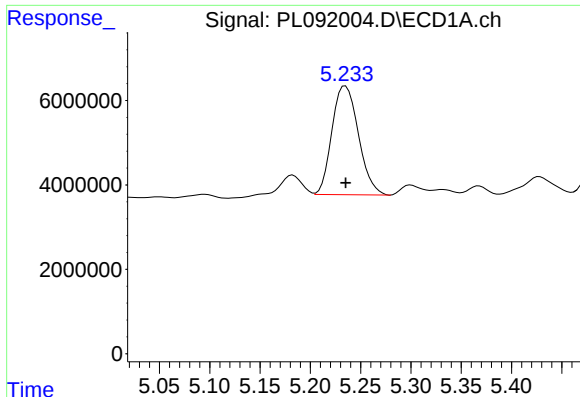

#24 Chlordane-2


R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 47245210
Conc: 440.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

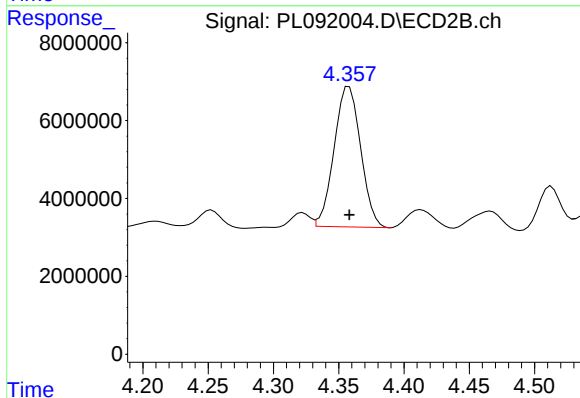


#24 Chlordane-2

R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 51014589
Conc: 454.57 ng/ml

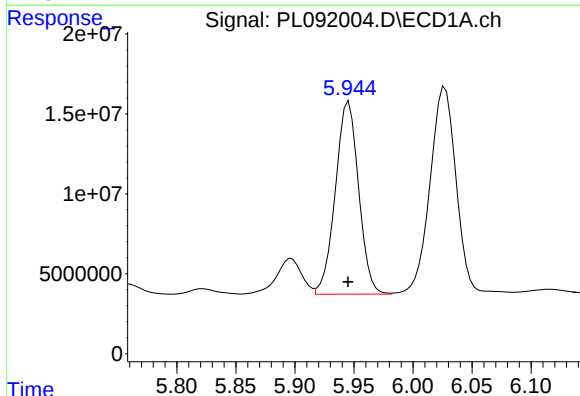


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 165092049
Conc: 440.74 ng/ml

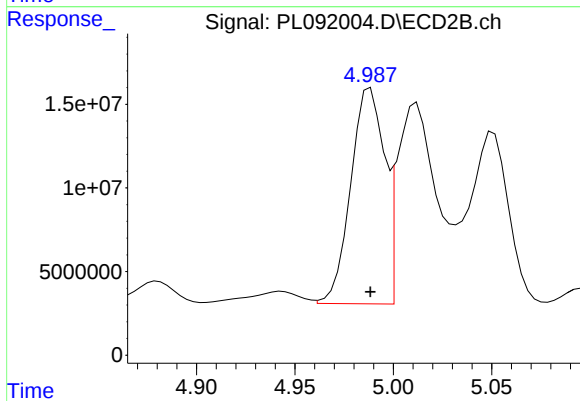

#25 Chlordane-3


R.T.: 4.989 min
Delta R.T.: 0.000 min
Response: 153019638
Conc: 461.98 ng/ml

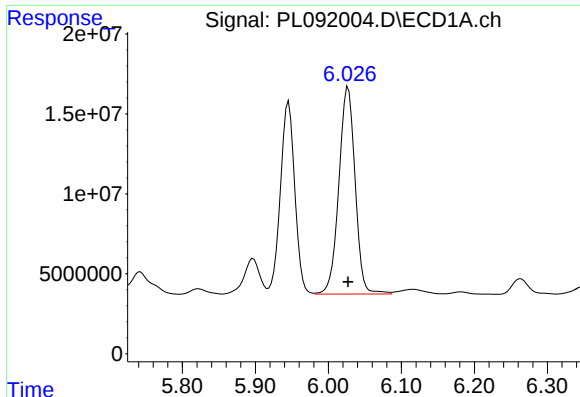

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 200275658
Conc: 442.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

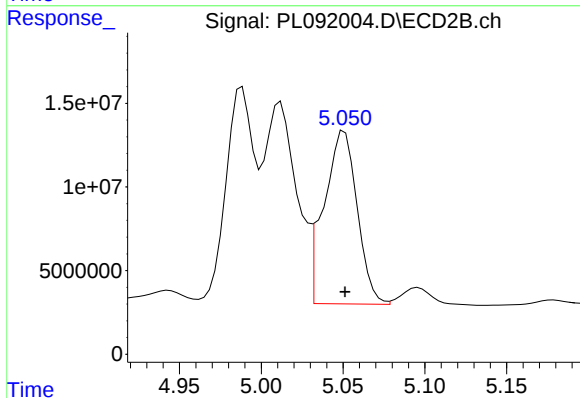


#26 Chlordane-4

R.T.: 5.051 min
Delta R.T.: 0.000 min
Response: 145765896
Conc: 459.42 ng/ml

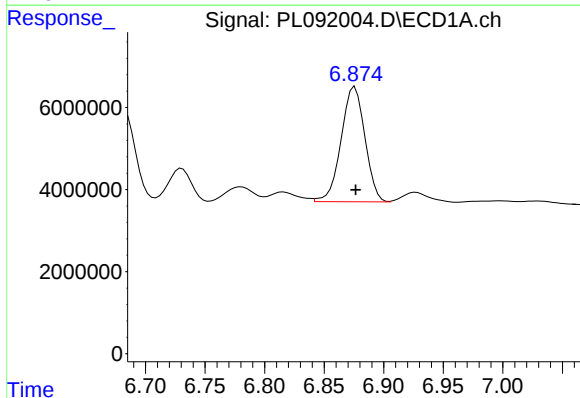


#27 Chlordane-5

R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 39006794
Conc: 447.25 ng/ml

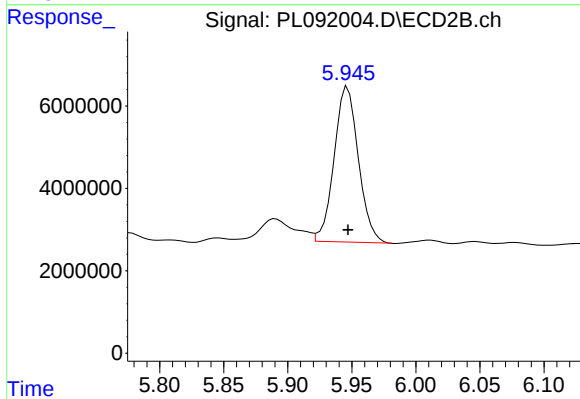

#27 Chlordane-5


R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 49726991
Conc: 458.53 ng/ml

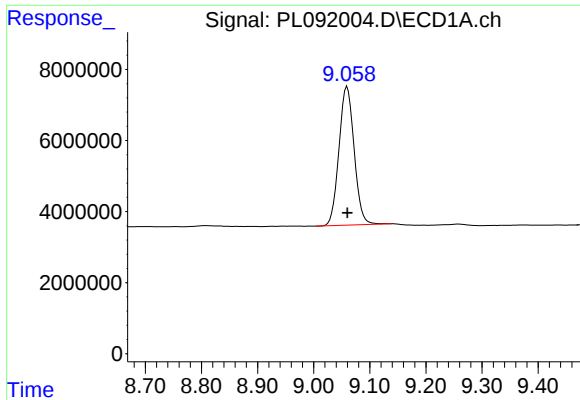

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.000 min
Response: 73319861
Conc: 44.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

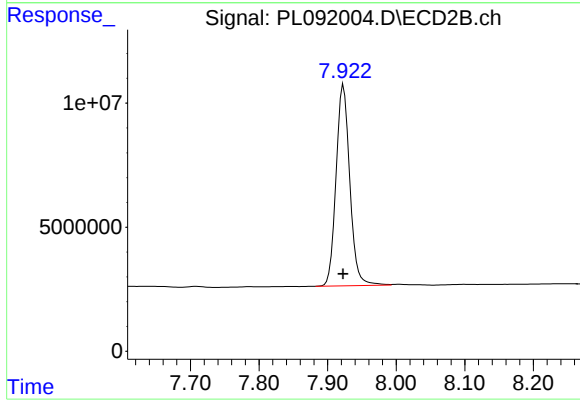

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: 0.000 min
Response: 113018494
Conc: 45.17 ng/ml