

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
 Data File : PL040294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 11:25
 Operator : AJ\SJ
 Sample : J4770-01
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:03:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.239	3.843	109.5E6	47483405	14.392	14.540
28)	SA Decachlor...	7.862	8.795	95391168	37839587	10.772	11.826
Target Compounds							
3)	MA gamma-BHC...	3.971f	0.000	200.7E6	0	18.182	N.D. #
7)	B delta-BHC	0.000	4.883	0	15499656	N.D.	3.427 #
8)	B Heptachlo...	4.960f	5.669	68441753	-75079	6.733	N.D. #
10)	B gamma-Chl...	0.000	5.895	0	4693801	N.D.	1.219 #
16)	A 4,4'-DDD	5.909f	6.566f	70402052	22238274	8.147	6.944
21)	B Endrin ke...	6.789f	0.000	7313964	0	0.748	N.D. #
25)	Chlordane-3	0.000	5.895	0	4693801	N.D.	8.777 #
27)	Chlordane-5	5.909	0.000	70402052	0	169.748	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
Data File : PL040294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 11:25
Operator : AJ\SJ
Sample : J4770-01
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:03:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

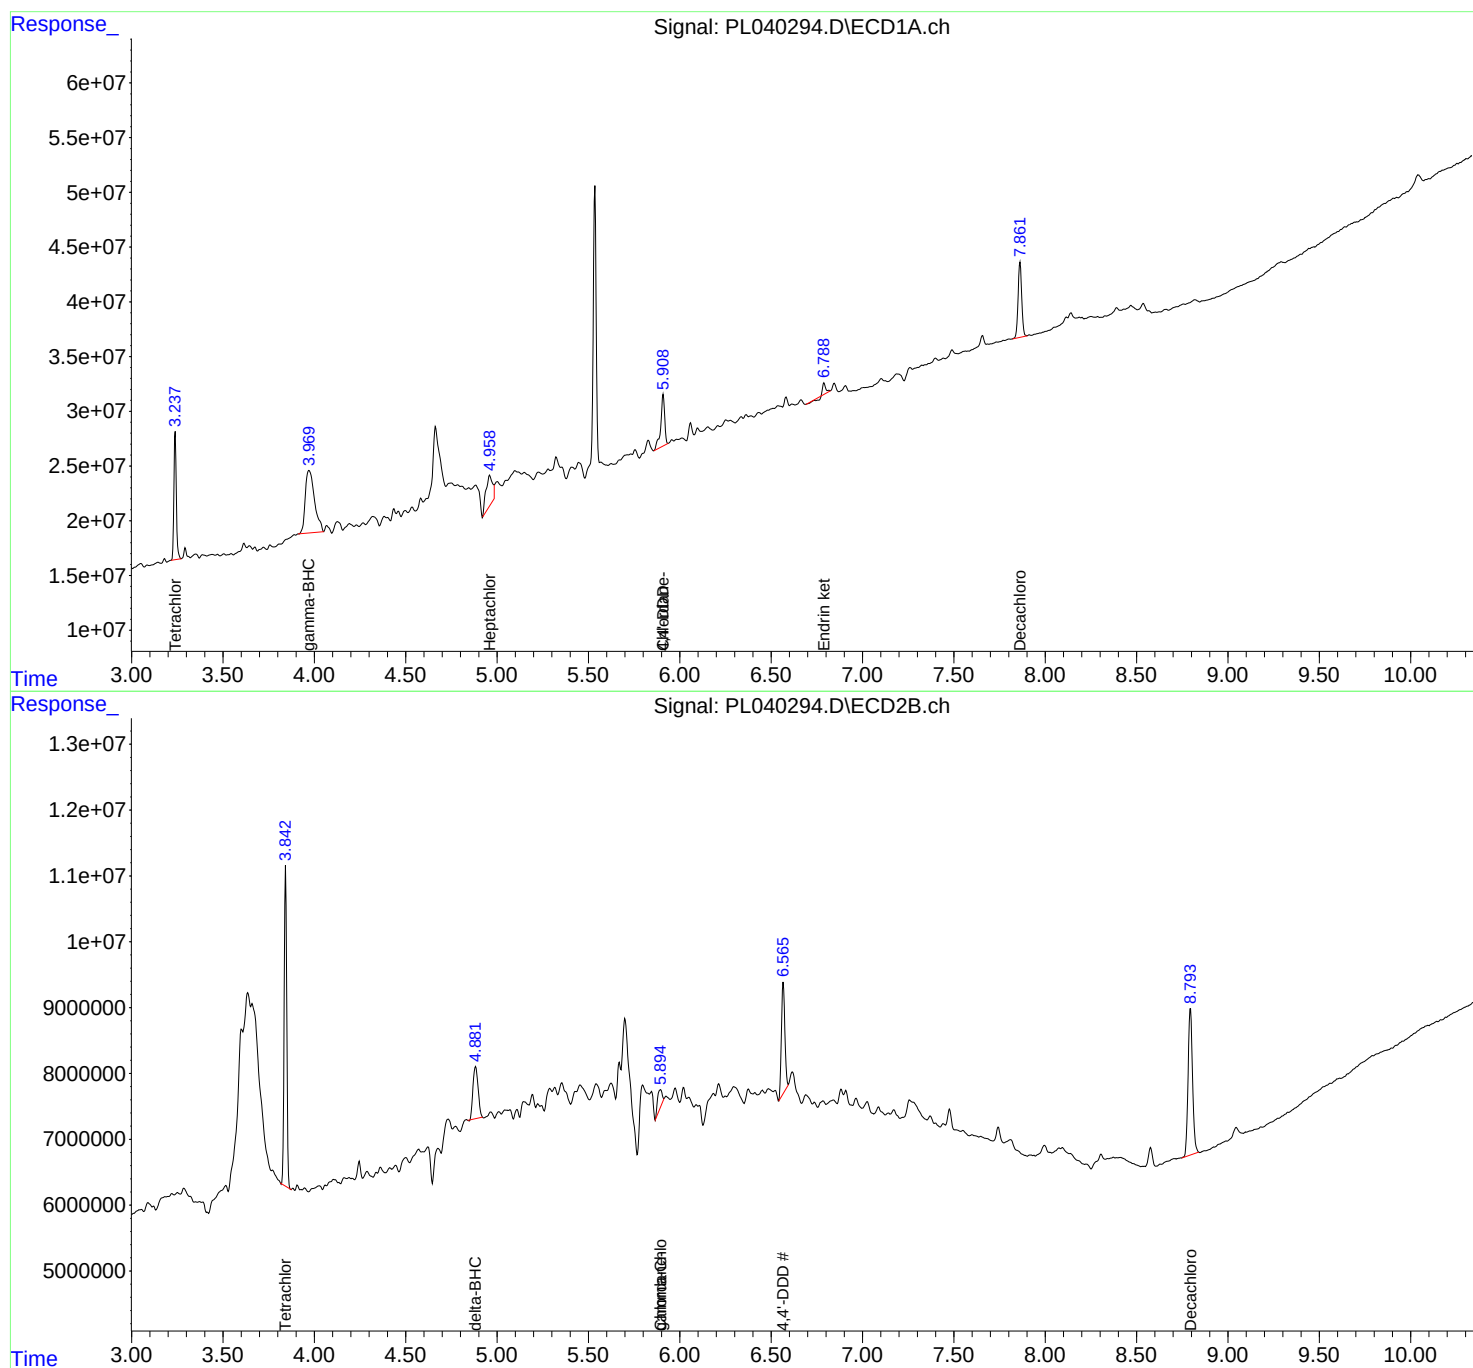


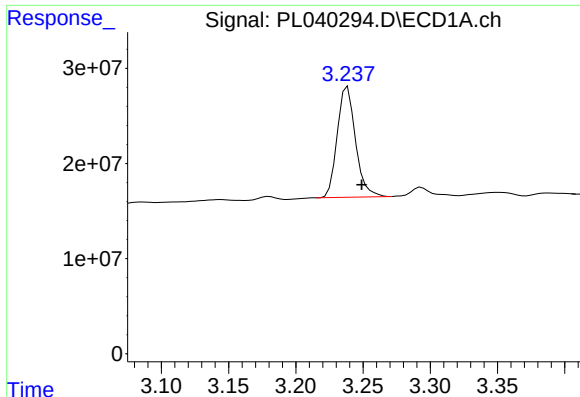

#1 Tetrachloro-m-xylene


R.T.: 3.239 min
Delta R.T.: -0.010 min
Response: 109492924
Conc: 14.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

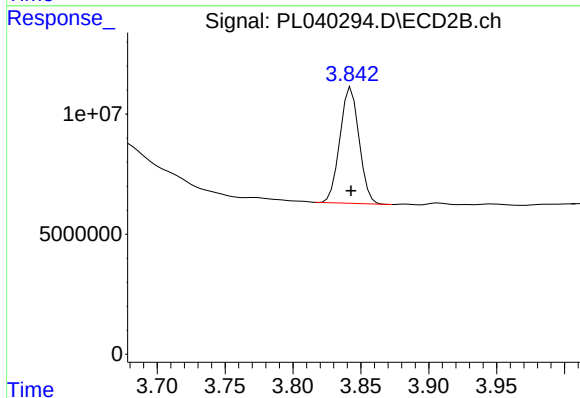


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 47483405
Conc: 14.54 ng/ml

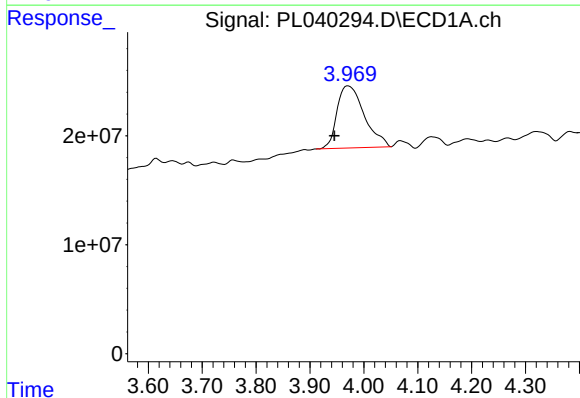


#3 gamma-BHC (Lindane)

R.T.: 3.971 min
Delta R.T.: 0.025 min
Response: 200677184
Conc: 18.18 ng/ml

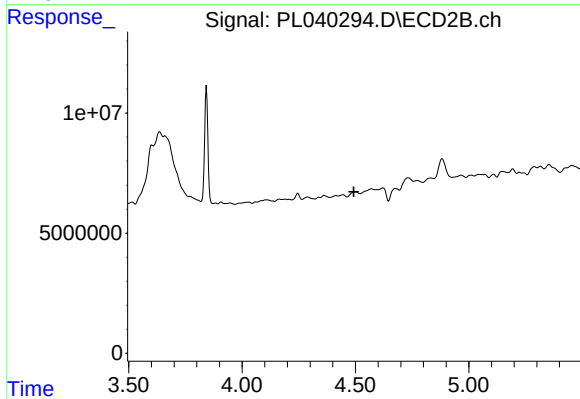

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.493 min
Response: 0
Conc: N.D.

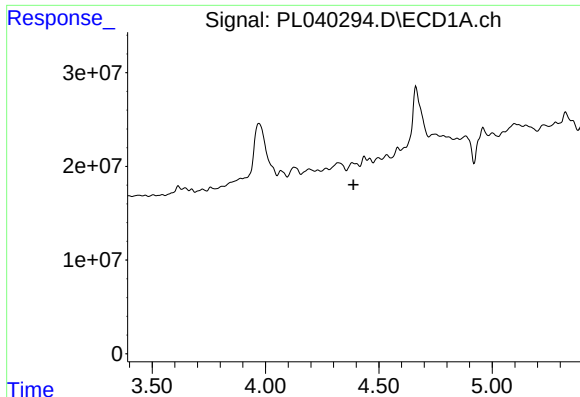

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

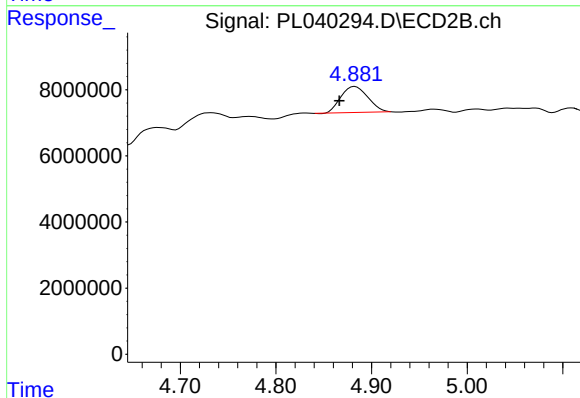


#7 delta-BHC

R.T.: 4.883 min
Delta R.T.: 0.016 min
Response: 15499656
Conc: 3.43 ng/ml

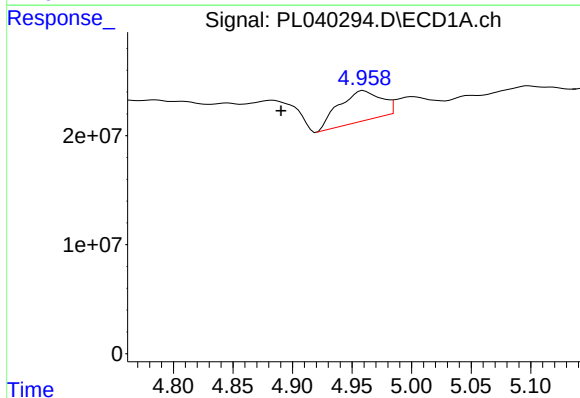


#8 Heptachlor epoxide

R.T.: 4.960 min
Delta R.T.: 0.069 min
Response: 68441753
Conc: 6.73 ng/ml

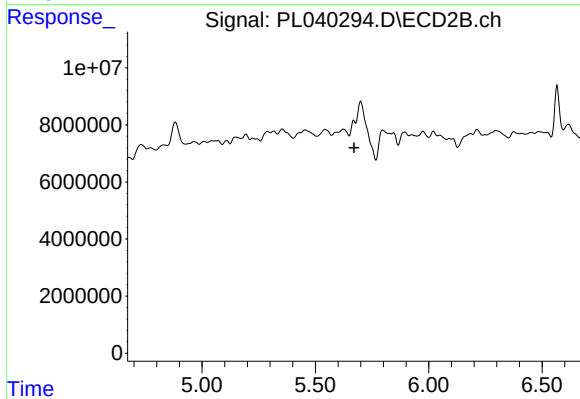

#8 Heptachlor epoxide


R.T.: 5.669 min
Delta R.T.: -0.002 min
Response: -75079
Conc: N.D.

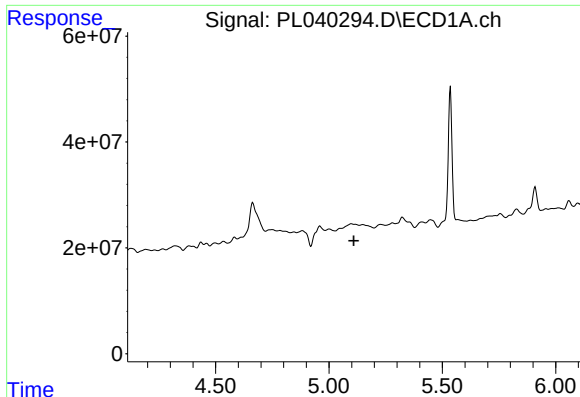

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.110 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

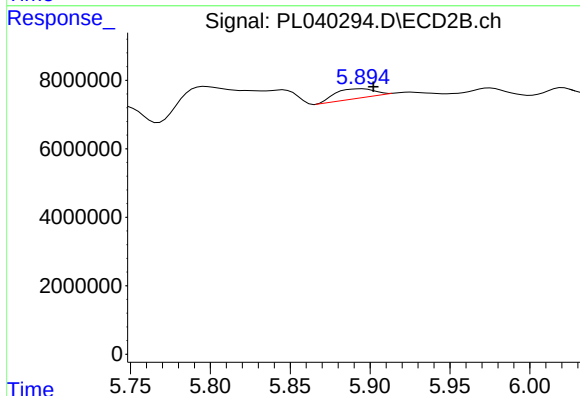


#10 gamma-Chlordane

R.T.: 5.895 min
Delta R.T.: -0.007 min
Response: 4693801
Conc: 1.22 ng/ml

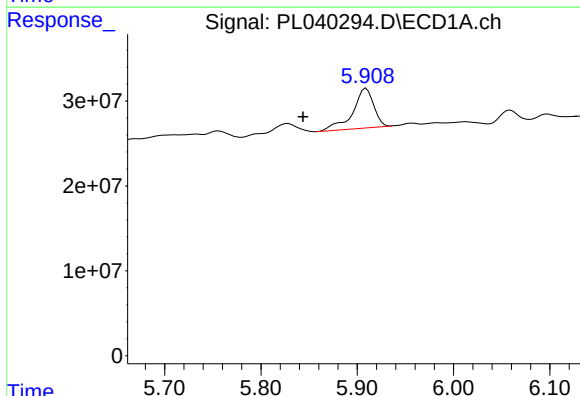


#16 4,4'-DDD

R.T.: 5.909 min
Delta R.T.: 0.066 min
Response: 70402052
Conc: 8.15 ng/ml

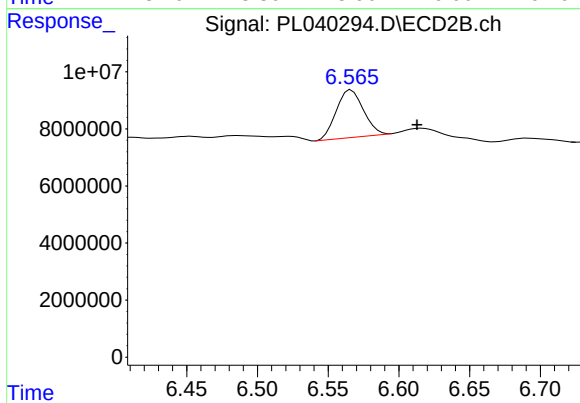

#16 4,4'-DDD


R.T.: 6.566 min
Delta R.T.: -0.047 min
Response: 22238274
Conc: 6.94 ng/ml

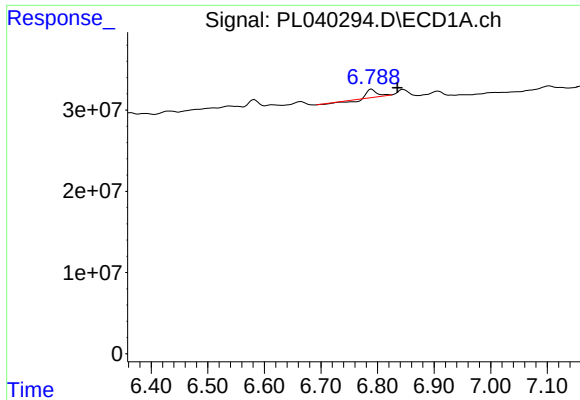

#21 Endrin ketone


R.T.: 6.789 min
Delta R.T.: -0.046 min
Response: 7313964
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

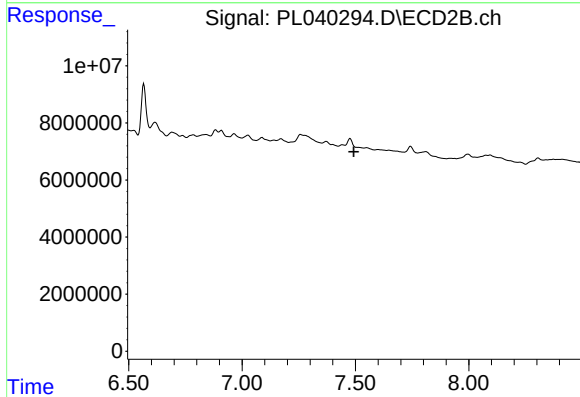


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

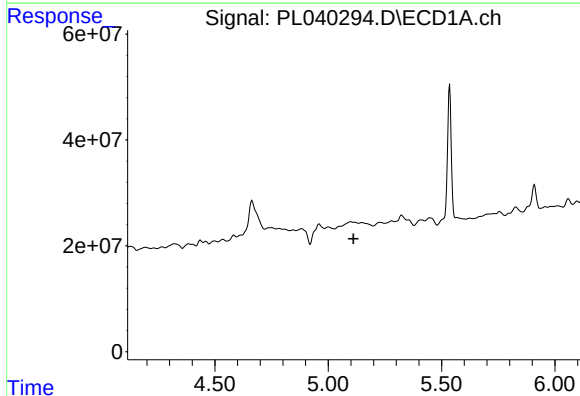


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

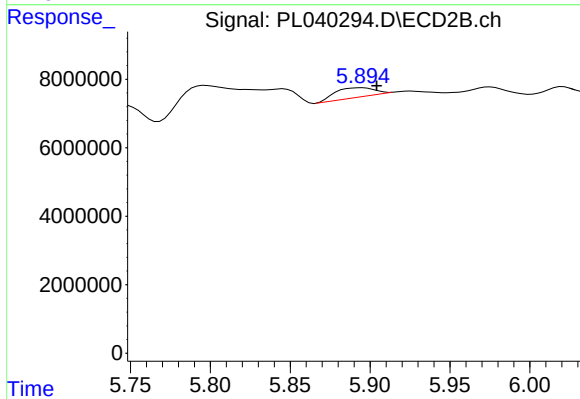

#25 Chlordane-3


R.T.: 5.895 min
Delta R.T.: -0.009 min
Response: 4693801
Conc: 8.78 ng/ml

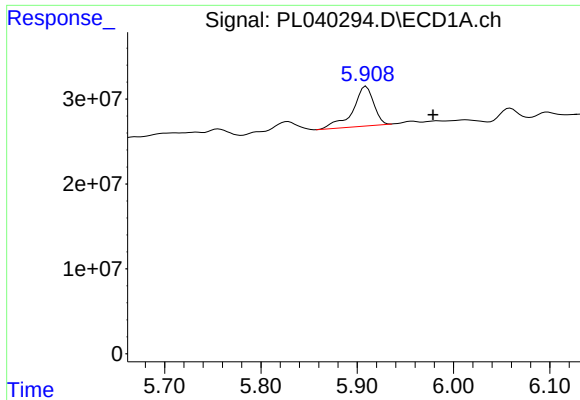

#27 Chlordane-5


R.T.: 5.909 min
Delta R.T.: -0.070 min
Response: 70402052
Conc: 169.75 ng/ml

Instrument :
ECD_L
ClientSampleId :

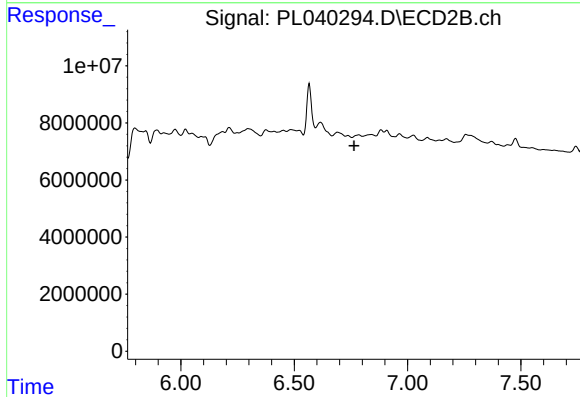


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

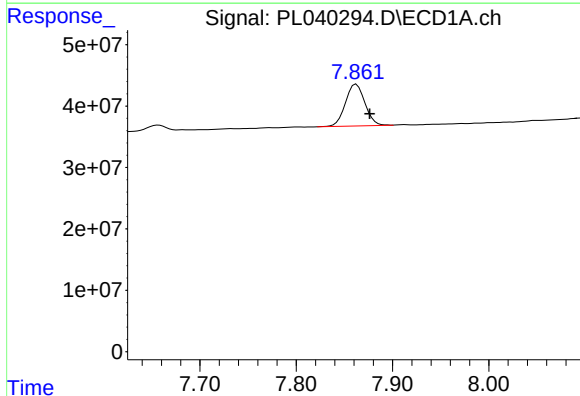

#28 Decachlorobiphenyl

R.T.: 7.862 min
Delta R.T.: -0.014 min
Response: 95391168
Conc: 10.77 ng/ml

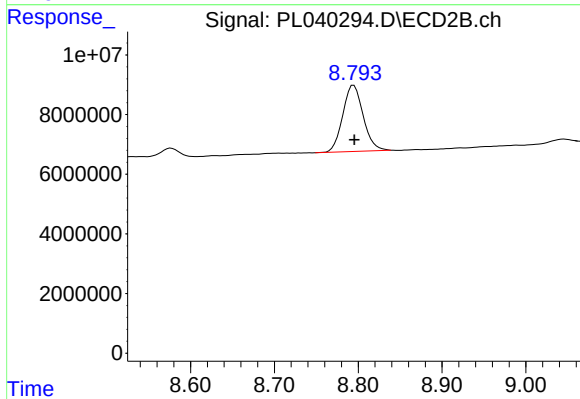

#28 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 37839587
Conc: 11.83 ng/ml