

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
 Data File : PL040296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 11:53
 Operator : AJ\SJ
 Sample : J4770-05
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:03:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.238	3.843	99602219	38273096	13.092	11.720
28)	SA Decachlor...	7.862	8.795	77509833	32258251	8.752	10.082
Target Compounds							
3)	MA gamma-BHC...	3.975f	0.000	191.5E6	0	17.350	N.D. #
7)	B delta-BHC	0.000	4.884	0	16672855	N.D.	3.686 #
9)	A Endosulfan I	0.000	5.977f	0	5336023	N.D.	1.506 #
11)	B alpha-Chl...	0.000	5.977	0	5336023	N.D.	1.403 #
16)	A 4,4'-DDD	5.909f	6.566f	57000178	28377209	6.596	8.861 #
21)	B Endrin ke...	6.787f	0.000	9198044	0	0.941	N.D. #
26)	Chlordane-4	0.000	5.977	0	5336023	N.D.	8.356 #
27)	Chlordane-5	5.909	0.000	57000178	0	137.434	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
Data File : PL040296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 11:53
Operator : AJ\SJ
Sample : J4770-05
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:03:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

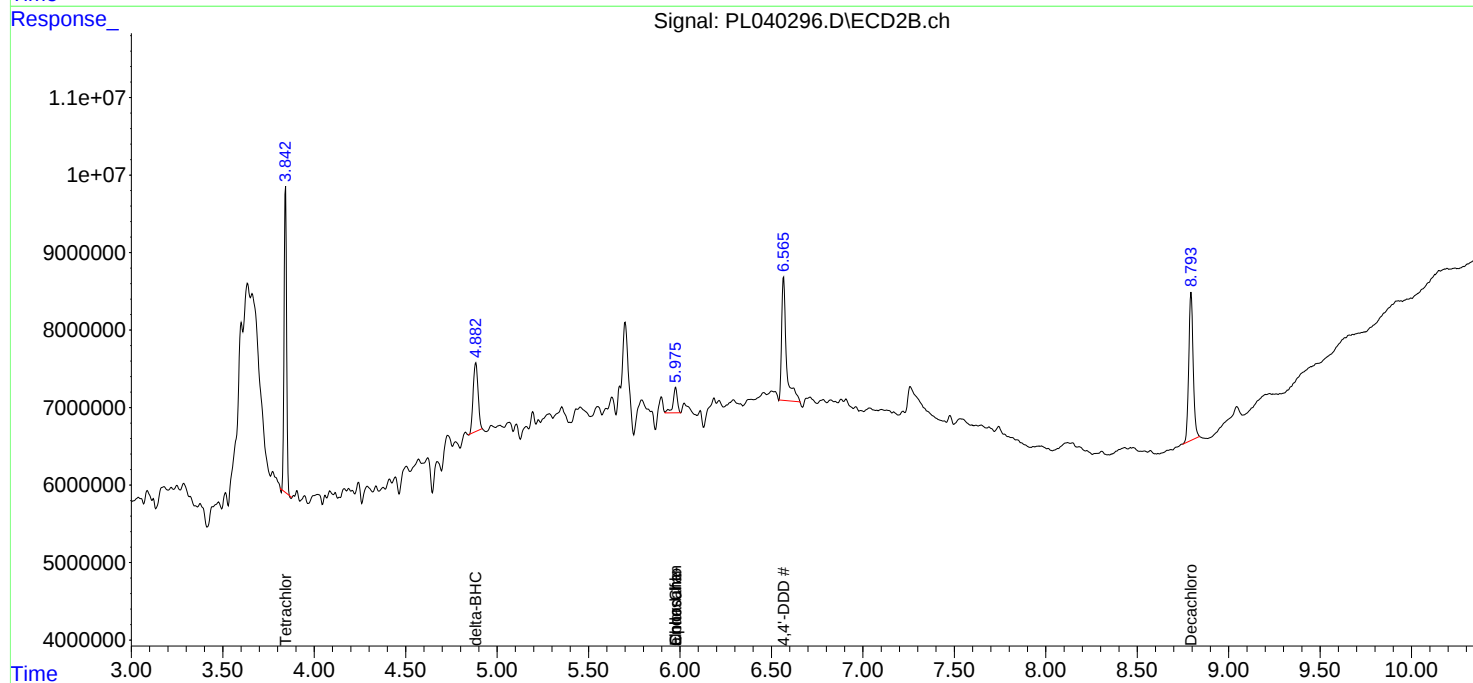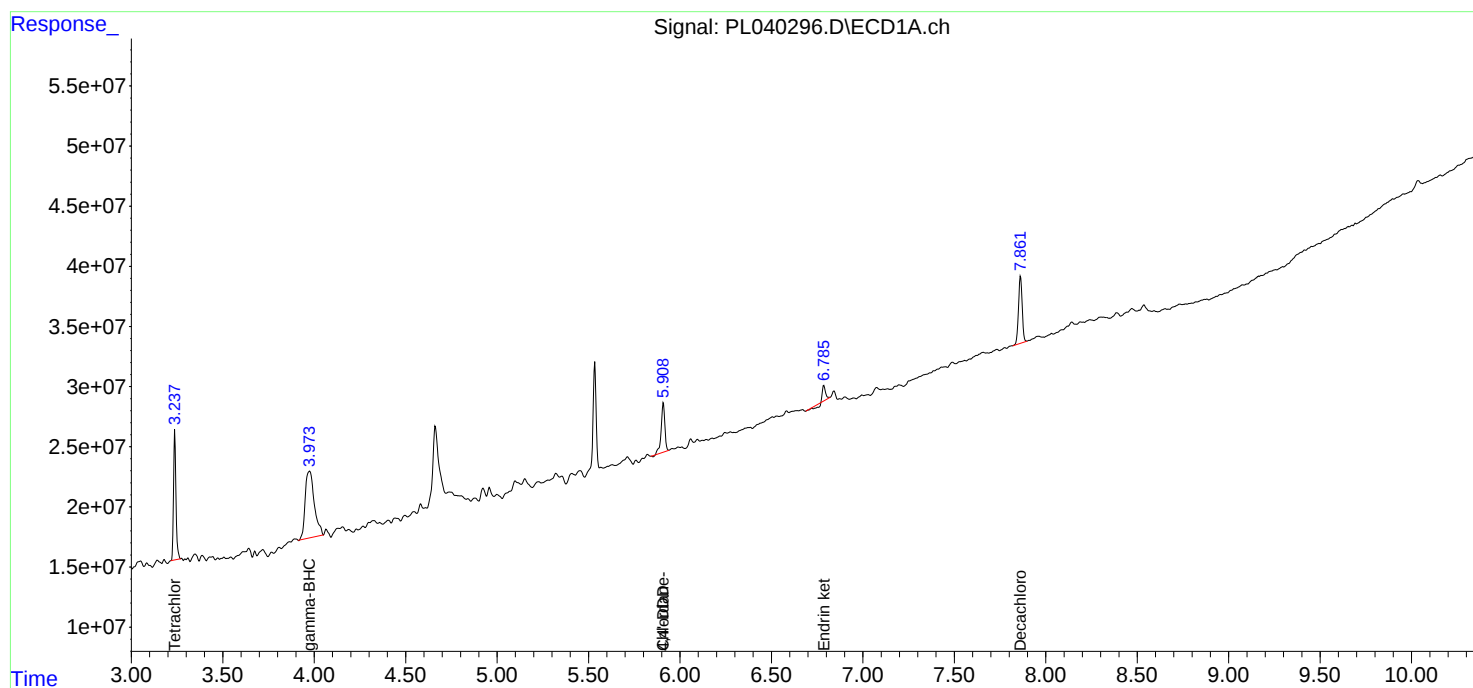


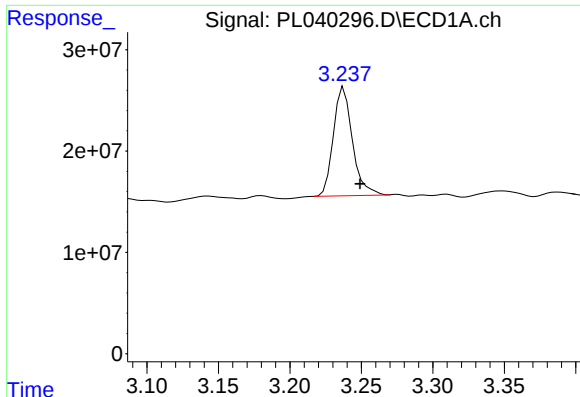

#1 Tetrachloro-m-xylene


R.T.: 3.238 min
Delta R.T.: -0.011 min
Response: 99602219
Conc: 13.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

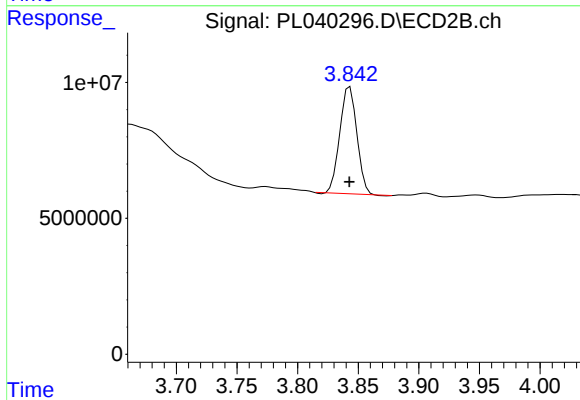


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 38273096
Conc: 11.72 ng/ml

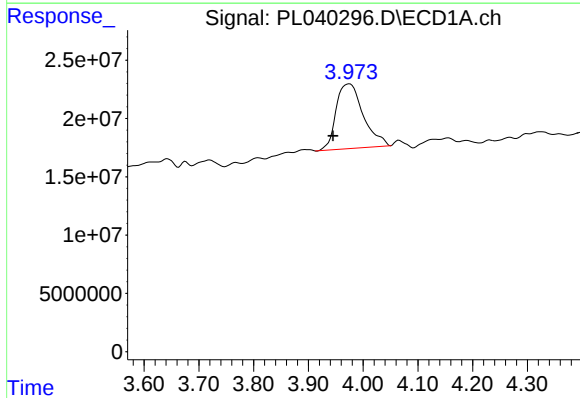


#3 gamma-BHC (Lindane)

R.T.: 3.975 min
Delta R.T.: 0.030 min
Response: 191487222
Conc: 17.35 ng/ml

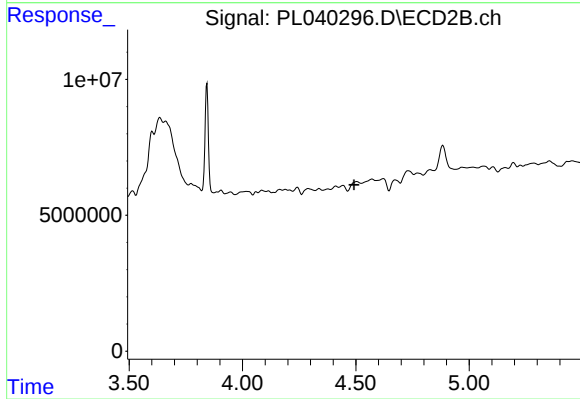

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.493 min
Response: 0
Conc: N.D.

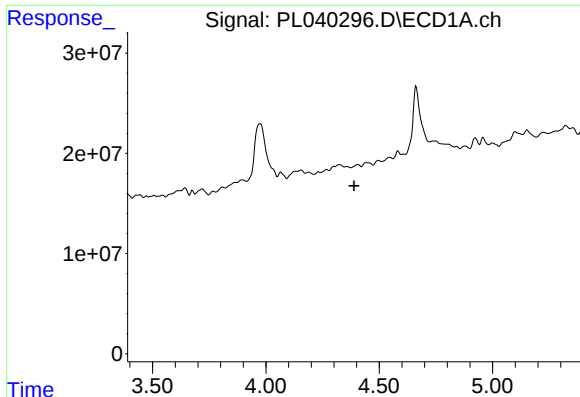

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

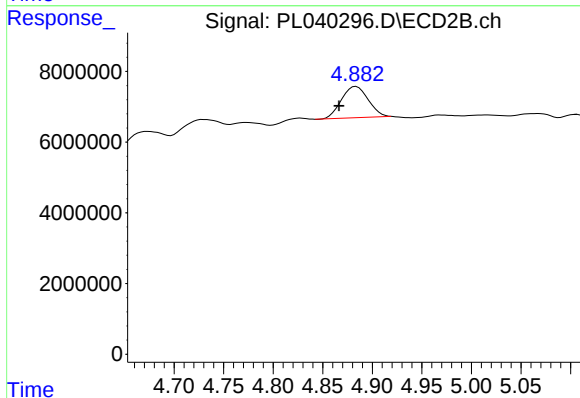


#7 delta-BHC

R.T.: 4.884 min
Delta R.T.: 0.017 min
Response: 16672855
Conc: 3.69 ng/ml

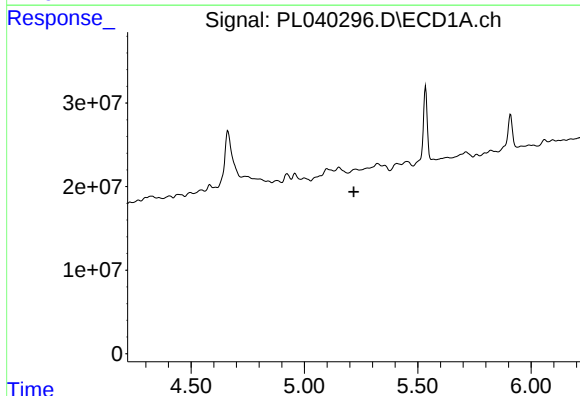


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.217 min
Response: 0
Conc: N.D.

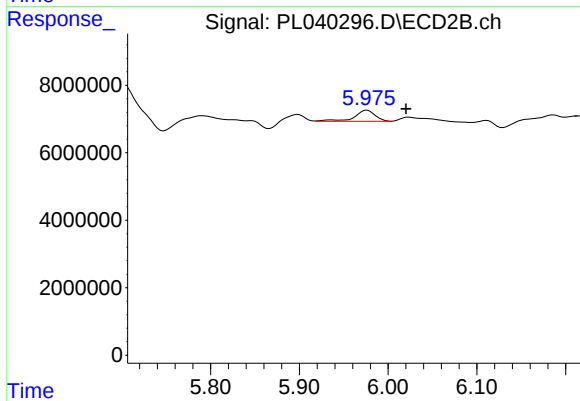

#9 Endosulfan I


R.T.: 5.977 min
Delta R.T.: -0.044 min
Response: 5336023
Conc: 1.51 ng/ml

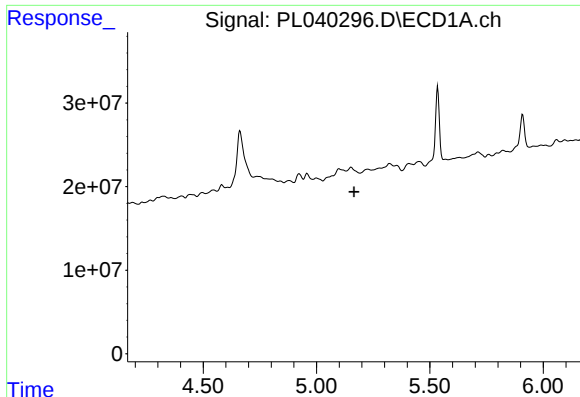

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

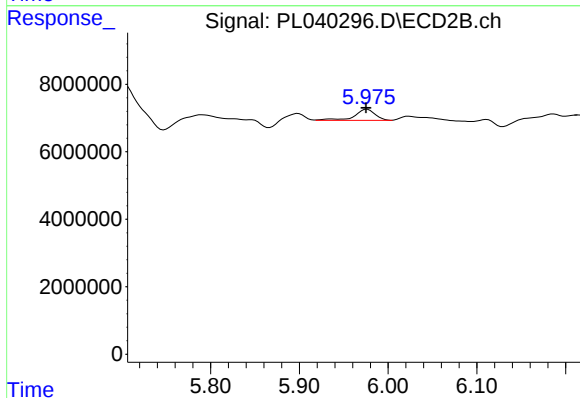


#11 alpha-Chlordane

R.T.: 5.977 min
Delta R.T.: 0.001 min
Response: 5336023
Conc: 1.40 ng/ml

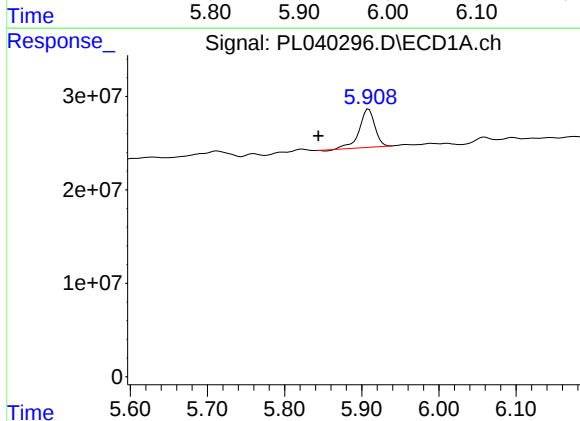


#16 4,4'-DDD

R.T.: 5.909 min
Delta R.T.: 0.065 min
Response: 57000178
Conc: 6.60 ng/ml

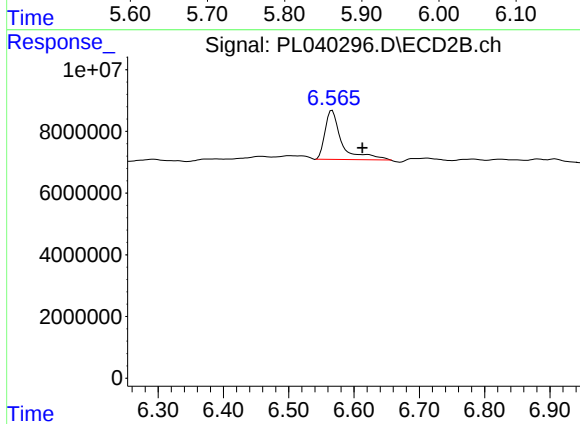

#16 4,4'-DDD


R.T.: 6.566 min
Delta R.T.: -0.047 min
Response: 28377209
Conc: 8.86 ng/ml

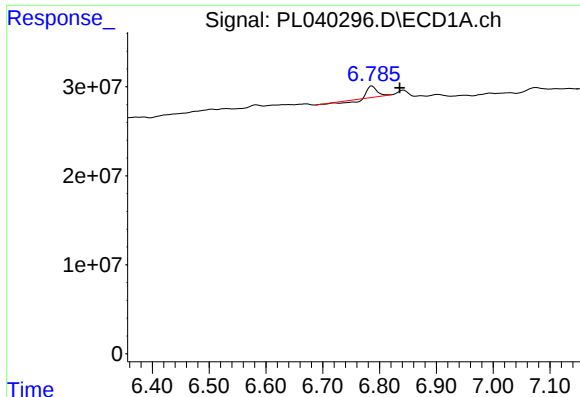

#21 Endrin ketone


R.T.: 6.787 min
Delta R.T.: -0.048 min
Response: 9198044
Conc: 0.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

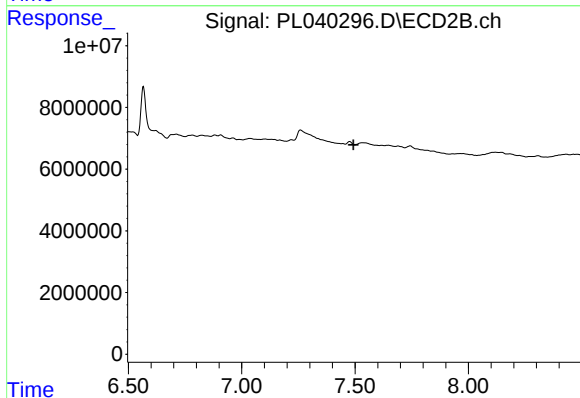


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

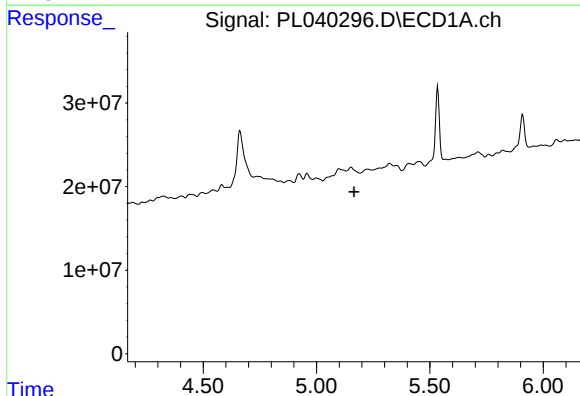


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.166 min
Response: 0
Conc: N.D.

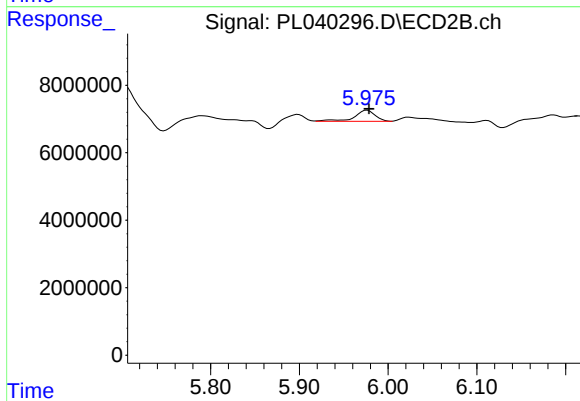

#26 Chlordane-4


R.T.: 5.977 min
Delta R.T.: -0.002 min
Response: 5336023
Conc: 8.36 ng/ml

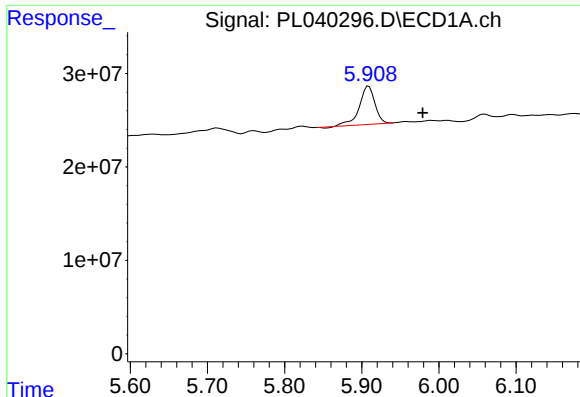

#27 Chlordane-5


R.T.: 5.909 min
Delta R.T.: -0.070 min
Response: 57000178
Conc: 137.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

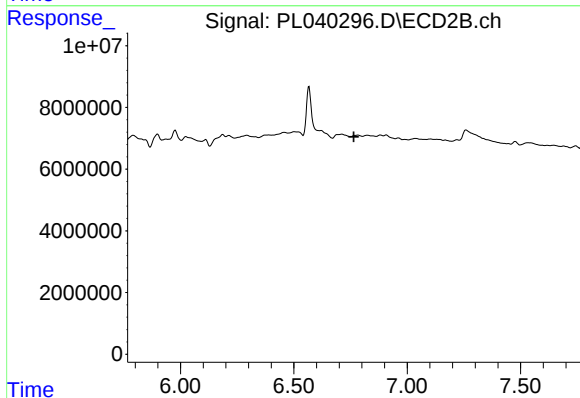


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

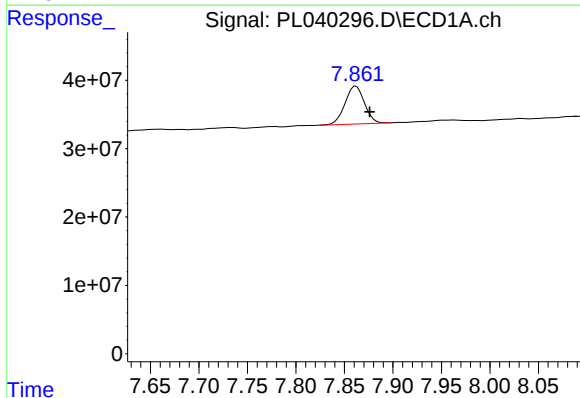

#28 Decachlorobiphenyl

R.T.: 7.862 min
Delta R.T.: -0.014 min
Response: 77509833
Conc: 8.75 ng/ml

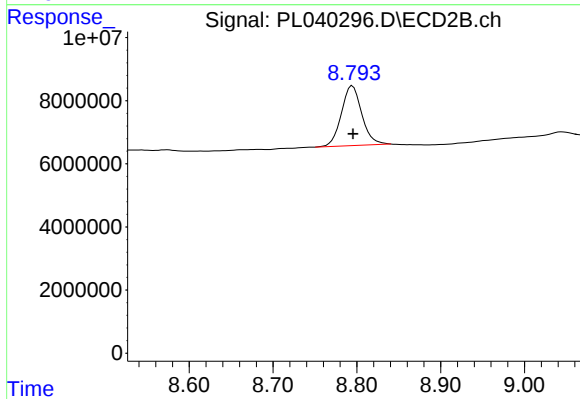

#28 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 32258251
Conc: 10.08 ng/ml