

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
 Data File : PL040304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 13:46
 Operator : AJ\SJ
 Sample : J5042-01
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:05:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.239	3.844	105.1E6	39006134	13.817	11.944
28)	SA Decachlor...	7.863	8.796	56519483	22434988	6.382	7.012
Target Compounds							
3)	MA gamma-BHC...	3.982f	0.000	179.4E6	0	16.257	N.D. #
6)	B beta-BHC	0.000	4.677	0	1754167	N.D.	0.889 #
7)	B delta-BHC	0.000	4.887	0	14434157	N.D.	3.191 #
13)	MA Dieldrin	0.000	6.229f	0	3139595	N.D.	0.862 #
15)	B Endosulfa...	5.910f	0.000	48498257	0	4.668	N.D. #
16)	A 4,4'-DDD	5.830	6.614	71695241	24526894	8.296	7.658
24)	Chlordane-2	4.583	0.000	22799267	0	59.427	N.D. #
27)	Chlordane-5	5.910	0.000	48498257	0	116.935	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
Data File : PL040304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 13:46
Operator : AJ\SJ
Sample : J5042-01
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:05:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

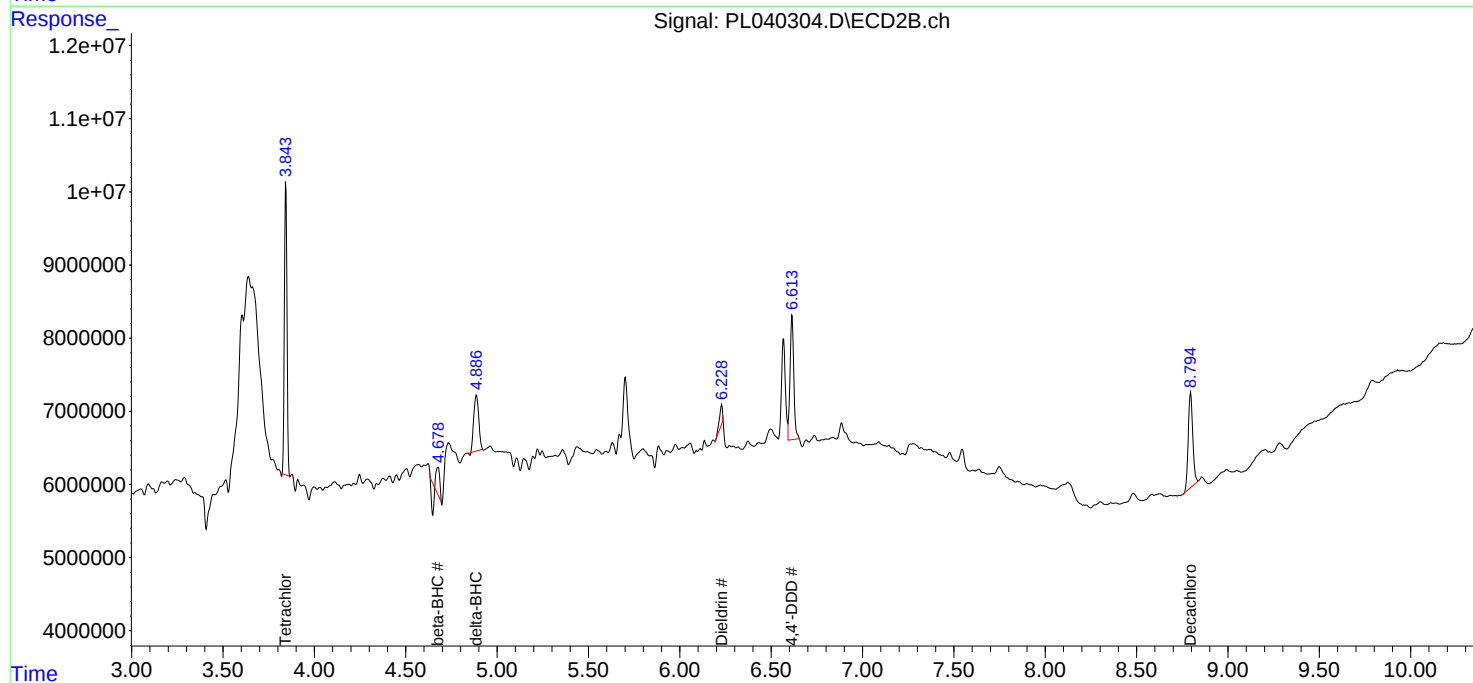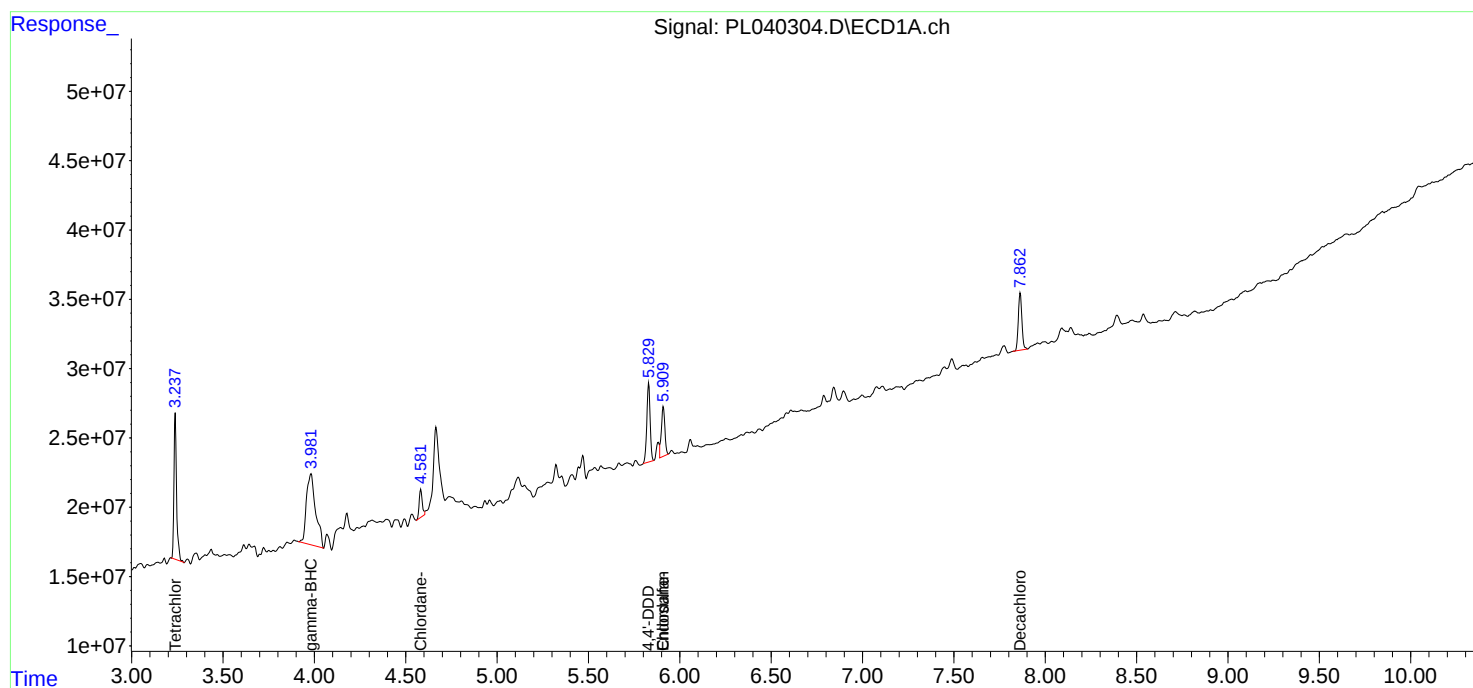


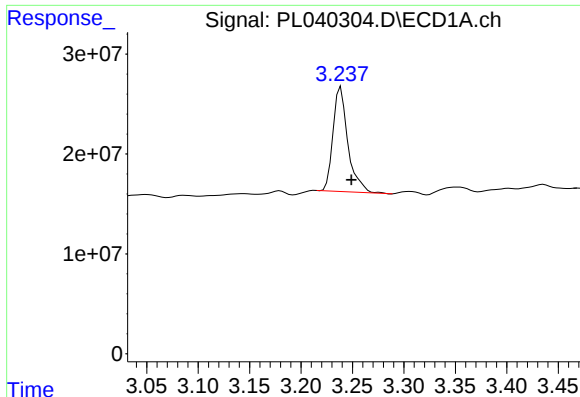

#1 Tetrachloro-m-xylene


R.T.: 3.239 min
Delta R.T.: -0.010 min
Response: 105119333
Conc: 13.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

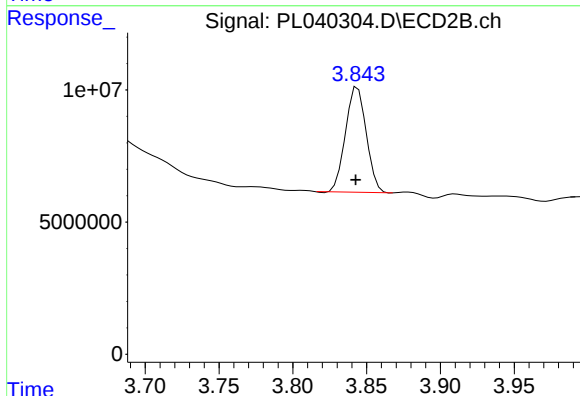


#1 Tetrachloro-m-xylene

R.T.: 3.844 min
Delta R.T.: 0.001 min
Response: 39006134
Conc: 11.94 ng/ml

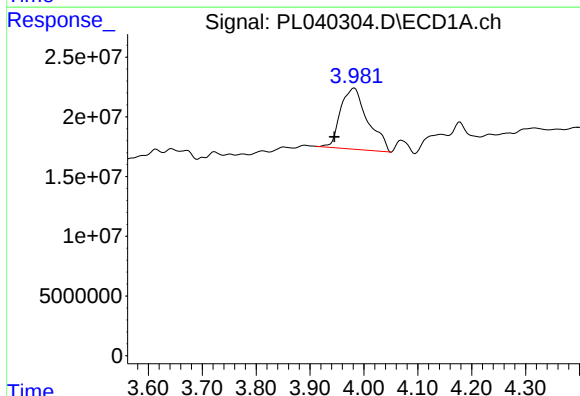


#3 gamma-BHC (Lindane)

R.T.: 3.982 min
Delta R.T.: 0.037 min
Response: 179428926
Conc: 16.26 ng/ml

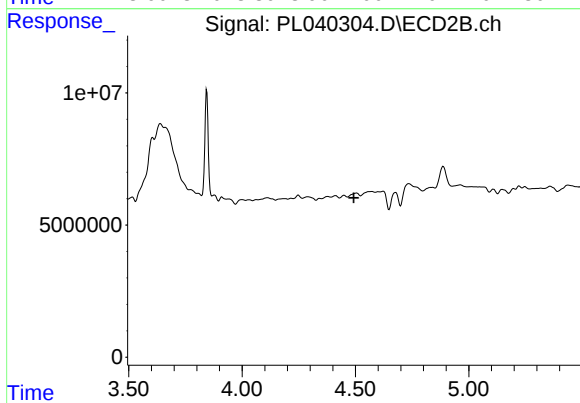

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.493 min
Response: 0
Conc: N.D.

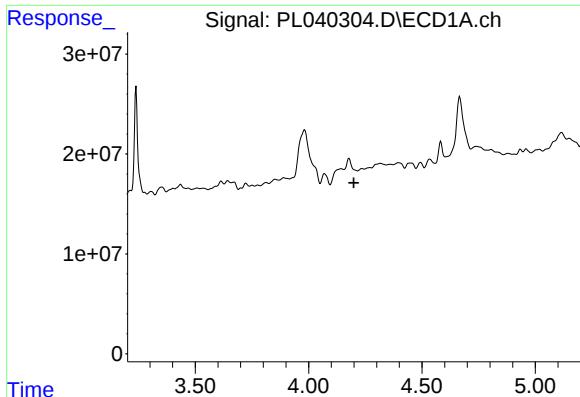

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

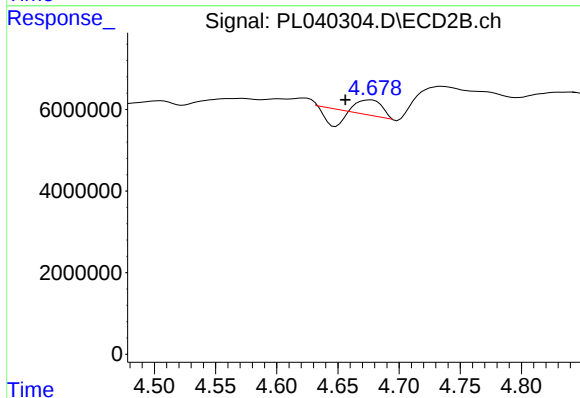


#6 beta-BHC

R.T.: 4.677 min
Delta R.T.: 0.021 min
Response: 1754167
Conc: 0.89 ng/ml

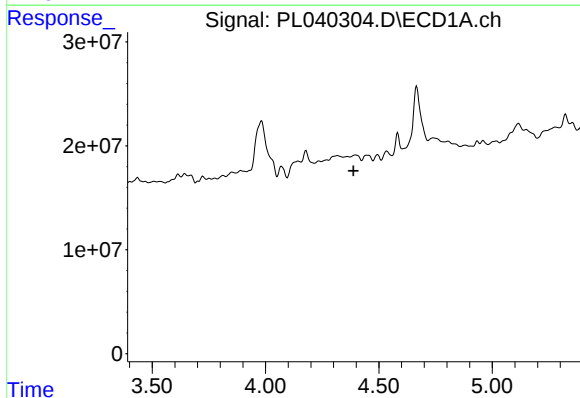


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.389 min
Response: 0
Conc: N.D.

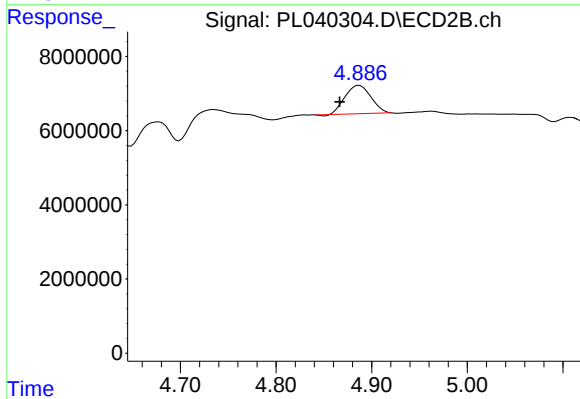

#7 delta-BHC


R.T.: 4.887 min
Delta R.T.: 0.020 min
Response: 14434157
Conc: 3.19 ng/ml

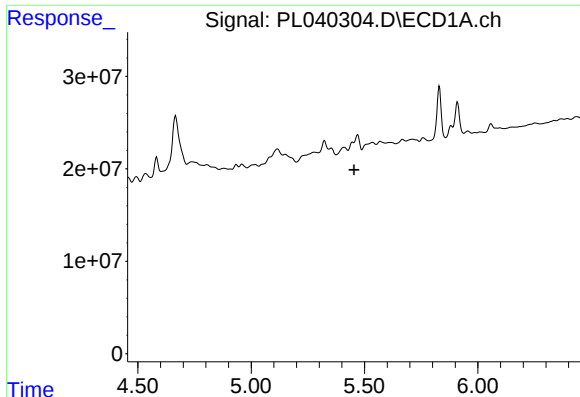

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.454 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

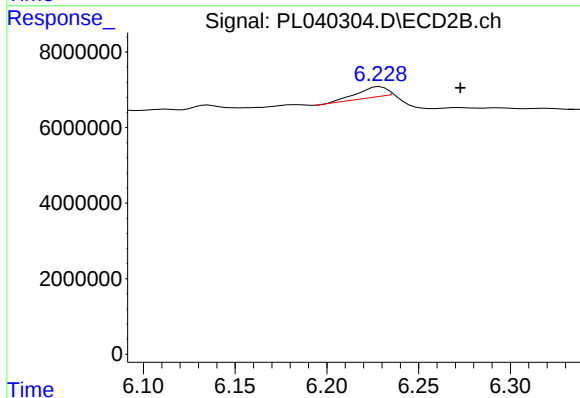


#13 Dieldrin

R.T.: 6.229 min
Delta R.T.: -0.044 min
Response: 3139595
Conc: 0.86 ng/ml

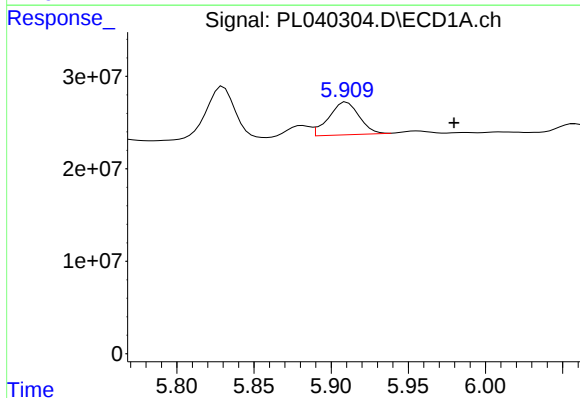


#15 Endosulfan II

R.T.: 5.910 min
Delta R.T.: -0.070 min
Response: 48498257
Conc: 4.67 ng/ml

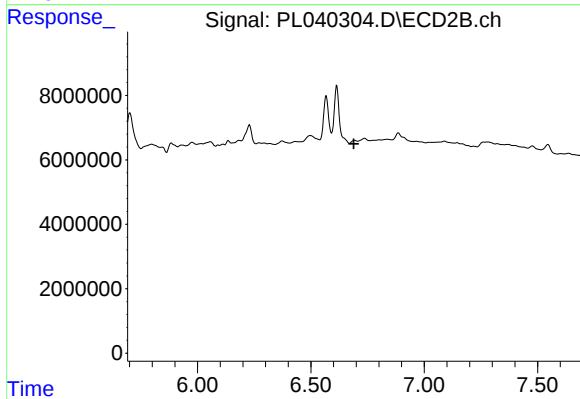

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.690 min
Response: 0
Conc: N.D.

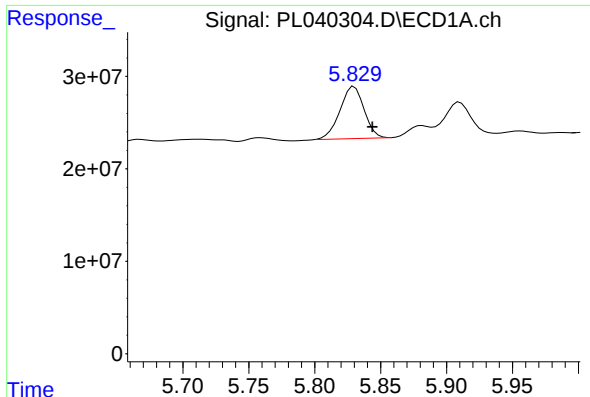

#16 4,4'-DDD


R.T.: 5.830 min
Delta R.T.: -0.014 min
Response: 71695241
Conc: 8.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

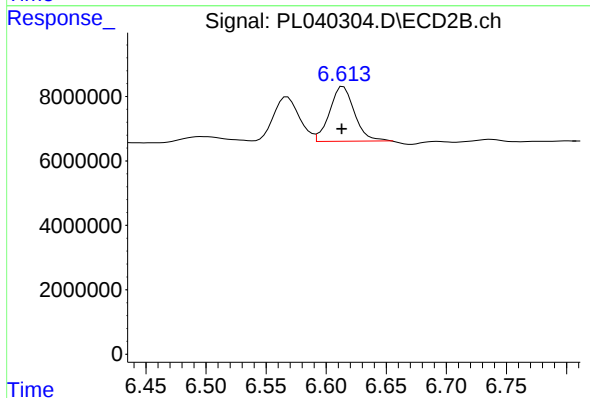


#16 4,4'-DDD

R.T.: 6.614 min
Delta R.T.: 0.001 min
Response: 24526894
Conc: 7.66 ng/ml

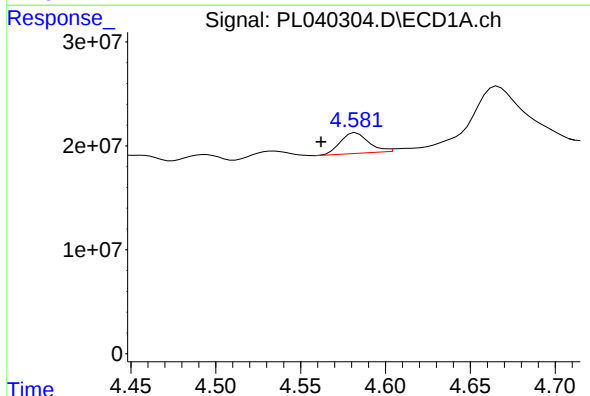


#24 Chlordane-2

R.T.: 4.583 min
Delta R.T.: 0.021 min
Response: 22799267
Conc: 59.43 ng/ml

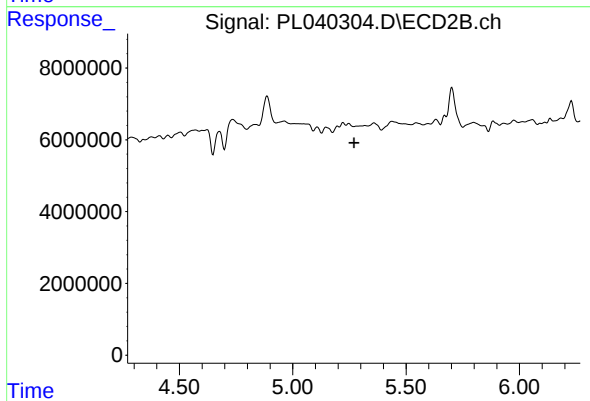

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

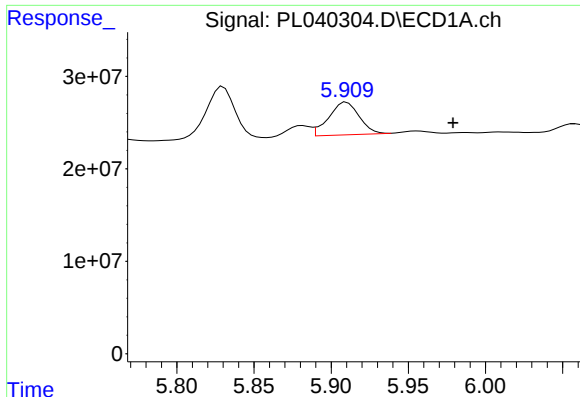

#27 Chlordane-5


R.T.: 5.910 min
Delta R.T.: -0.069 min
Response: 48498257
Conc: 116.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

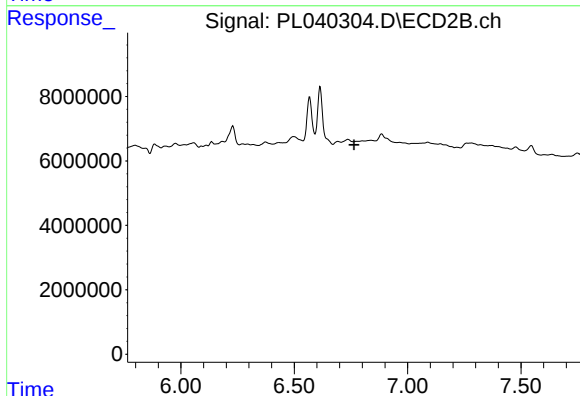


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

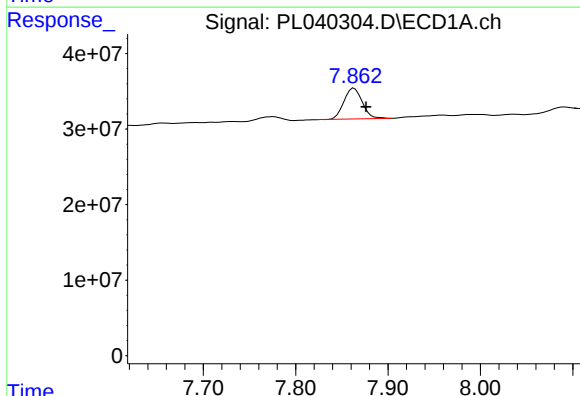

#28 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: -0.013 min
Response: 56519483
Conc: 6.38 ng/ml

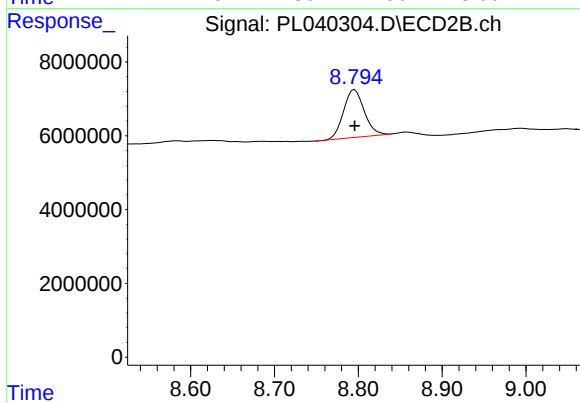

#28 Decachlorobiphenyl

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 22434988
Conc: 7.01 ng/ml