

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
 Data File : PL040324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2018 20:04
 Operator : AJ\SJ
 Sample : J5061-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:09:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.238	3.843	167.7E6	74334930	22.039	22.763
28)	SA Decachlor...	7.862	8.795	171.8E6	60812617	19.395	19.006
Target Compounds							
3)	MA gamma-BHC...	3.982f	0.000	117.0E6	0	10.600	N.D. #
7)	B delta-BHC	0.000	4.887	0	9636559	N.D.	2.130 #
8)	B Heptachlo...	4.956f	5.667	29694455	7426342	2.921	2.012 #
12)	B 4,4'-DDE	0.000	6.187f	0	5397120	N.D.	1.424 #
14)	MA Endrin	5.713	0.000	9429437	0	0.958	N.D. #
16)	A 4,4'-DDD	5.908f	6.571f	57125413	90075164	6.610	28.126 #
21)	B Endrin ke...	6.788f	0.000	573.2E6	0	58.647	N.D. #
24)	Chlordane-2	0.000	5.208	0	10079957	N.D.	61.104 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
Data File : PL040324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2018 20:04
Operator : AJ\SJ
Sample : J5061-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:09:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

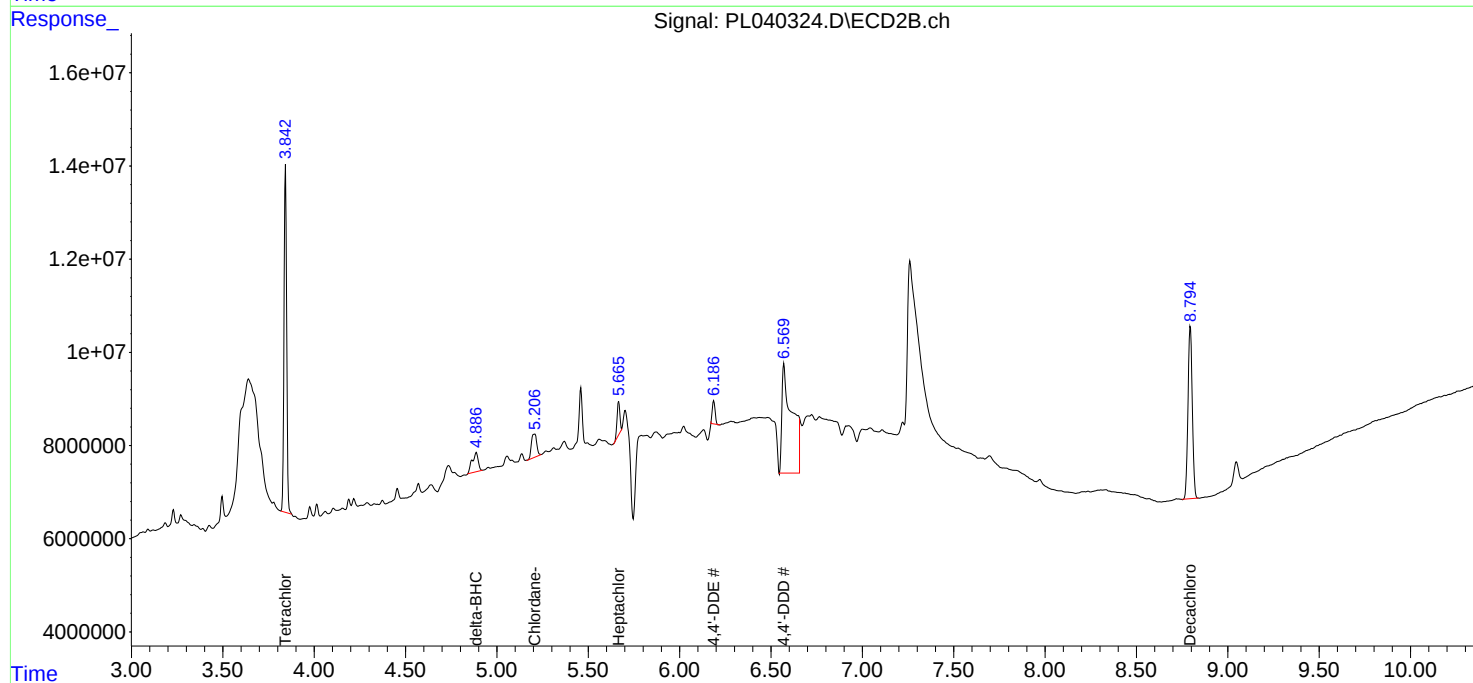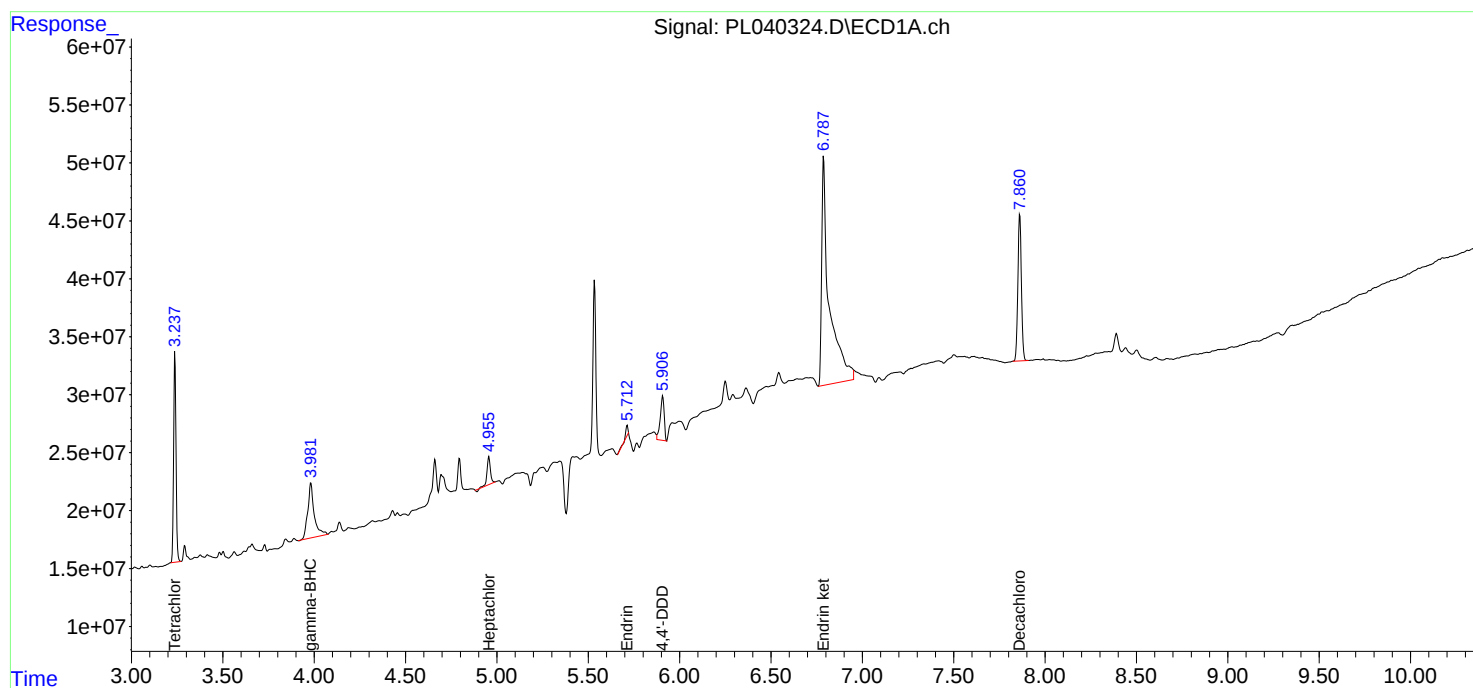


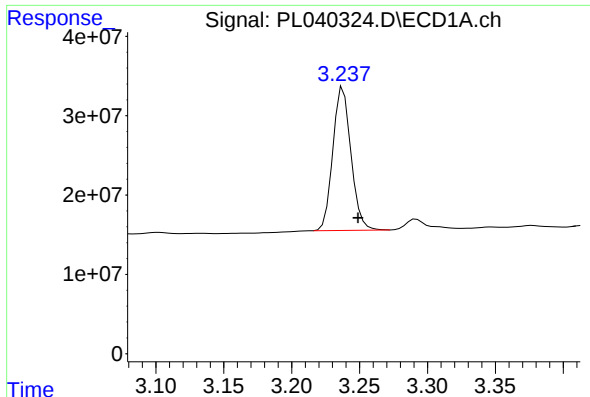

#1 Tetrachloro-m-xylene


R.T.: 3.238 min
Delta R.T.: -0.011 min
Response: 167673633
Conc: 22.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

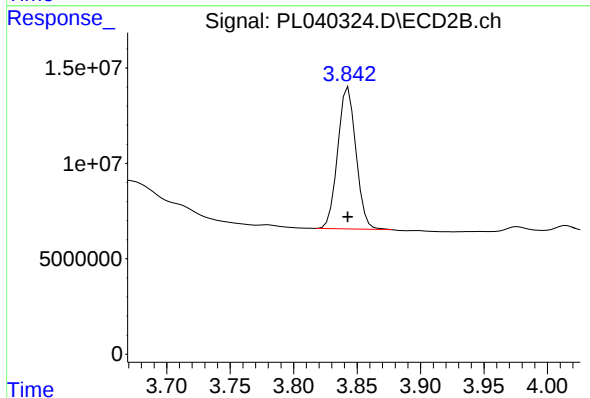


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 74334930
Conc: 22.76 ng/ml

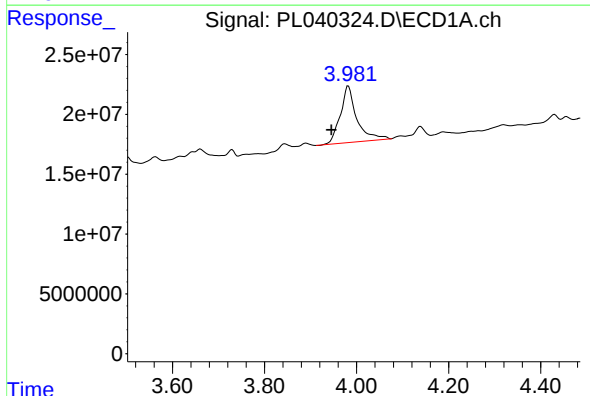


#3 gamma-BHC (Lindane)

R.T.: 3.982 min
Delta R.T.: 0.037 min
Response: 116996023
Conc: 10.60 ng/ml

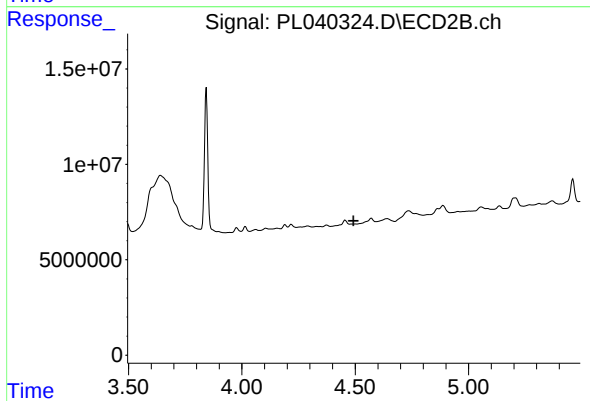

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.493 min
Response: 0
Conc: N.D.

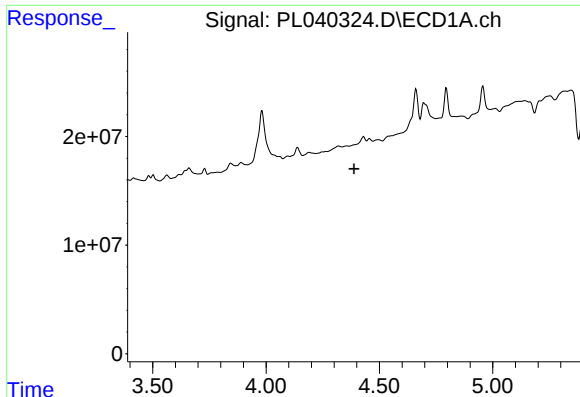

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

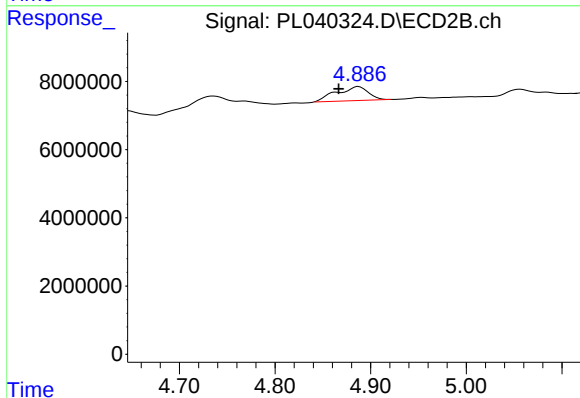


#7 delta-BHC

R.T.: 4.887 min
Delta R.T.: 0.021 min
Response: 9636559
Conc: 2.13 ng/ml

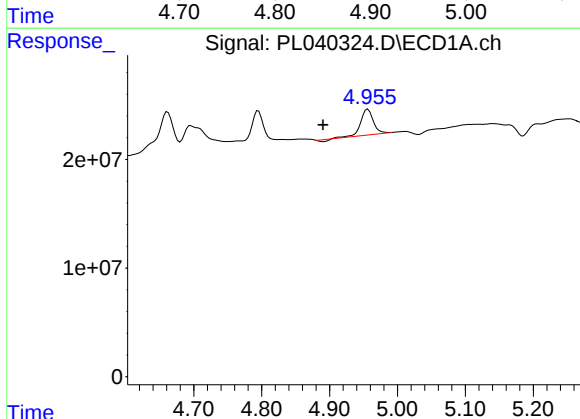


#8 Heptachlor epoxide

R.T.: 4.956 min
Delta R.T.: 0.066 min
Response: 29694455
Conc: 2.92 ng/ml

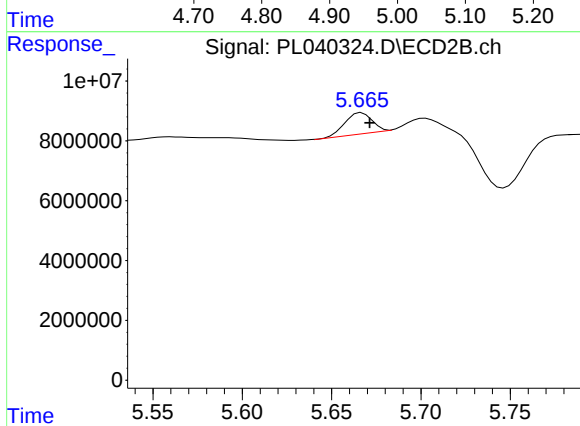

#8 Heptachlor epoxide


R.T.: 5.667 min
Delta R.T.: -0.005 min
Response: 7426342
Conc: 2.01 ng/ml

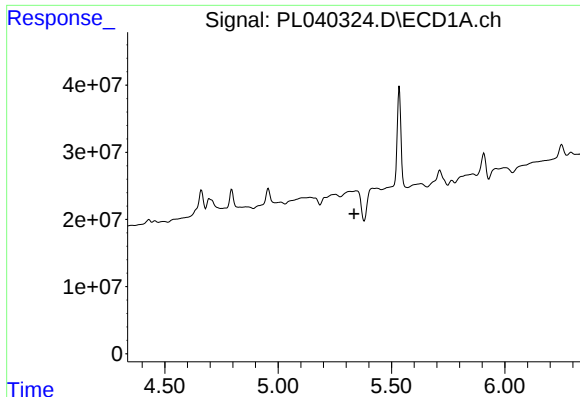

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

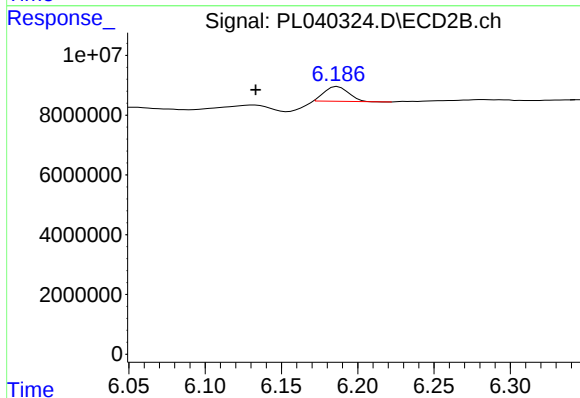


#12 4,4'-DDE

R.T.: 6.187 min
Delta R.T.: 0.054 min
Response: 5397120
Conc: 1.42 ng/ml

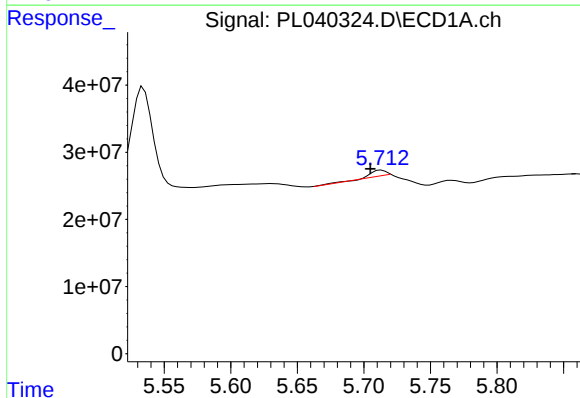


#14 Endrin

R.T.: 5.713 min
Delta R.T.: 0.008 min
Response: 9429437
Conc: 0.96 ng/ml

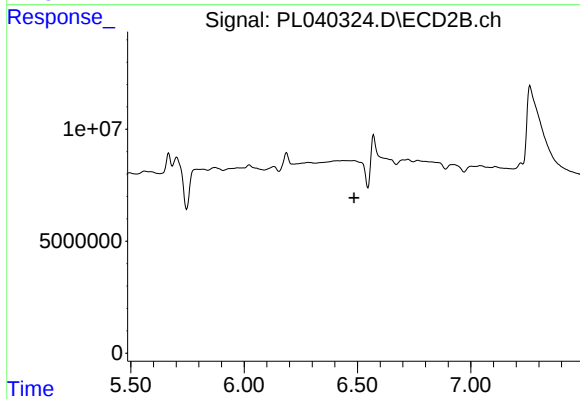

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.485 min
Response: 0
Conc: N.D.

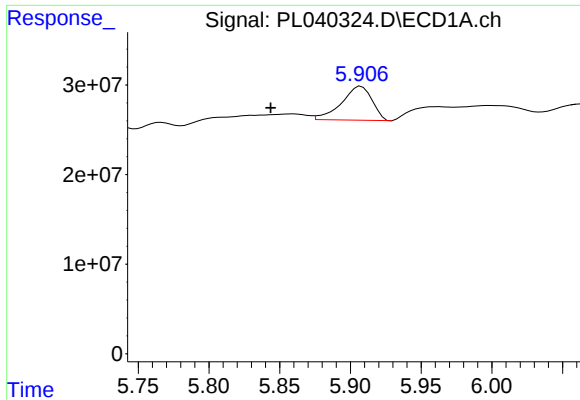

#16 4,4'-DDD


R.T.: 5.908 min
Delta R.T.: 0.064 min
Response: 57125413
Conc: 6.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

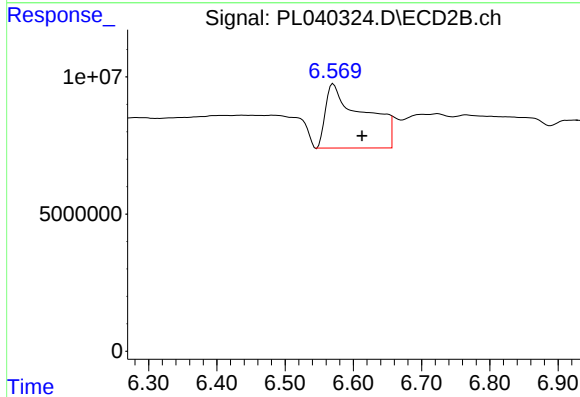


#16 4,4'-DDD

R.T.: 6.571 min
Delta R.T.: -0.042 min
Response: 90075164
Conc: 28.13 ng/ml

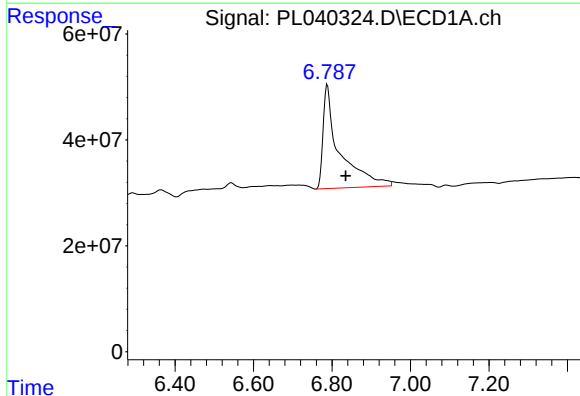


#21 Endrin ketone

R.T.: 6.788 min
Delta R.T.: -0.047 min
Response: 573171613
Conc: 58.65 ng/ml

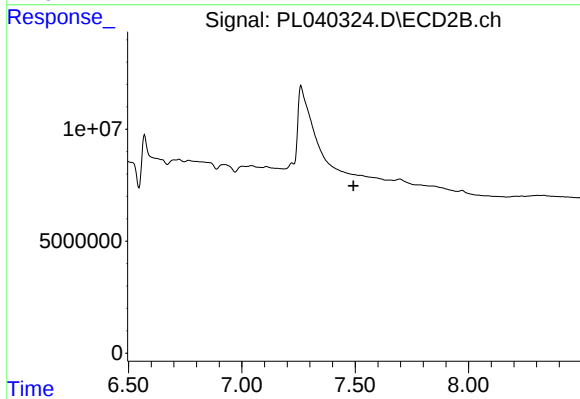

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

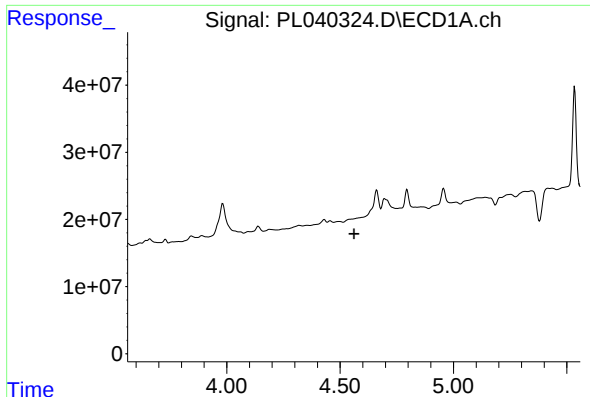

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.562 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

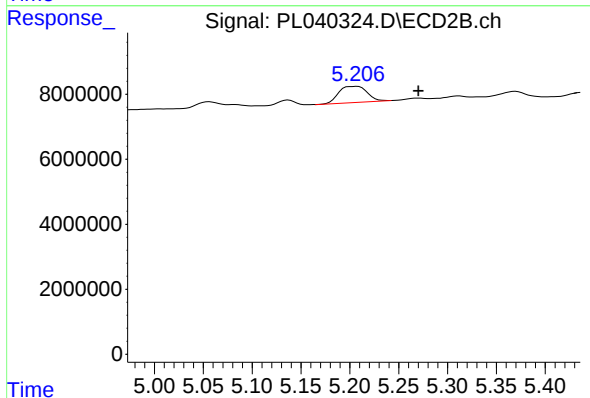


#24 Chlordane-2

R.T.: 5.208 min
Delta R.T.: -0.063 min
Response: 10079957
Conc: 61.10 ng/ml

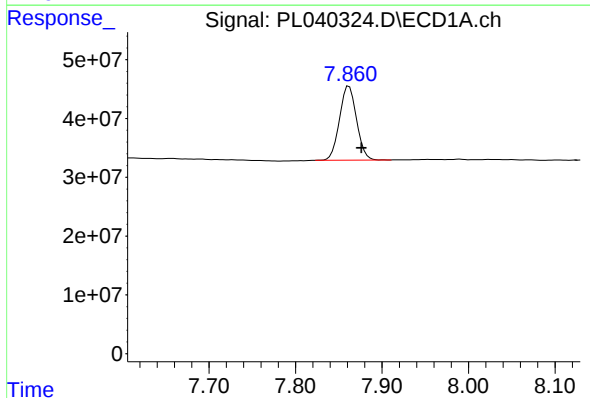

#28 Decachlorobiphenyl

R.T.: 7.862 min
Delta R.T.: -0.014 min
Response: 171755444
Conc: 19.39 ng/ml

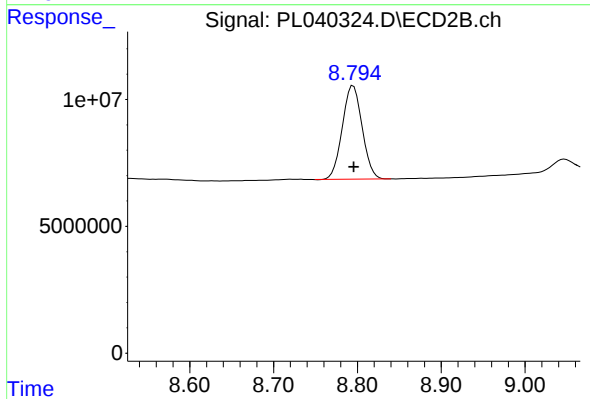

#28 Decachlorobiphenyl

R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 60812617
Conc: 19.01 ng/ml