

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
 Data File : PL040352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2018 03:09
 Operator : AJ\SJ
 Sample : J5055-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 04:02:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.239	3.844	81707505	30887158	10.740	9.458
28)	SA Decachlor...	7.863	8.796	112.3E6	41800820	12.685	13.064
Target Compounds							
4)	MA Heptachlor	4.158f	0.000	4376424	0	0.381	N.D. #
5)	MB Aldrin	4.440	0.000	35519399	0	3.360	N.D. #
6)	B beta-BHC	4.158f	0.000	4376424	0	0.996	N.D. #
7)	B delta-BHC	4.348f	4.888	24869551	8162406	2.229	1.805
15)	B Endosulfa...	5.910f	0.000	40745076	0	3.922	N.D. #
16)	A 4,4'-DDD	5.910f	6.567f	40745076	13253113	4.715	4.138
21)	B Endrin ke...	6.894f	0.000	2658683	0	0.272	N.D. #
23)	Chlordane-1	4.079	0.000	36587331	0	97.208	N.D. #
27)	Chlordane-5	5.910	0.000	40745076	0	98.241	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
Data File : PL040352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2018 03:09
Operator : AJ\SJ
Sample : J5055-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 04:02:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

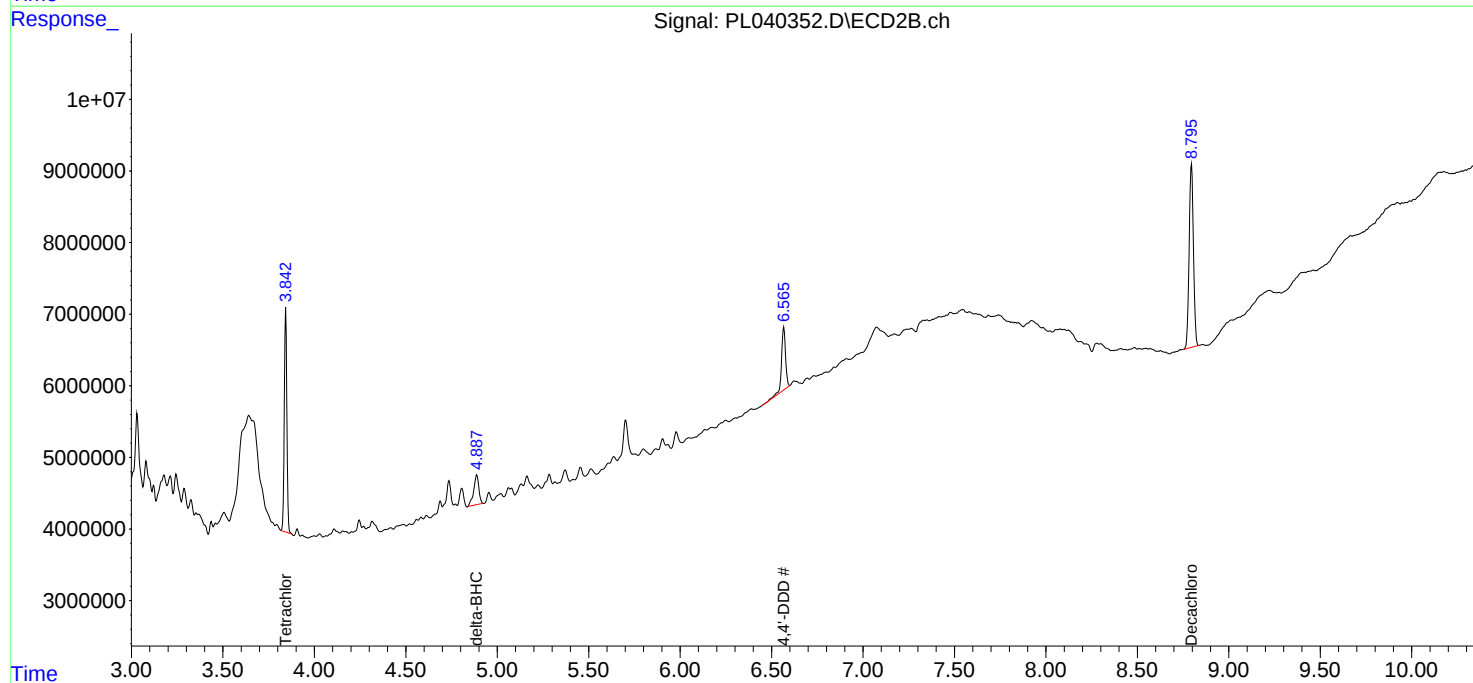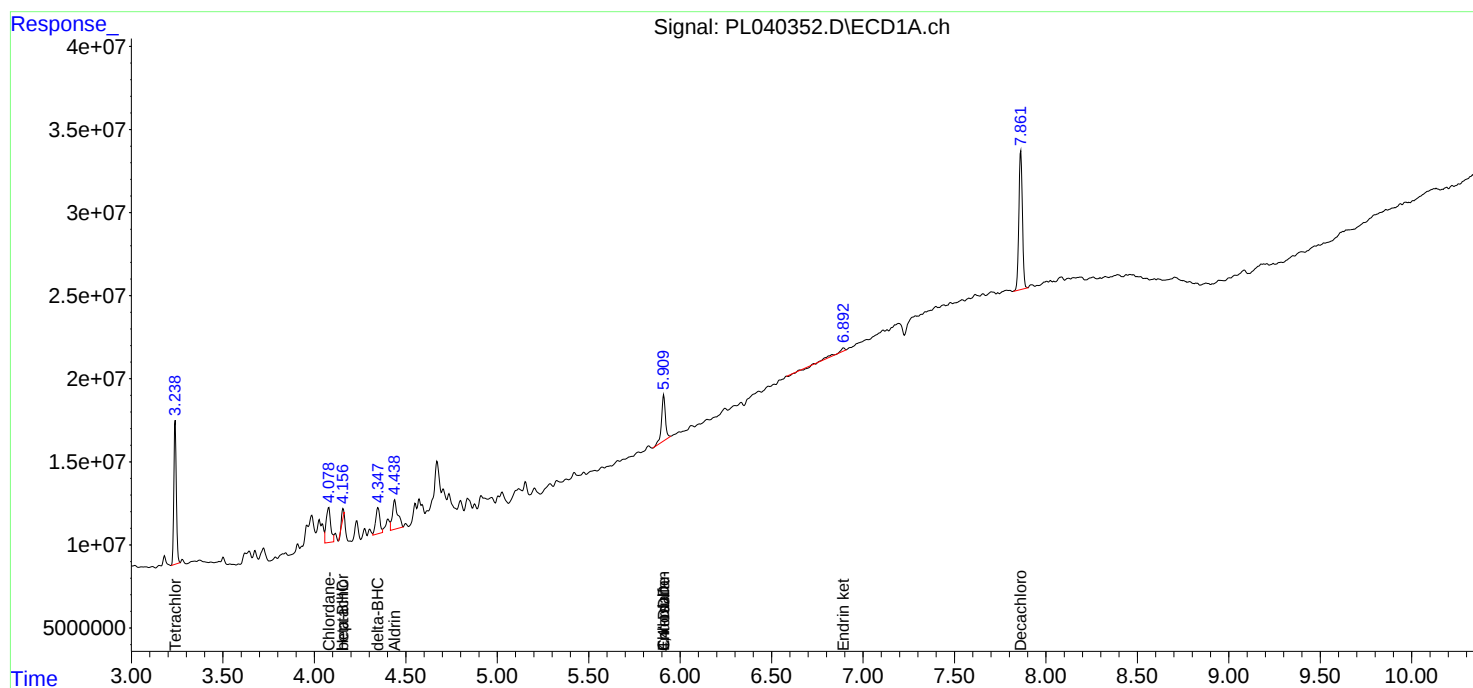


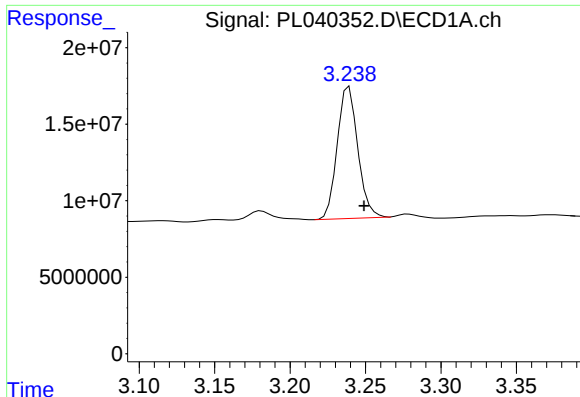

#1 Tetrachloro-m-xylene


R.T.: 3.239 min
Delta R.T.: -0.010 min
Response: 81707505
Conc: 10.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

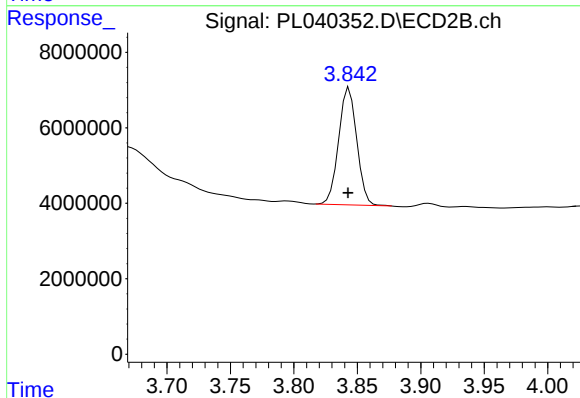


#1 Tetrachloro-m-xylene

R.T.: 3.844 min
Delta R.T.: 0.001 min
Response: 30887158
Conc: 9.46 ng/ml

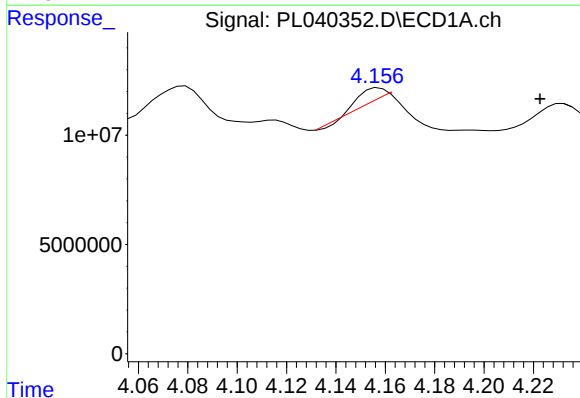


#4 Heptachlor

R.T.: 4.158 min
Delta R.T.: -0.065 min
Response: 4376424
Conc: 0.38 ng/ml

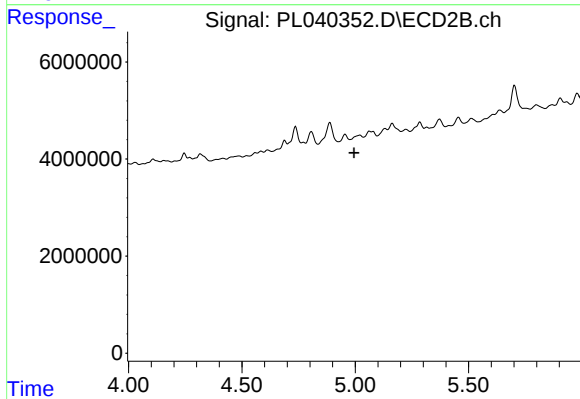

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.995 min
Response: 0
Conc: N.D.

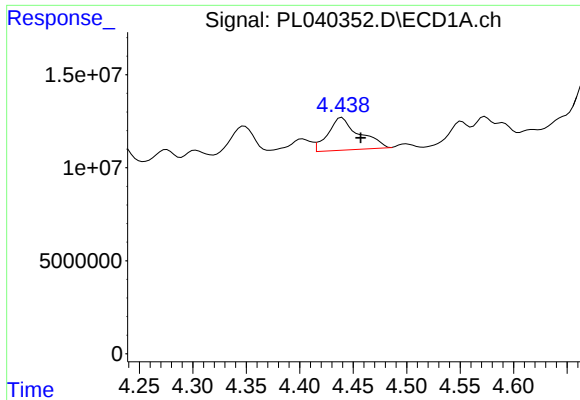

#5 Aldrin


R.T.: 4.440 min
Delta R.T.: -0.018 min
Response: 35519399
Conc: 3.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

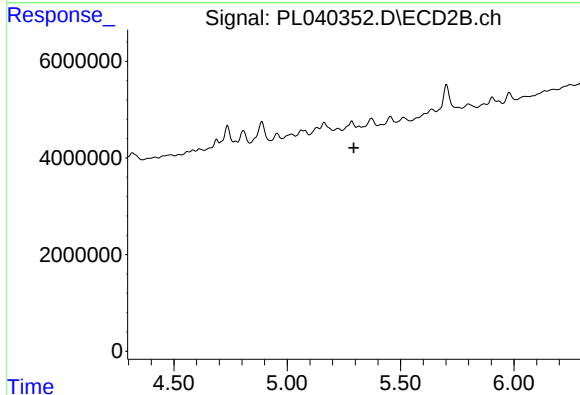


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

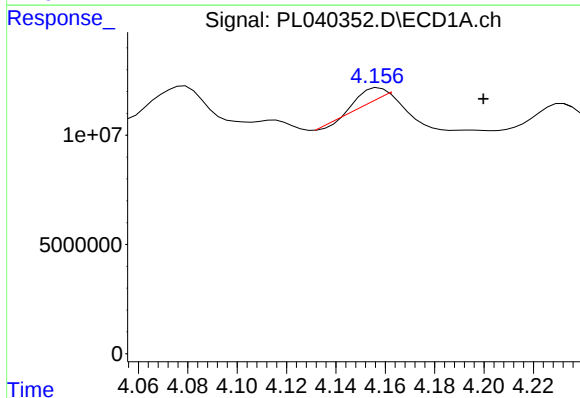


#6 beta-BHC

R.T.: 4.158 min
Delta R.T.: -0.042 min
Response: 4376424
Conc: 1.00 ng/ml

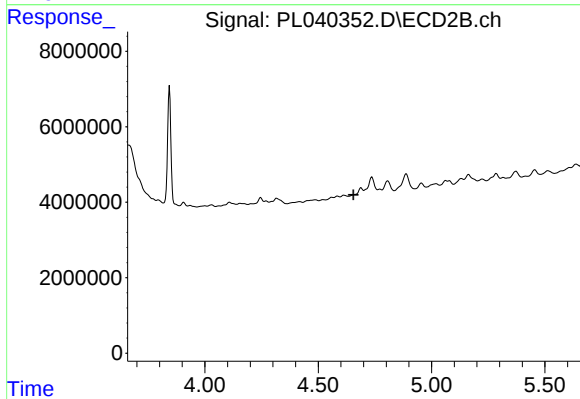

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.656 min
Response: 0
Conc: N.D.

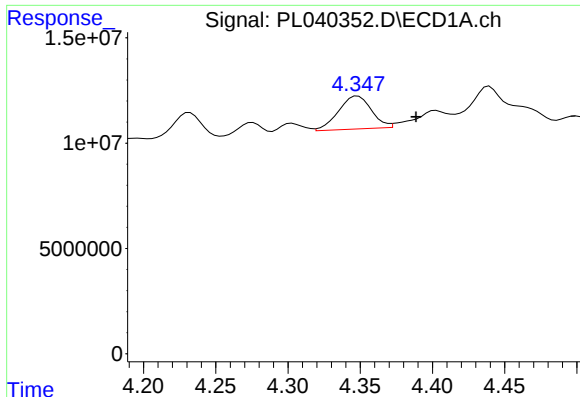

#7 delta-BHC


R.T.: 4.348 min
Delta R.T.: -0.040 min
Response: 24869551
Conc: 2.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

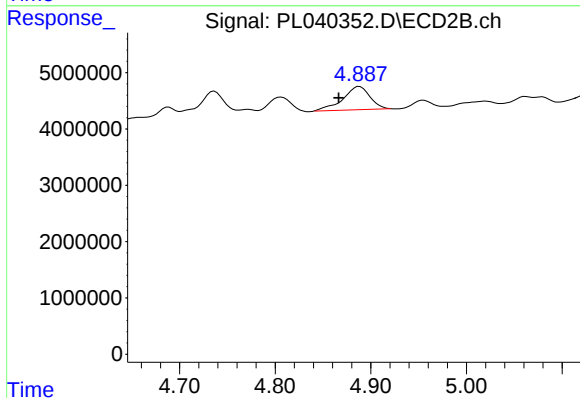


#7 delta-BHC

R.T.: 4.888 min
Delta R.T.: 0.022 min
Response: 8162406
Conc: 1.80 ng/ml

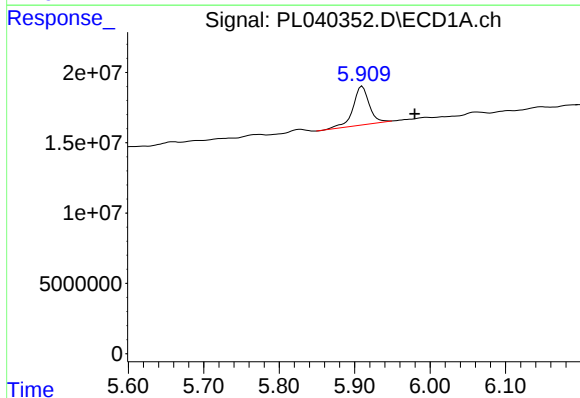


#15 Endosulfan II

R.T.: 5.910 min
Delta R.T.: -0.069 min
Response: 40745076
Conc: 3.92 ng/ml

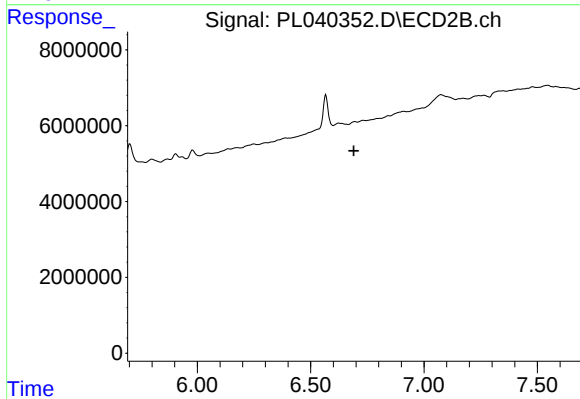

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.690 min
Response: 0
Conc: N.D.

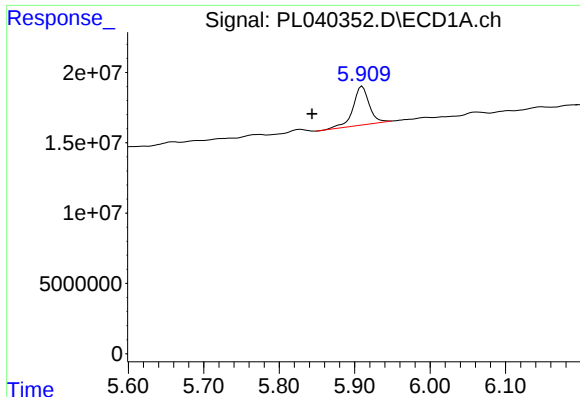

#16 4,4'-DDD


R.T.: 5.910 min
Delta R.T.: 0.067 min
Response: 40745076
Conc: 4.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

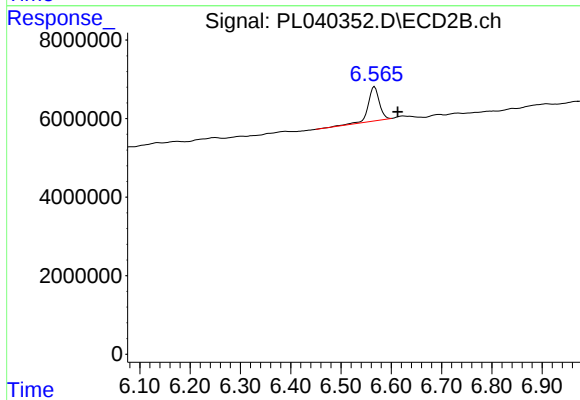


#16 4,4'-DDD

R.T.: 6.567 min
Delta R.T.: -0.046 min
Response: 13253113
Conc: 4.14 ng/ml

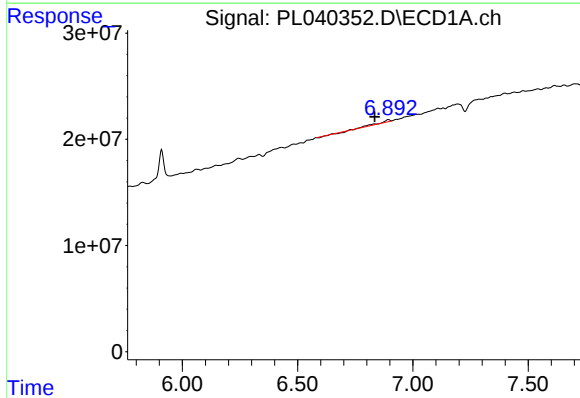


#21 Endrin ketone

R.T.: 6.894 min
Delta R.T.: 0.058 min
Response: 2658683
Conc: 0.27 ng/ml

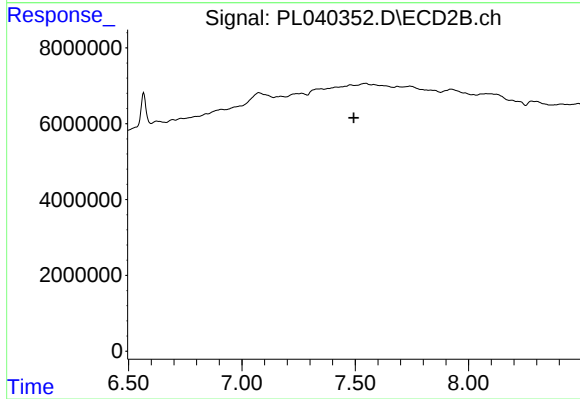

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

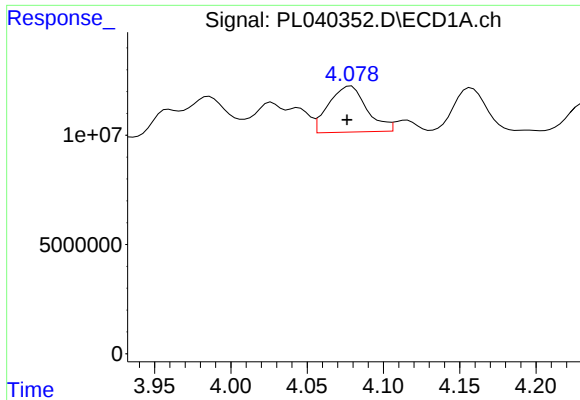

#23 Chlordane-1


R.T.: 4.079 min
Delta R.T.: 0.003 min
Response: 36587331
Conc: 97.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

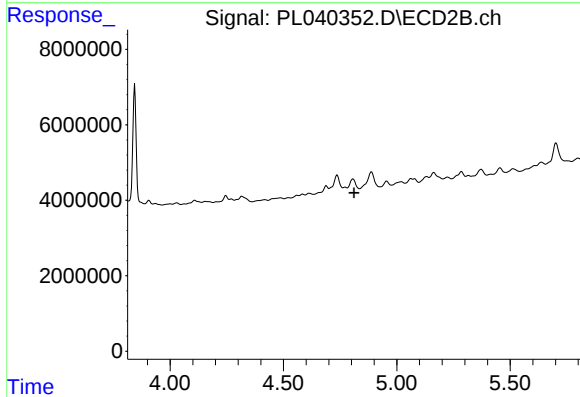


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.812 min
Response: 0
Conc: N.D.

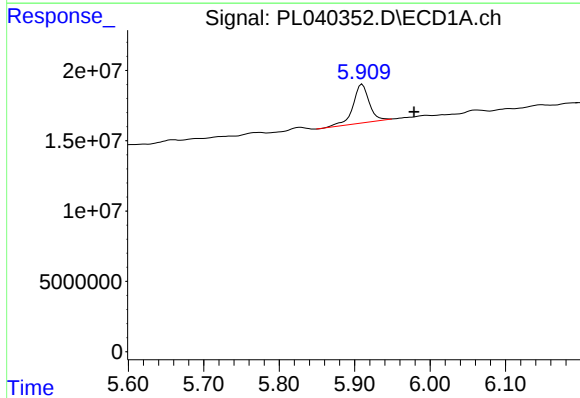


#27 Chlordane-5

R.T.: 5.910 min
Delta R.T.: -0.069 min
Response: 40745076
Conc: 98.24 ng/ml

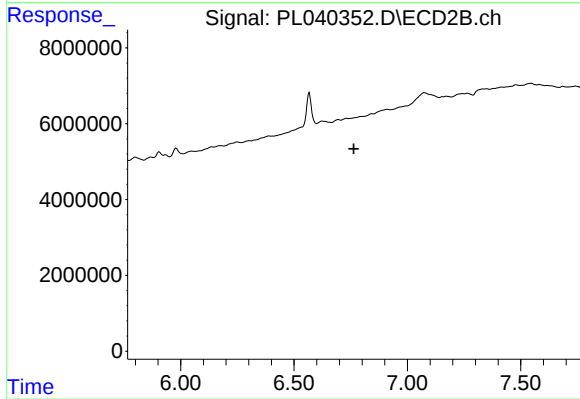

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.764 min
Response: 0
Conc: N.D.

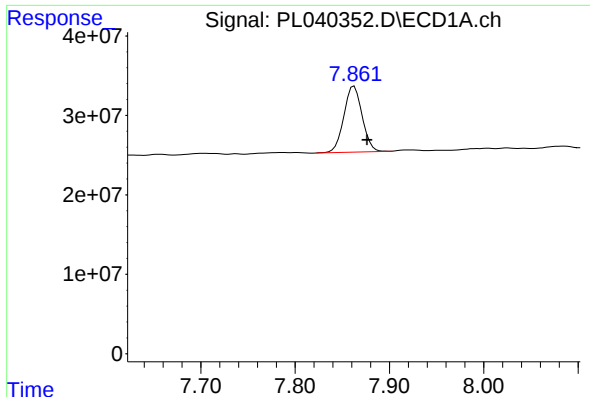

#28 Decachlorobiphenyl

R.T.: 7.863 min
Delta R.T.: -0.014 min
Response: 112334497
Conc: 12.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

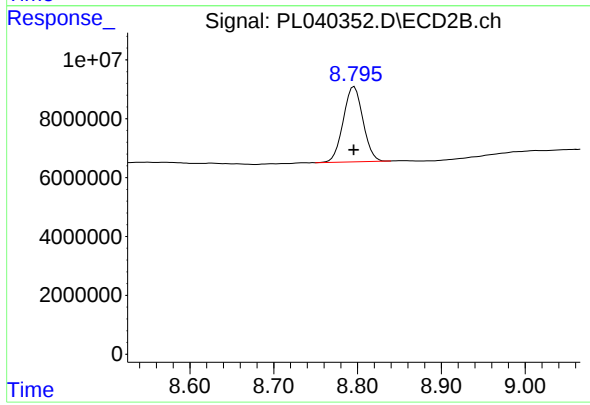

#28 Decachlorobiphenyl

R.T.: 8.796 min
Delta R.T.: 0.000 min
Response: 41800820
Conc: 13.06 ng/ml