

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
 Data File : PL040369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Sep 2018 08:26
 Operator : AJ\SJ
 Sample : J4774-05 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 09:38:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 22 05:31:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	3.843	0	4132743	N.D.	1.266 #
Target Compounds							
3)	MA gamma-BHC...	3.987f	0.000	85625166	0	7.758	N.D. #
6)	B beta-BHC	0.000	4.679	0	199553	N.D.	0.101 #
9)	A Endosulfan I	0.000	6.018	0	1529764	N.D.	0.432 #
10)	B gamma-Chl...	0.000	5.899	0	11858894	N.D.	3.080 #
11)	B alpha-Chl...	0.000	5.977	0	17367421	N.D.	4.567 #
16)	A 4,4'-DDD	5.909f	6.566f	47071227	18480417	5.447	5.770
25)	Chlordane-3	0.000	5.899	0	11858894	N.D.	22.176 #
26)	Chlordane-4	0.000	5.977	0	17367421	N.D.	27.196 #
27)	Chlordane-5	5.909	0.000	47071227	0	113.494	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092518\
Data File : PL040369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Sep 2018 08:26
Operator : AJ\SJ
Sample : J4774-05 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 09:38:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092218.M
Quant Title : GC Extractables
QLast Update : Sat Sep 22 05:31:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

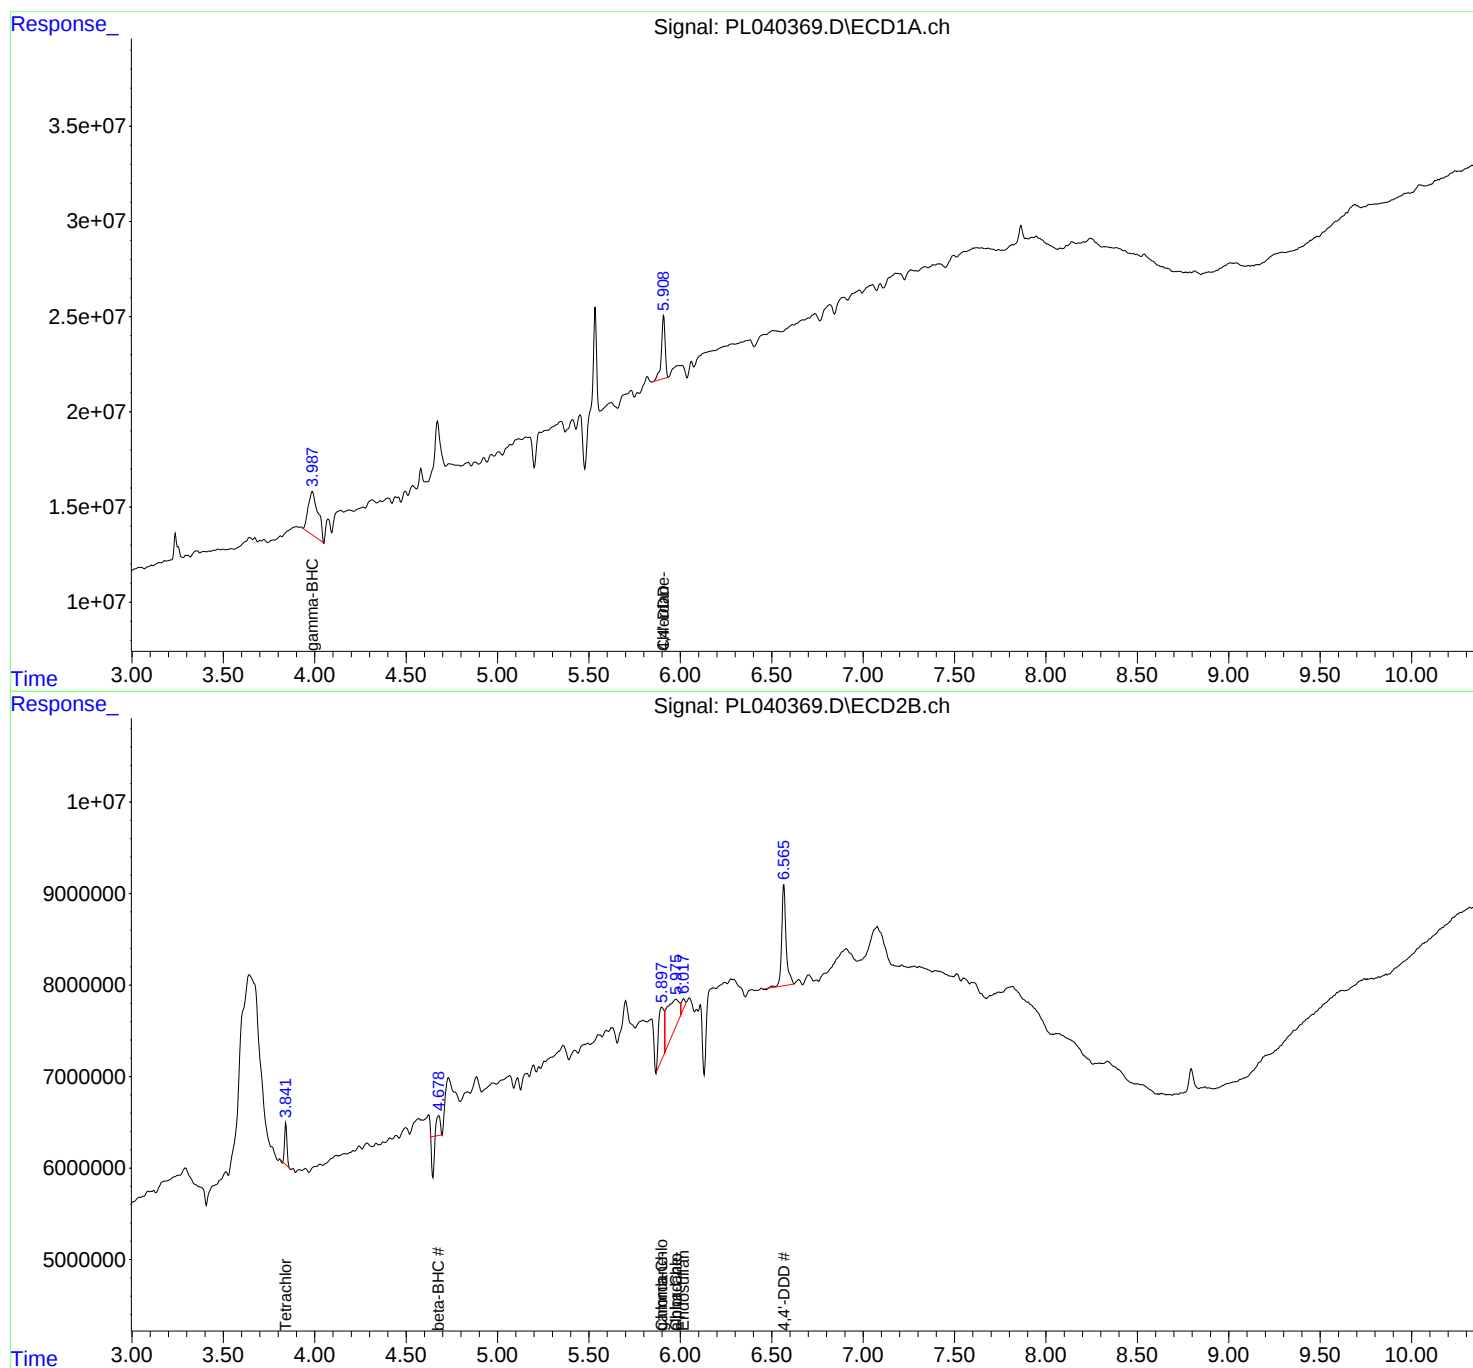


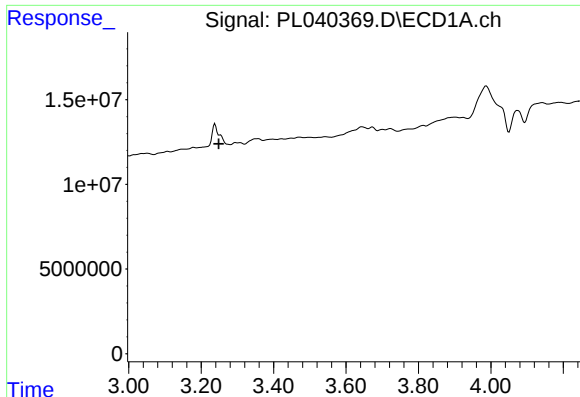

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.249 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

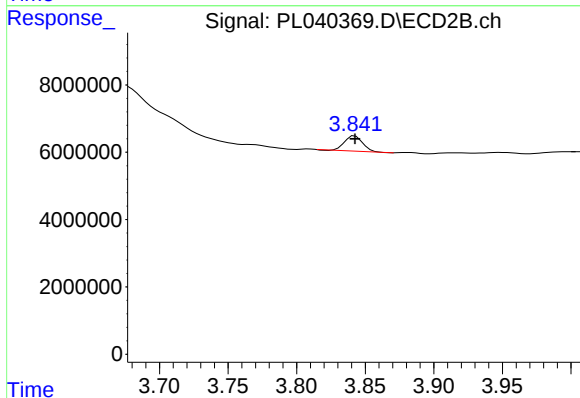


#1 Tetrachloro-m-xylene

R.T.: 3.843 min
Delta R.T.: 0.000 min
Response: 4132743
Conc: 1.27 ng/ml

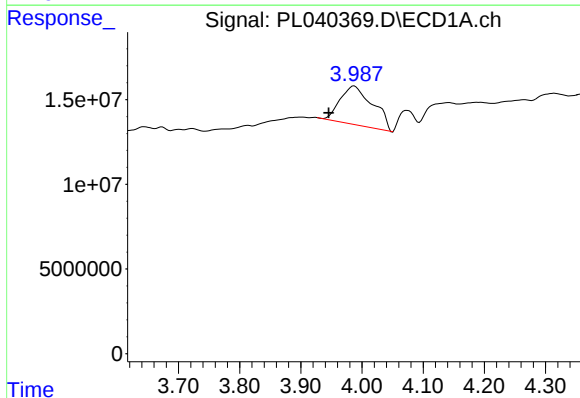


#3 gamma-BHC (Lindane)

R.T.: 3.987 min
Delta R.T.: 0.042 min
Response: 85625166
Conc: 7.76 ng/ml

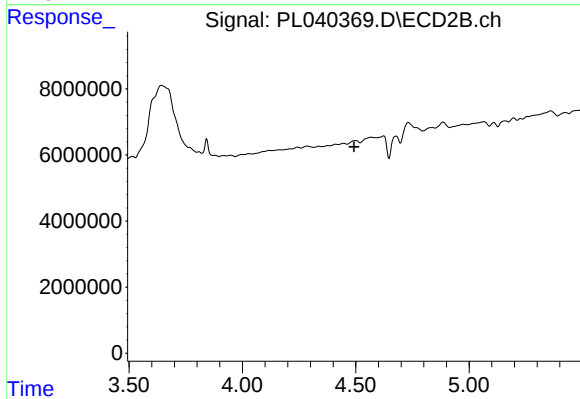

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.493 min
Response: 0
Conc: N.D.

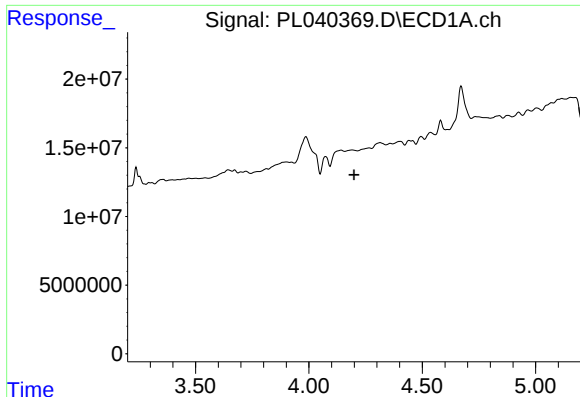

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

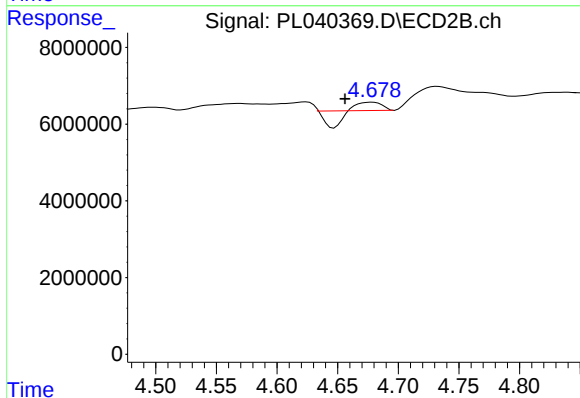


#6 beta-BHC

R.T.: 4.679 min
Delta R.T.: 0.023 min
Response: 199553
Conc: 0.10 ng/ml

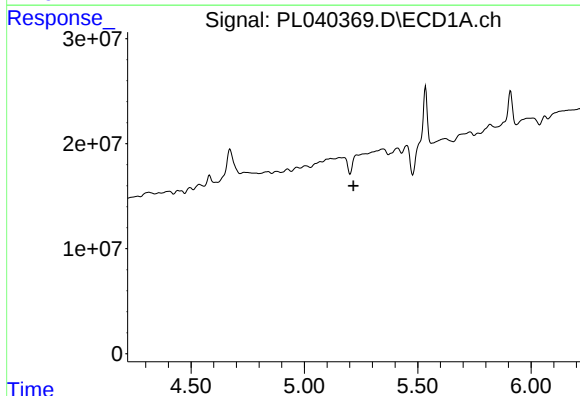


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.217 min
Response: 0
Conc: N.D.

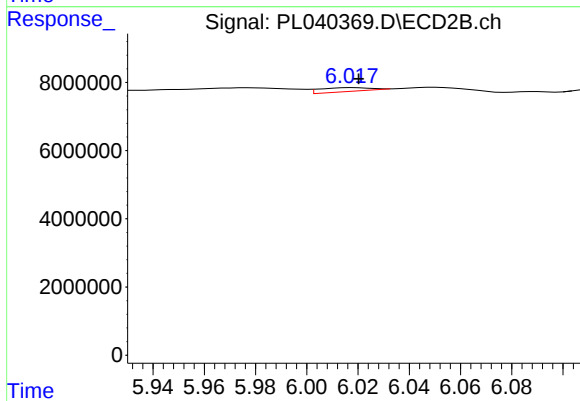

#9 Endosulfan I


R.T.: 6.018 min
Delta R.T.: -0.002 min
Response: 1529764
Conc: 0.43 ng/ml

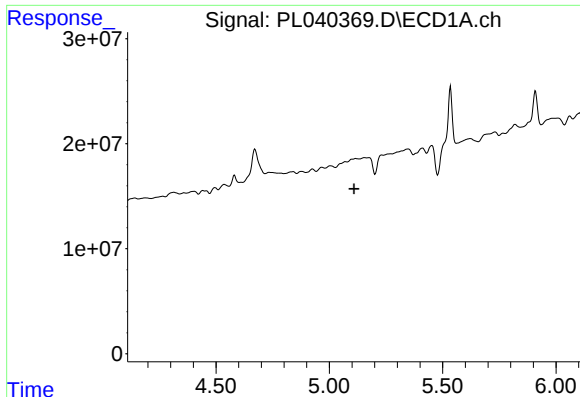

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.110 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

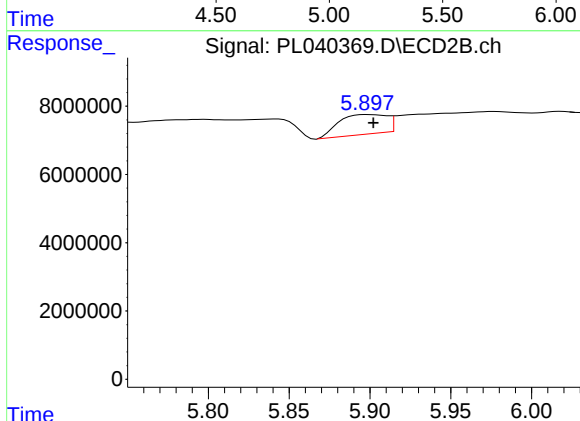


#10 gamma-Chlordane

R.T.: 5.899 min
Delta R.T.: -0.003 min
Response: 11858894
Conc: 3.08 ng/ml

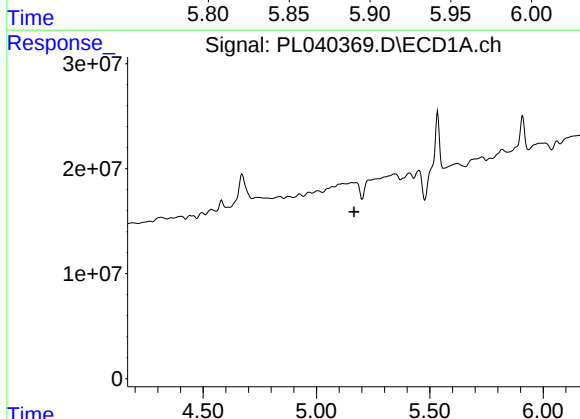


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.166 min
Response: 0
Conc: N.D.

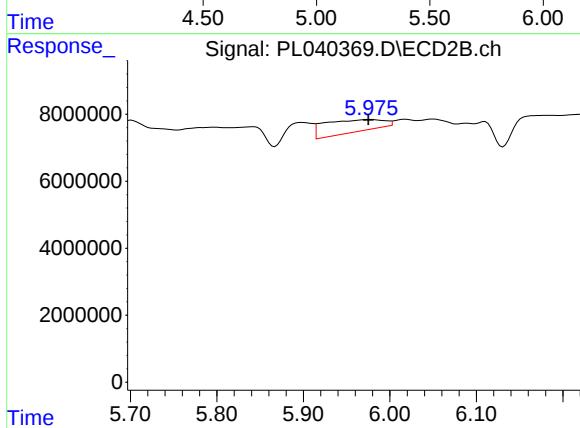

#11 alpha-Chlordane


R.T.: 5.977 min
Delta R.T.: 0.002 min
Response: 17367421
Conc: 4.57 ng/ml

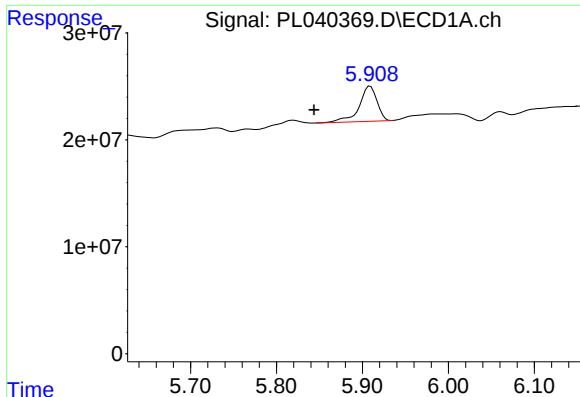

#16 4,4'-DDD


R.T.: 5.909 min
Delta R.T.: 0.065 min
Response: 47071227
Conc: 5.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

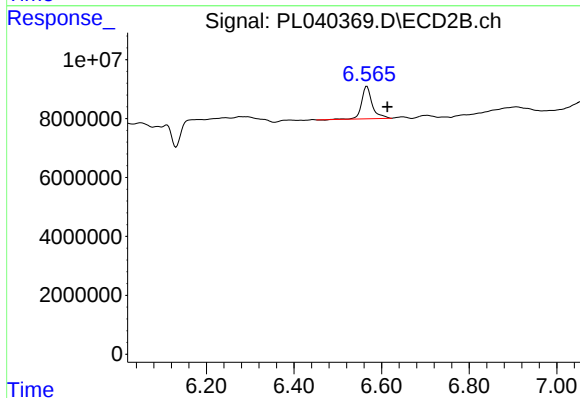


#16 4,4'-DDD

R.T.: 6.566 min
Delta R.T.: -0.046 min
Response: 18480417
Conc: 5.77 ng/ml

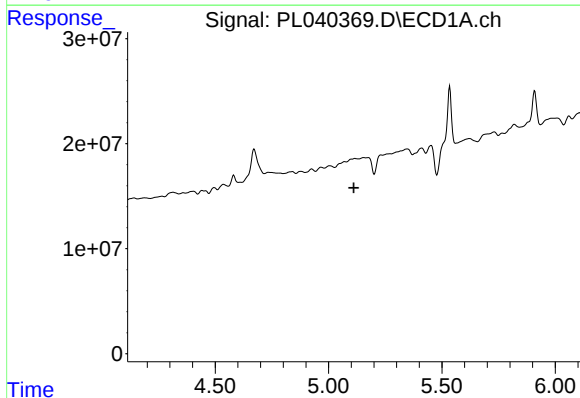


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.112 min
Response: 0
Conc: N.D.

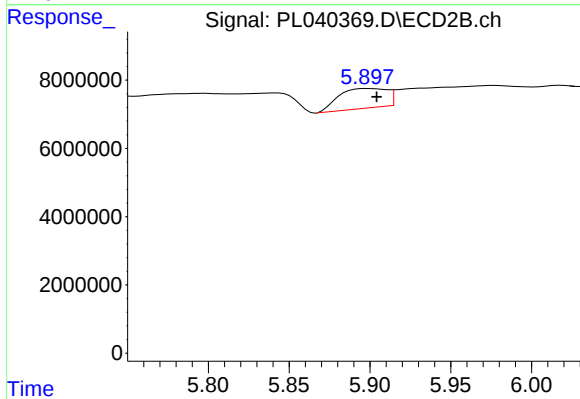

#25 Chlordane-3


R.T.: 5.899 min
Delta R.T.: -0.005 min
Response: 11858894
Conc: 22.18 ng/ml

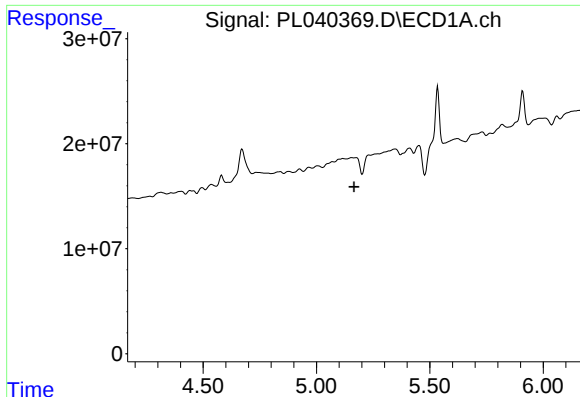

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.166 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

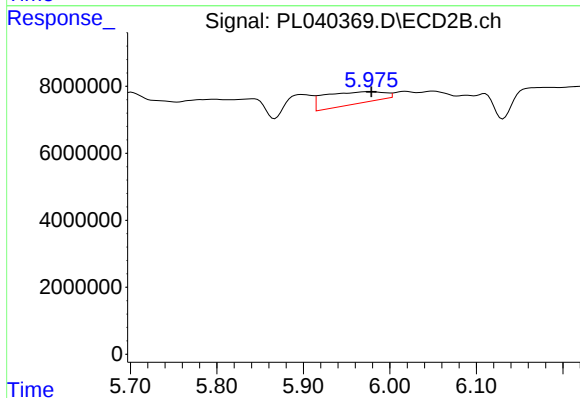


#26 Chlordane-4

R.T.: 5.977 min
Delta R.T.: -0.002 min
Response: 17367421
Conc: 27.20 ng/ml

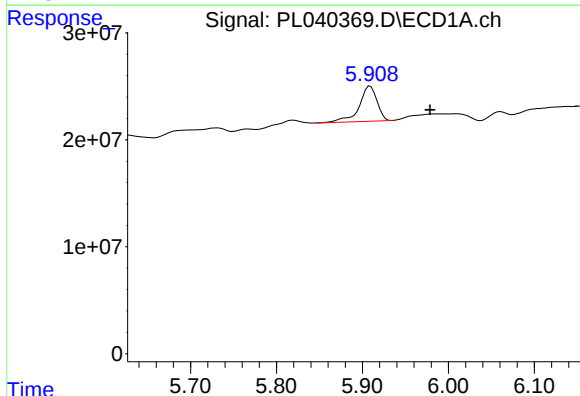


#27 Chlordane-5

R.T.: 5.909 min
Delta R.T.: -0.070 min
Response: 47071227
Conc: 113.49 ng/ml

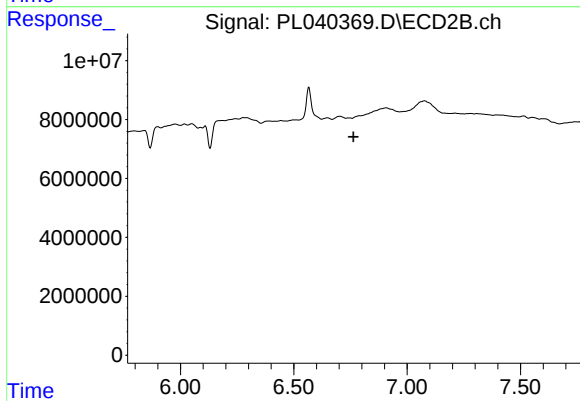

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

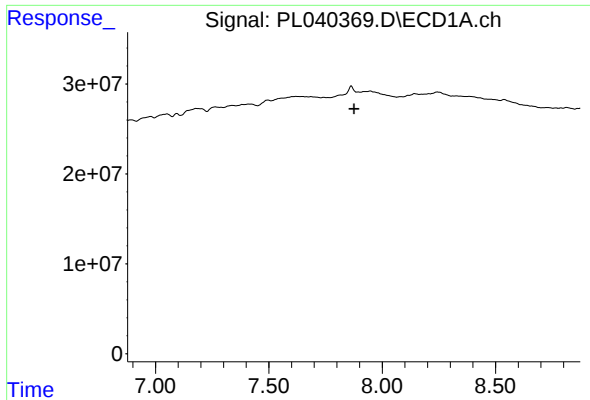

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.876 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

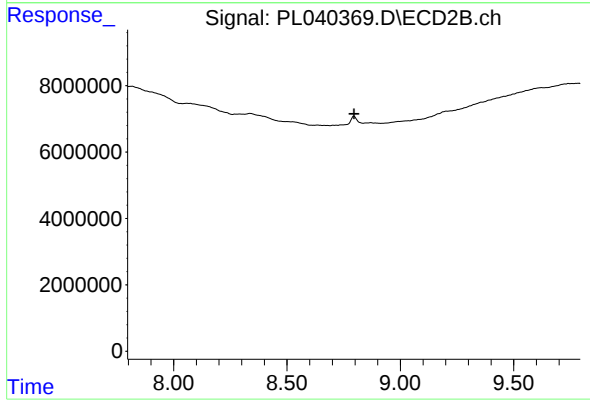

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.796 min
Response: 0
Conc: N.D.