

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092520\
 Data File : PL061814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2020 14:54
 Operator : DD\AJ
 Sample : L4132-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-20413

Manual Integrations
 APPROVED

Ankita
 9/28/2020 4:20:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 00:46:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	4.007	26926130	42535597	15.783	15.591
28)	SA Decachlor...	8.209	9.093	33896343	46228647	20.837	21.000
Target Compounds							
10)	B gamma-Chl...	5.394	6.108	1015037	19835823	0.584m	6.755m#
11)	B alpha-Chl...	5.452	6.195	1787467	9378634	1.029m	3.123 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092520\
Data File : PL061814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2020 14:54
Operator : DD\AJ
Sample : L4132-04
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-20413


Manual Integrations
APPROVED

Ankita
9/28/2020 4:20:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 00:46:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

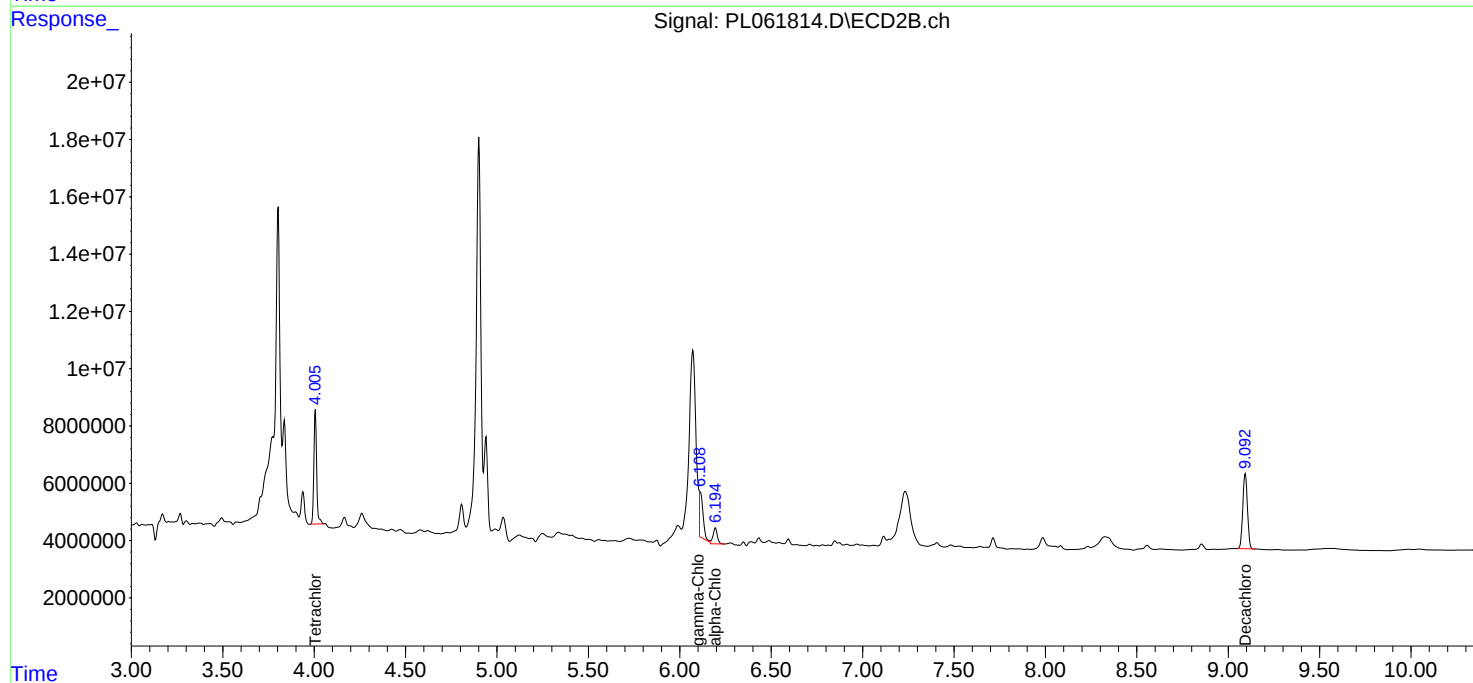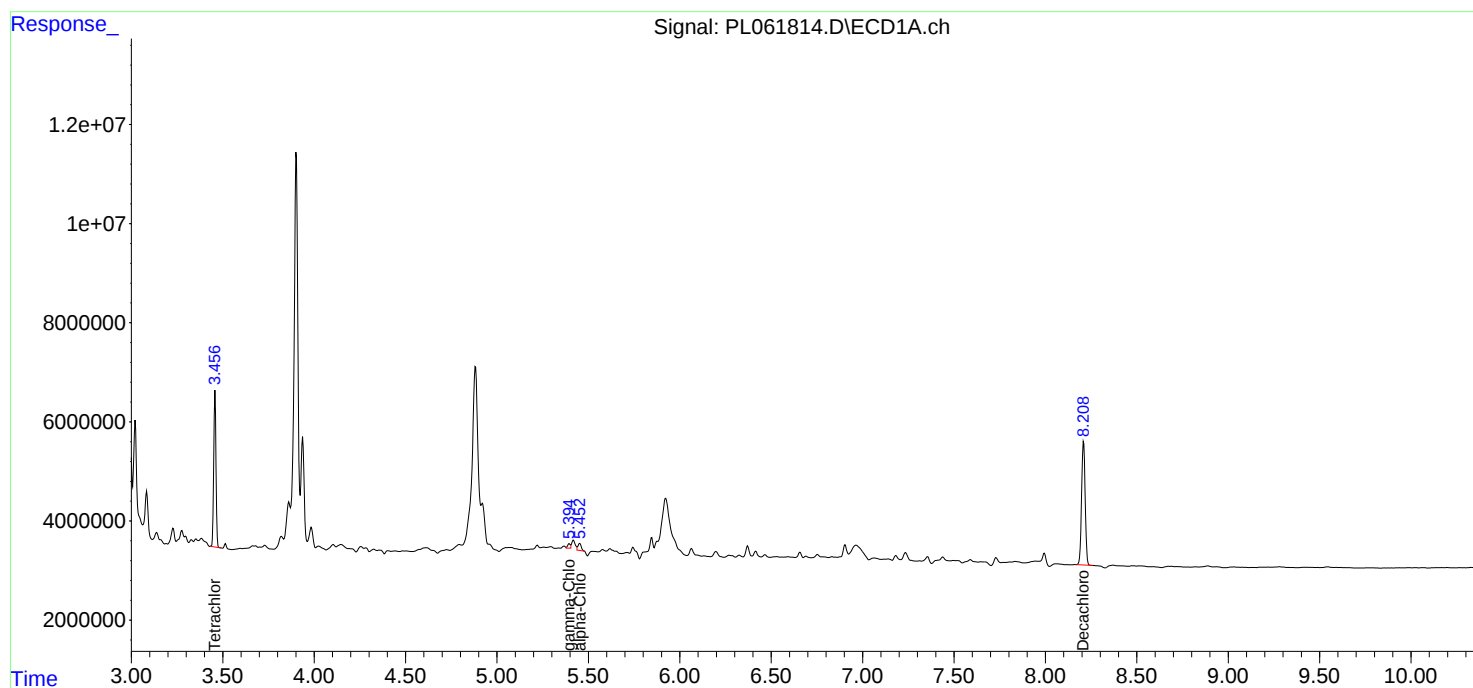

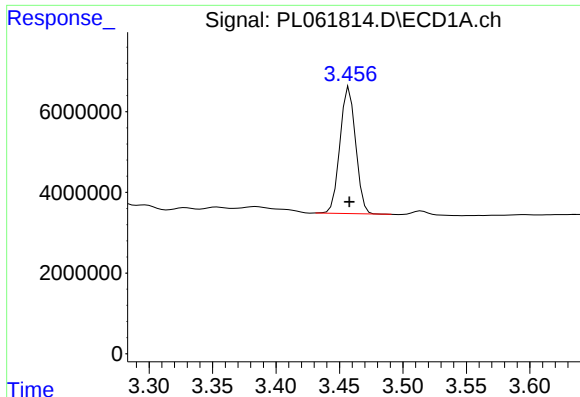


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 26926130
Conc: 15.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-20413


Manual Integrations
APPROVED

Ankita
9/28/2020 4:20:42 PM

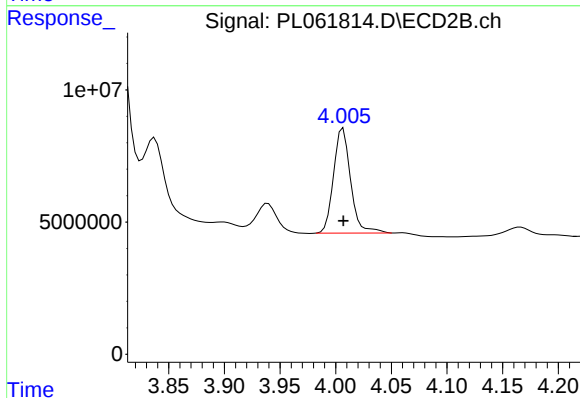


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: 0.000 min
Response: 42535597
Conc: 15.59 ng/ml

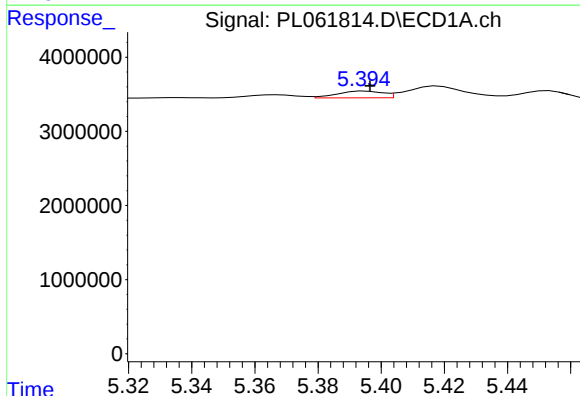


#10 gamma-Chlordane

R.T.: 5.394 min
Delta R.T.: -0.003 min
Response: 1015037
Conc: 0.58 ng/ml m

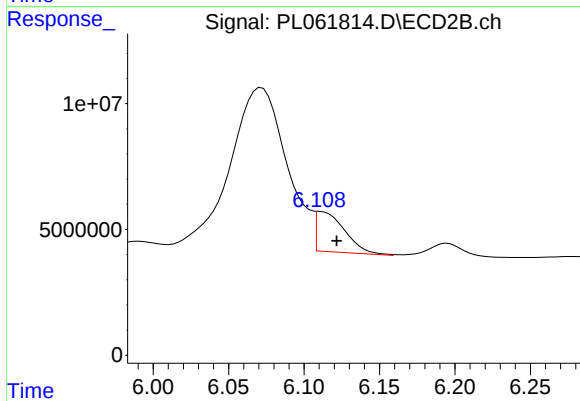

#10 gamma-Chlordane

R.T.: 6.108 min
Delta R.T.: -0.013 min
Response: 19835823
Conc: 6.75 ng/ml m

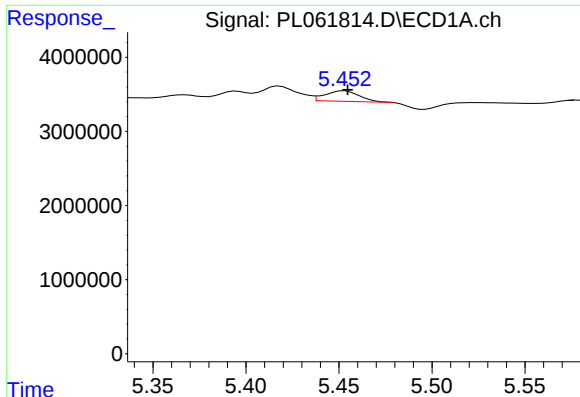


#11 alpha-Chlordane

R.T.: 5.452 min
Delta R.T.: -0.003 min
Response: 1787467
Conc: 1.03 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CHRT-20413


Manual Integrations
APPROVED

Ankita
9/28/2020 4:20:42 PM

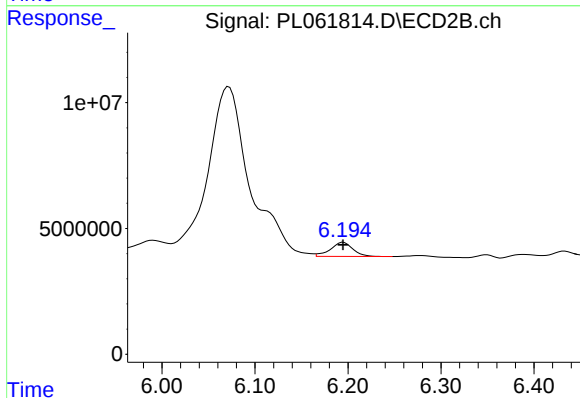


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 9378634
Conc: 3.12 ng/ml

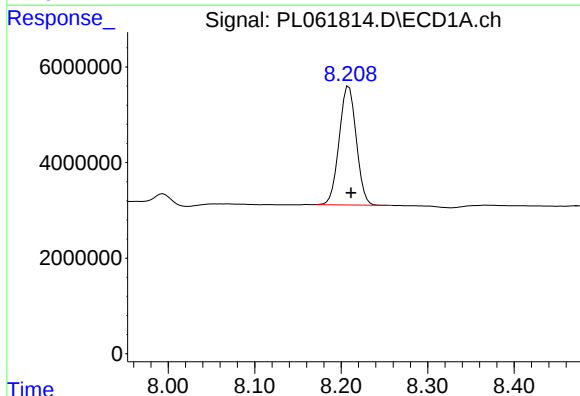

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: -0.002 min
Response: 33896343
Conc: 20.84 ng/ml

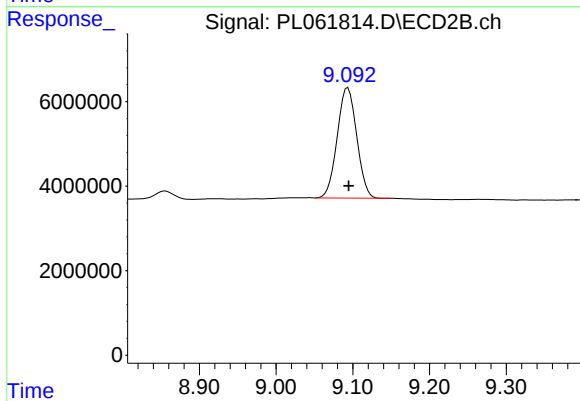

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.001 min
Response: 46228647
Conc: 21.00 ng/ml