

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092520\
 Data File : PL061817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2020 15:36
 Operator : DD\AJ
 Sample : L4152-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WR-PILE-5-7

Manual Integrations
 APPROVED

Ankita
 9/28/2020 4:20:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 00:47:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 23 13:58:40 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.457	4.005	25046414	26581490	14.682	9.743m#
28) SA Decachlor...	8.207	9.092	27072047	31532068	16.642	14.324
Target Compounds						
12) B 4,4'-DDE	5.617	6.348	21088542	32457103	13.418m	11.890m
14) MA Endrin	6.007	6.712	4174357	5086219	2.623	2.085m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092520\
Data File : PL061817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2020 15:36
Operator : DD\AJ
Sample : L4152-03
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WR-PILE-5-7


Manual Integrations
APPROVED

Ankita
9/28/2020 4:20:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 00:47:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092320.M
Quant Title : GC Extractables
QLast Update : Wed Sep 23 13:58:40 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

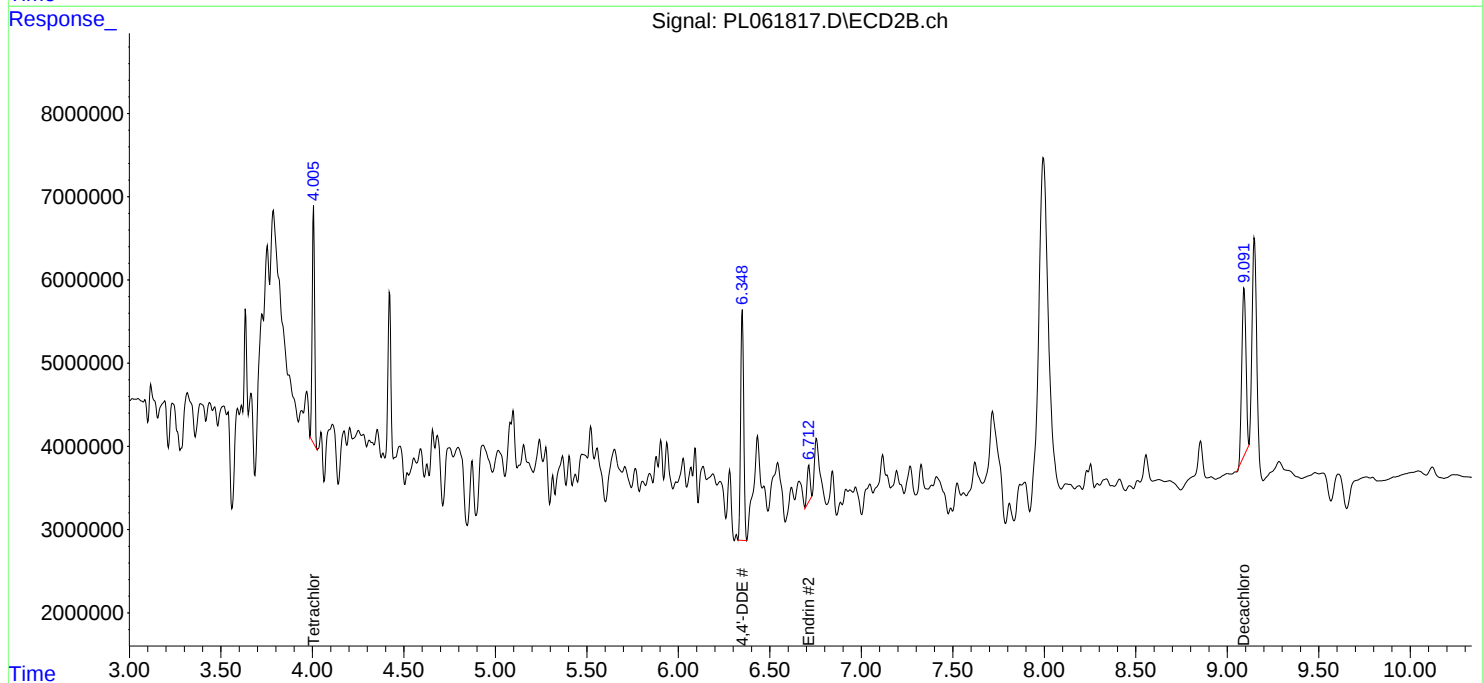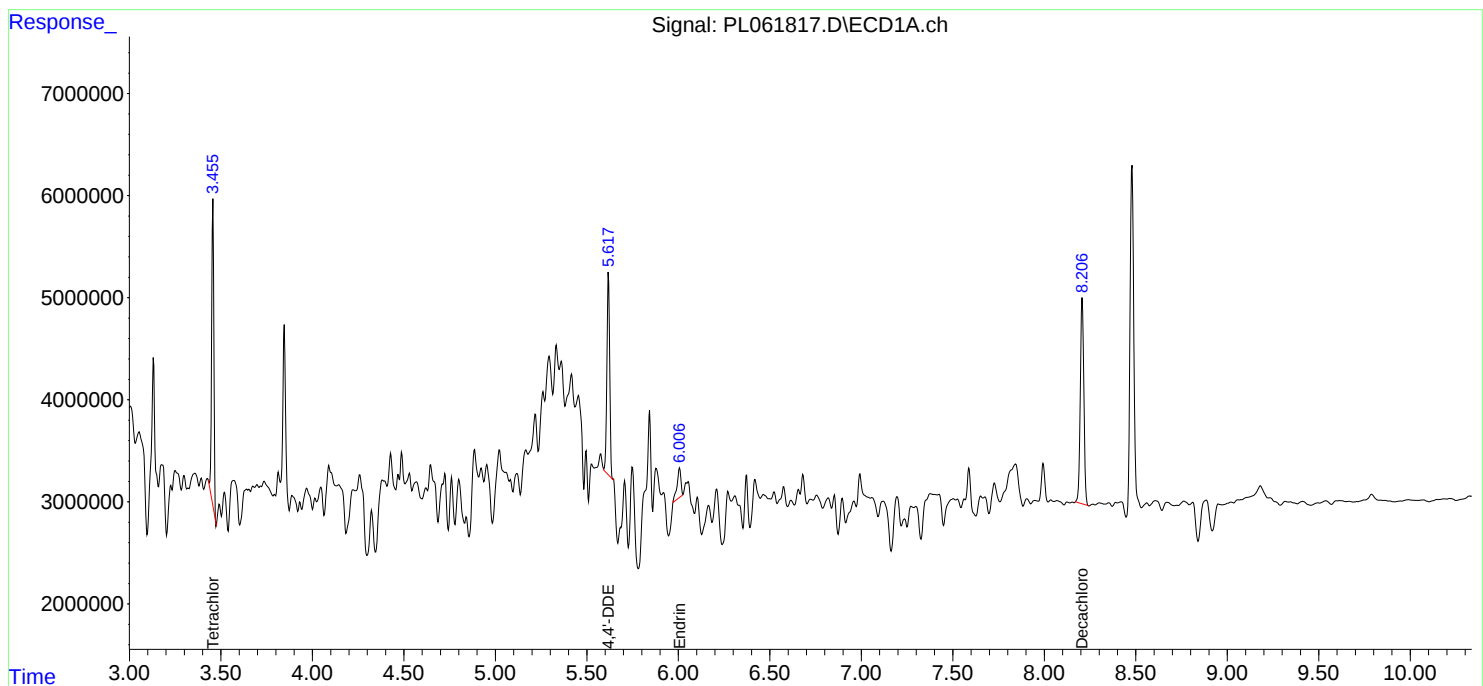

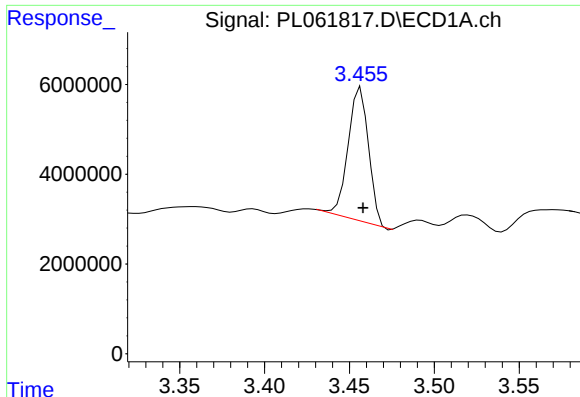


#1 Tetrachloro-m-xylene

R.T.: 3.457 min
Delta R.T.: -0.001 min
Response: 25046414
Conc: 14.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
WR-PILE-5-7


Manual Integrations
APPROVED

Ankita
9/28/2020 4:20:50 PM

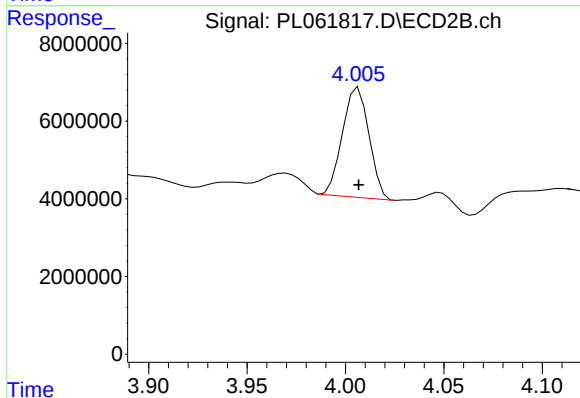


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.002 min
Response: 26581490
Conc: 9.74 ng/ml m

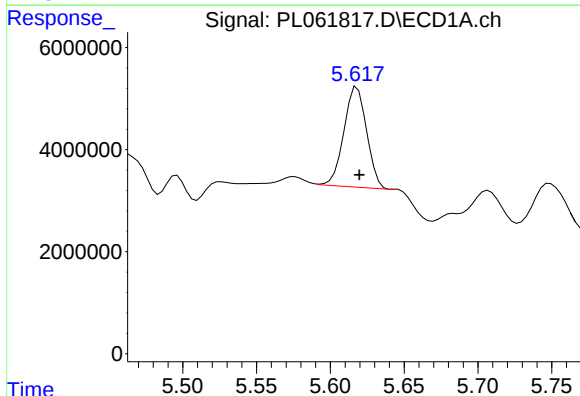


#12 4,4'-DDE

R.T.: 5.617 min
Delta R.T.: -0.003 min
Response: 21088542
Conc: 13.42 ng/ml m

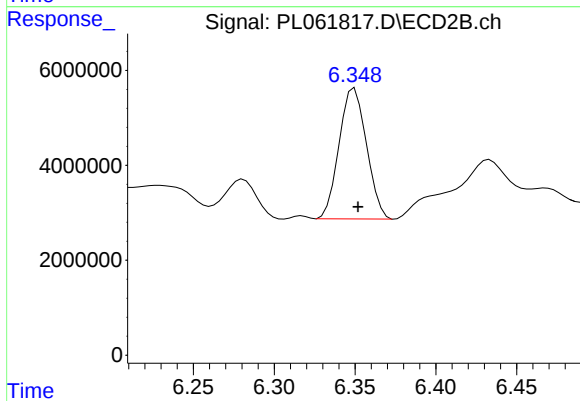

#12 4,4'-DDE

R.T.: 6.348 min
Delta R.T.: -0.004 min
Response: 32457103
Conc: 11.89 ng/ml m

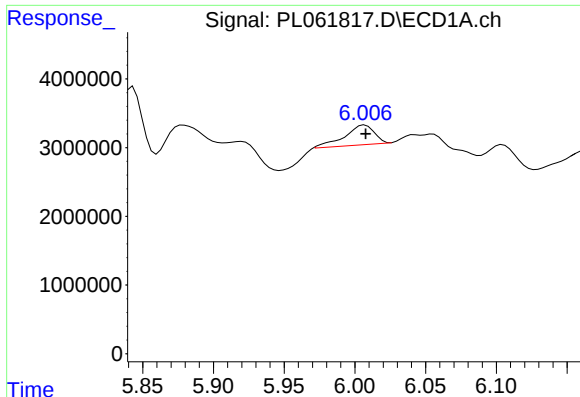


#14 Endrin

R.T.: 6.007 min
Delta R.T.: 0.000 min
Response: 4174357
Conc: 2.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
WR-PILE-5-7


Manual Integrations
APPROVED

Ankita
9/28/2020 4:20:50 PM

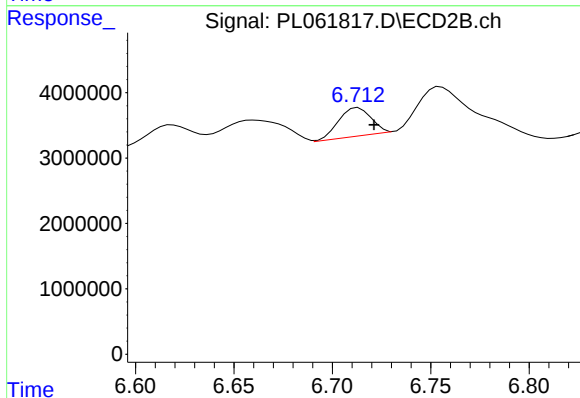


#14 Endrin

R.T.: 6.712 min
Delta R.T.: -0.009 min
Response: 5086219
Conc: 2.08 ng/ml m

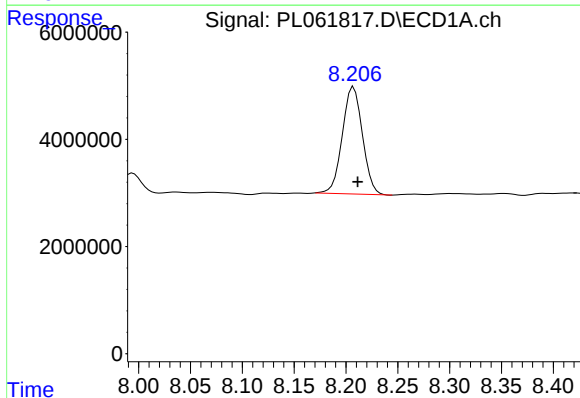

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: -0.004 min
Response: 27072047
Conc: 16.64 ng/ml

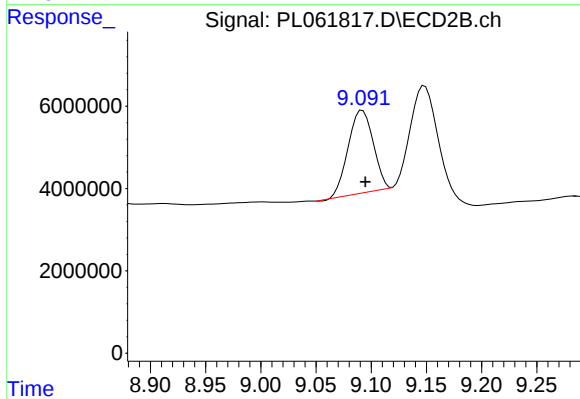

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.003 min
Response: 31532068
Conc: 14.32 ng/ml