

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
 Data File : PL085477.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 15:28
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 16:17:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 16:14:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.404	2.649	239.8E6	135.2E6	99.649	100.549
28)	SA Decachlor...	8.936	7.822	174.5E6	110.5E6	96.471	98.209
Target Compounds							
23)	Chlordane-1	4.566	3.646	102.0E6	38131589	984.626	1006.546
24)	Chlordane-2	5.098	4.227	102.9E6	44572761	966.645	976.519
25)	Chlordane-3	5.812	4.857	404.0E6	136.2E6	1003.043	1014.112
26)	Chlordane-4	5.895	4.920	484.9E6	148.6E6	996.009	1018.131
27)	Chlordane-5	6.745	5.592	85748801	38464454	981.716	1002.268



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
Data File : PL085477.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 15:28
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 16:17:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 16:14:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

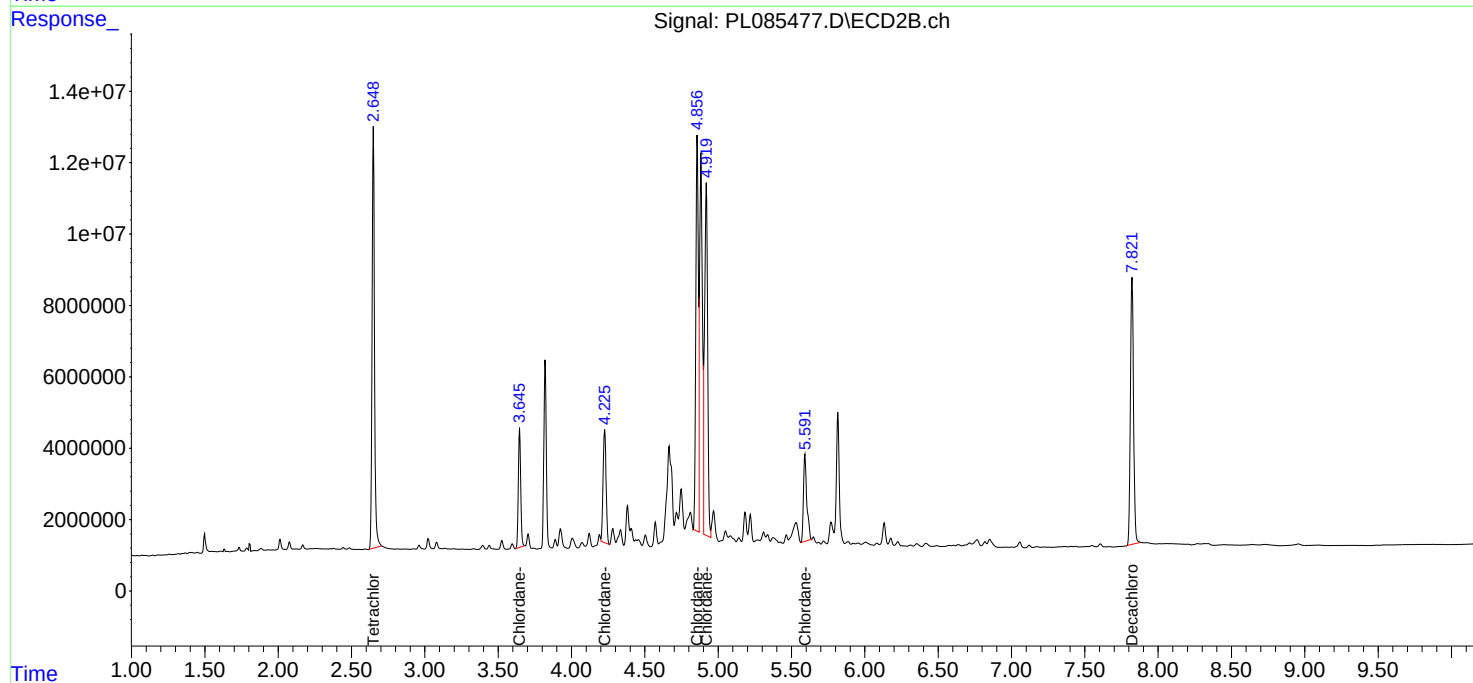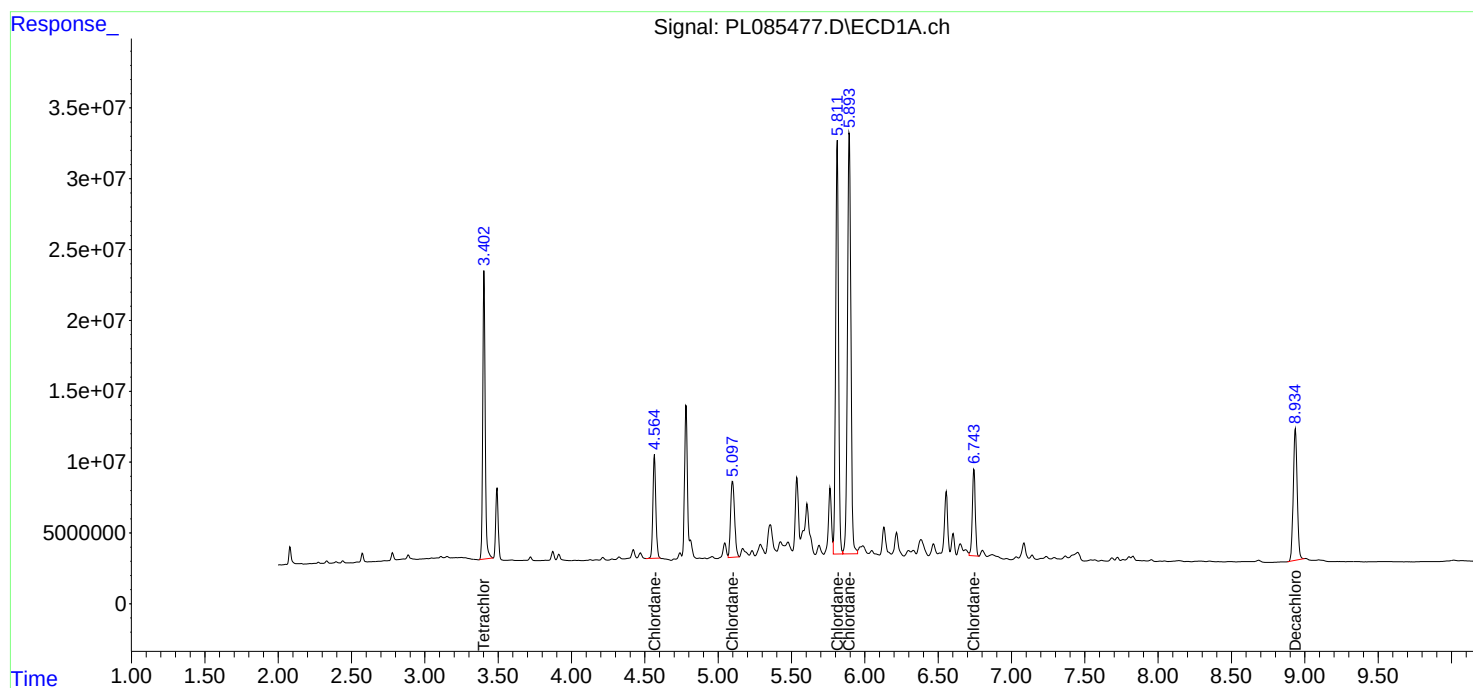


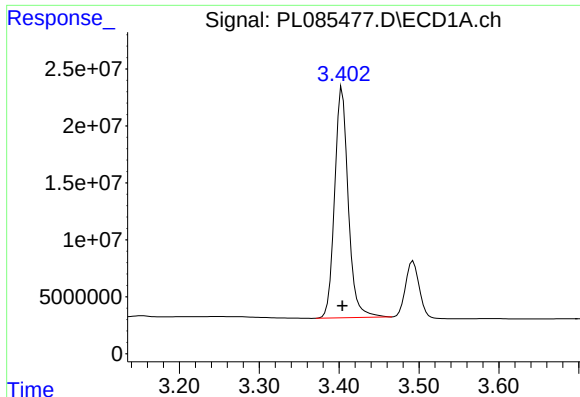

#1 Tetrachloro-m-xylene


R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 239803724
Conc: 99.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

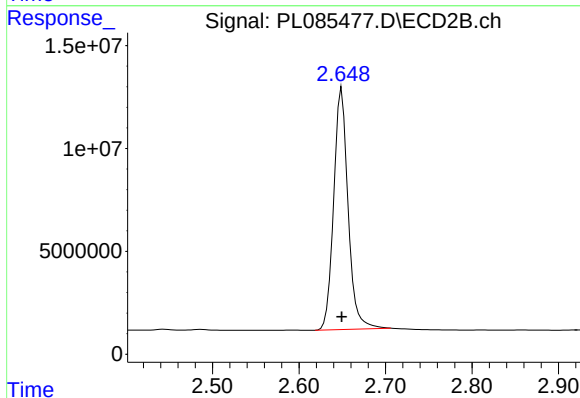


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 135215003
Conc: 100.55 ng/ml

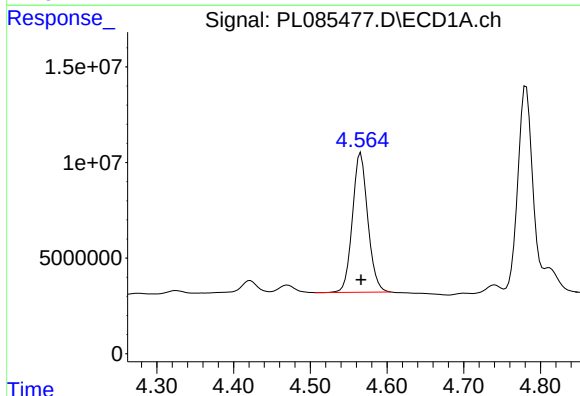


#23 Chlordane-1

R.T.: 4.566 min
Delta R.T.: 0.000 min
Response: 102025367
Conc: 984.63 ng/ml

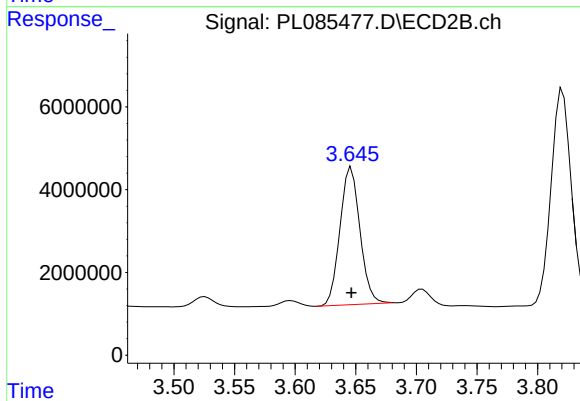

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 38131589
Conc: 1006.55 ng/ml

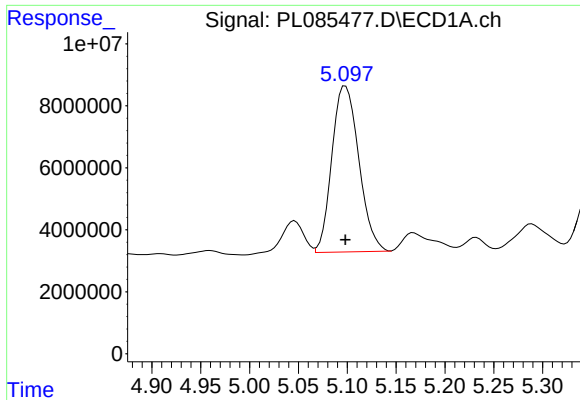

#24 Chlordane-2


R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 102870416
Conc: 966.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

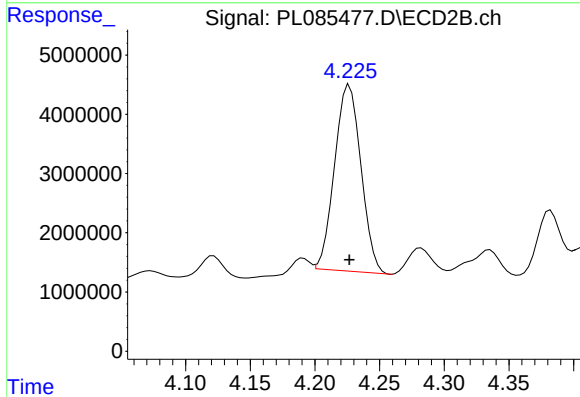


#24 Chlordane-2

R.T.: 4.227 min
Delta R.T.: 0.000 min
Response: 44572761
Conc: 976.52 ng/ml

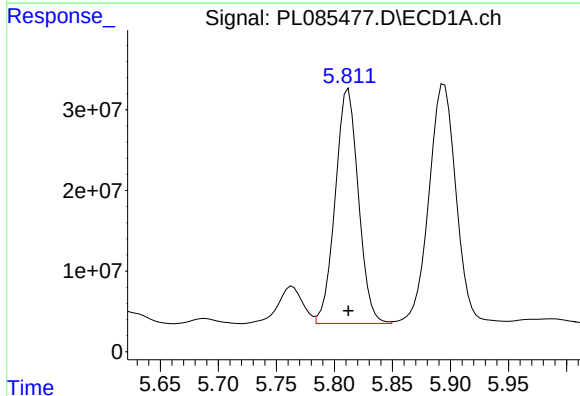


#25 Chlordane-3

R.T.: 5.812 min
Delta R.T.: 0.000 min
Response: 404003307
Conc: 1003.04 ng/ml

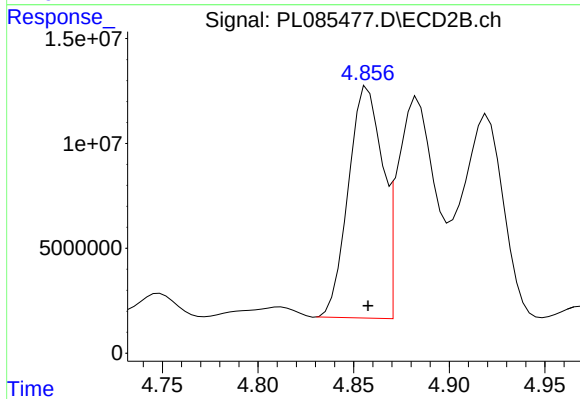

#25 Chlordane-3


R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 136160936
Conc: 1014.11 ng/ml

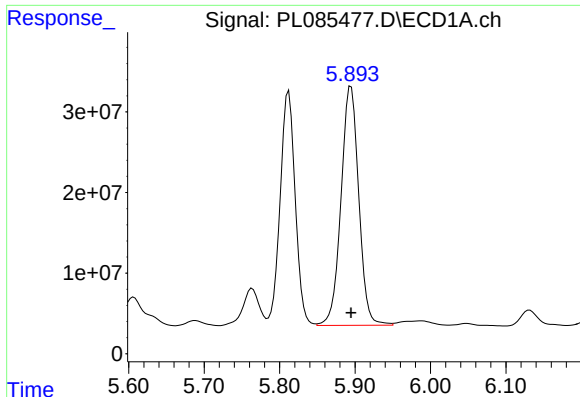

#26 Chlordane-4


R.T.: 5.895 min
Delta R.T.: 0.000 min
Response: 484936938
Conc: 996.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

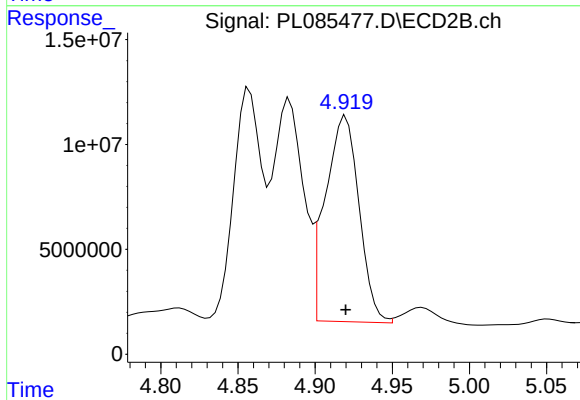


#26 Chlordane-4

R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 148584217
Conc: 1018.13 ng/ml

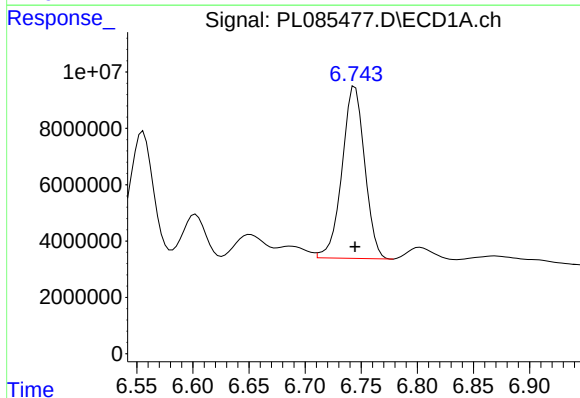


#27 Chlordane-5

R.T.: 6.745 min
Delta R.T.: 0.000 min
Response: 85748801
Conc: 981.72 ng/ml

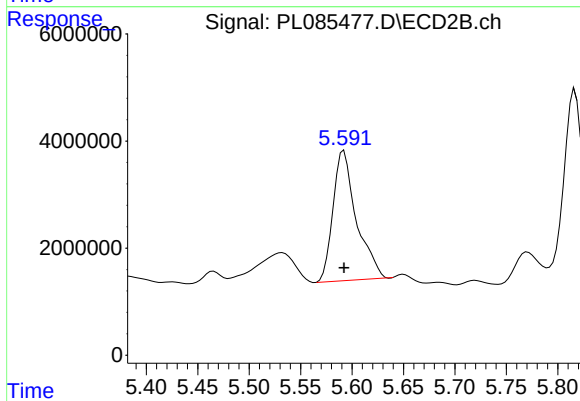

#27 Chlordane-5

R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 38464454
Conc: 1002.27 ng/ml

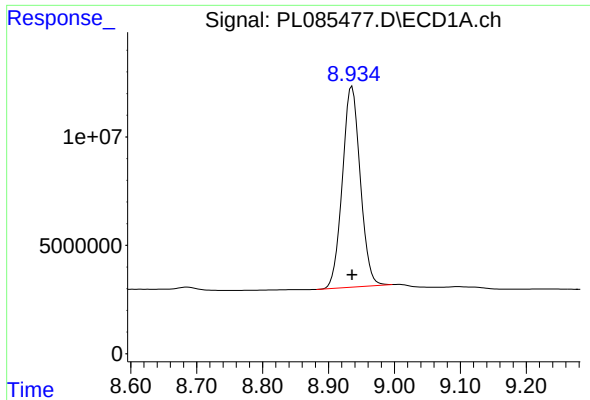

#28 Decachlorobiphenyl


R.T.: 8.936 min

Delta R.T.: 0.000 min

Response: 174456910

Conc: 96.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

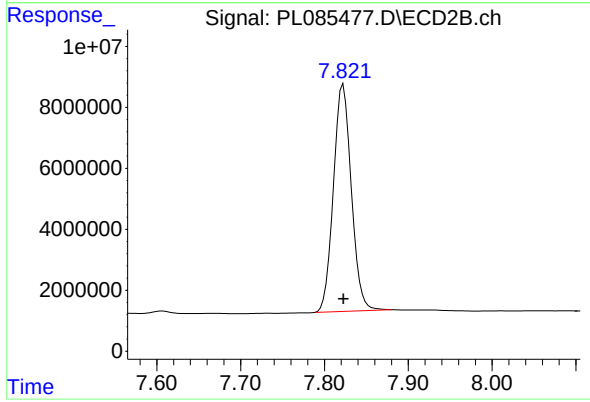

#28 Decachlorobiphenyl

R.T.: 7.822 min

Delta R.T.: 0.000 min

Response: 110495758

Conc: 98.21 ng/ml