

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
 Data File : PL085478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 15:42
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 16:19:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 16:14:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.403	2.649	176.8E6	99204948	73.983	74.176
28)	SA Decachlor...	8.935	7.822	132.6E6	82014525	73.888	73.583
Target Compounds							
23)	Chlordane-1	4.565	3.645	75586766	27840648	736.189	739.865
24)	Chlordane-2	5.098	4.226	77693469	33226666	736.590	735.150
25)	Chlordane-3	5.811	4.857	296.2E6	98797313	740.116	740.495
26)	Chlordane-4	5.894	4.920	357.4E6	107.5E6	739.245	740.852
27)	Chlordane-5	6.744	5.592	64094240	27711987	739.121	731.160



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
Data File : PL085478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 15:42
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 16:19:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 16:14:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

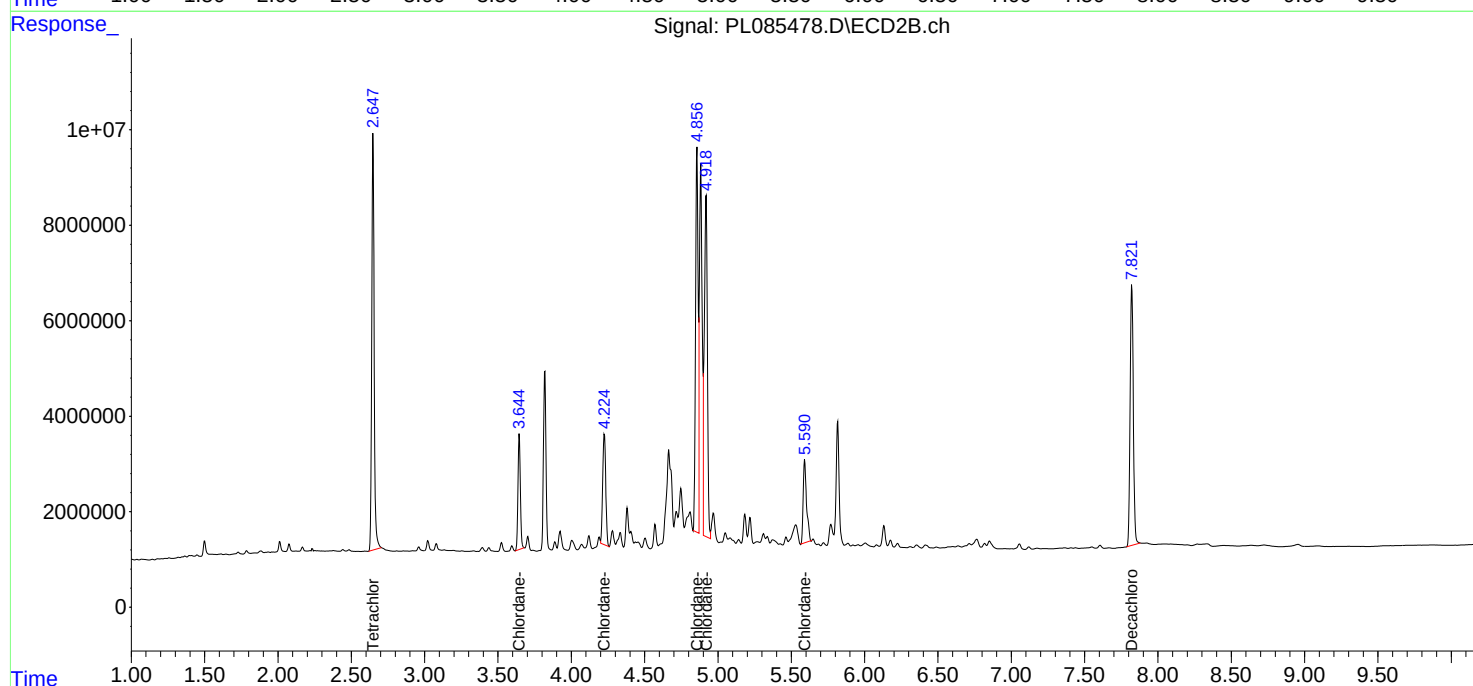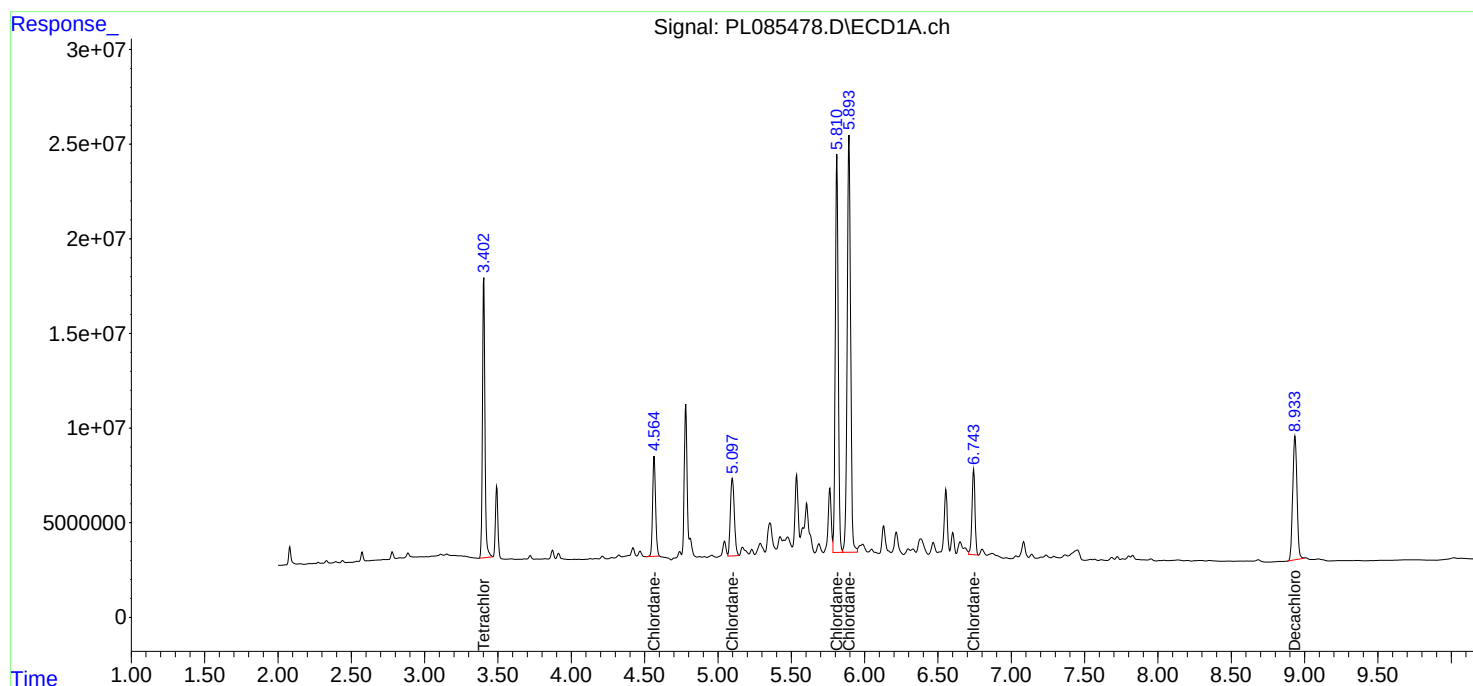


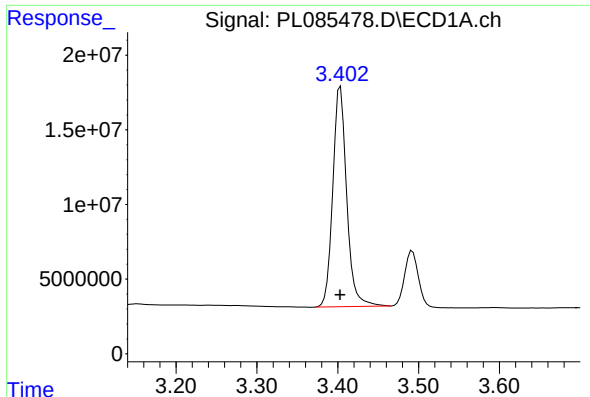

#1 Tetrachloro-m-xylene


R.T.: 3.403 min
Delta R.T.: 0.000 min
Response: 176839532
Conc: 73.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

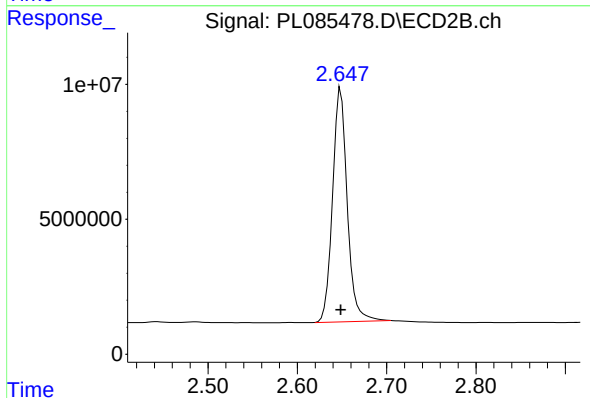


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 99204948
Conc: 74.18 ng/ml

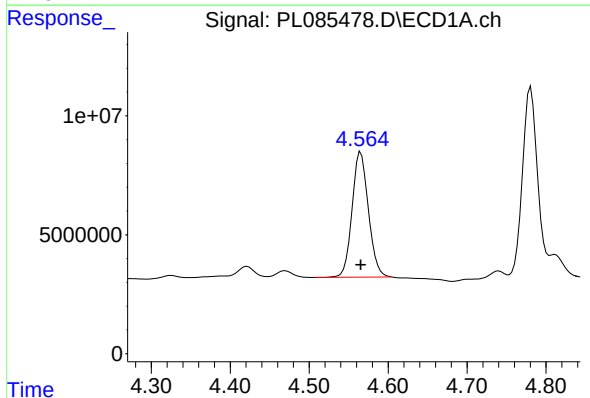


#23 Chlordane-1

R.T.: 4.565 min
Delta R.T.: 0.000 min
Response: 75586766
Conc: 736.19 ng/ml

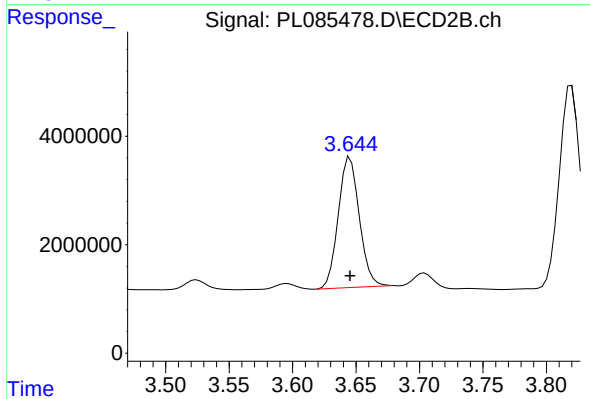

#23 Chlordane-1


R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 27840648
Conc: 739.87 ng/ml

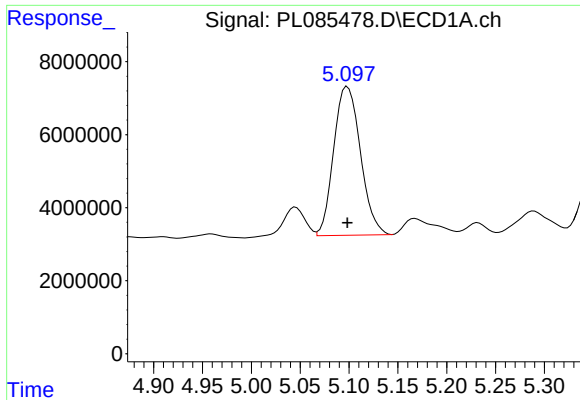

#24 Chlordane-2


R.T.: 5.098 min
Delta R.T.: 0.000 min
Response: 77693469
Conc: 736.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

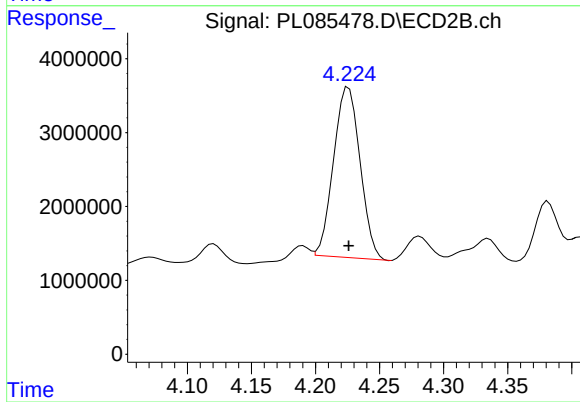


#24 Chlordane-2

R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 33226666
Conc: 735.15 ng/ml

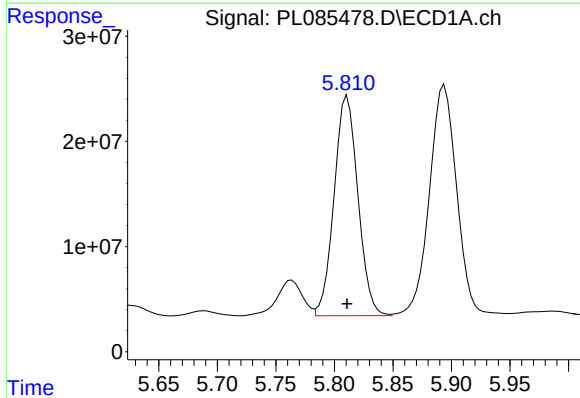


#25 Chlordane-3

R.T.: 5.811 min
Delta R.T.: 0.000 min
Response: 296150883
Conc: 740.12 ng/ml

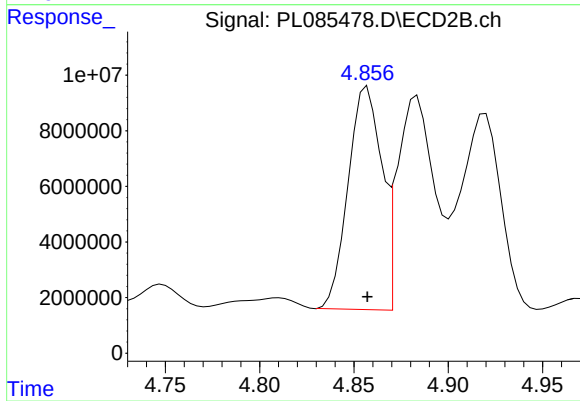

#25 Chlordane-3


R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 98797313
Conc: 740.49 ng/ml

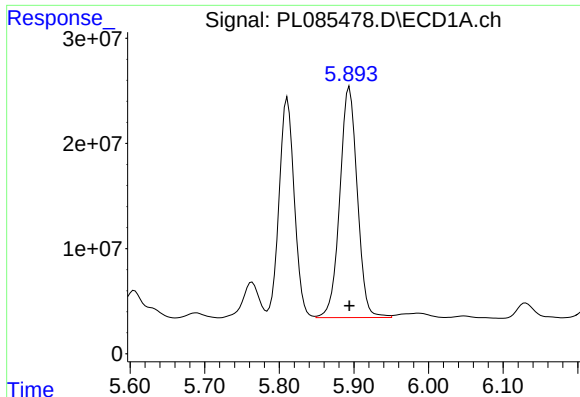

#26 Chlordane-4


R.T.: 5.894 min
Delta R.T.: 0.000 min
Response: 357361430
Conc: 739.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

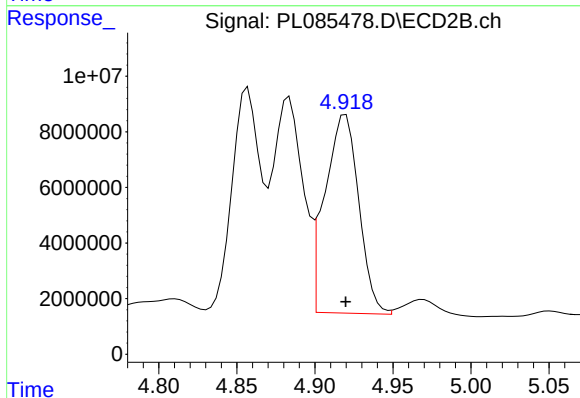


#26 Chlordane-4

R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 107463135
Conc: 740.85 ng/ml

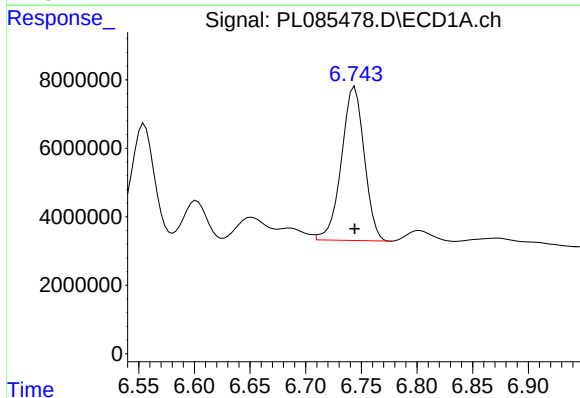


#27 Chlordane-5

R.T.: 6.744 min
Delta R.T.: 0.000 min
Response: 64094240
Conc: 739.12 ng/ml

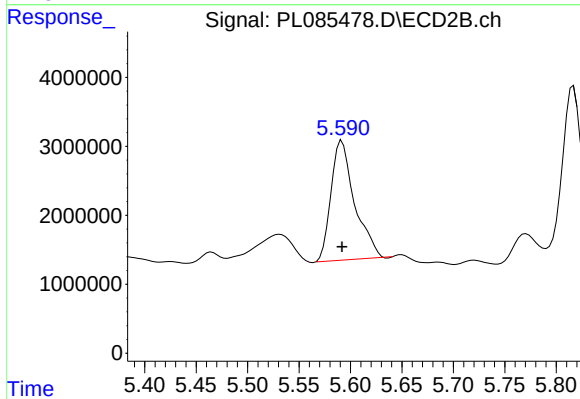

#27 Chlordane-5


R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 27711987
Conc: 731.16 ng/ml

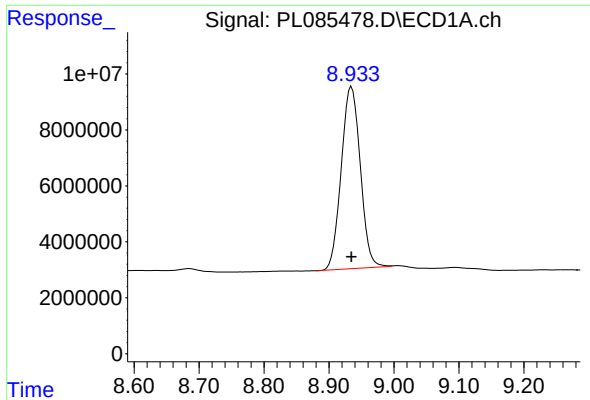

#28 Decachlorobiphenyl

R.T.: 8.935 min
Delta R.T.: 0.000 min
Response: 132634823
Conc: 73.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

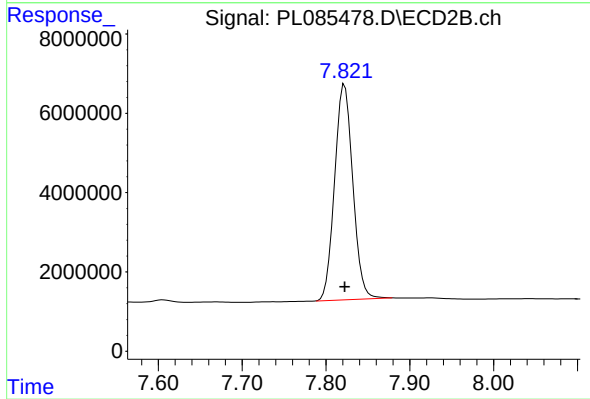

#28 Decachlorobiphenyl

R.T.: 7.822 min
Delta R.T.: 0.000 min
Response: 82014525
Conc: 73.58 ng/ml