

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
 Data File : PL085479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 15:56
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 16:14:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 16:14:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.404	2.649	120.7E6	66869717	50.000	50.000
28)	SA Decachlor...	8.937	7.823	93609509	57263122	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.566	3.646	52605764	18817794	500.000	500.000
24)	Chlordane-2	5.099	4.226	54984896	23358181	500.000	500.000
25)	Chlordane-3	5.813	4.857	200.8E6	66185708	500.000	500.000
26)	Chlordane-4	5.896	4.920	244.4E6	71646094	500.000	500.000
27)	Chlordane-5	6.746	5.592	44471443	19145206	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
Data File : PL085479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 15:56
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 16:14:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 16:14:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

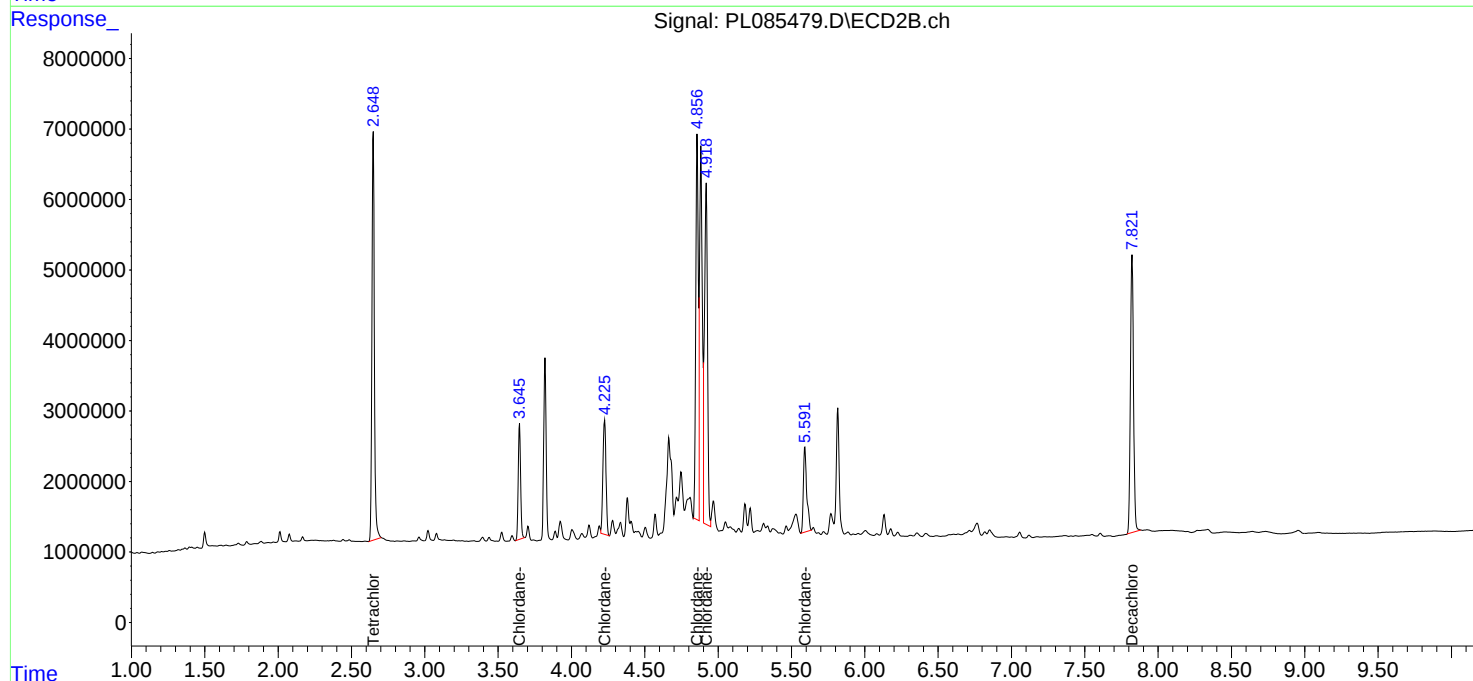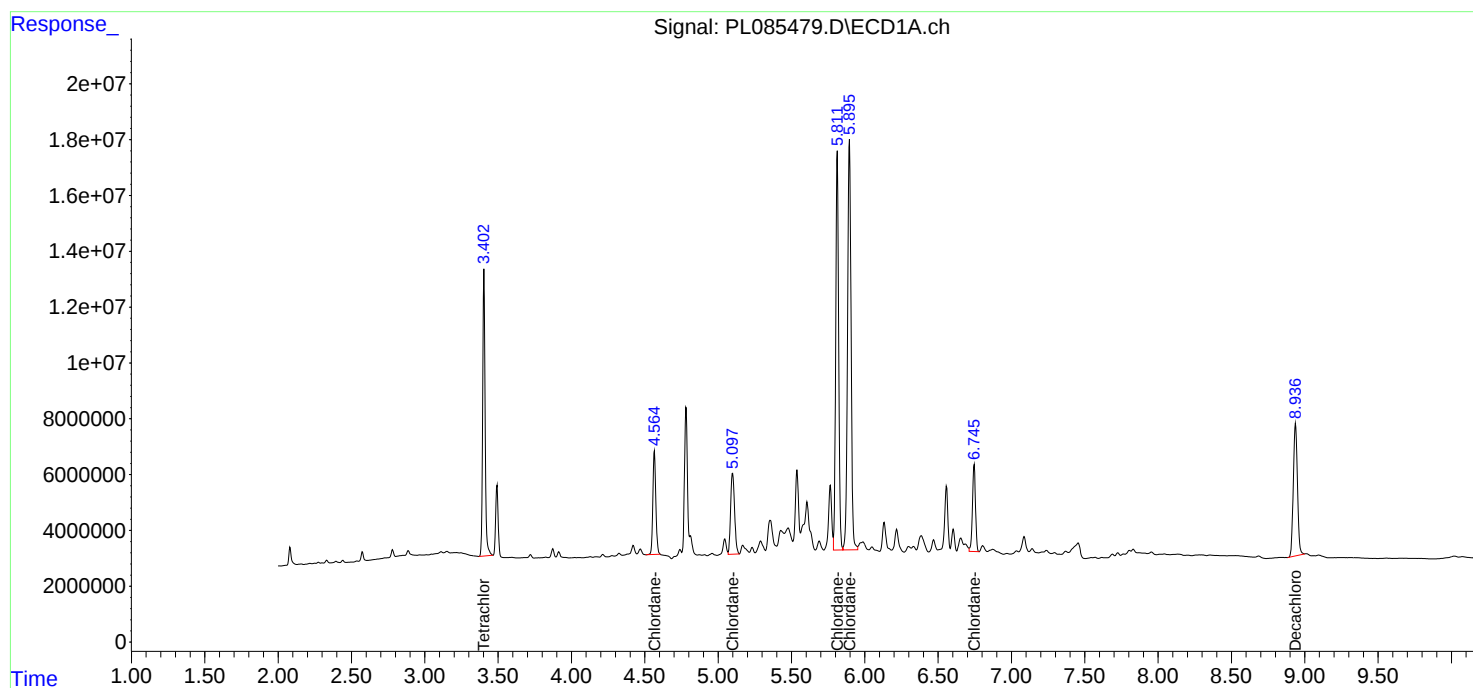


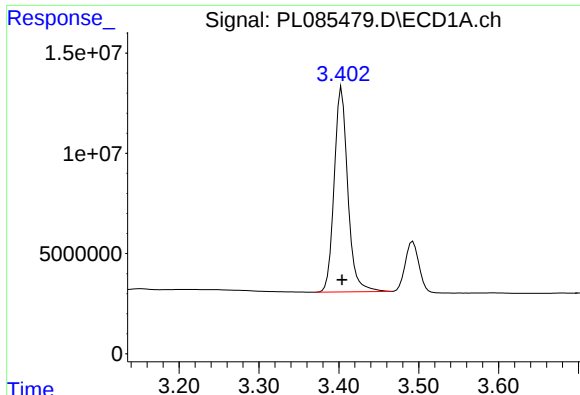

#1 Tetrachloro-m-xylene


R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 120746941
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

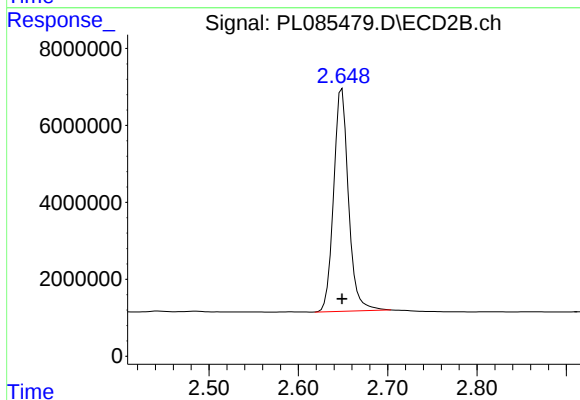


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 66869717
Conc: 50.00 ng/ml

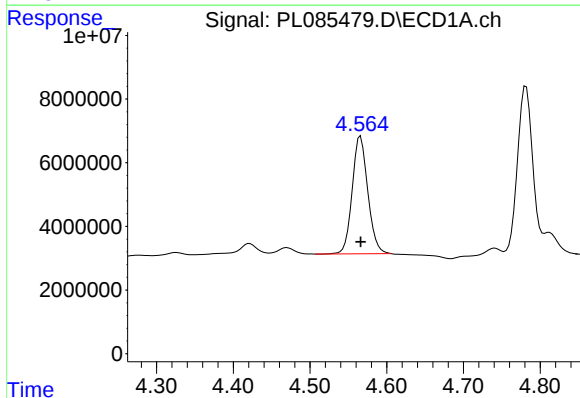


#23 Chlordane-1

R.T.: 4.566 min
Delta R.T.: 0.000 min
Response: 52605764
Conc: 500.00 ng/ml

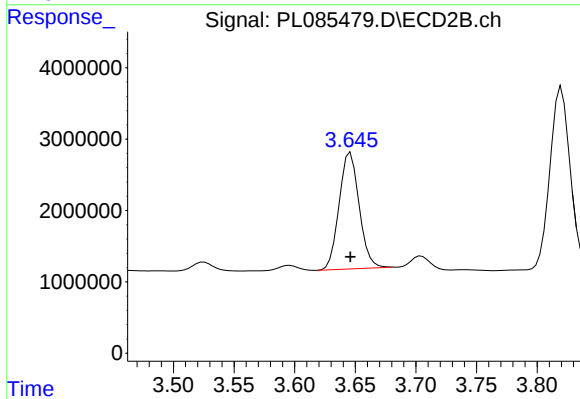

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 18817794
Conc: 500.00 ng/ml

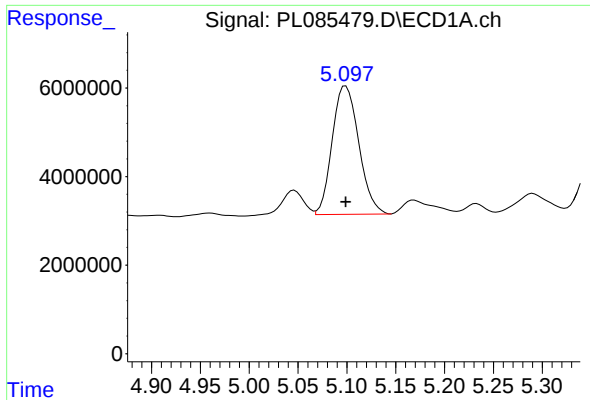

#24 Chlordane-2


R.T.: 5.099 min
Delta R.T.: 0.000 min
Response: 54984896
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

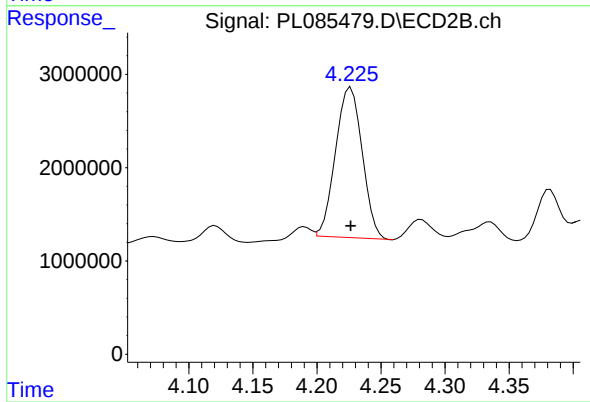


#24 Chlordane-2

R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 23358181
Conc: 500.00 ng/ml

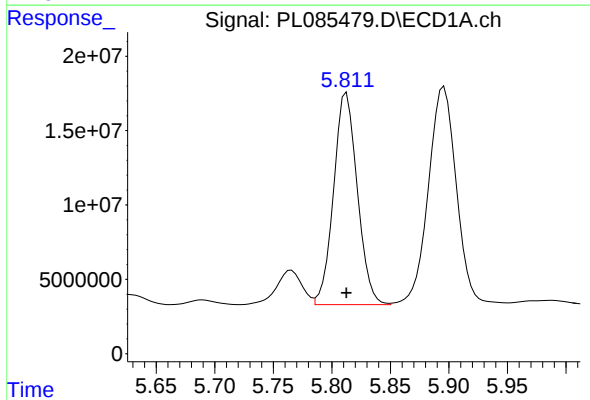


#25 Chlordane-3

R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 200775988
Conc: 500.00 ng/ml

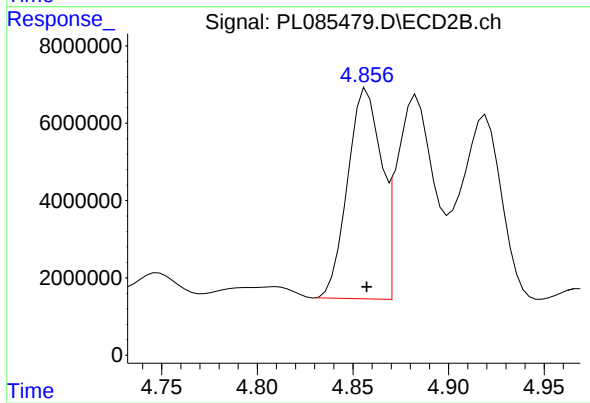

#25 Chlordane-3


R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 66185708
Conc: 500.00 ng/ml

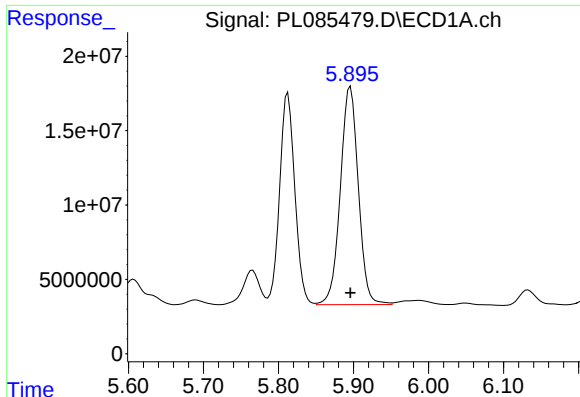

#26 Chlordane-4


R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 244411633
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

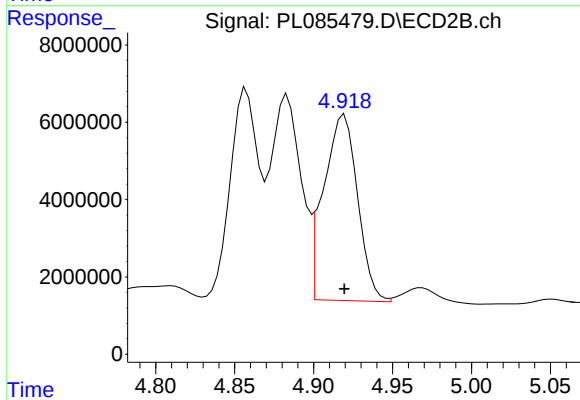


#26 Chlordane-4

R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 71646094
Conc: 500.00 ng/ml

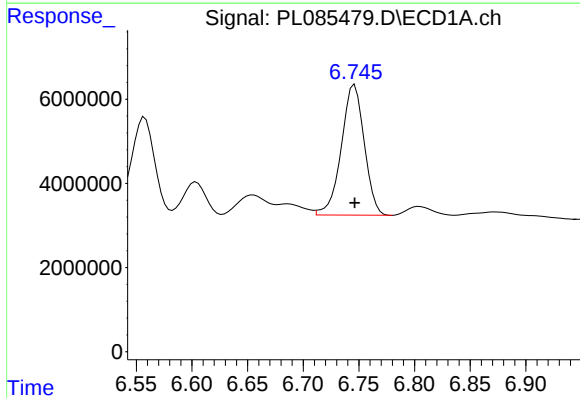


#27 Chlordane-5

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 44471443
Conc: 500.00 ng/ml

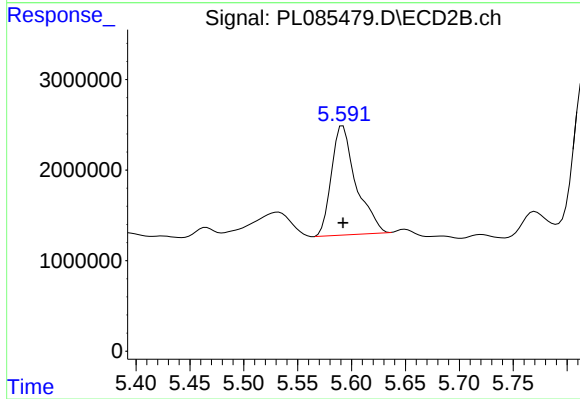

#27 Chlordane-5


R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 19145206
Conc: 500.00 ng/ml

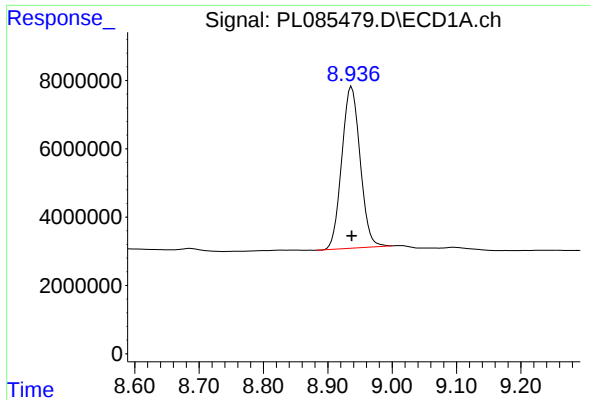

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 93609509
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

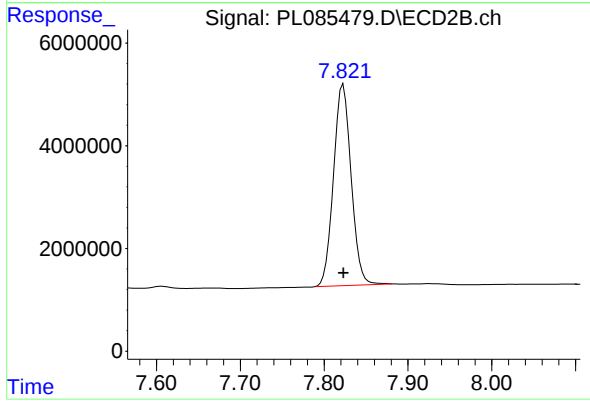

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 57263122
Conc: 50.00 ng/ml