

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
 Data File : PL085480.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 16:10
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 16:22:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 16:14:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.407	2.649	59209599	32313941	24.828	24.366
28)	SA Decachlor...	8.939	7.824	48945931	29034846	26.662	25.779
Target Compounds							
23)	Chlordane-1	4.569	3.646	25868497	9120788	251.460	244.245
24)	Chlordane-2	5.103	4.227	28114324	11719271	262.206	256.905
25)	Chlordane-3	5.816	4.858	97192680	31277235	244.634	238.134
26)	Chlordane-4	5.899	4.920	119.5E6	33719810	247.902	236.614
27)	Chlordane-5	6.748	5.593	22957789	9064405	260.897	241.779



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
Data File : PL085480.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 16:10
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 16:22:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 16:14:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

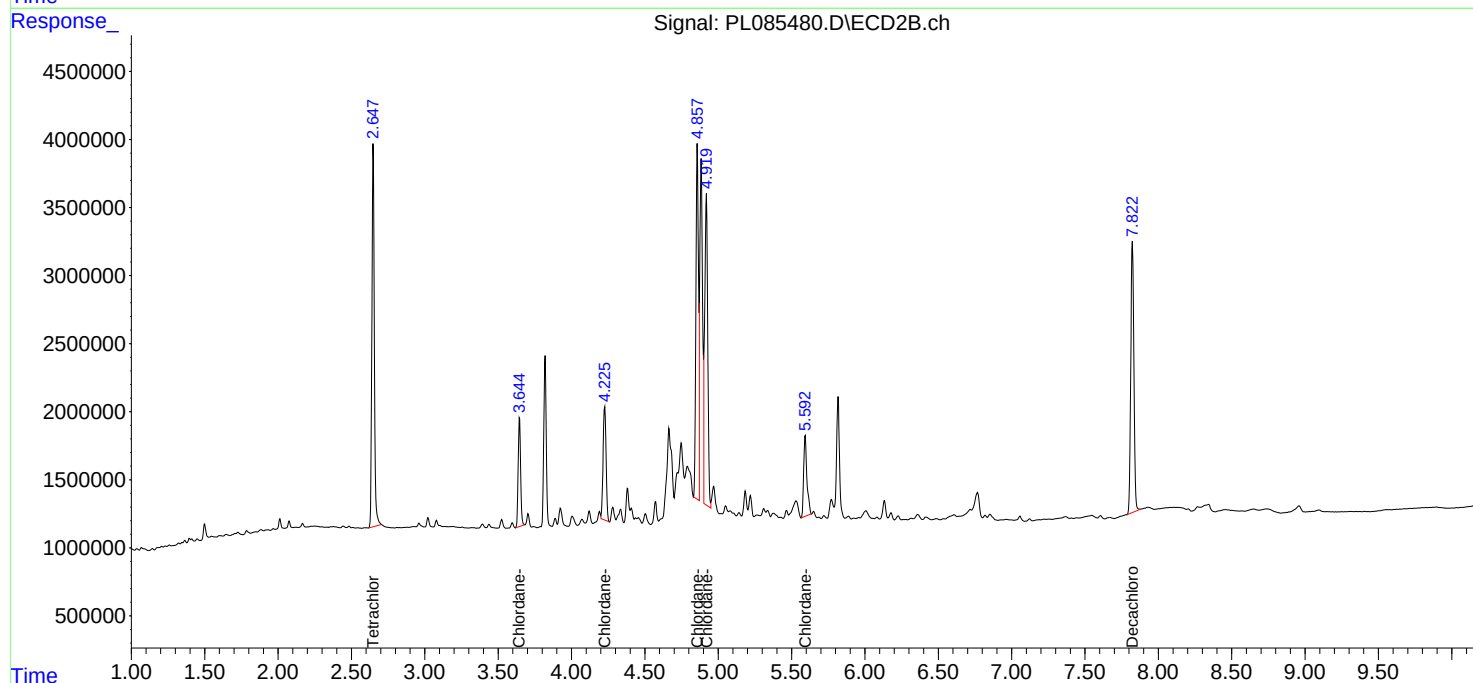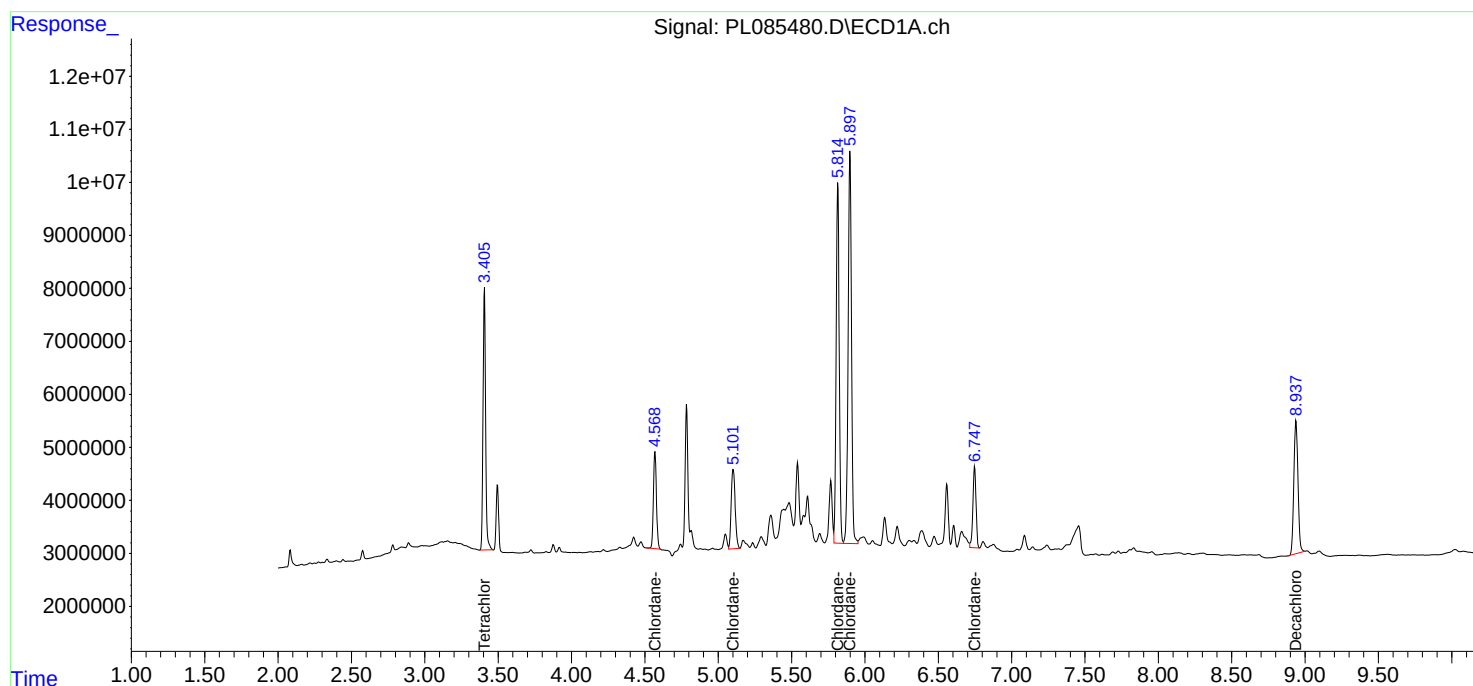


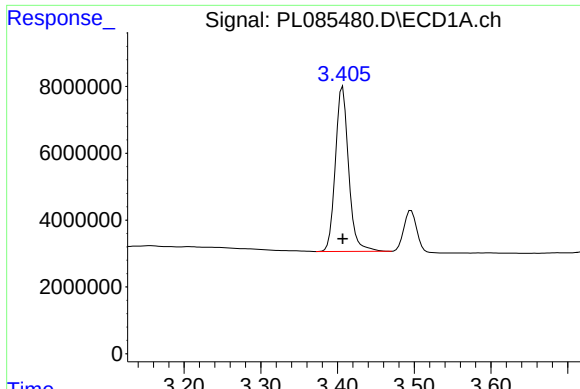

#1 Tetrachloro-m-xylene


R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 59209599
Conc: 24.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

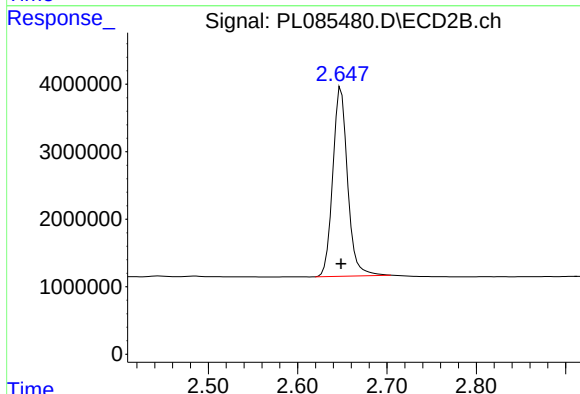


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 32313941
Conc: 24.37 ng/ml

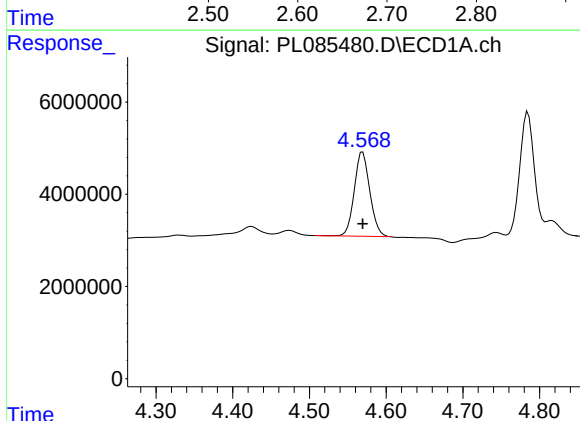


#23 Chlordane-1

R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 25868497
Conc: 251.46 ng/ml

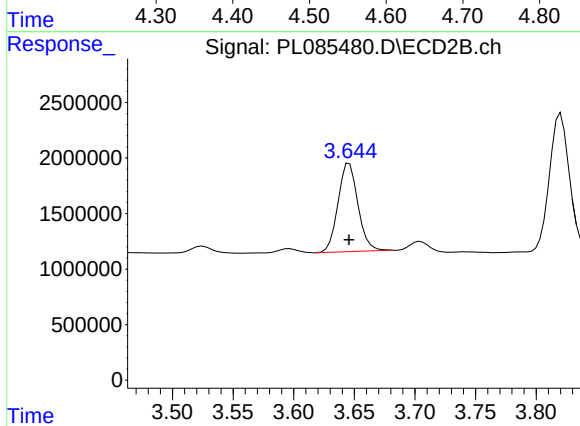

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 9120788
Conc: 244.24 ng/ml

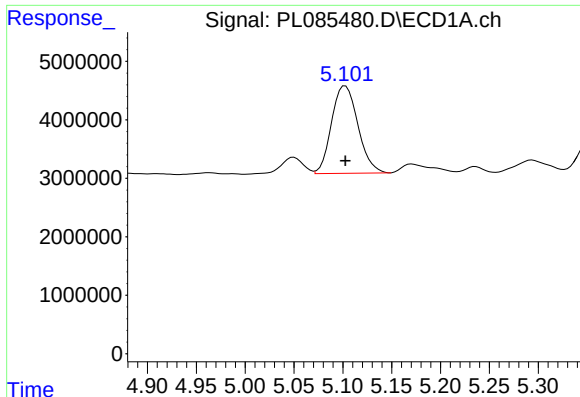

#24 Chlordane-2


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 28114324
Conc: 262.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

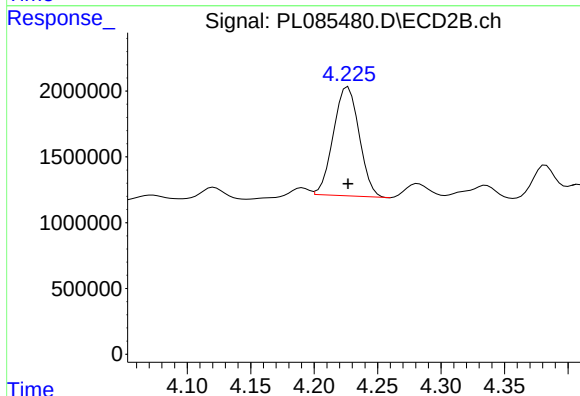


#24 Chlordane-2

R.T.: 4.227 min
Delta R.T.: 0.000 min
Response: 11719271
Conc: 256.91 ng/ml

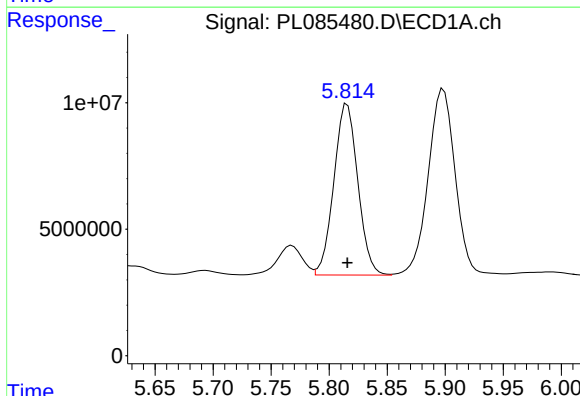


#25 Chlordane-3

R.T.: 5.816 min
Delta R.T.: 0.000 min
Response: 97192680
Conc: 244.63 ng/ml

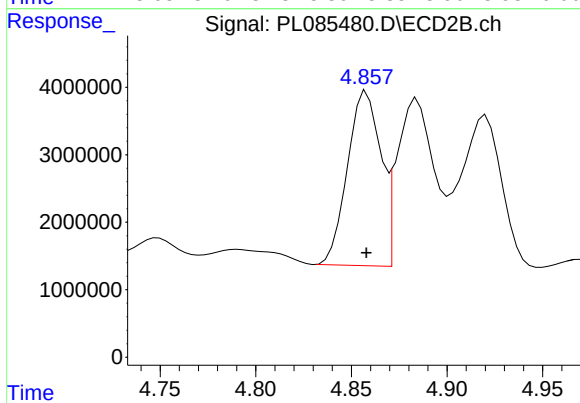

#25 Chlordane-3


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 31277235
Conc: 238.13 ng/ml

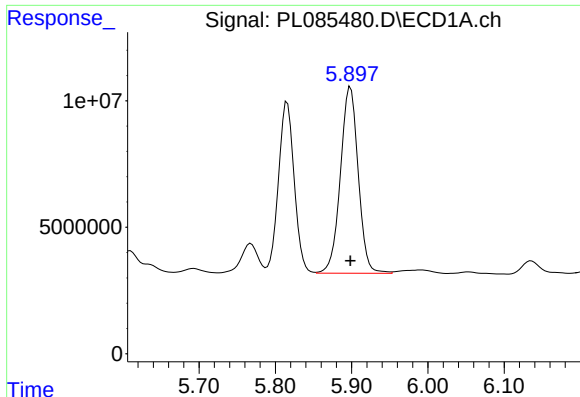

#26 Chlordane-4


R.T.: 5.899 min
Delta R.T.: 0.000 min
Response: 119504947
Conc: 247.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

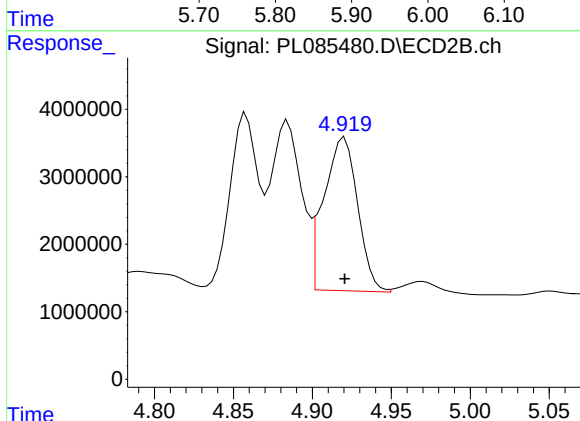


#26 Chlordane-4

R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 33719810
Conc: 236.61 ng/ml

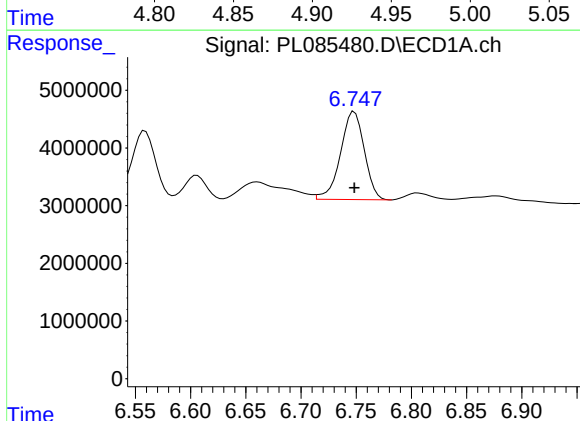


#27 Chlordane-5

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 22957789
Conc: 260.90 ng/ml

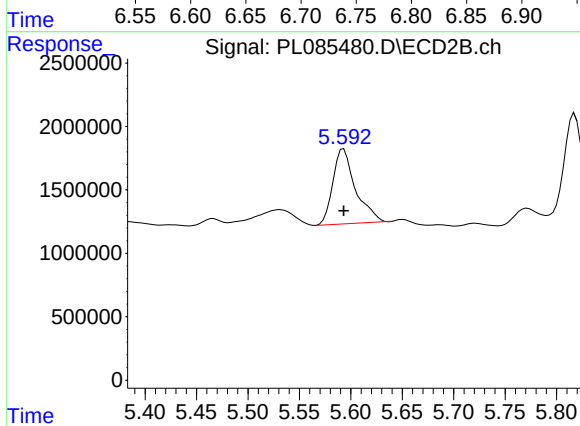

#27 Chlordane-5


R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 9064405
Conc: 241.78 ng/ml

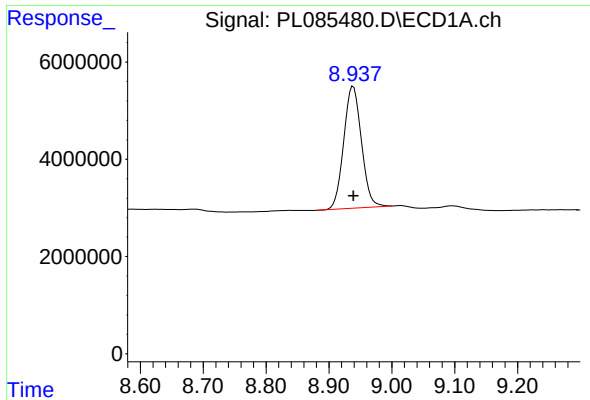

#28 Decachlorobiphenyl

R.T.: 8.939 min
Delta R.T.: 0.000 min
Response: 48945931
Conc: 26.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

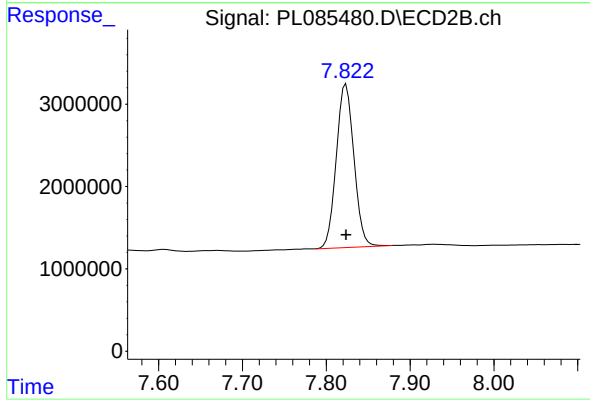

#28 Decachlorobiphenyl

R.T.: 7.824 min
Delta R.T.: 0.000 min
Response: 29034846
Conc: 25.78 ng/ml