

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
 Data File : PL085481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 16:24
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 25 16:34:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 25 16:34:46 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.407	2.649	12630949	6714276	5.234	5.050
28)	SA Decachlor...	8.938	7.823	12040711	6345655	6.174	5.495
Target Compounds							
23)	Chlordane-1	4.569	3.646	5470138	1869958	52.507	50.060
24)	Chlordane-2	5.102	4.226	6301795	2464530	56.781	53.170
25)	Chlordane-3	5.816	4.857	20993843	6009660	52.248	46.546
26)	Chlordane-4	5.898	4.920	25958798	6547324	53.033	46.701
27)	Chlordane-5	6.748	5.592	5473876	1792806	59.310	48.241



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
Data File : PL085481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 16:24
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 25 16:34:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Mon Sep 25 16:34:46 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

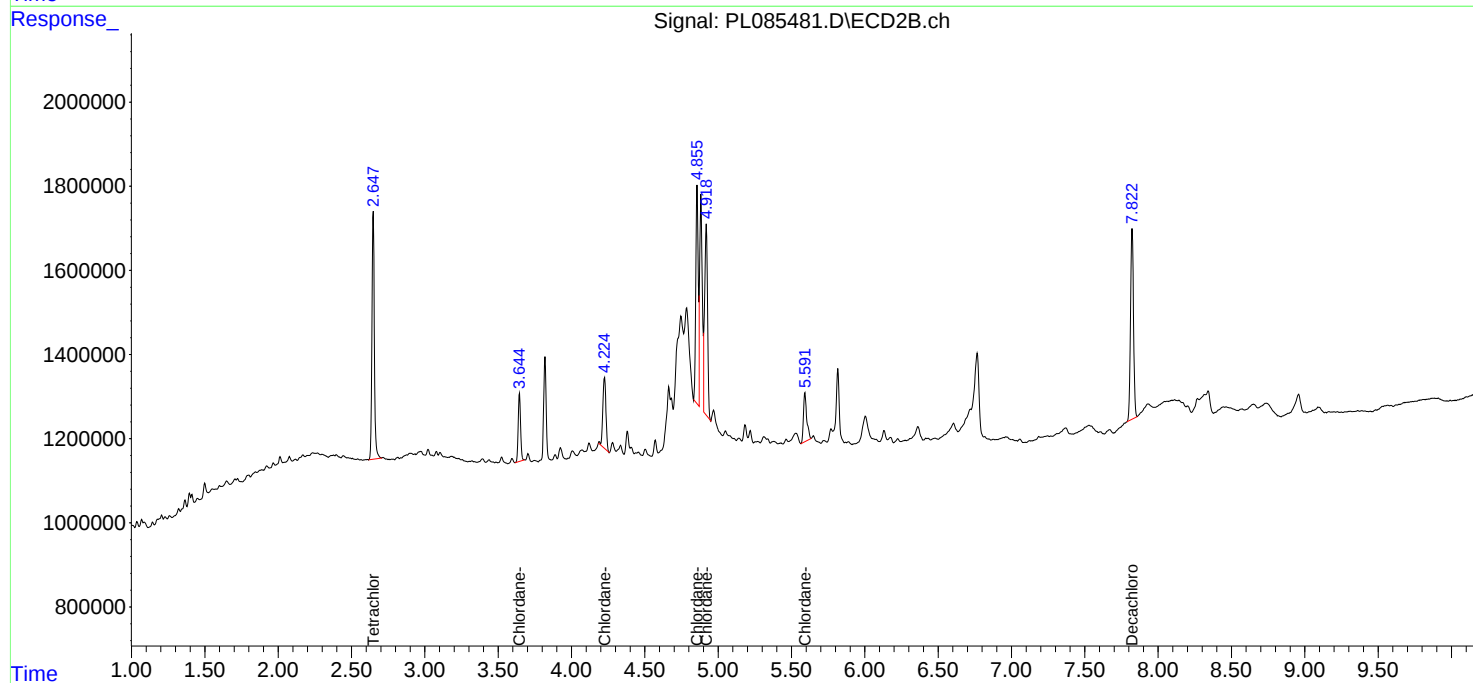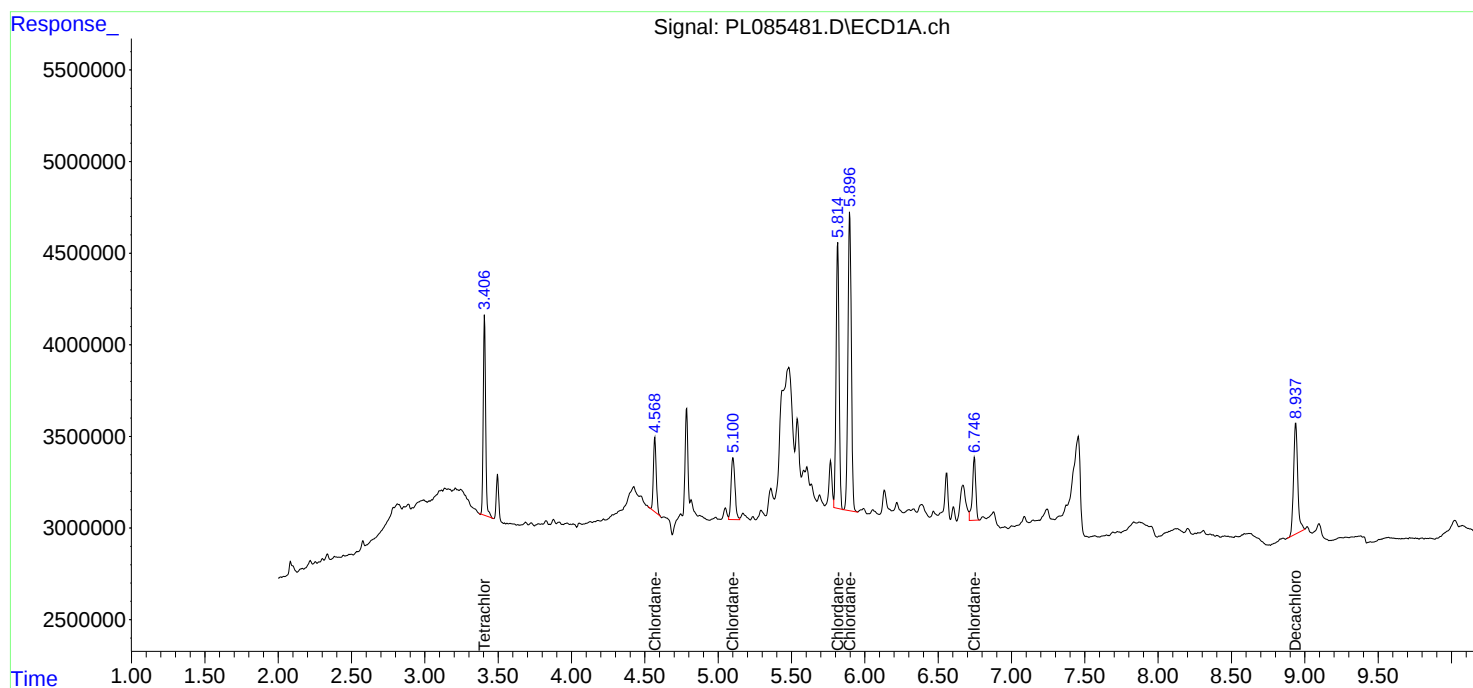


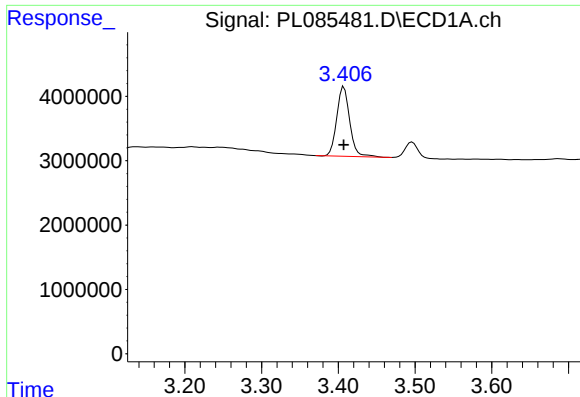

#1 Tetrachloro-m-xylene


R.T.: 3.407 min
Delta R.T.: 0.000 min
Response: 12630949
Conc: 5.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

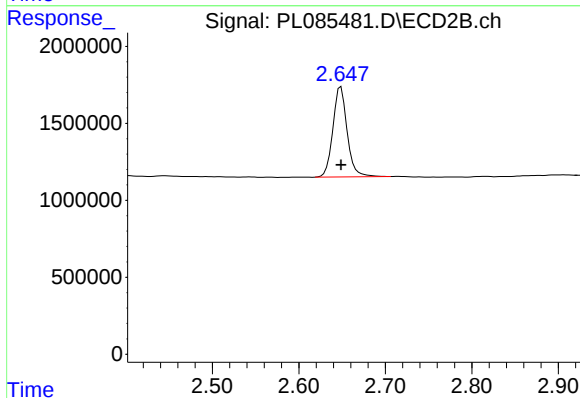


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 6714276
Conc: 5.05 ng/ml

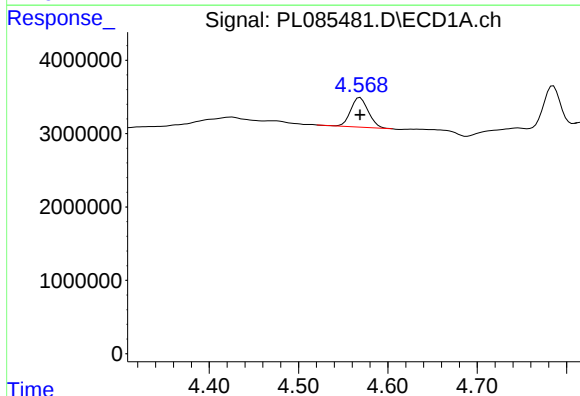


#23 Chlordane-1

R.T.: 4.569 min
Delta R.T.: 0.000 min
Response: 5470138
Conc: 52.51 ng/ml

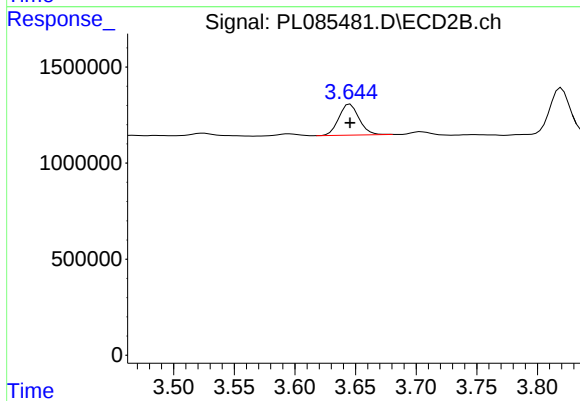

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 1869958
Conc: 50.06 ng/ml

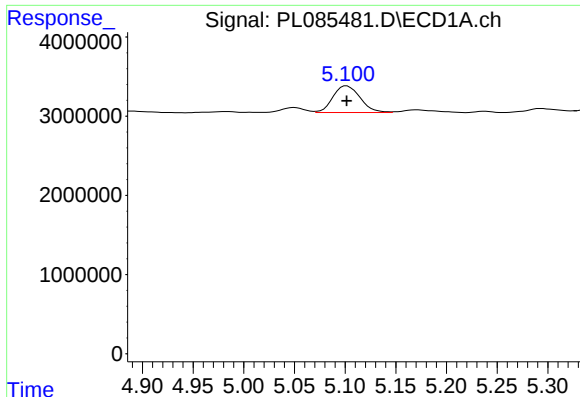

#24 Chlordane-2


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 6301795
Conc: 56.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

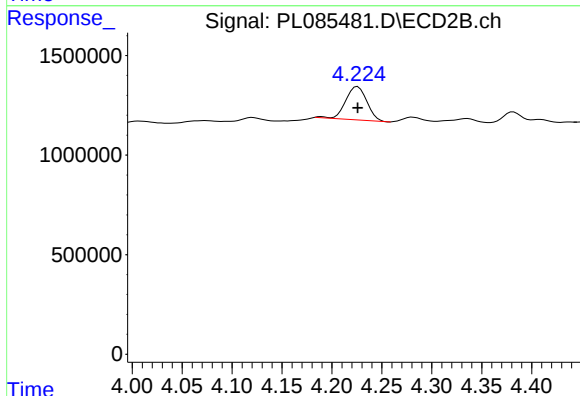


#24 Chlordane-2

R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 2464530
Conc: 53.17 ng/ml

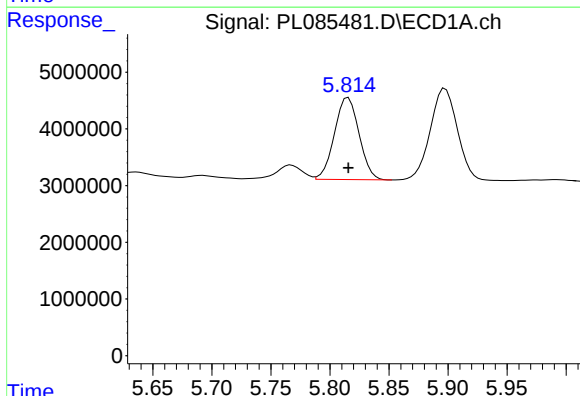


#25 Chlordane-3

R.T.: 5.816 min
Delta R.T.: 0.000 min
Response: 20993843
Conc: 52.25 ng/ml

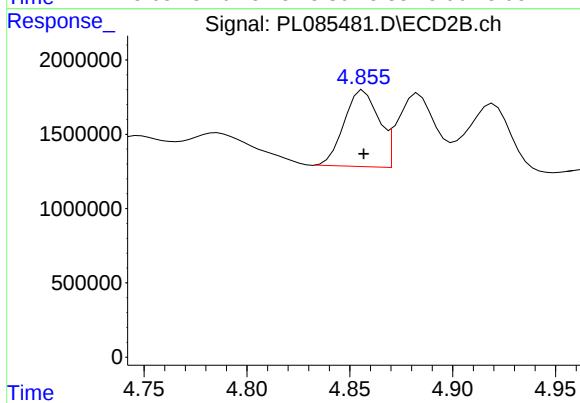

#25 Chlordane-3


R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 6009660
Conc: 46.55 ng/ml

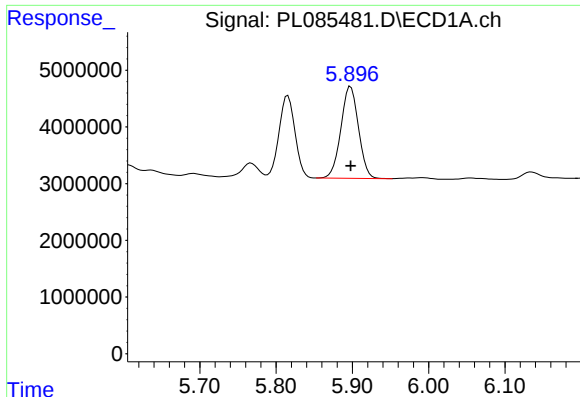

#26 Chlordane-4


R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 25958798
Conc: 53.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

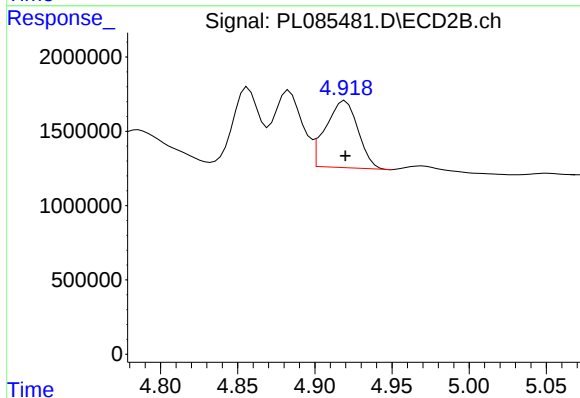


#26 Chlordane-4

R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 6547324
Conc: 46.70 ng/ml

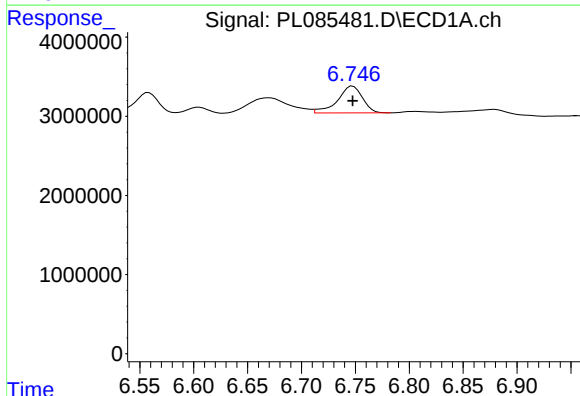


#27 Chlordane-5

R.T.: 6.748 min
Delta R.T.: 0.000 min
Response: 5473876
Conc: 59.31 ng/ml

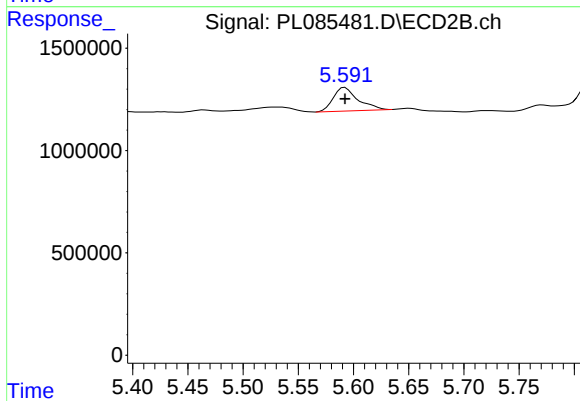

#27 Chlordane-5


R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 1792806
Conc: 48.24 ng/ml

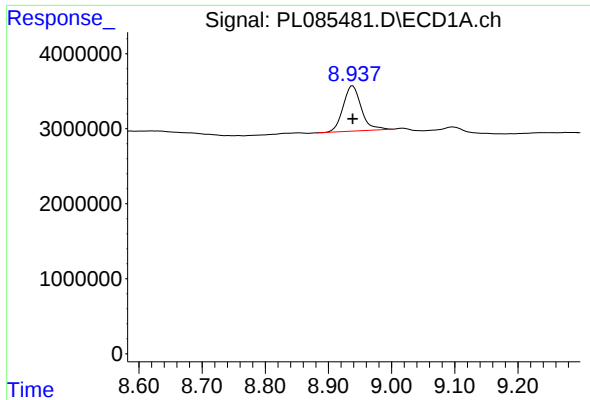

#28 Decachlorobiphenyl

R.T.: 8.938 min
Delta R.T.: 0.000 min
Response: 12040711
Conc: 6.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

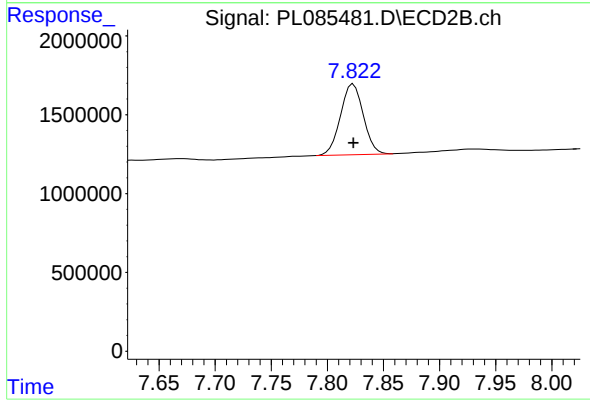

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 6345655
Conc: 5.49 ng/ml