

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
 Data File : PL085488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2023 19:56
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL092523

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 01:23:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 26 01:21:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.414	2.649	118.6E6	66156779	49.132	49.759
28)	SA Decachlor...	8.941	7.823	93144037	57342284	47.760	49.653
Target Compounds							
23)	Chlordane-1	4.576	3.646	48743976	18529056	467.886	496.038
24)	Chlordane-2	5.108	4.226	53030102	22814849	477.814	492.211
25)	Chlordane-3	5.820	4.857	190.8E6	65220039	474.834	505.140
26)	Chlordane-4	5.903	4.920	232.2E6	70898489	474.475	505.705
27)	Chlordane-5	6.751	5.592	42645785	18542752	462.075	498.950



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092523\
Data File : PL085488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2023 19:56
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL092523

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 01:23:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092523.M
Quant Title : GC Extractables
QLast Update : Tue Sep 26 01:21:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

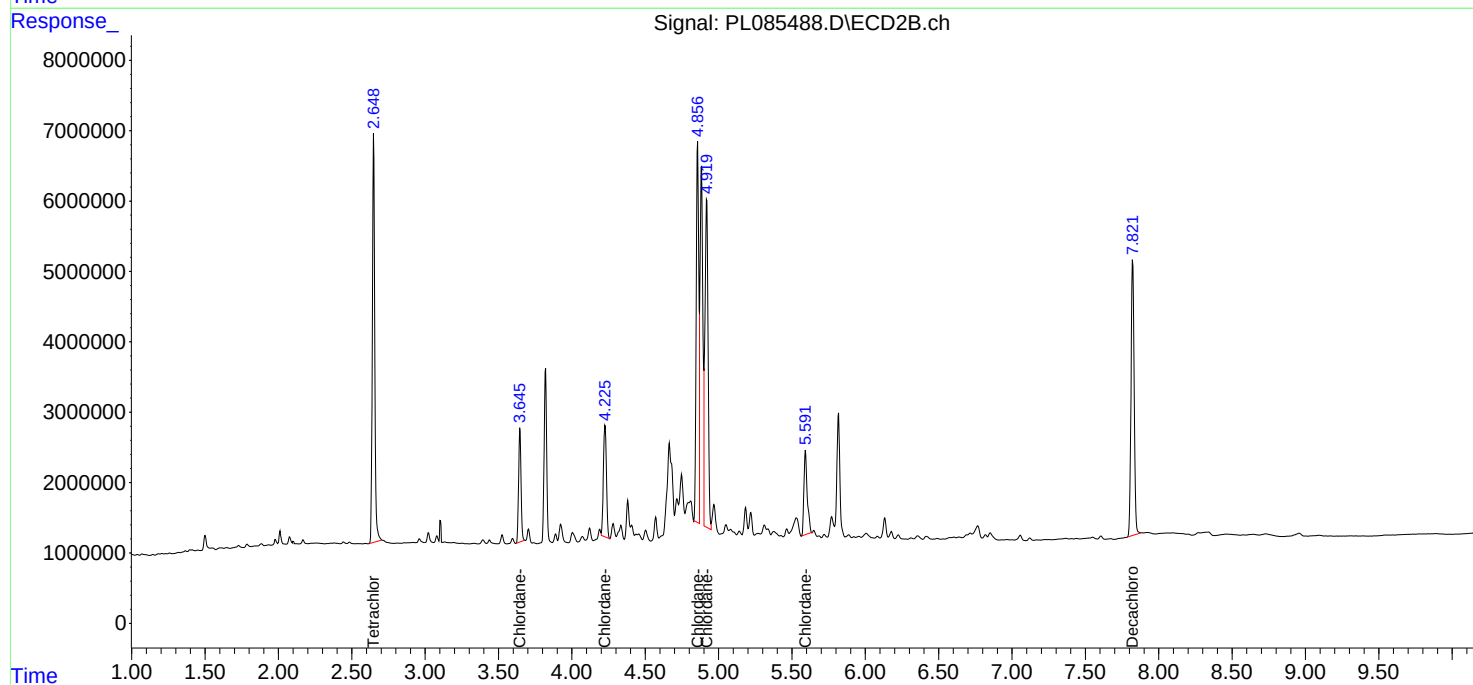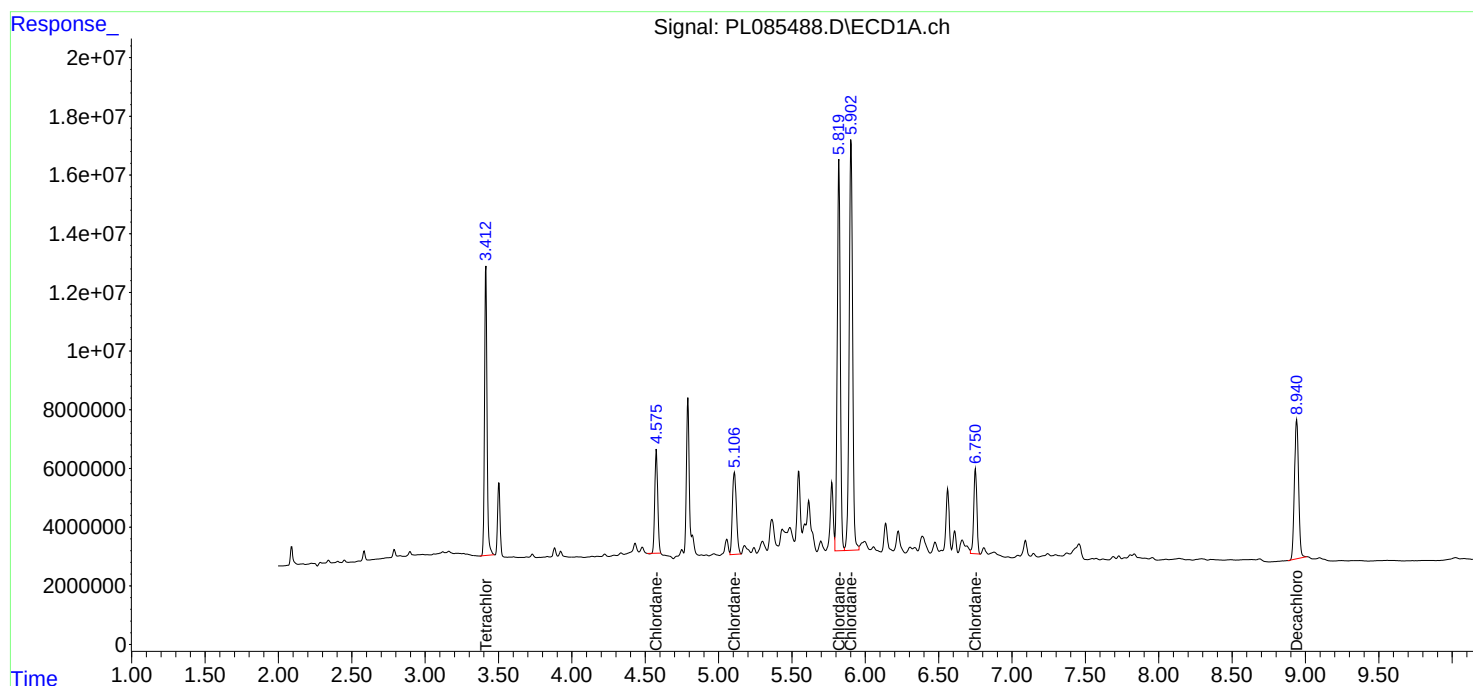


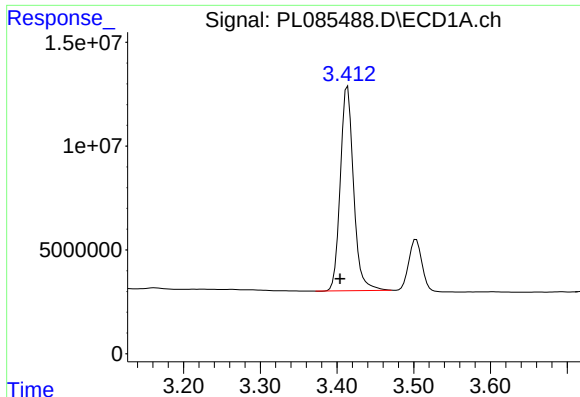

#1 Tetrachloro-m-xylene


R.T.: 3.414 min
Delta R.T.: 0.010 min
Response: 118558394
Conc: 49.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092523

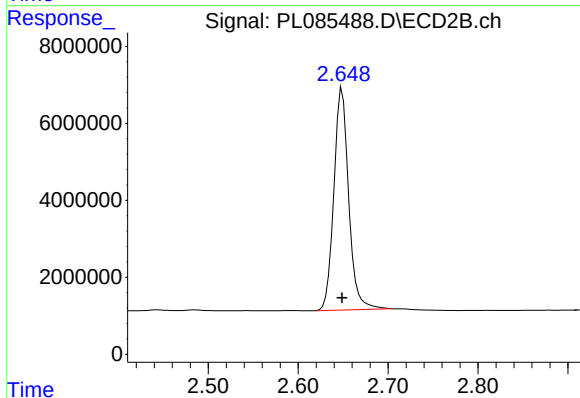


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 66156779
Conc: 49.76 ng/ml

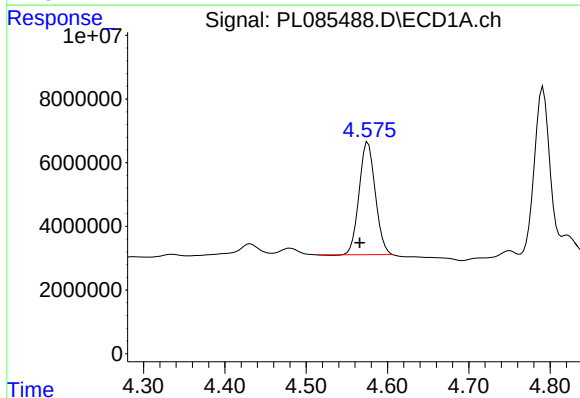


#23 Chlordane-1

R.T.: 4.576 min
Delta R.T.: 0.010 min
Response: 48743976
Conc: 467.89 ng/ml

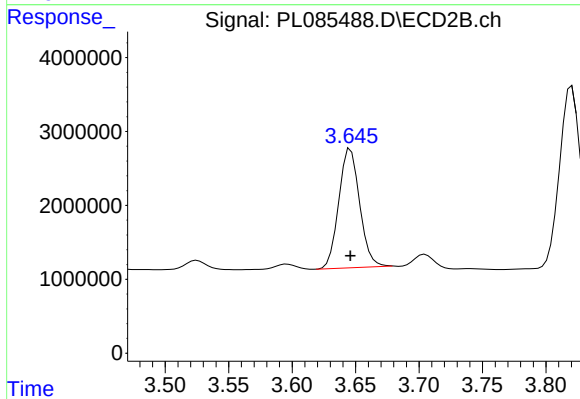

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 18529056
Conc: 496.04 ng/ml

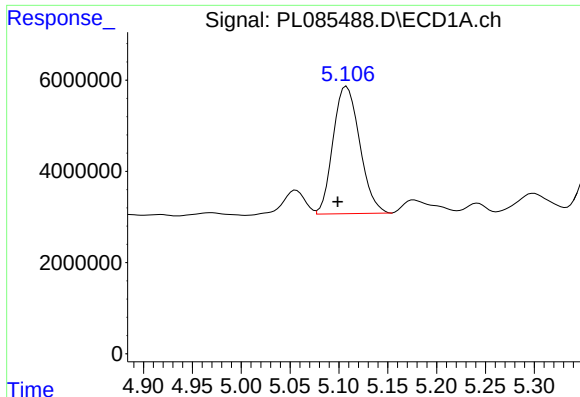

#24 Chlordane-2


R.T.: 5.108 min
Delta R.T.: 0.009 min
Response: 53030102
Conc: 477.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092523

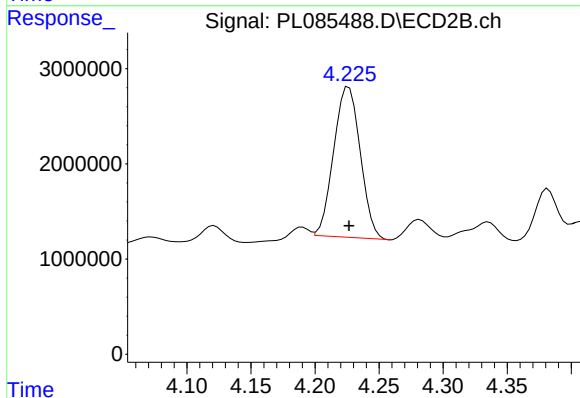


#24 Chlordane-2

R.T.: 4.226 min
Delta R.T.: 0.000 min
Response: 22814849
Conc: 492.21 ng/ml

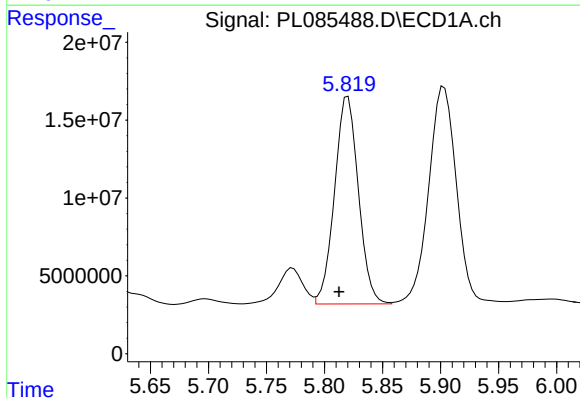


#25 Chlordane-3

R.T.: 5.820 min
Delta R.T.: 0.008 min
Response: 190794959
Conc: 474.83 ng/ml

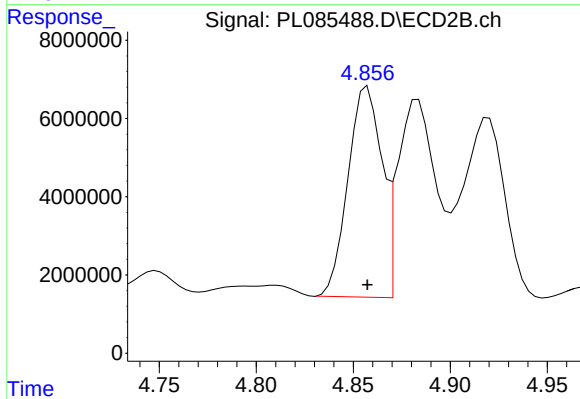

#25 Chlordane-3


R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 65220039
Conc: 505.14 ng/ml

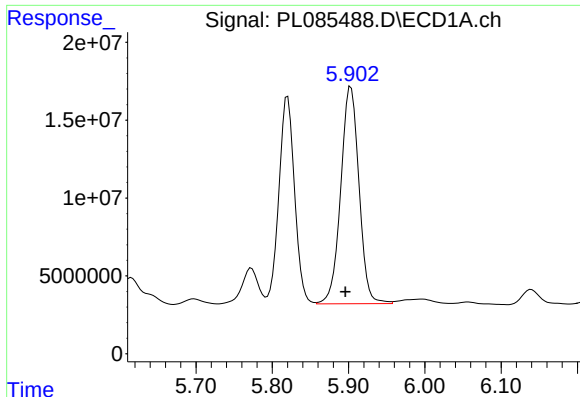

#26 Chlordane-4


R.T.: 5.903 min
Delta R.T.: 0.007 min
Response: 232249750
Conc: 474.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092523

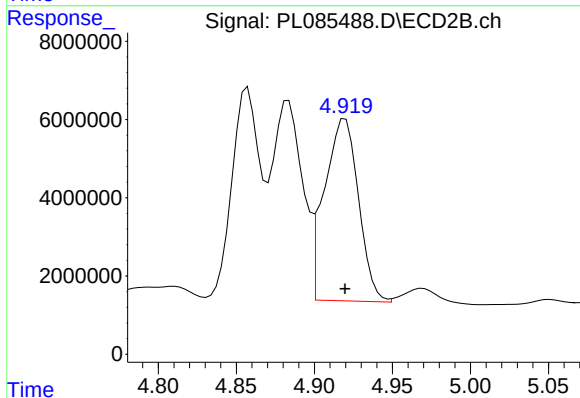


#26 Chlordane-4

R.T.: 4.920 min
Delta R.T.: 0.000 min
Response: 70898489
Conc: 505.71 ng/ml

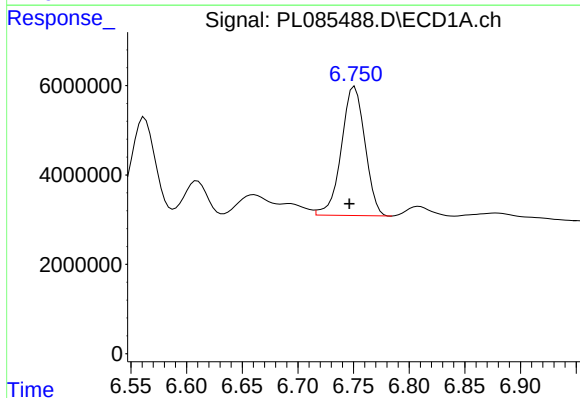


#27 Chlordane-5

R.T.: 6.751 min
Delta R.T.: 0.005 min
Response: 42645785
Conc: 462.08 ng/ml

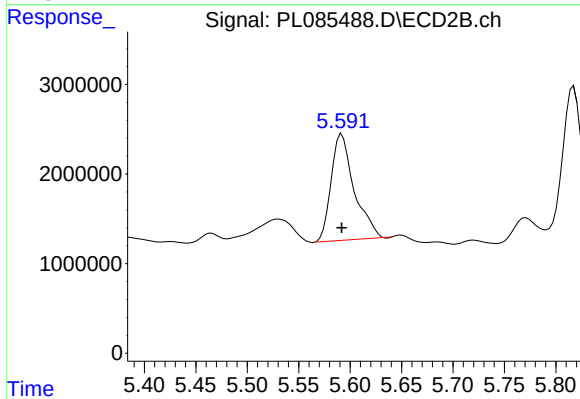

#27 Chlordane-5


R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 18542752
Conc: 498.95 ng/ml

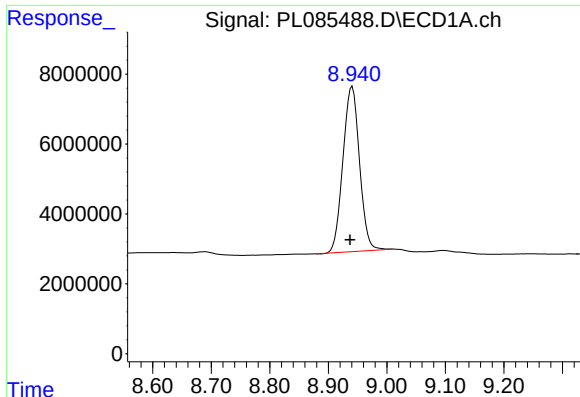

#28 Decachlorobiphenyl

R.T.: 8.941 min
Delta R.T.: 0.004 min
Response: 93144037
Conc: 47.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL092523

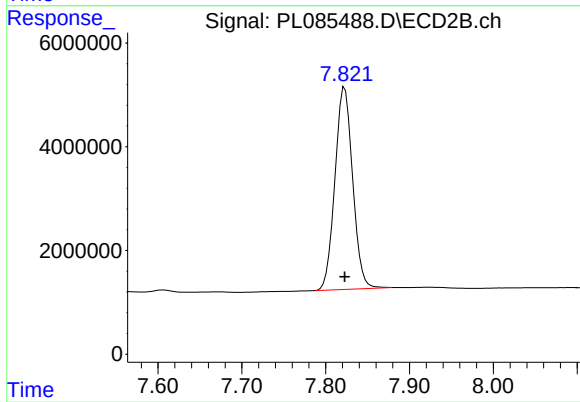

#28 Decachlorobiphenyl

R.T.: 7.823 min
Delta R.T.: 0.000 min
Response: 57342284
Conc: 49.65 ng/ml