

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 11:45
 Operator : AR\AJ
 Sample : P3879-05DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC59DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/26/2024
 Supervised By : Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:07:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.796	75754430	3444.8E6	43.374m	1618.413m#
2) SA Decachlor...	9.059	7.922	5627585	9113104	4.188	4.283
Target Compounds						
2) A alpha-BHC	3.999	3.285	133.3E6	163.9E6	52.479	54.763
5) MB Aldrin	5.276	4.246	11360202	11846250	5.060	4.525m
7) B delta-BHC	4.776	4.144	158.1E6	195.1E6	64.790	67.678
16) A 4,4'-DDD	6.695	5.795	1629966	2439645	1.143m	1.335m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 11:45
Operator : AR\AJ
Sample : P3879-05DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:07:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

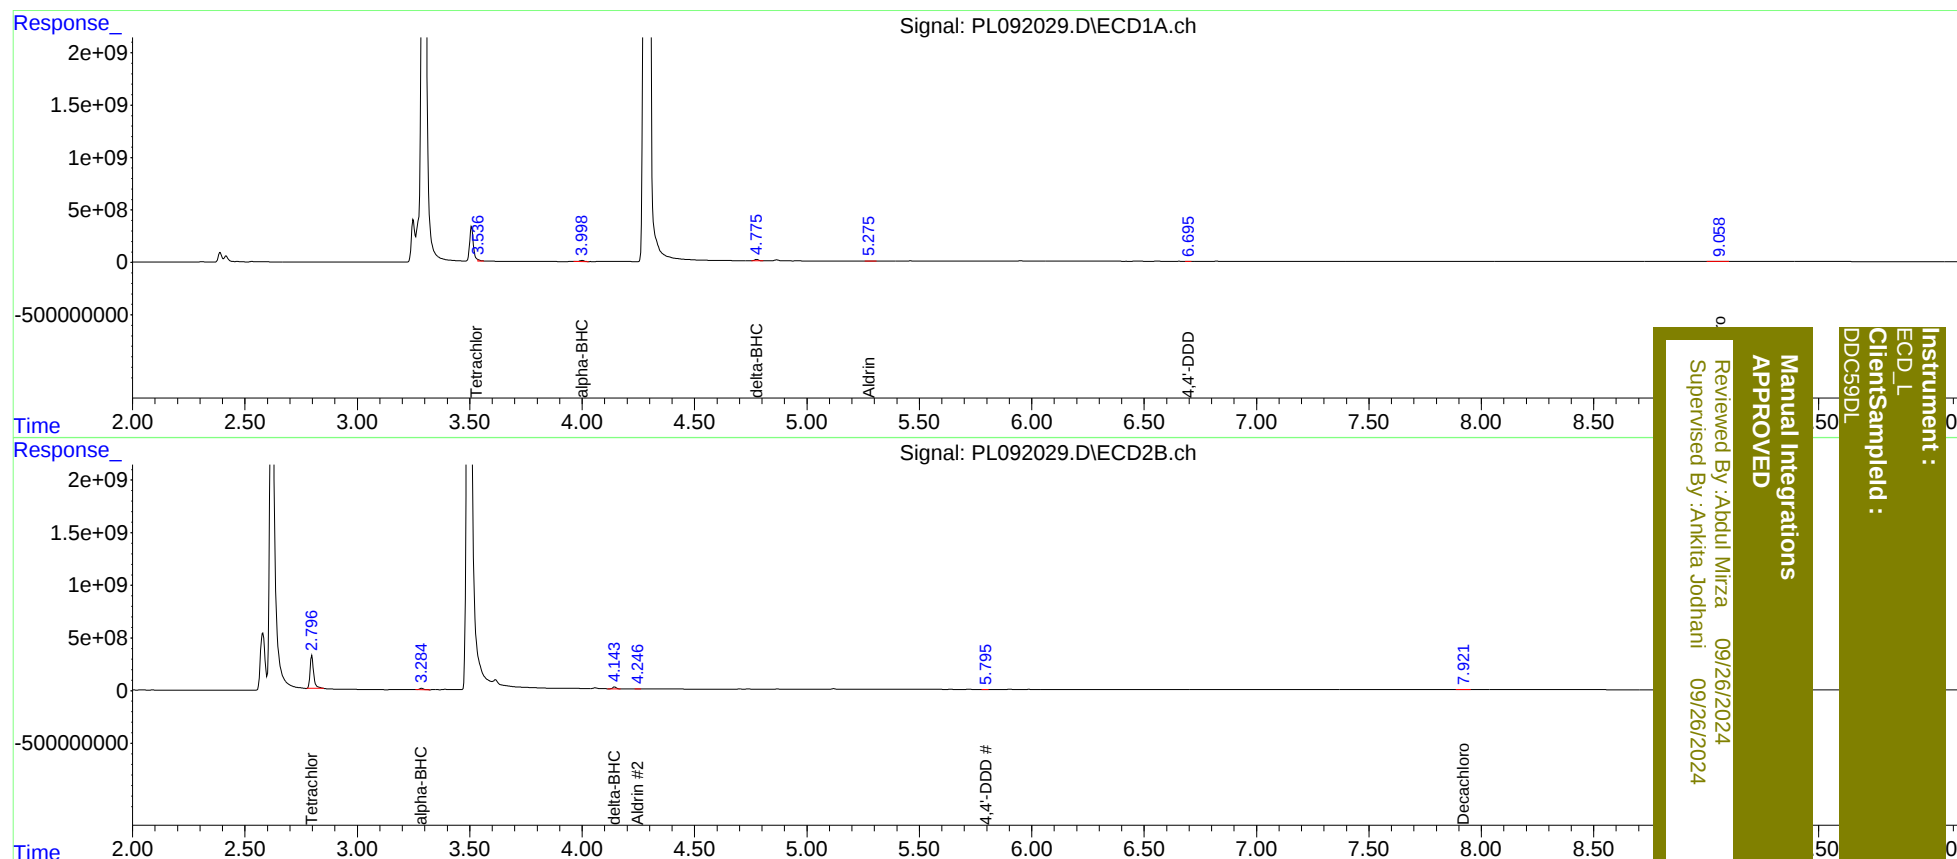

Instrument :
ECD_L
ClientSampled :
DDC59DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/26/2024
Supervised By :Ankita Jodhani 09/26/2024