

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 11:59
 Operator : AR\AJ
 Sample : P3879-08DL 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC78DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/26/2024
 Supervised By : Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:07:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.796	44493051	2210.2E6	25.475m	1038.365m#
2) SA Decachlor...	9.057	7.921	4380873	7598287	3.260m	3.571m
Target Compounds						
2) A alpha-BHC	4.000	3.285	143.1E6	189.0E6	56.315	63.149
5) MB Aldrin	5.277	4.247	12622135	10942606	5.622	4.180 #
7) B delta-BHC	4.774	4.143	176.8E6	183.9E6	72.425m	63.778m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 11:59
Operator : AR\AJ
Sample : P3879-08DL 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:07:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

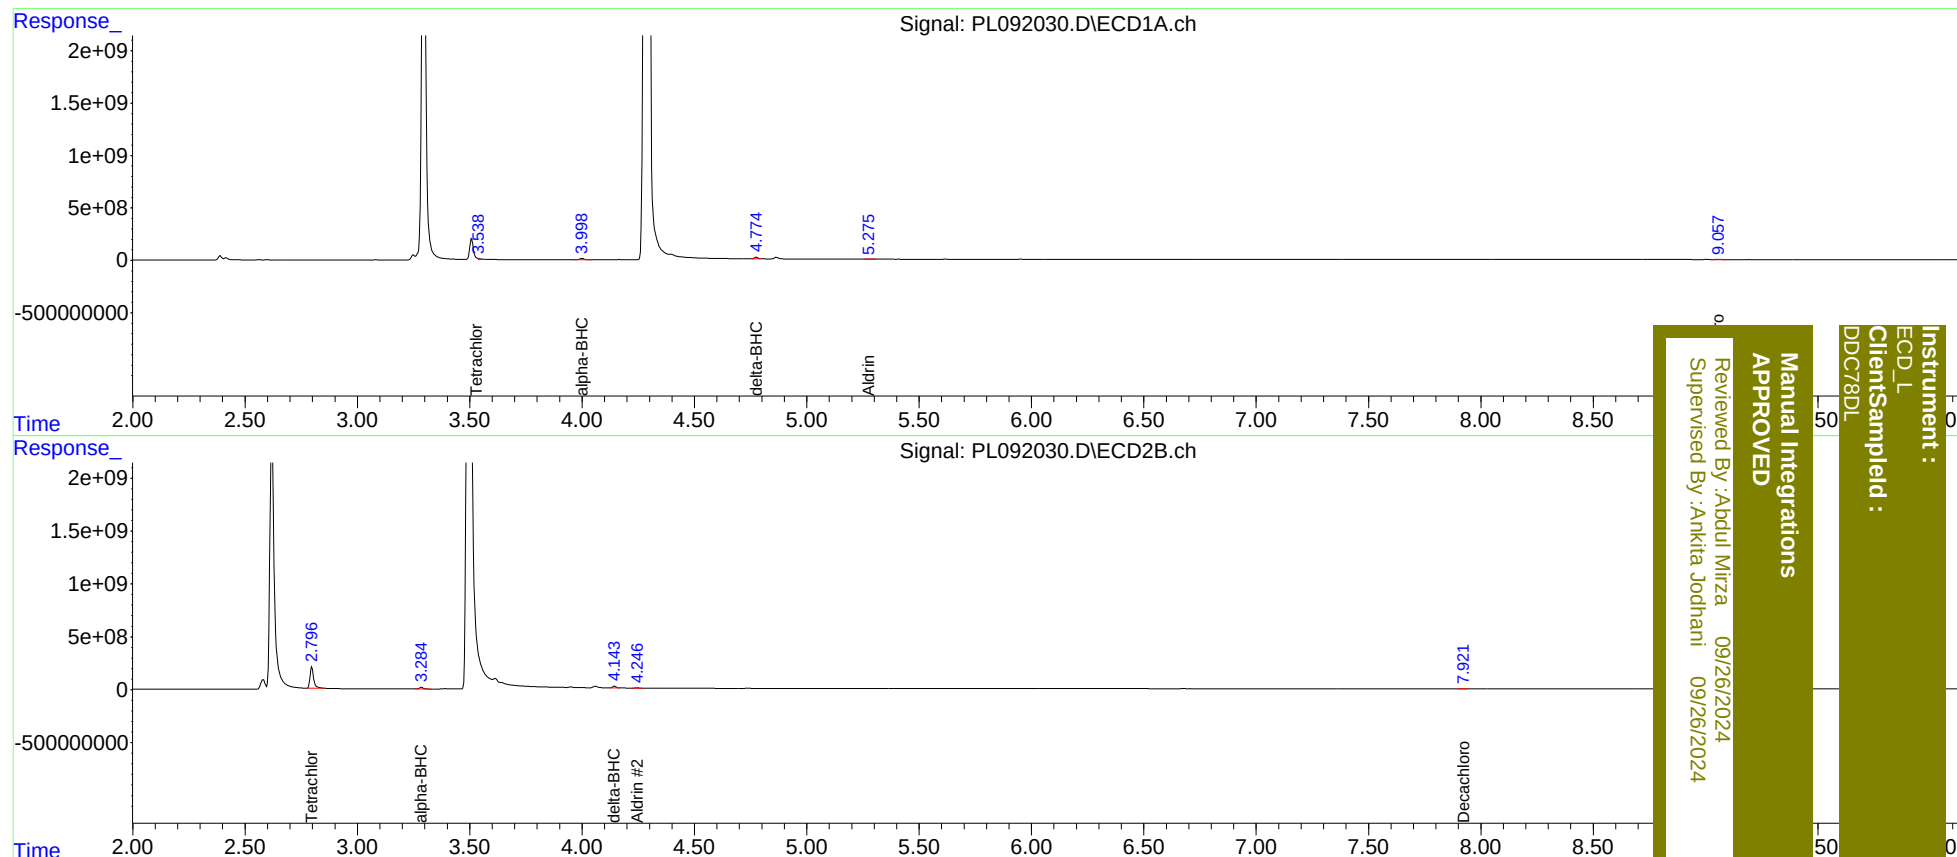

Reviewed By: Abdul Mirza 09/26/2024
Supervised By: Ankita Jodhani 09/26/2024

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
DDC78DL