

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 13:33
 Operator : AR\AJ
 Sample : P3879-15DL 3X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC33DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/26/2024
 Supervised By : Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:09:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.796	75000338	145.9E6	42.942m	68.555m#
2)	SA Decachlor...	9.060	7.922	8239363	17724779	6.132m	8.330 #
Target Compounds							
2)	A alpha-BHC	3.999	3.286	171.1E6	205.7E6	67.345	68.751
7)	B delta-BHC	4.775	4.143	188.1E6	190.1E6	77.082m	65.912m
16)	A 4,4'-DDD	6.695	5.797	9418475	16889673	6.607m	9.241m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 13:33
Operator : AR\AJ
Sample : P3879-15DL 3X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:09:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

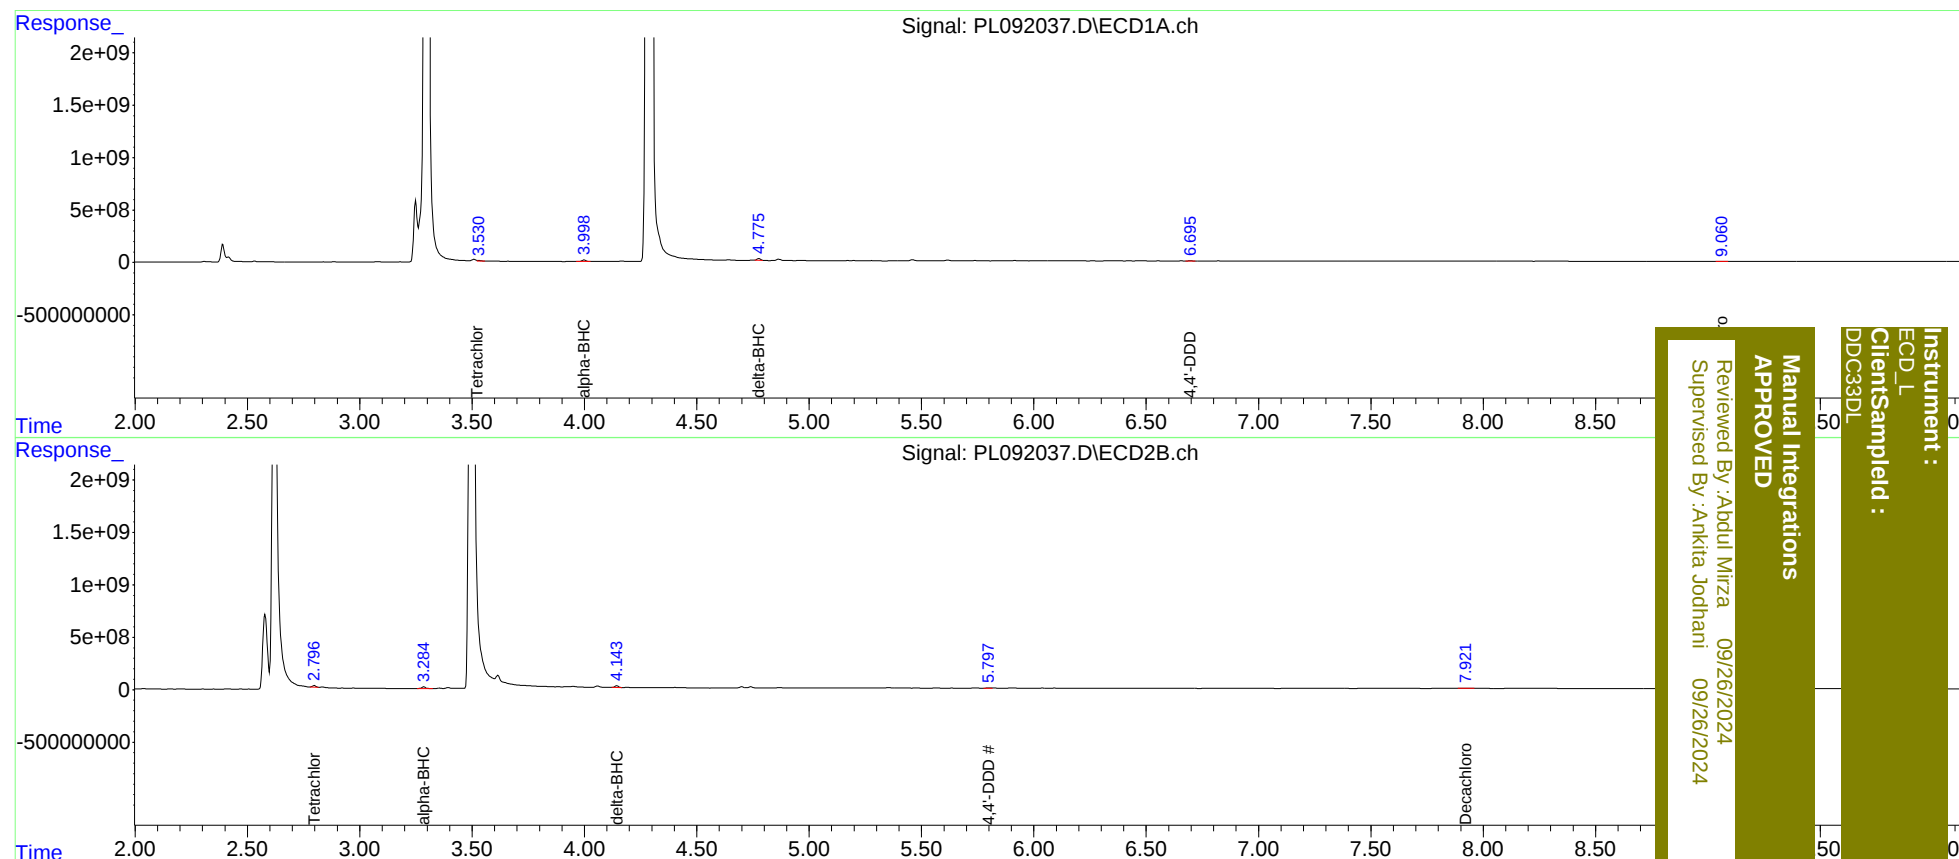

Instrument :
ECD_L
ClientSampled :
DDC33DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/26/2024
Supervised By :Ankita Jodhani 09/26/2024