

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 12:52
 Operator : AR\AJ
 Sample : P3879-11DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DCVZ9DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/26/2024
 Supervised By : Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:08:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.796	110.1E6	12140.6E6	63.023m	5703.846m#
2) SA Decachlor...	9.056	7.922	3404857	6286104	2.534m	2.954m
Target Compounds						
2) A alpha-BHC	3.999	3.285	96746505	123.7E6	38.075	41.329
6) B beta-BHC	4.527	3.915	4848561	8121740	4.188m	6.268m#
7) B delta-BHC	4.775	4.143	131.4E6	129.7E6	53.841m	44.994m
16) A 4,4'-DDD	6.696	5.797	28859744	40817525	20.246m	22.333m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 12:52
Operator : AR\AJ
Sample : P3879-11DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:08:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

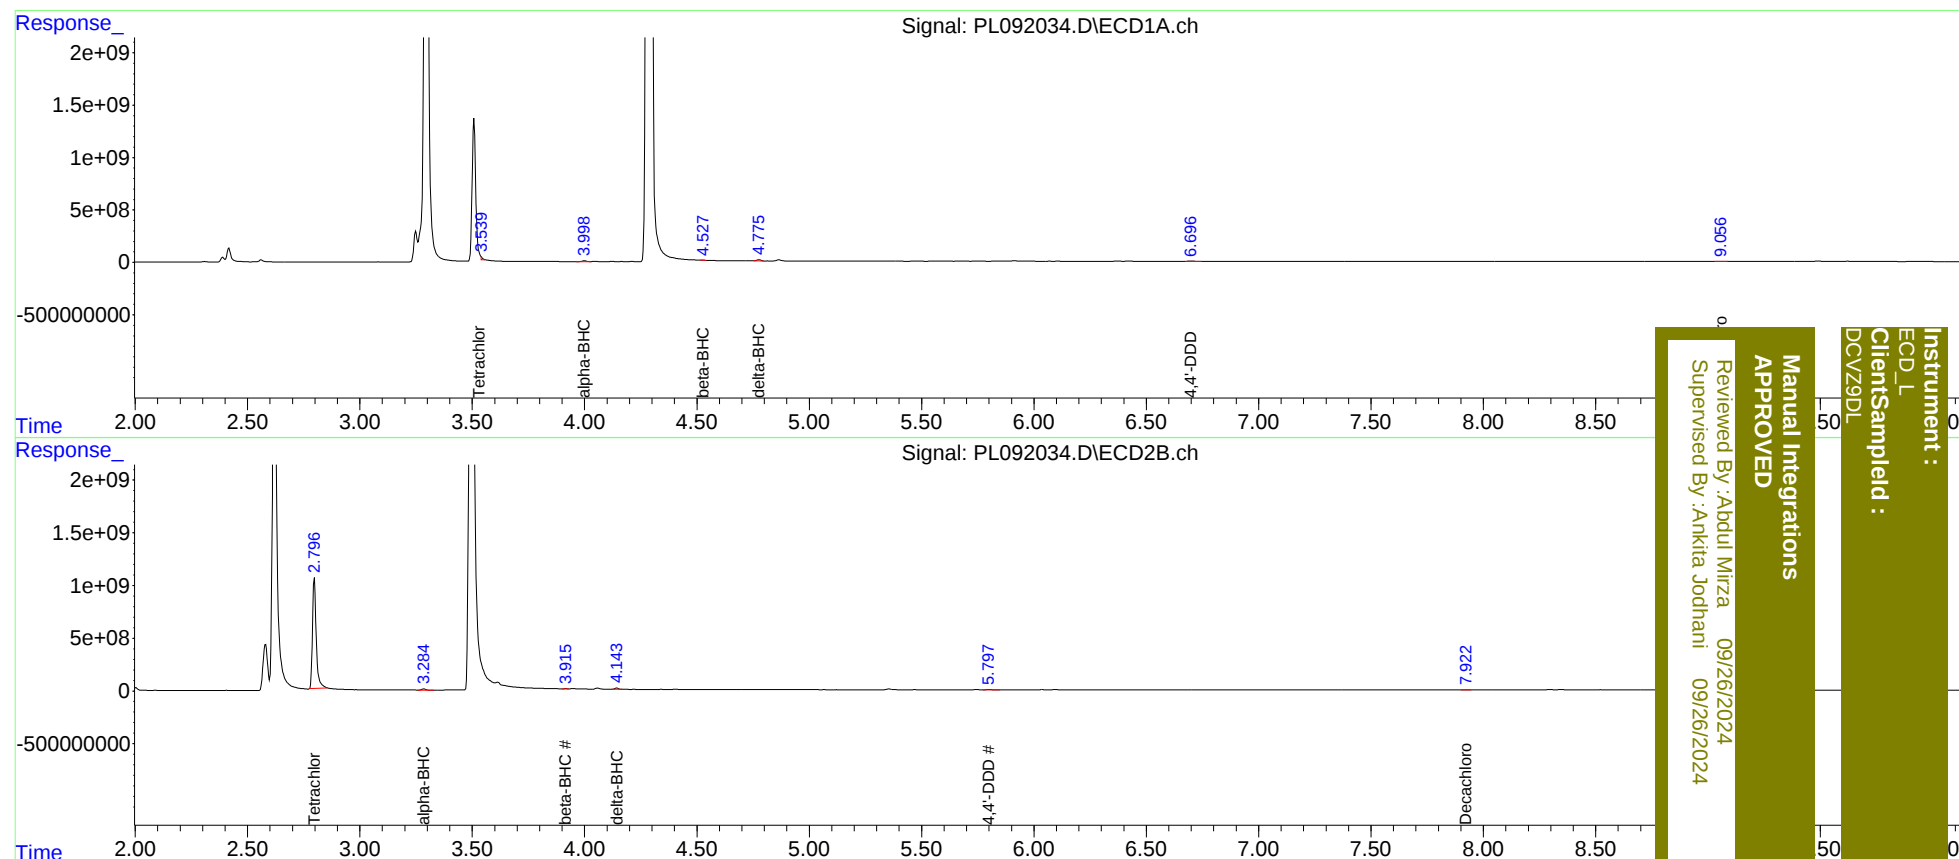

Instrument :
ECD_L
ClientSampled :
DCVZ9DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/26/2024
Supervised By :Ankita Jodhani 09/26/2024