

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
 Data File : PL092035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Sep 2024 13:06
 Operator : AR\AJ
 Sample : P3879-12DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DDC53DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/26/2024
 Supervised By :Ankita Jodhani 09/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 26 02:08:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 07:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.534	2.797	7597585	315.5E6	4.350m	148.237m#
Target Compounds						
2) A alpha-BHC	3.999	3.286	153.0E6	173.2E6	60.217	57.879
3) MA gamma-BHC...	4.324	3.613	775.5E6	213.1E6	315.394m	76.300m#
6) B beta-BHC	4.529	3.913	13751705	8231665	11.878m	6.353m#
7) B delta-BHC	4.776	4.144	146.7E6	179.6E6	60.125	62.295

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL092524\
Data File : PL092035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Sep 2024 13:06
Operator : AR\AJ
Sample : P3879-12DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 26 02:08:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092024CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 07:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

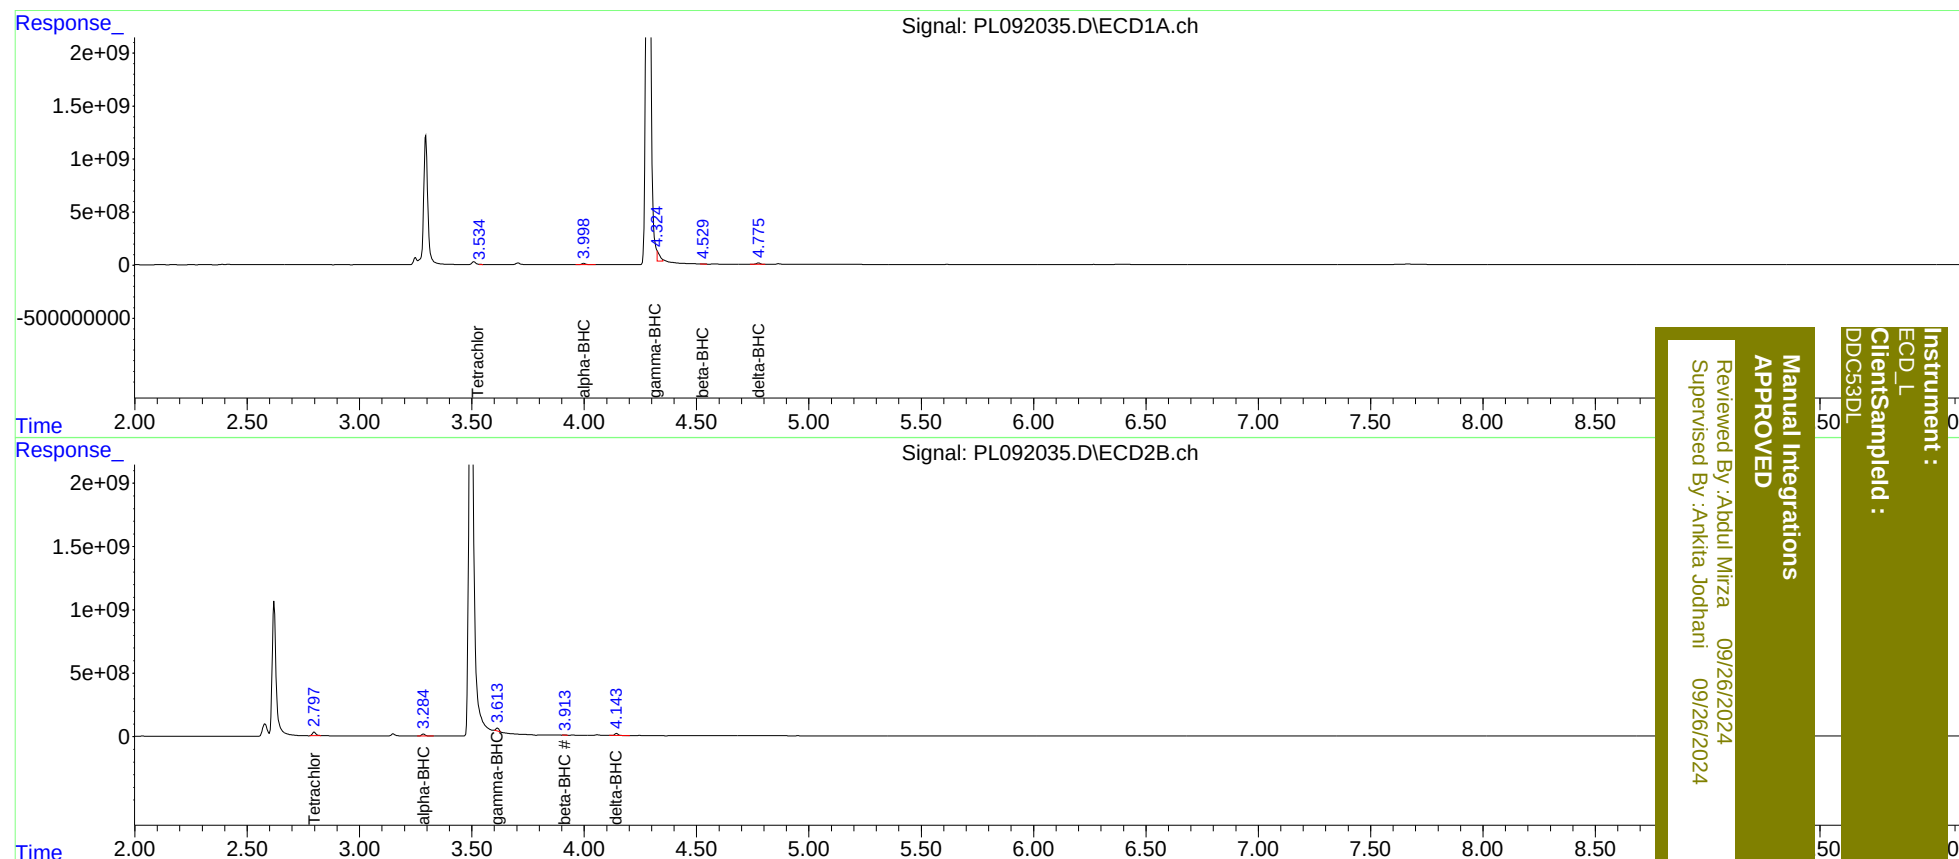

Instrument :
ECD_L
ClientSampled :
DDC53DL

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/26/2024
Supervised By :Ankita Jodhani 09/26/2024